


Data Path : Z:\HPCHEM1\BNA E\DATA\BE100716\
 Data File : BE092442.D
 Acq On : 7 Oct 2016 11:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 22 18:25:56 2016

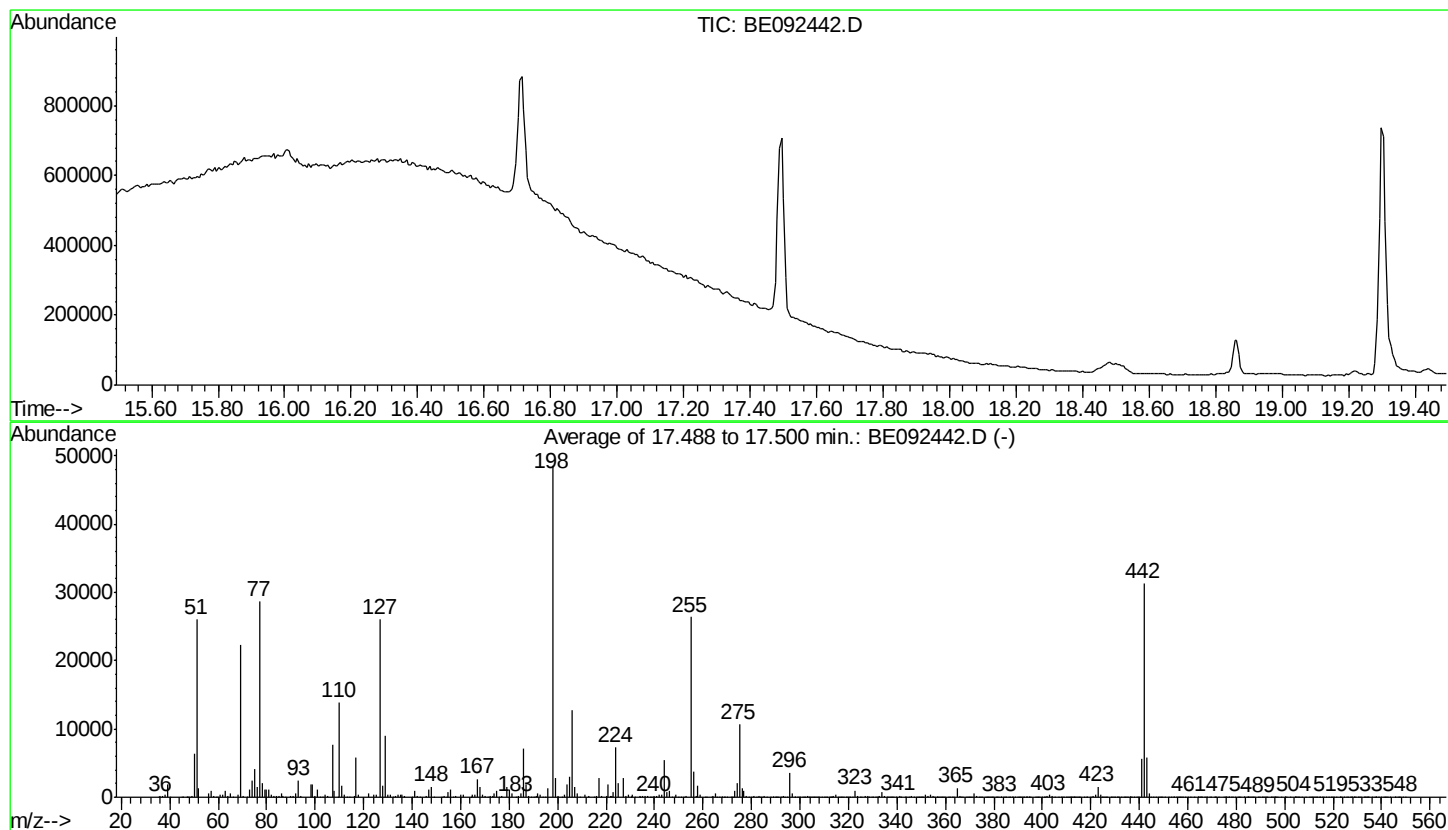

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.6	25998	PASS
68	69	0.00	2	1.9	428	PASS
69	198	0.00	100	46.1	22372	PASS
70	69	0.00	2	0.6	127	PASS
127	198	10	80	53.6	25997	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48534	PASS
199	198	5	9	5.9	2868	PASS
275	198	10	60	21.9	10605	PASS
365	198	1	100	2.9	1390	PASS
441	442	0.01	24	17.9	5605	PASS
442	198	50	100	64.4	31276	PASS
443	442	15	24	18.6	5803	PASS