

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:22:31 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

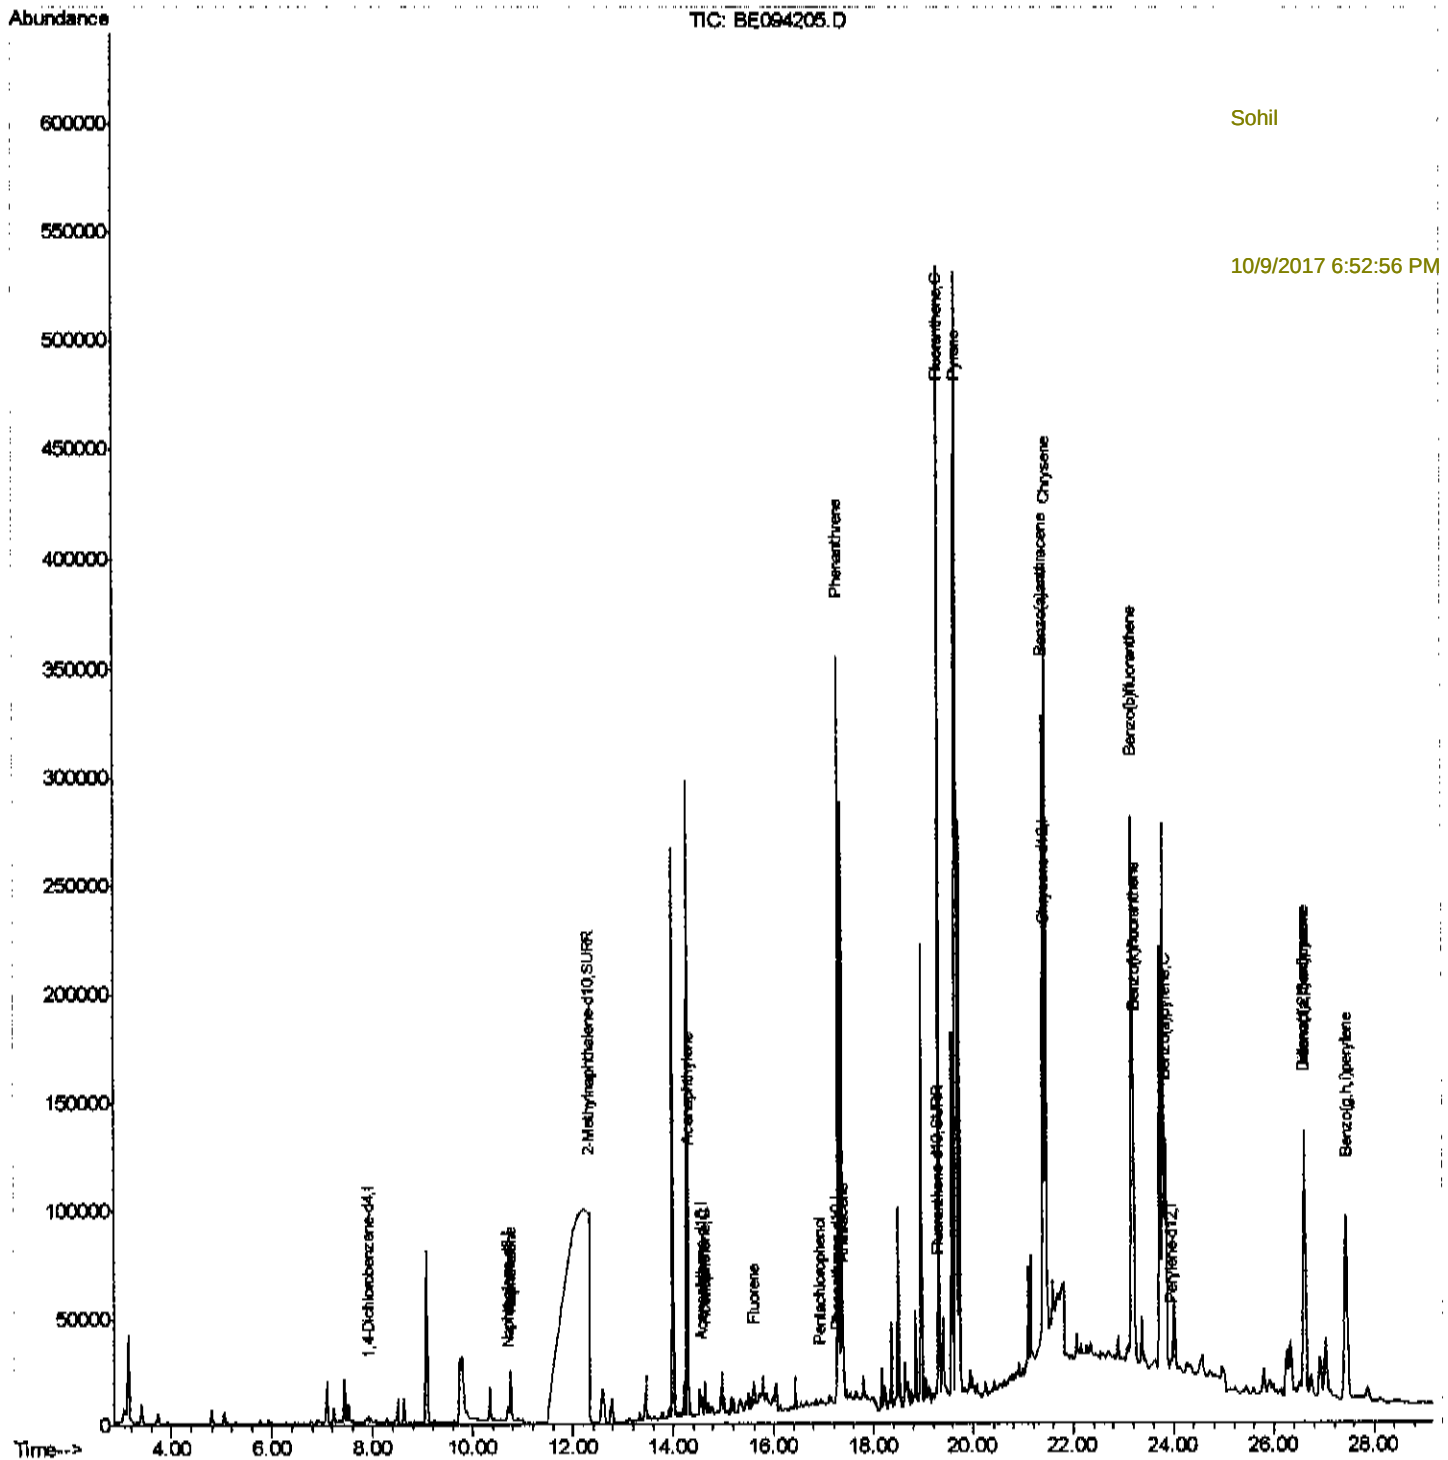

Sohil

10/9/2017 6:52:56 PM

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:11:13 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

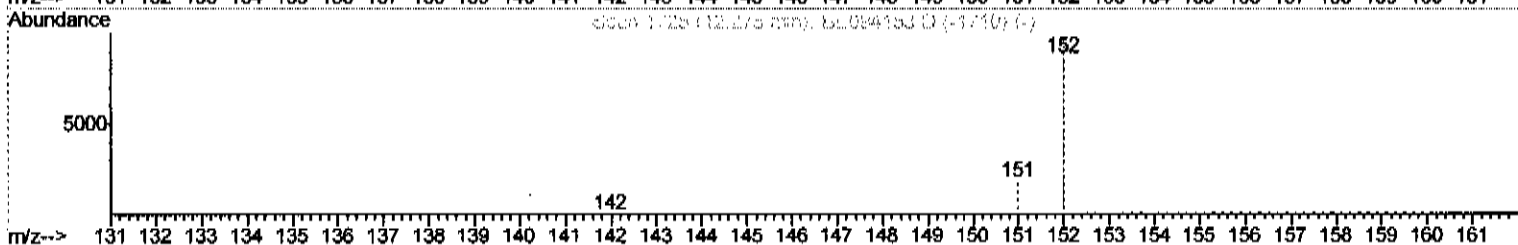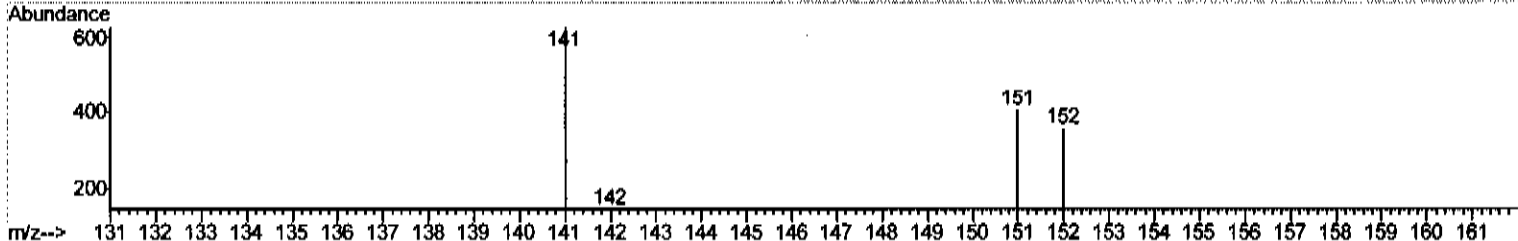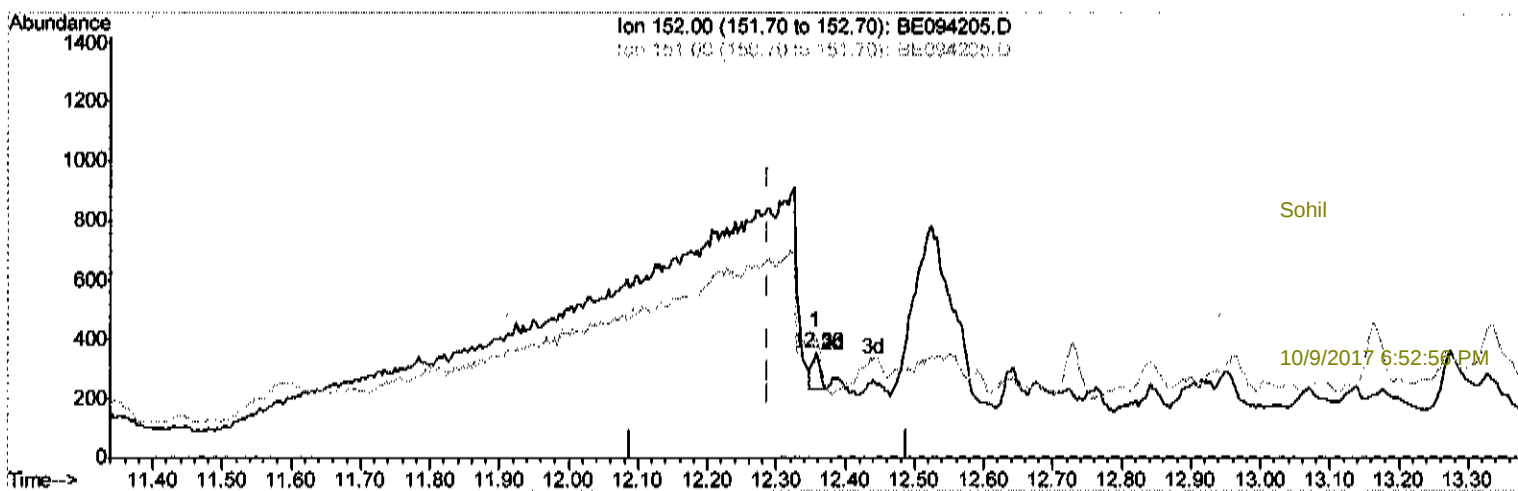

TIC: BE094205.D

(4) 2-Methylnaphthalene-d10 (SURR)

12.357min (+0.069) 0.01ng/ul

response 95

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:11:13 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

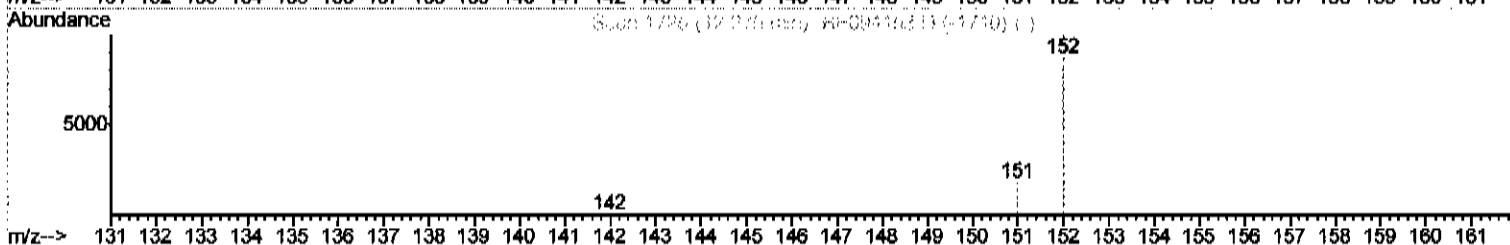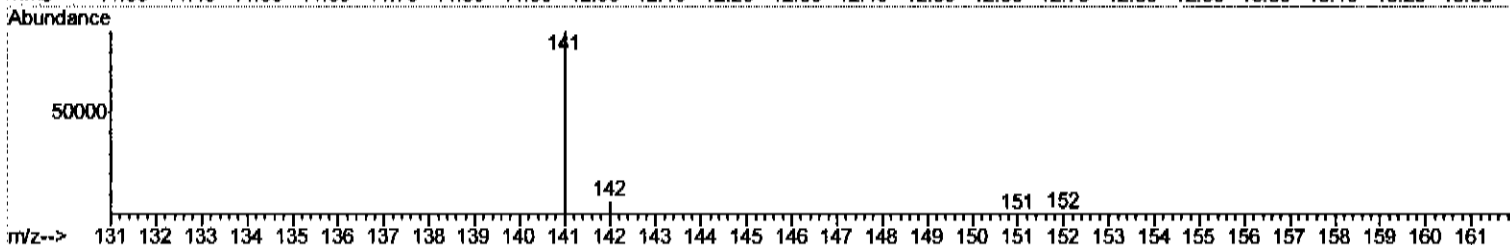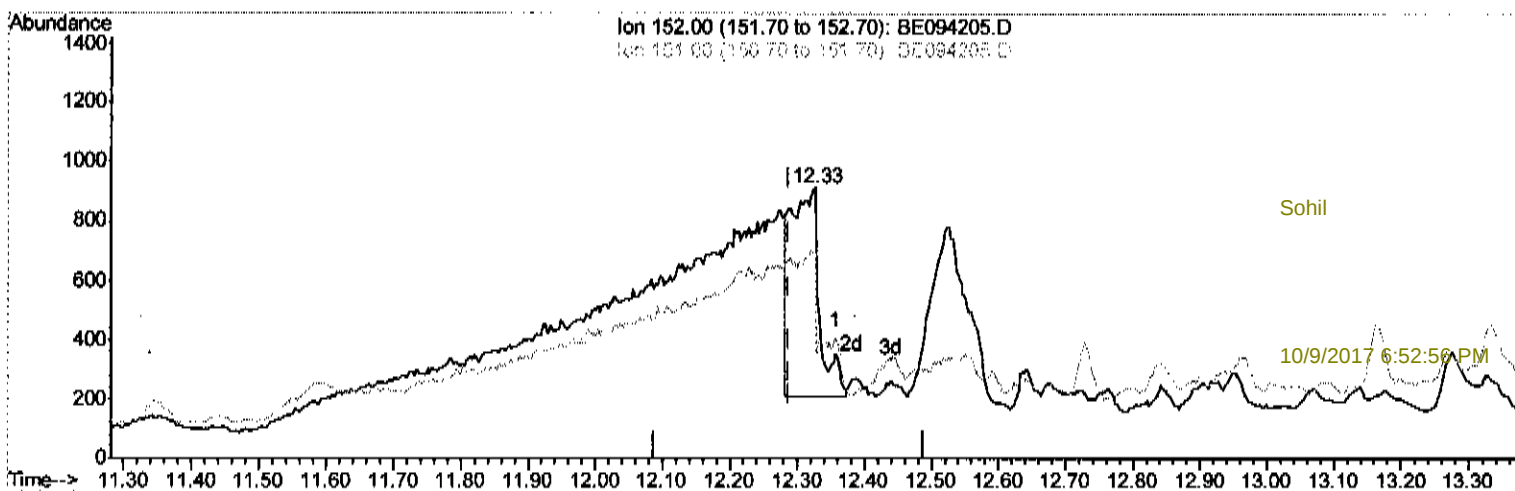

(4) 2-Methylnaphthalene-d10 (SURR)

12.326min (+0.038) 0.17ng/ul m

response 2128

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:11:13 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

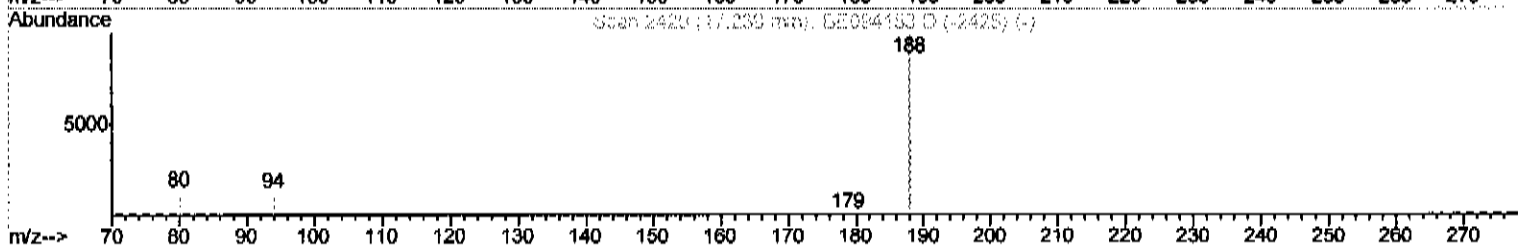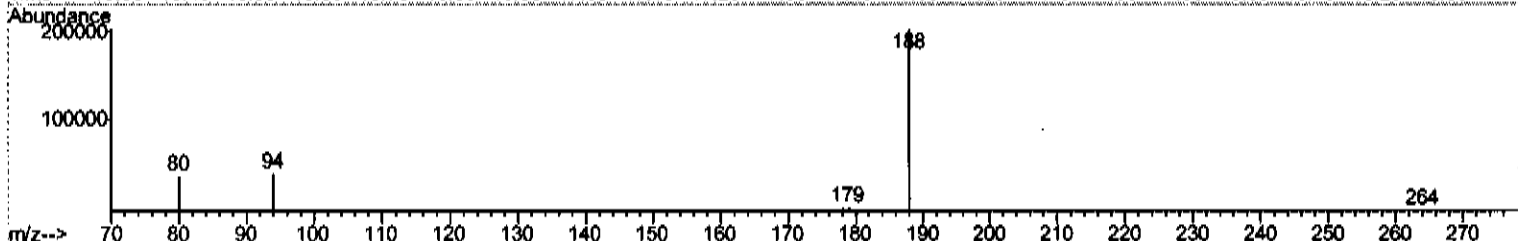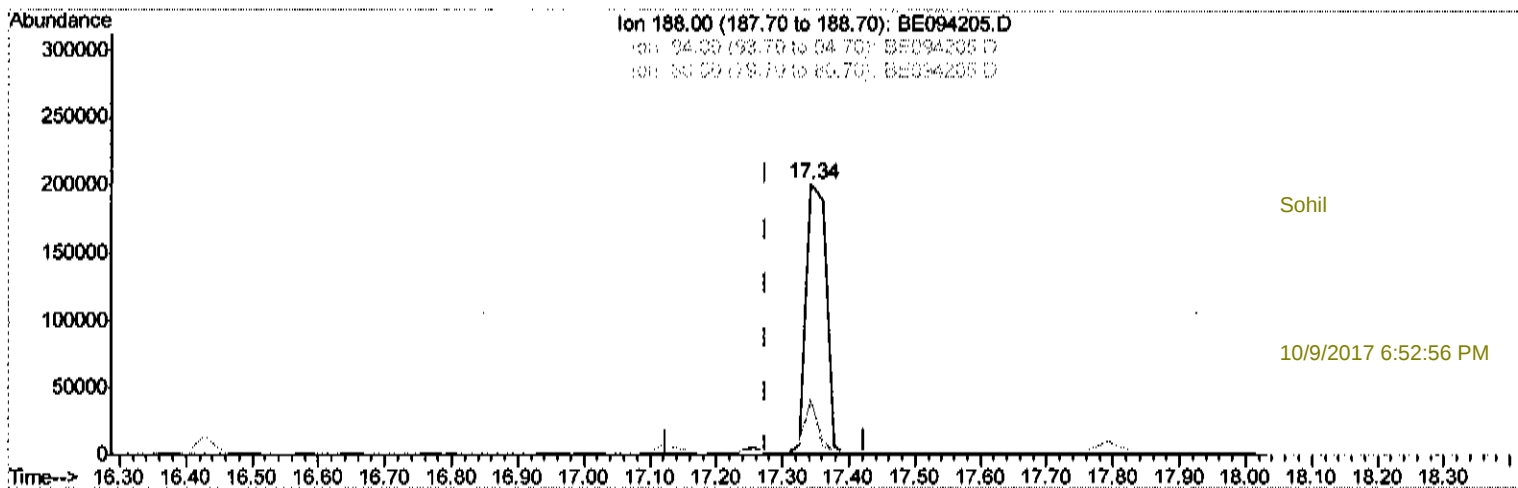

TIC: BE094205.D

(10) Phenanthrene-d10 (I)

17.343min (+0.069) 0.40ng/ul

response 418313

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	20.62#
80.00	11.80	19.48#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 B-40(0-1)-092617

Manual Integrations
 APPROVED



Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:11:13 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

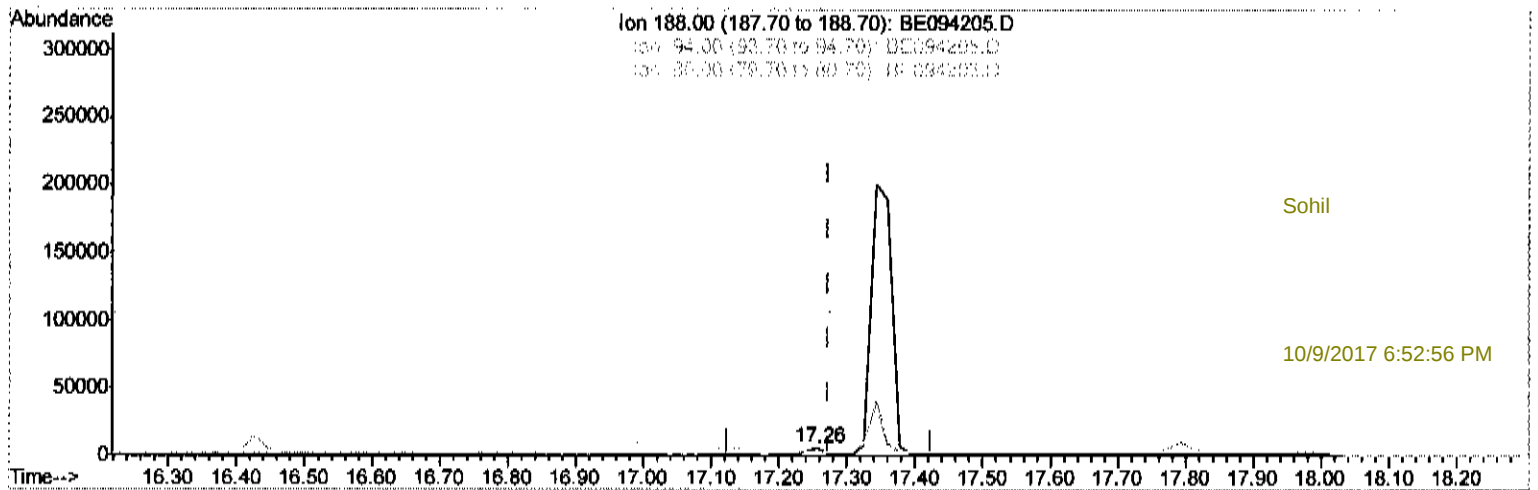

Sohil

10/9/2017 6:52:56 PM

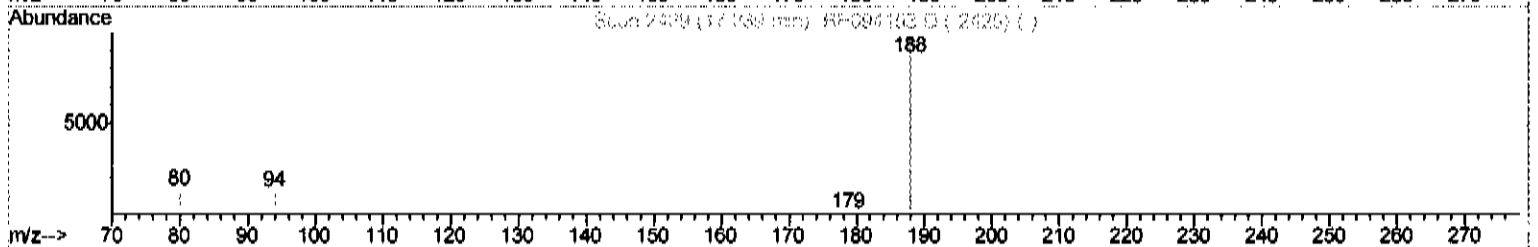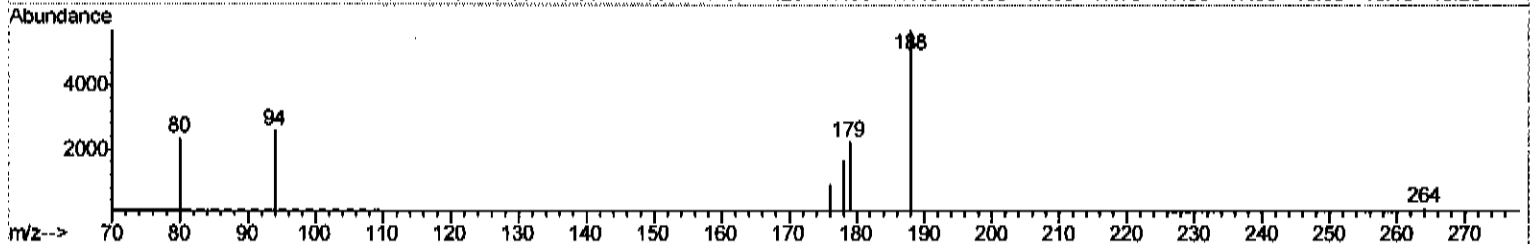

TIC: BE094205.D

(10) Phenanthrene-d10 (I)

17.256min (-0.018) 0.40ng/ul m

response 8381

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	45.42#
80.00	11.80	41.08#
0.00	0.00	0.00

ju 10/9/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

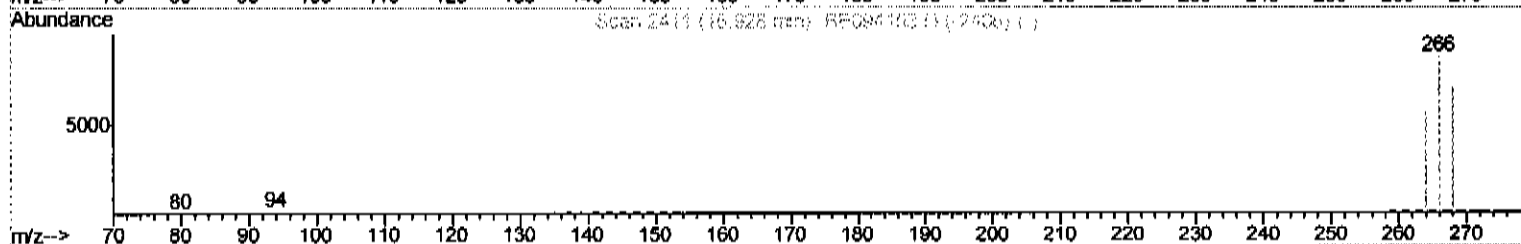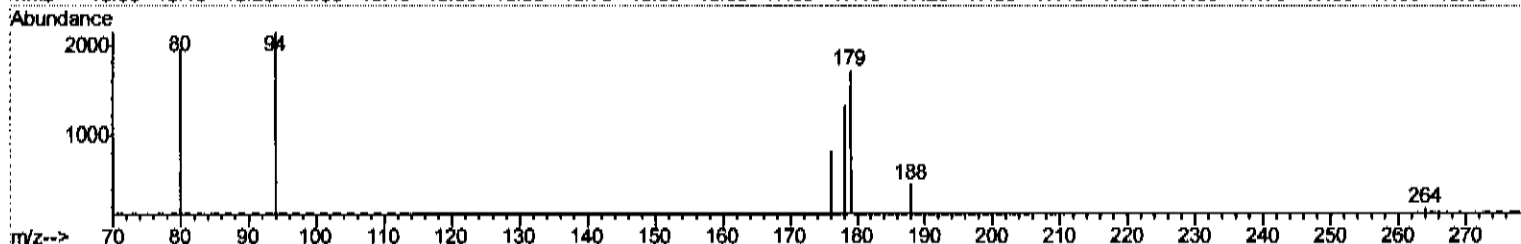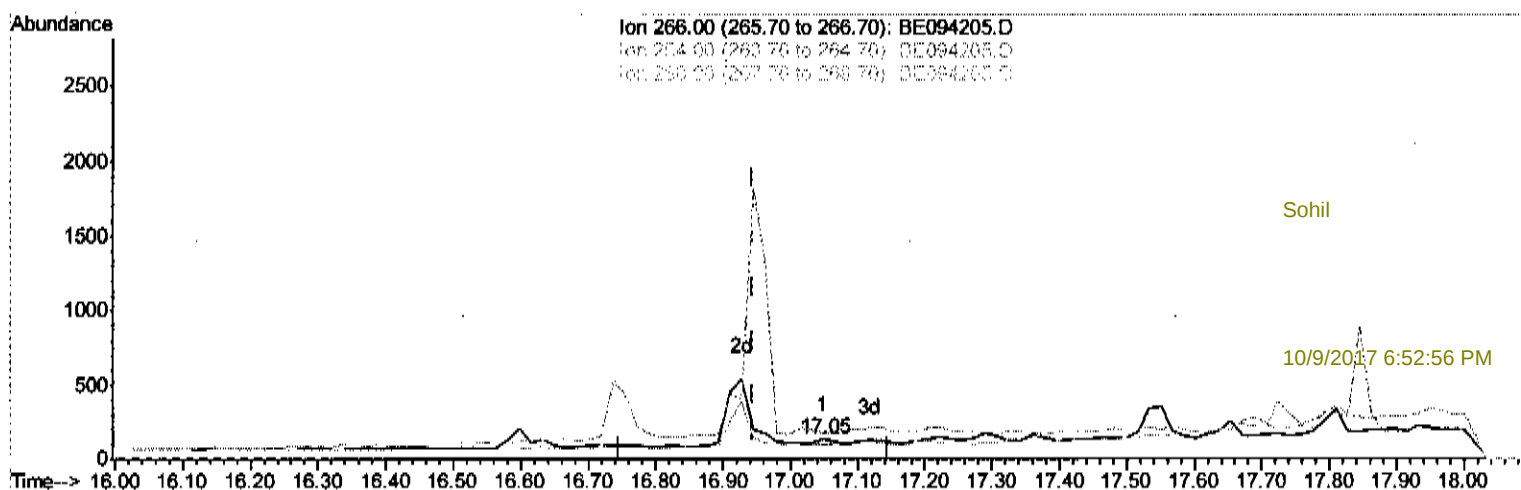

TIC: BE094205.D

(11) Pentachlorophenol

17.049min (+0.103) 0.08ng/ul

response 76

Ion	Exp%	Act%
266.00	100	100
264.00	59.90	0.00#
268.00	62.30	103.95#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

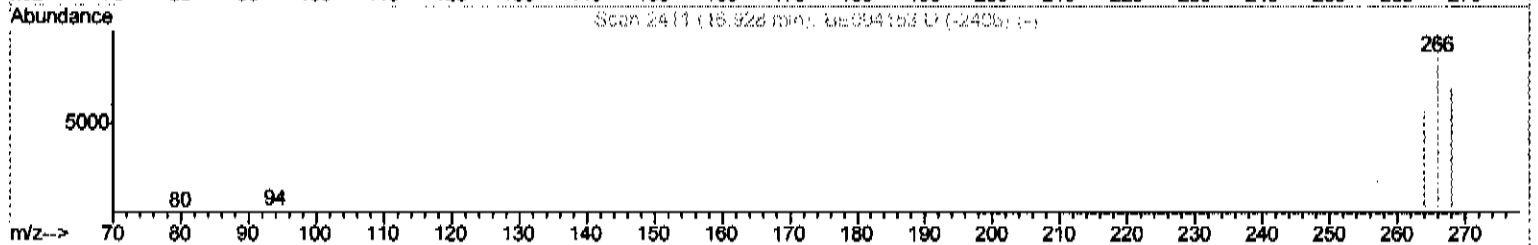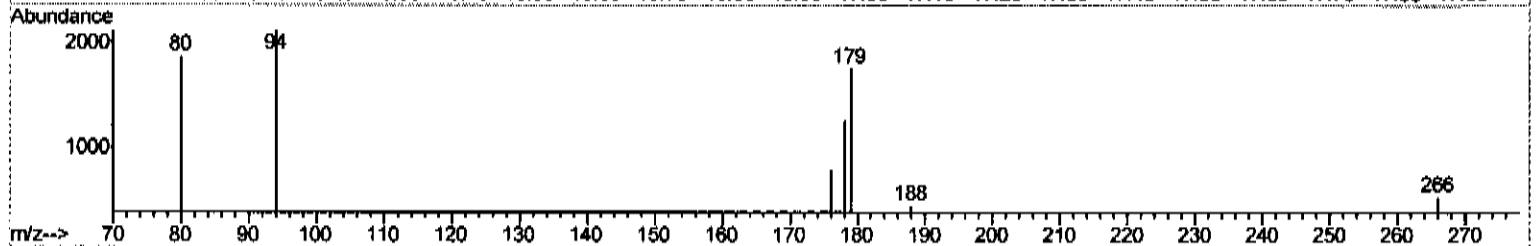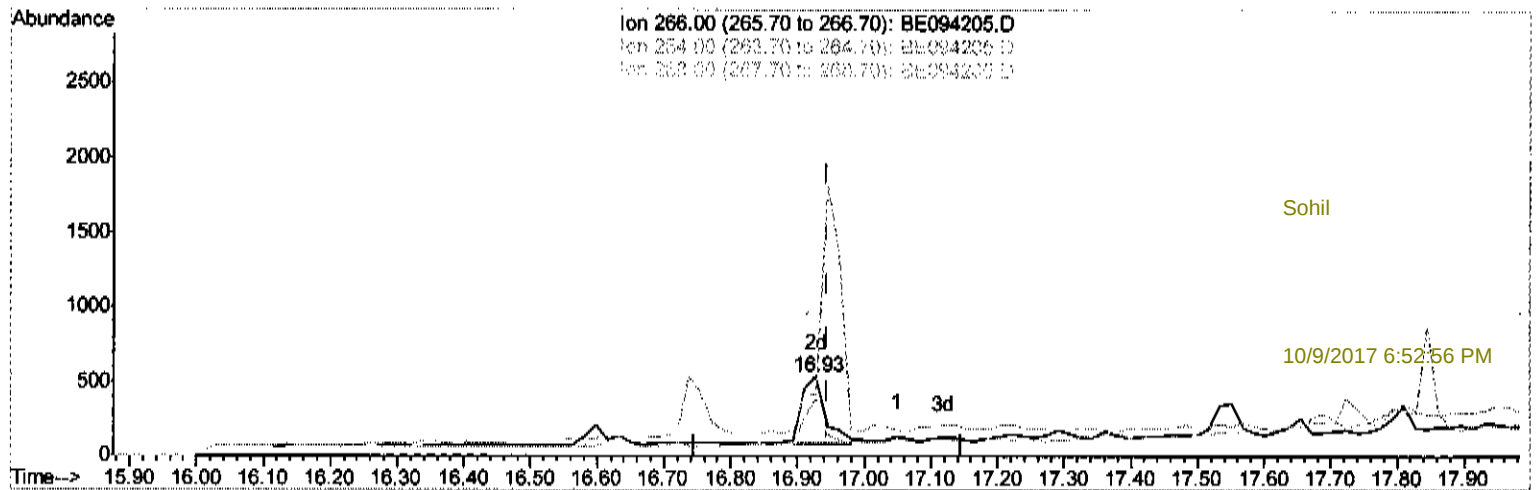

TIC: BE094205.D

(11) Pentachlorophenol

16.927min (-0.018) 1.16ng/ul m

response 1143

Ion	Exp%	Act%
266.00	100	100
264.00	59.90	0.00#
268.00	62.30	6.91#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED



Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

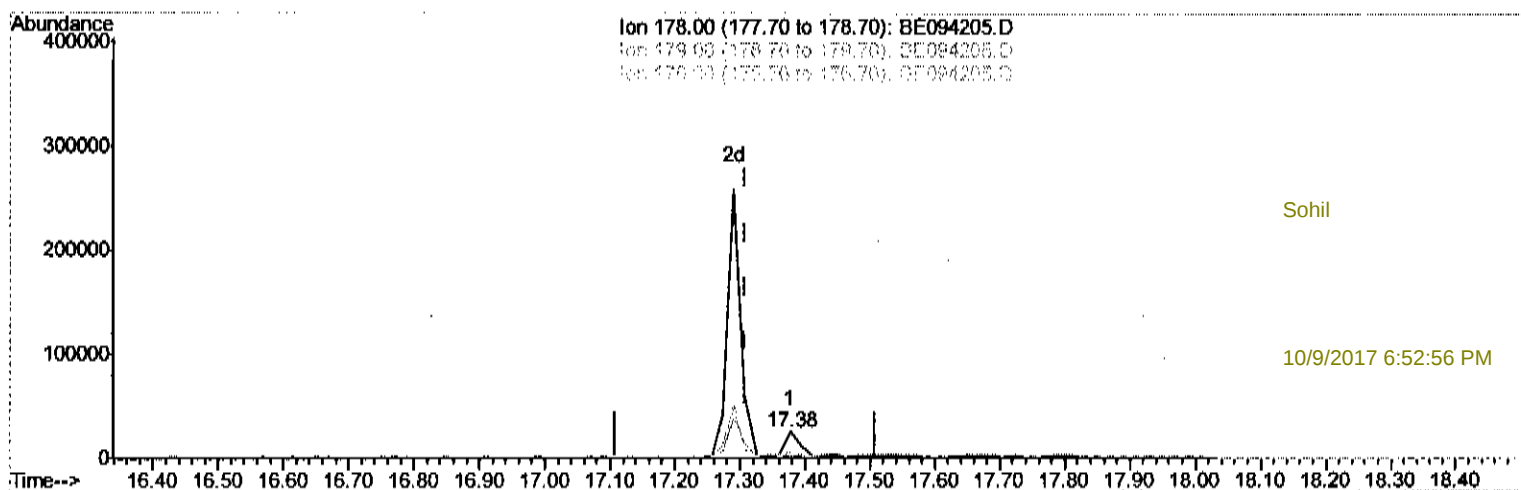

Sohil

10/9/2017 6:52:56 PM

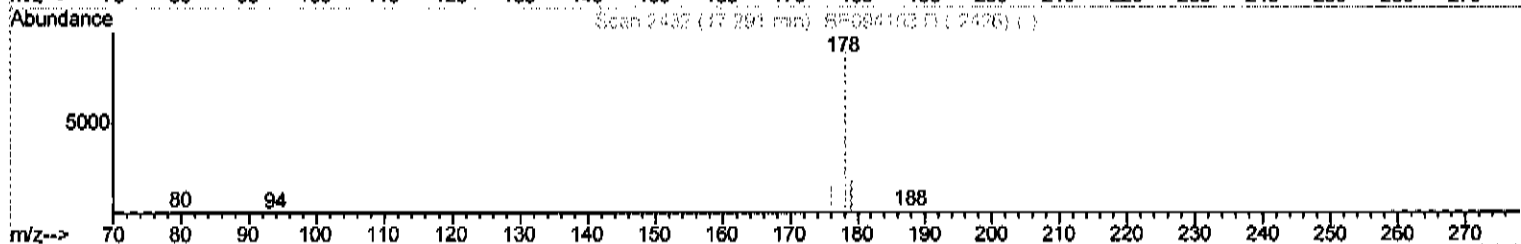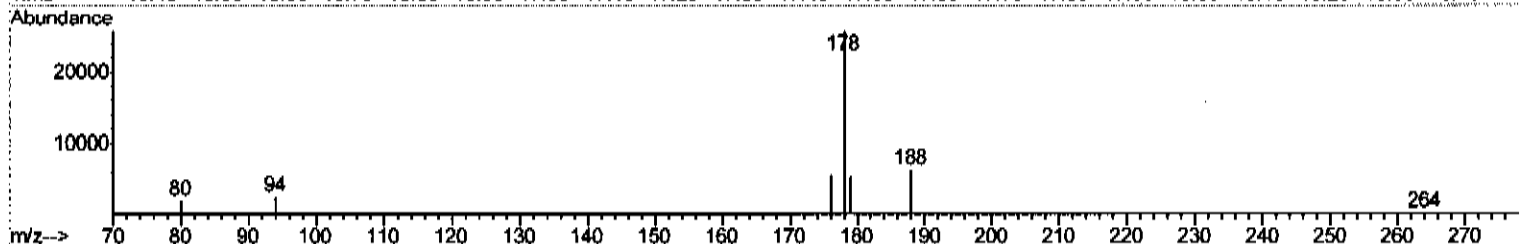

TIC: BE094205.D

(12) Phenanthrene

17.378min (+0.069) 1.87ng/ul

response 40861

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	21.04
176.00	17.00	21.77#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED



Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

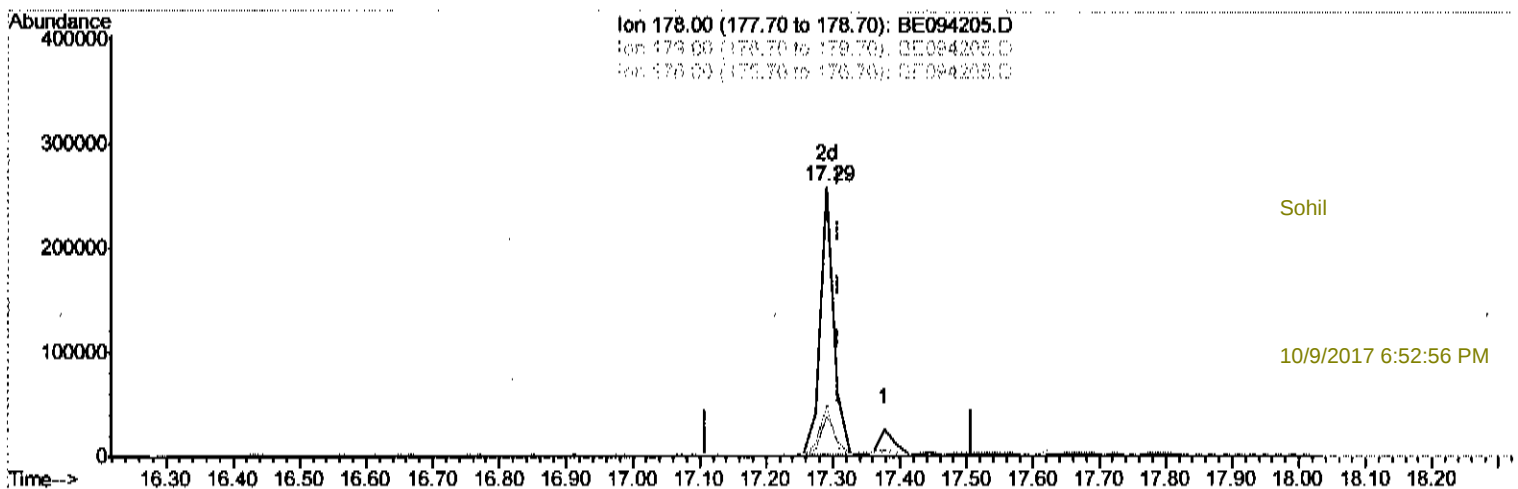

Sohil

10/9/2017 6:52:56 PM

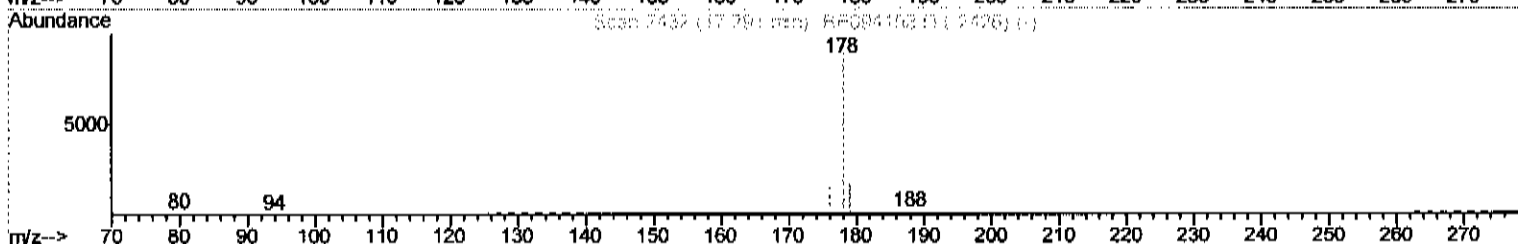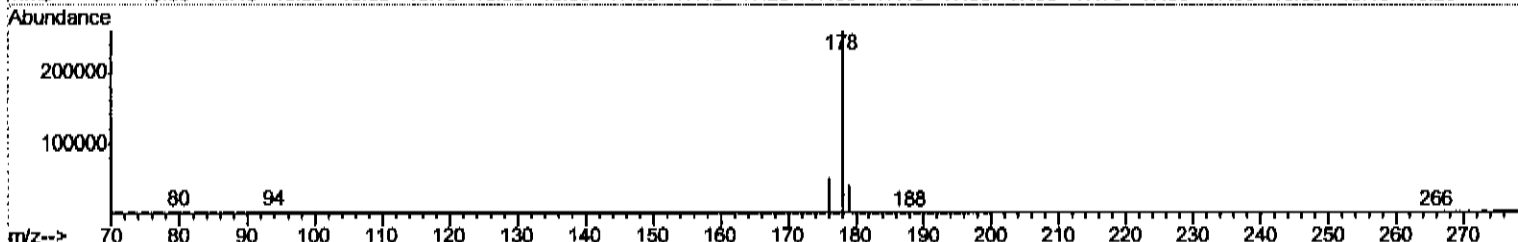

TIC: BE094205.D

(12) Phenanthrene

17.291min (-0.018) 17.06ng/ul m

response 373703

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.15#
176.00	17.00	19.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

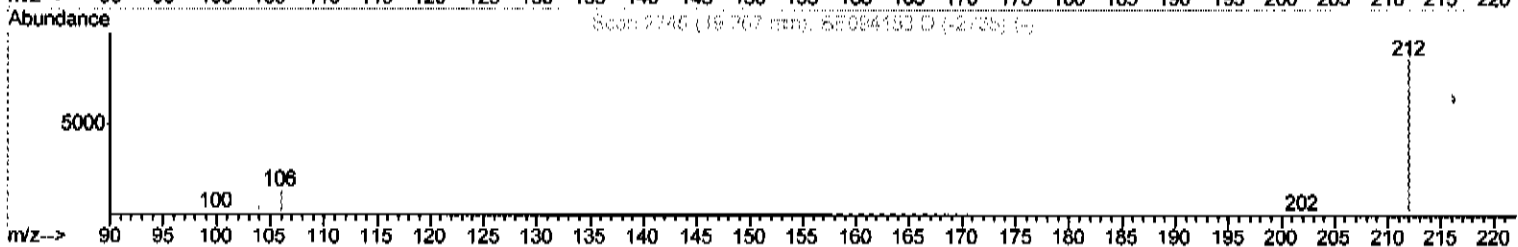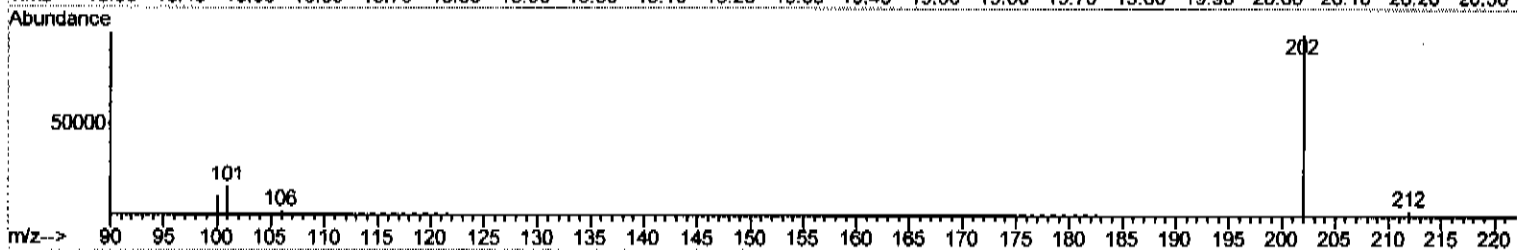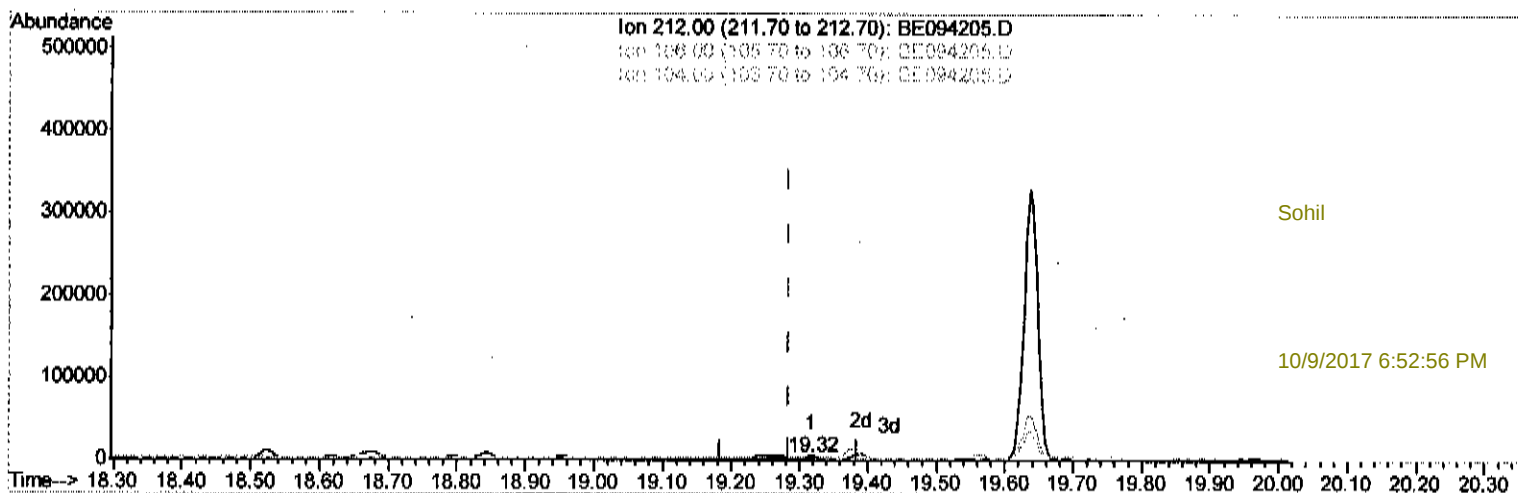

TIC: BE094205.D

(14) Fluoranthene-d10 (SURR)

19.318min (+0.033) 0.18ng/ul

response 4938

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	14.86
104.00	15.60	13.08
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

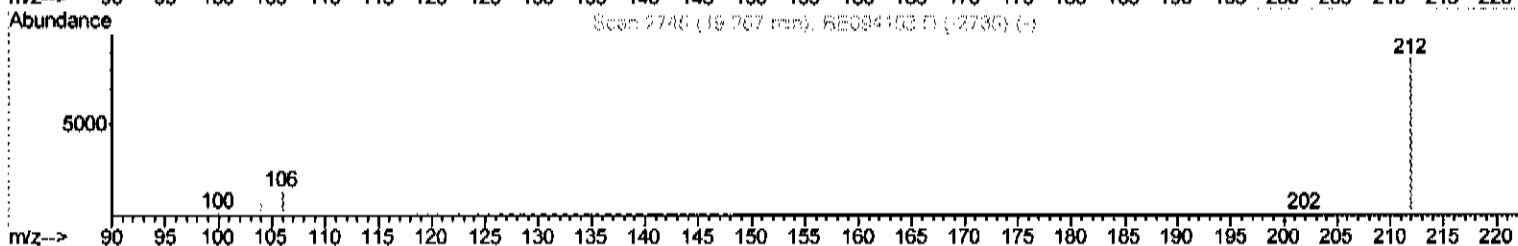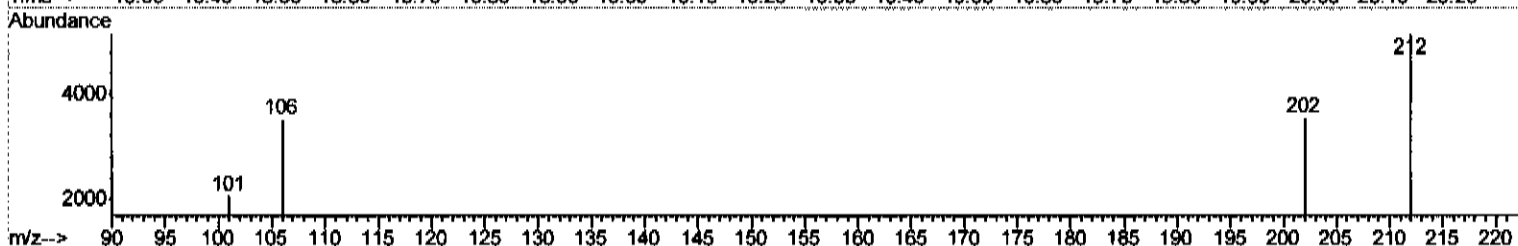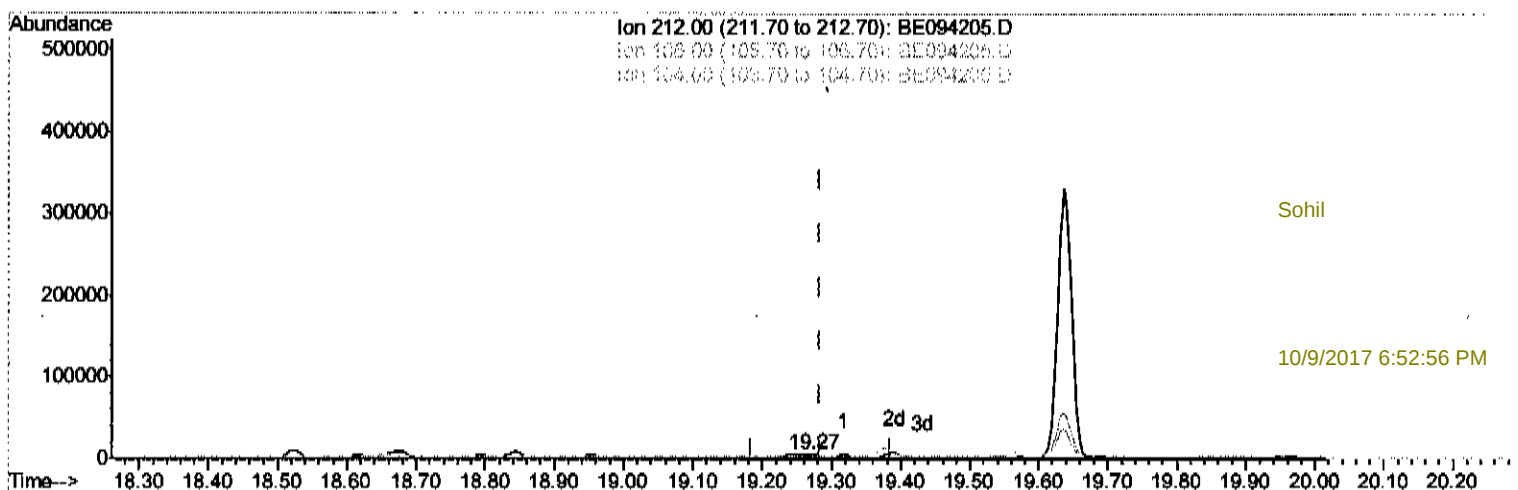

TIC: BE094205.D

(14) Fluoranthene-d10 (SURR)

19.272min (-0.013) 0.15ng/ul m

response 4323

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	16.98
104.00	15.60	14.94
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

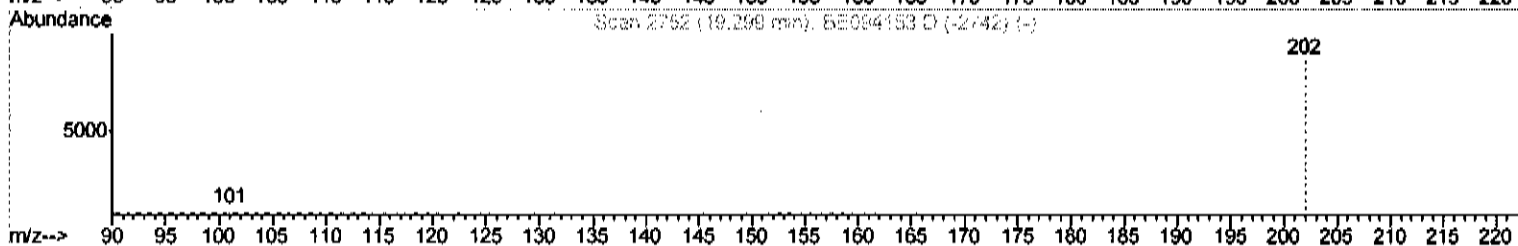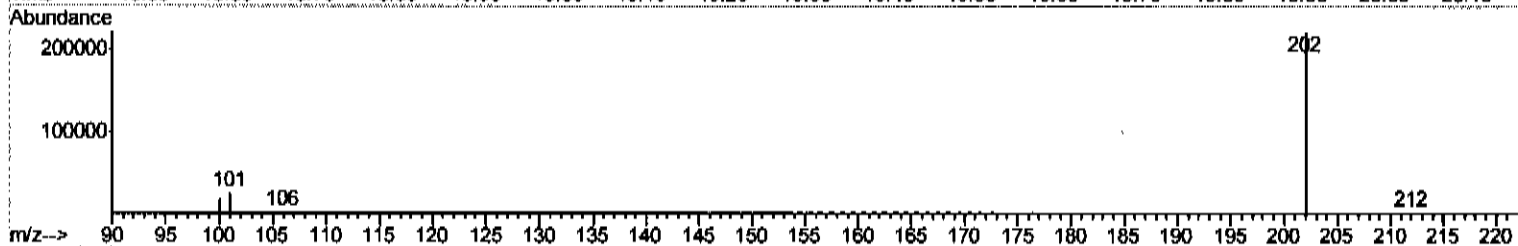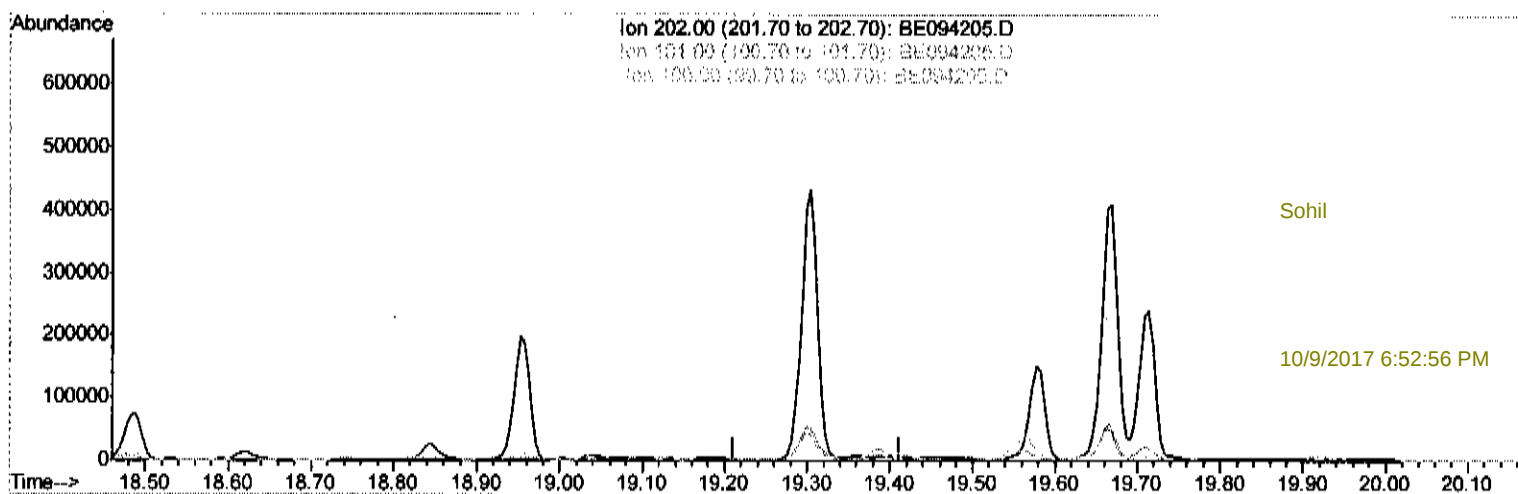

TIC: BE094205.D

(15) Fluoranthene (C)

19.312min (-19.312) 0.00ng/ui

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.30	0.00
100.00	19.50	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

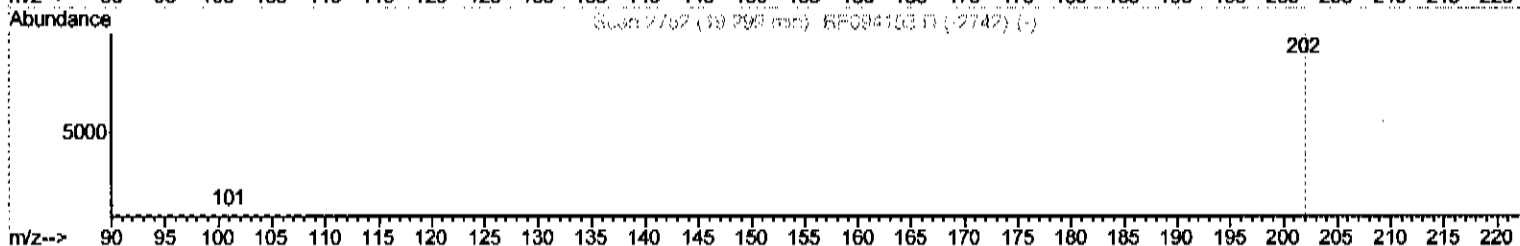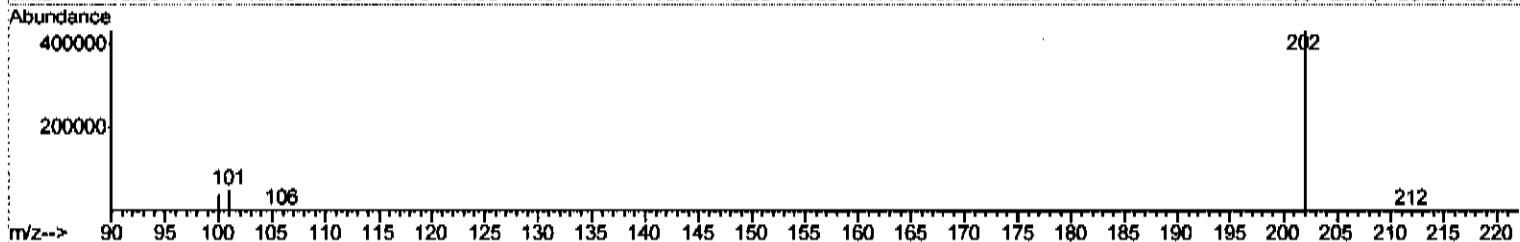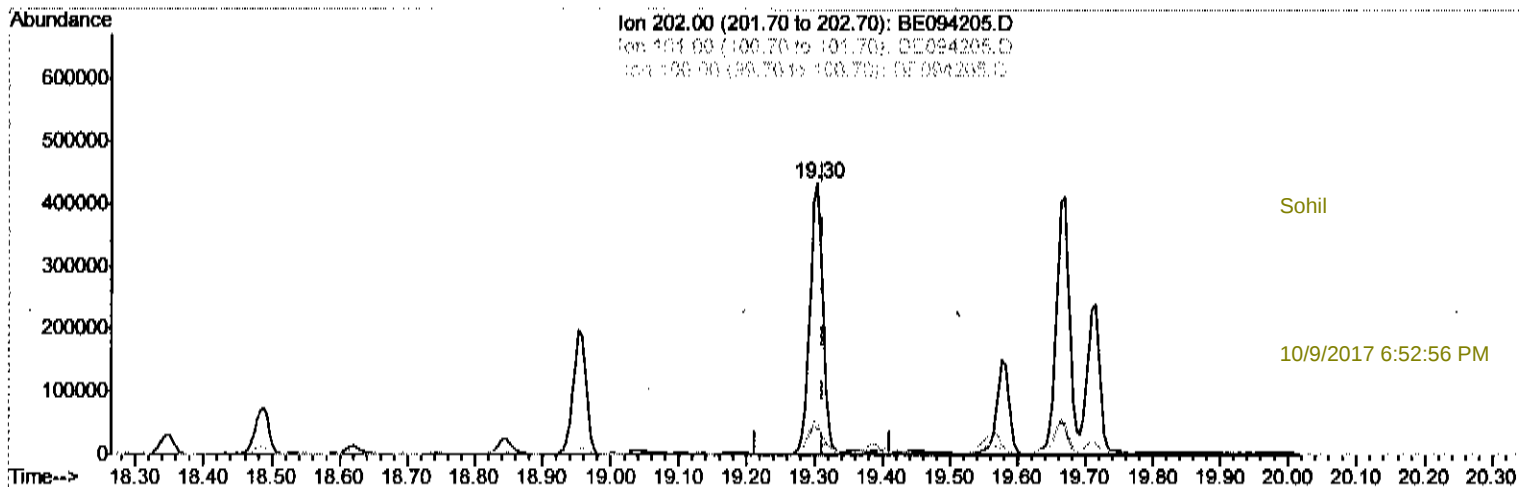

TIC: BE094205.D

(15) Fluoranthene (C)

19.304min (-0.008) 20.10ng/ul m

response 578332

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	11.99
100.00	19.50	9.49
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 B-40(0-1)-092617

Manual Integrations
 APPROVED



Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

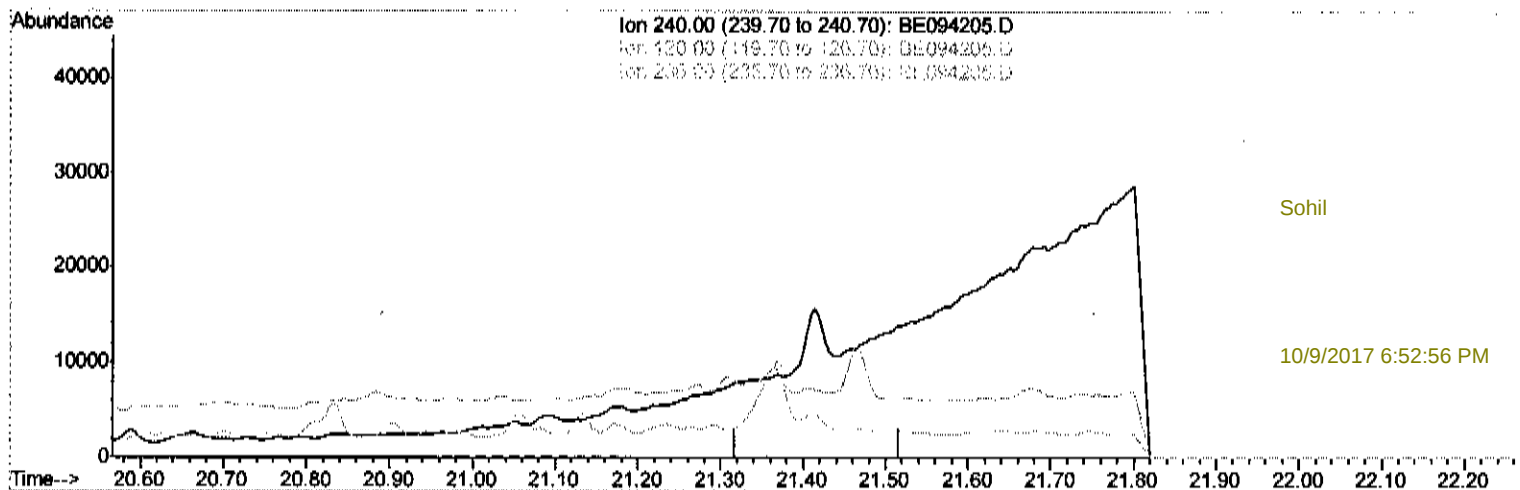

Sohil

10/9/2017 6:52:56 PM

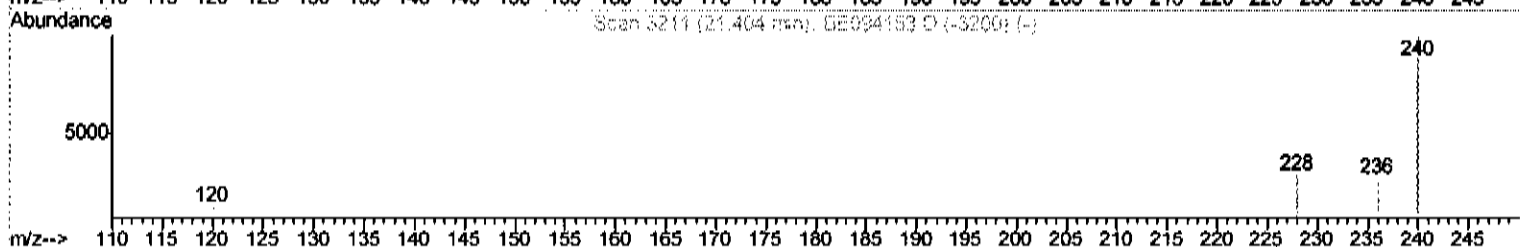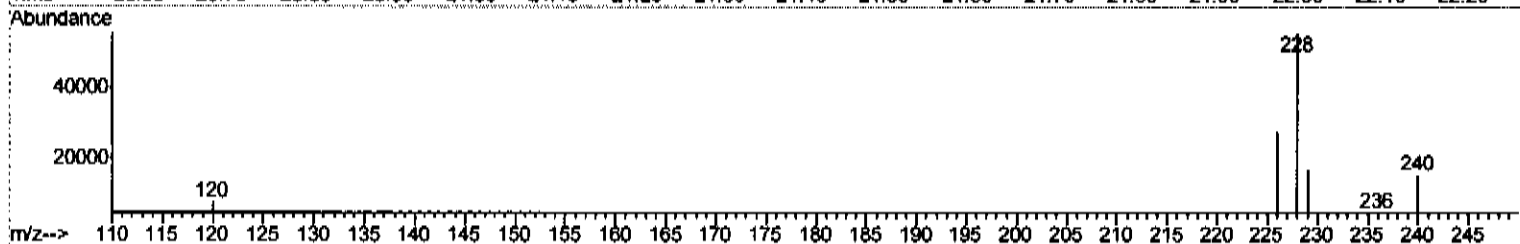

TIC: BE094205.D

(16) Chrysene-d12 (I)

21.417min (-21.417) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 B-40(0-1)-092617

Manual Integrations
 APPROVED



Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:16:03 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

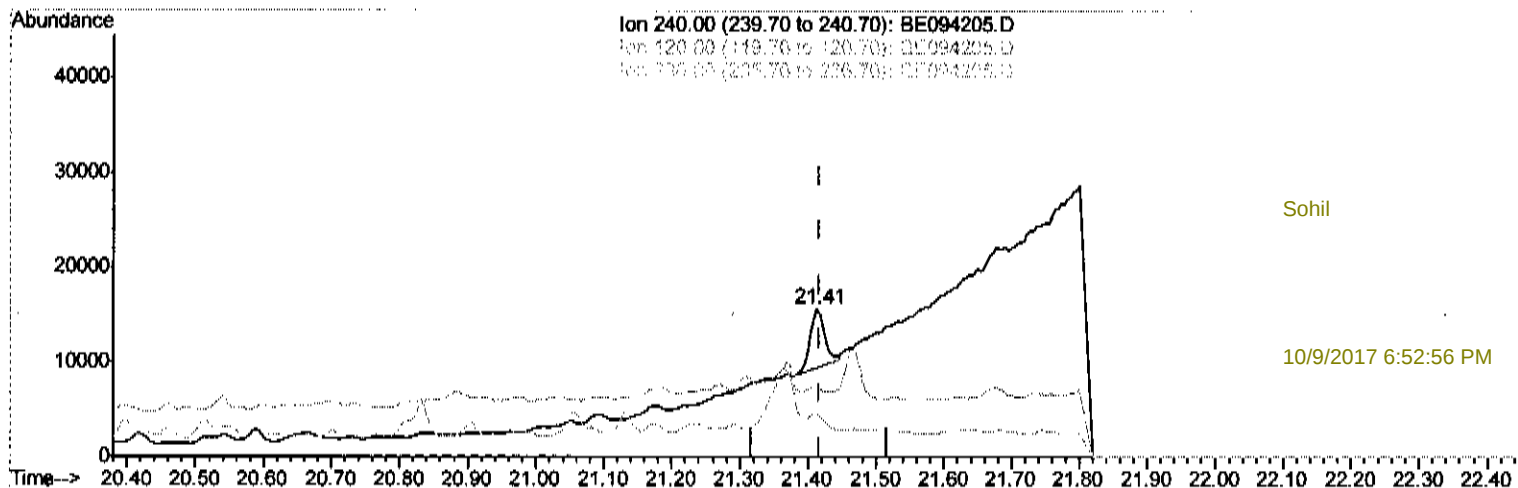

Sohil

10/9/2017 6:52:56 PM

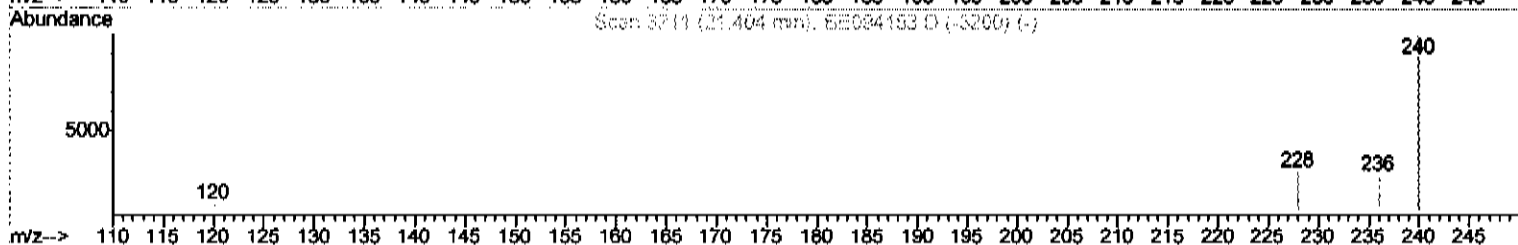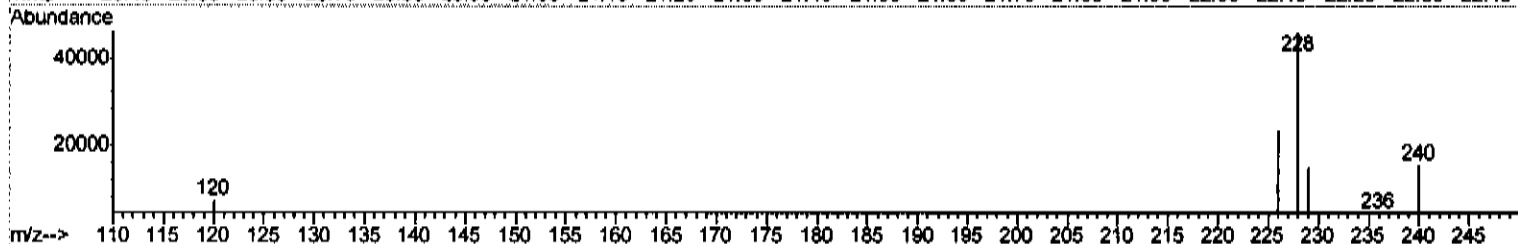

TIC: BE094205.D

(16) Chrysene-d12 (I)

21.413min (-0.004) 0.40ng/ul m

response 9394

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	46.18#
236.00	34.90	29.43
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:18:43 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

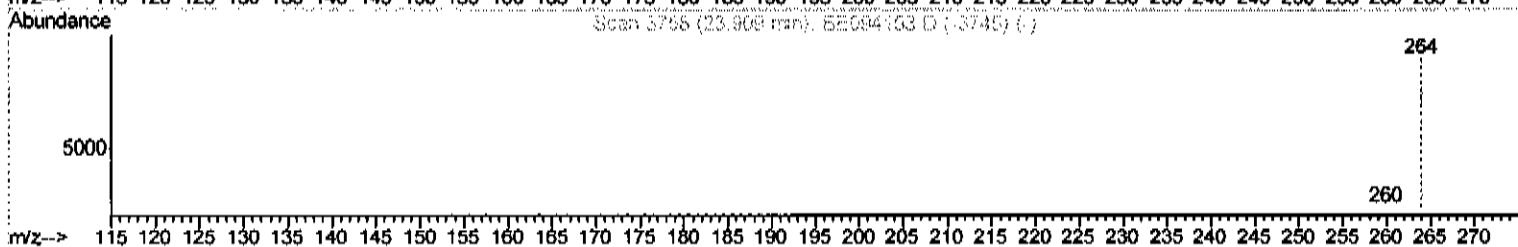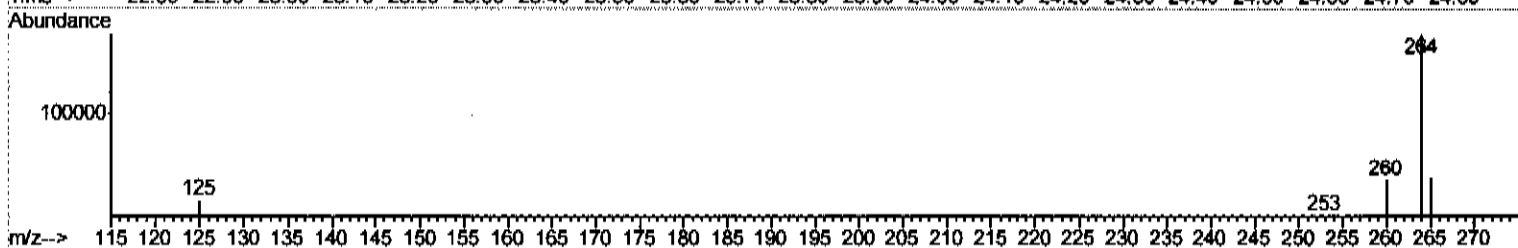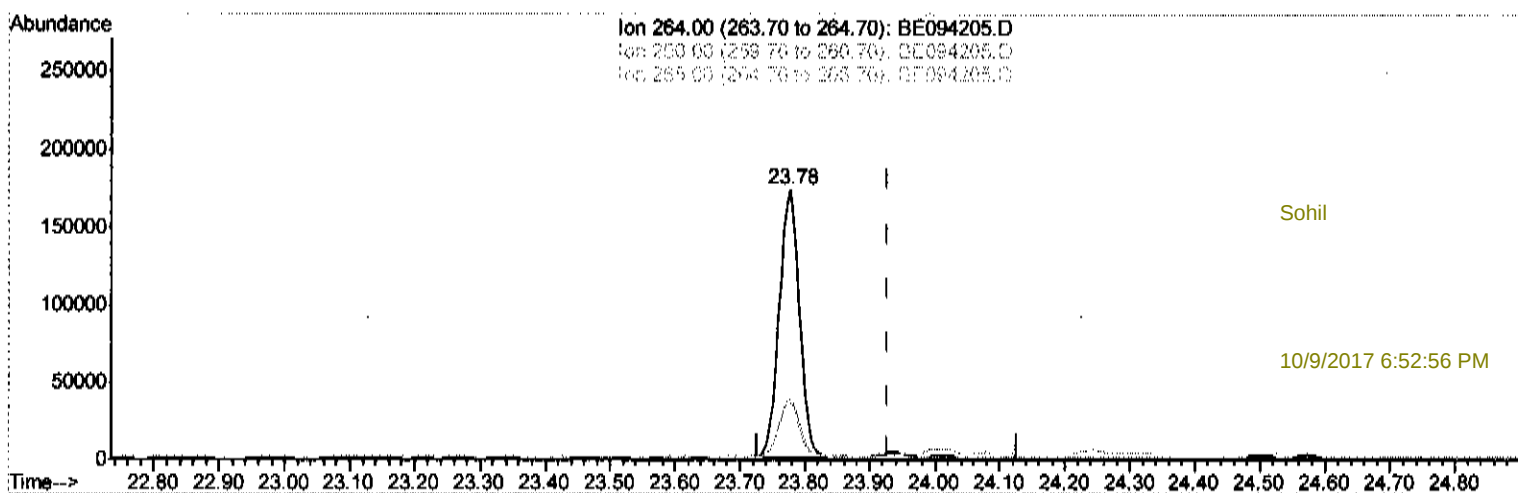

TIC: BE094205.D

(20) Perylene-d12 (I)

23.778min (-0.150) 0.40ng/ul

response 372892

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.74#
265.00	103.50	22.56#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED



Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:18:43 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

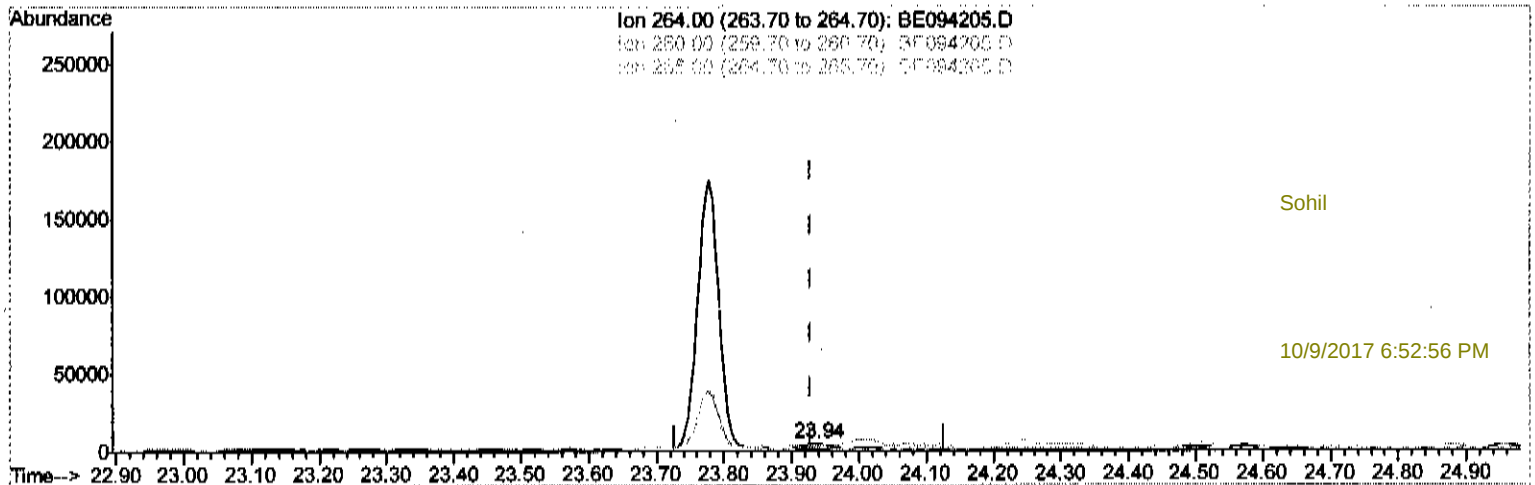

Sohil

10/9/2017 6:52:56 PM

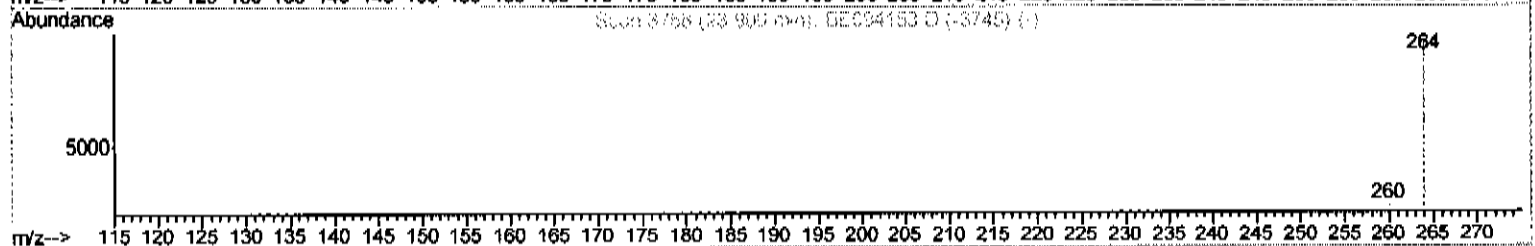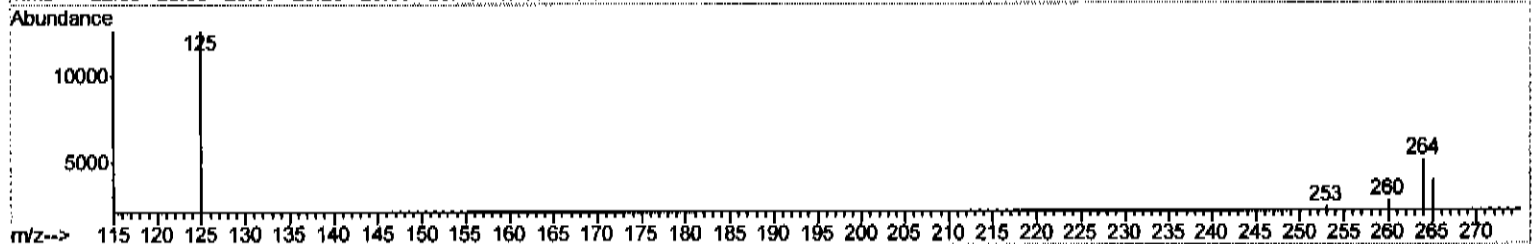

TIC: BE094205.D

(20) Perylene-d12 (I)

23.937min (+0.010) 0.40ng/ul m

response 7517

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	52.42#
265.00	103.50	75.13#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

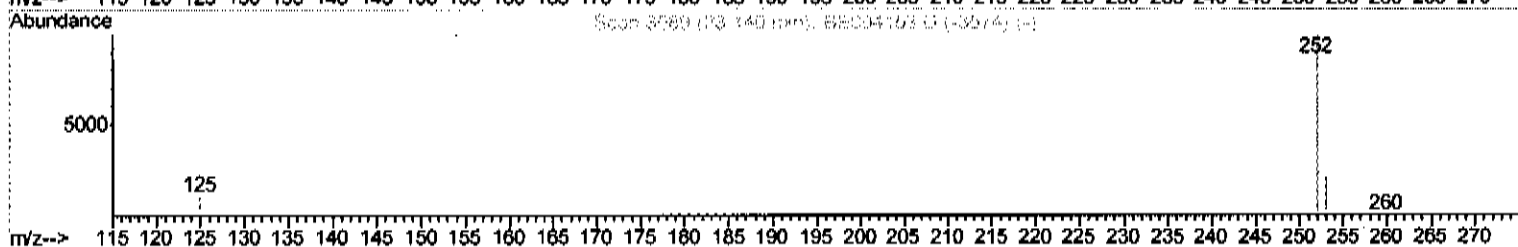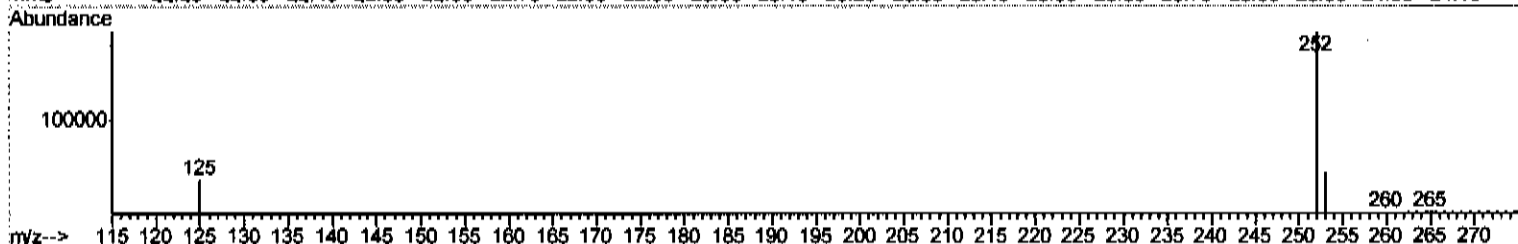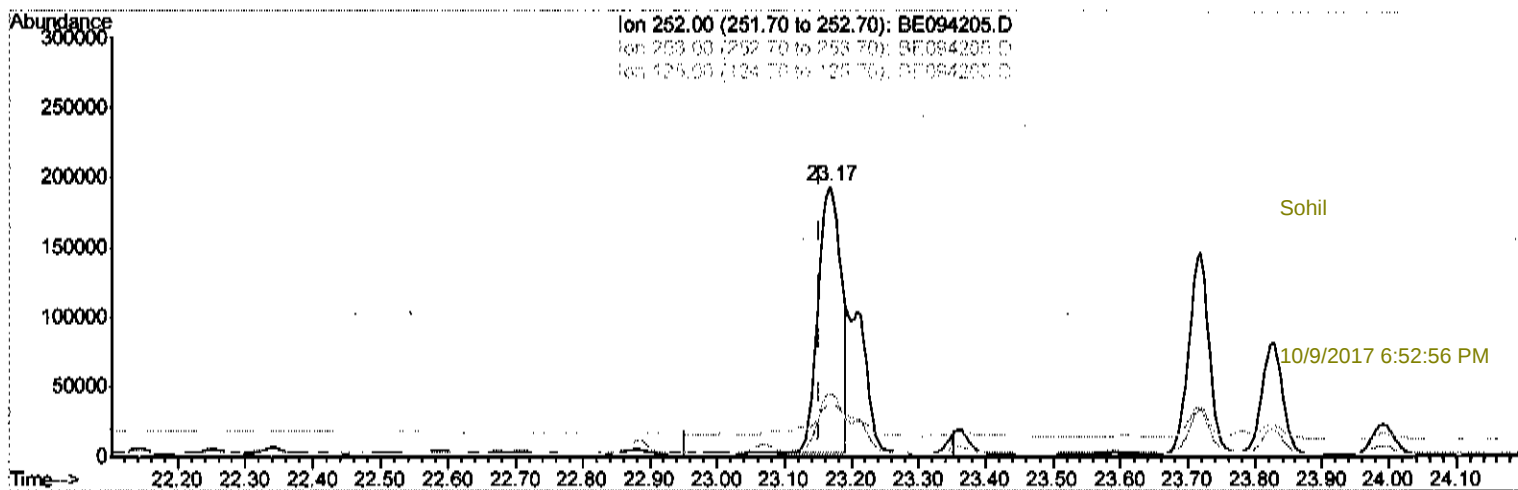

TIC: BE094205.D

(21) Benzo(b)fluoranthene

23.167min (+0.014) 22.12ng/ul

response 451733

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.11
125.00	17.50	19.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleID :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

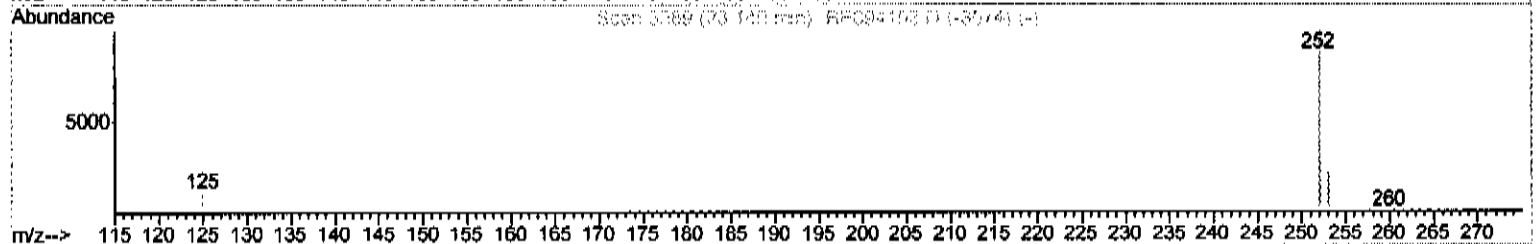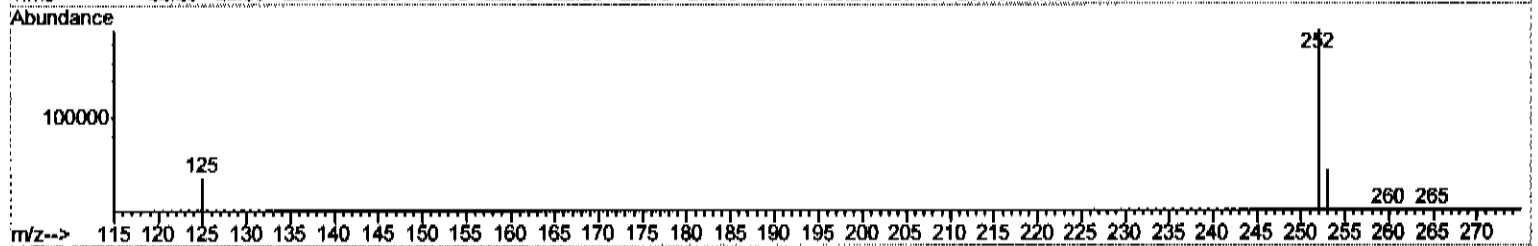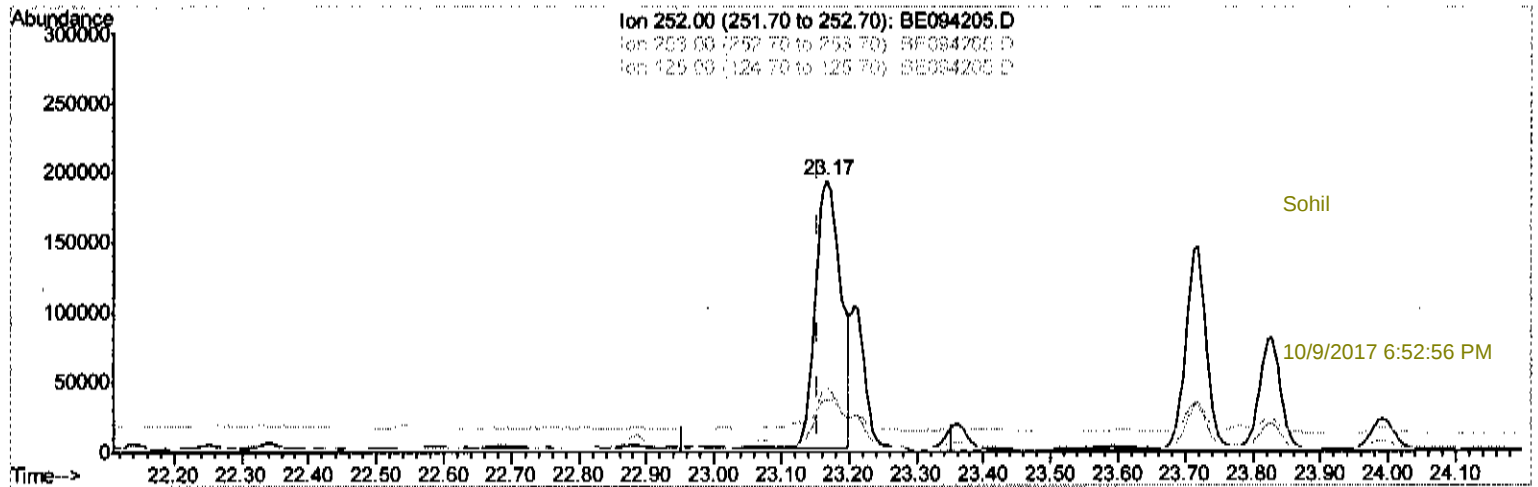

TIC: BE094205.D

(21) Benzo(b)fluoranthene

23.167min (+0.014) 24.82ng/ul m

response 506752

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.11
125.00	17.50	19.16
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

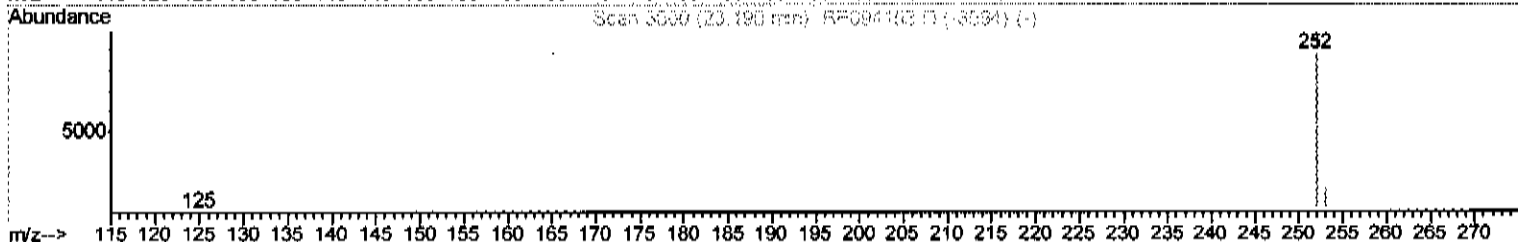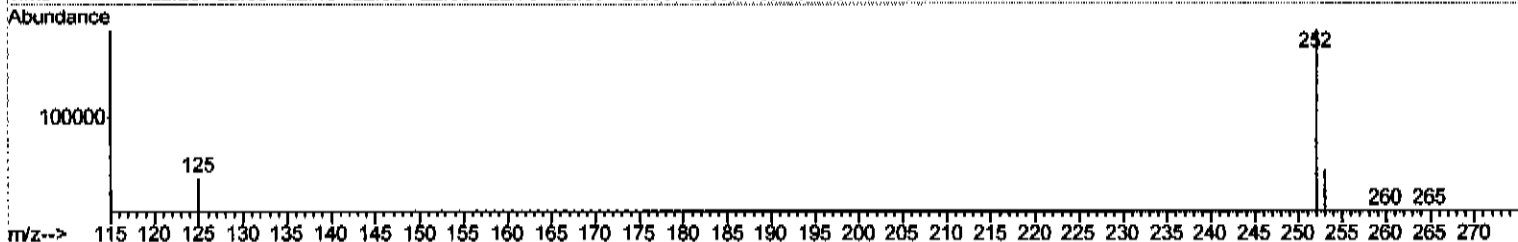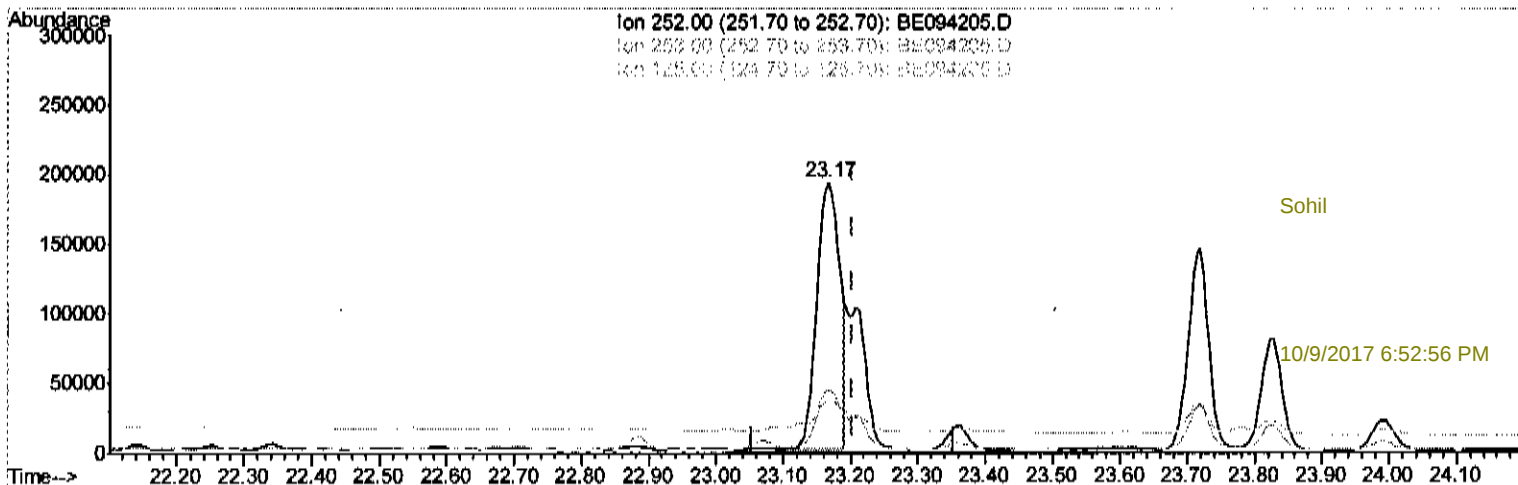

TIC: BE094205.D

(22) Benzo(k)fluoranthene

23.167min (-0.036) 19.14ng/ui

response 451733

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.11#
125.00	17.10	19.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
B-40(0-1)-092617

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

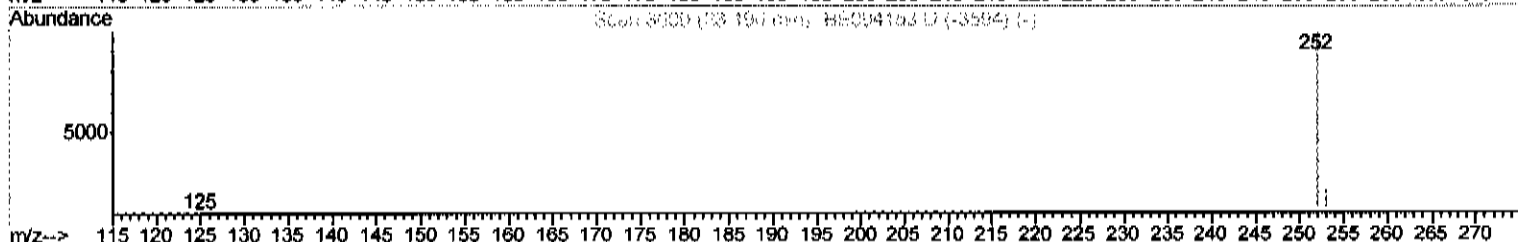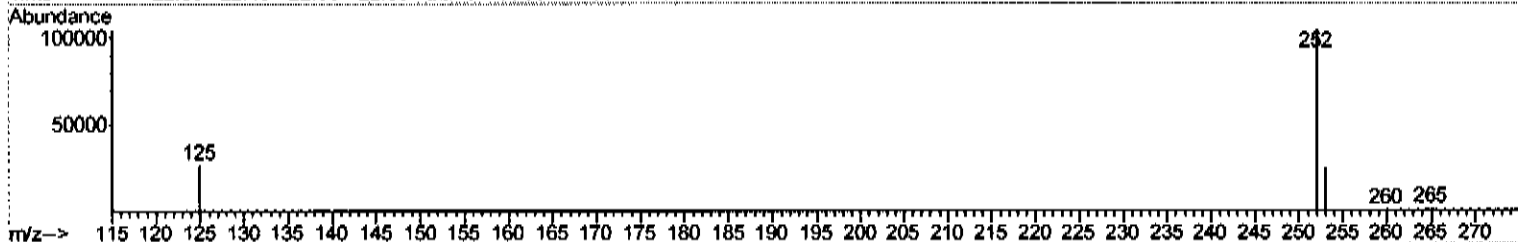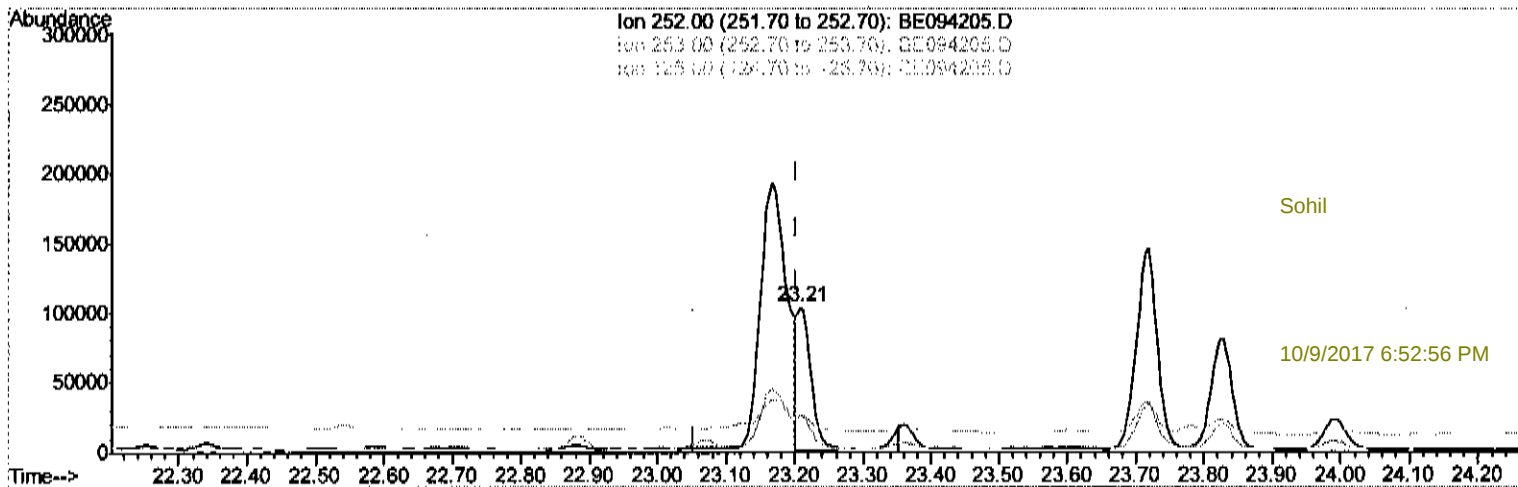

TIC: BE094205.D

(22) Benzo(k)fluoranthene

23.208min (+0.005) 6.32ng/ul m

response 149127

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.70
125.00	17.10	26.48#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleID :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

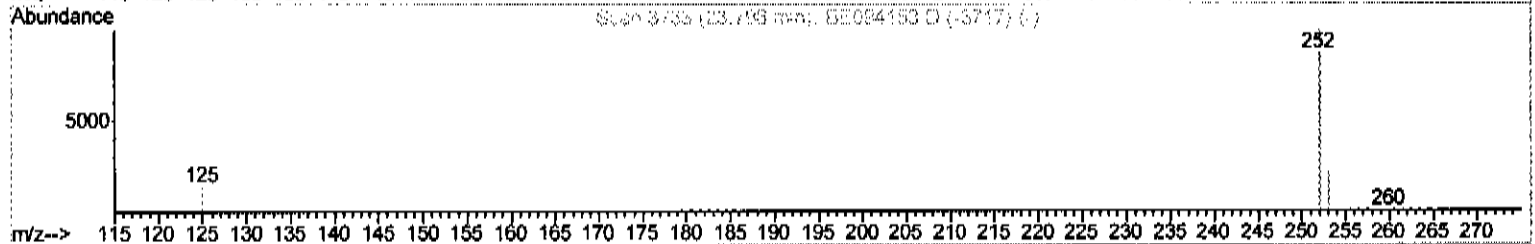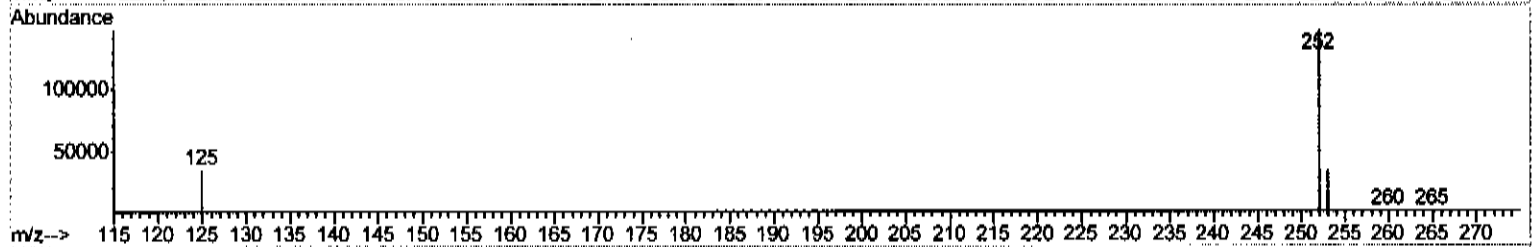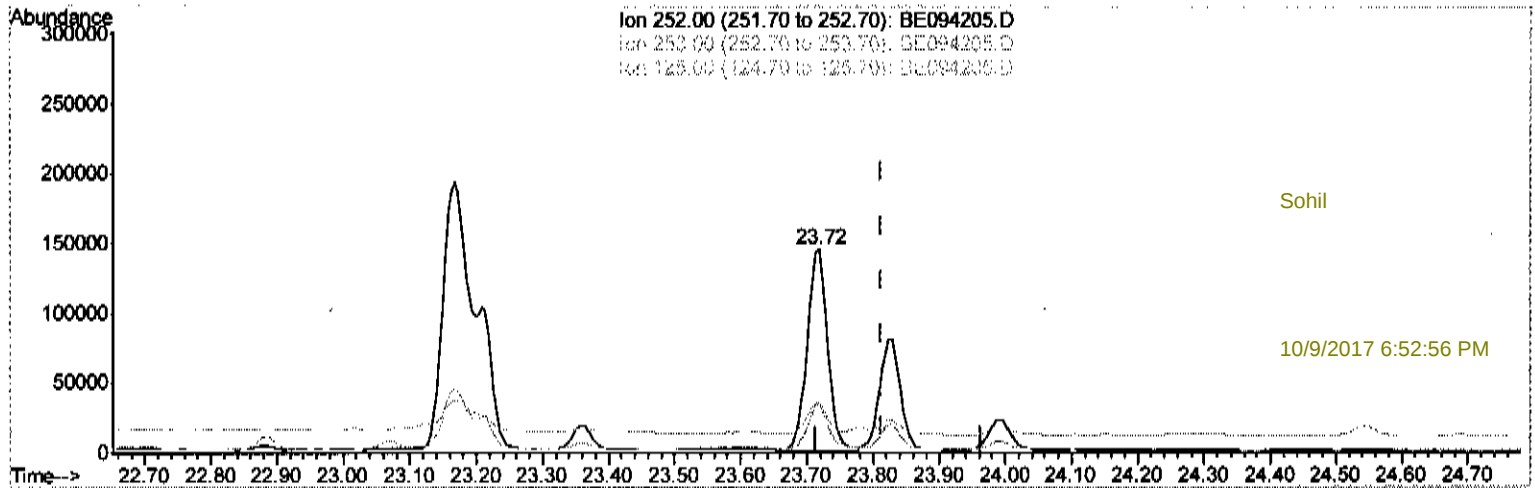

TIC: BE094205.D

(23) Benzo(a)pyrene (C)

23.718min (-0.095) 14.28ng/ul

response 302959

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	23.39#
125.00	22.60	24.29
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

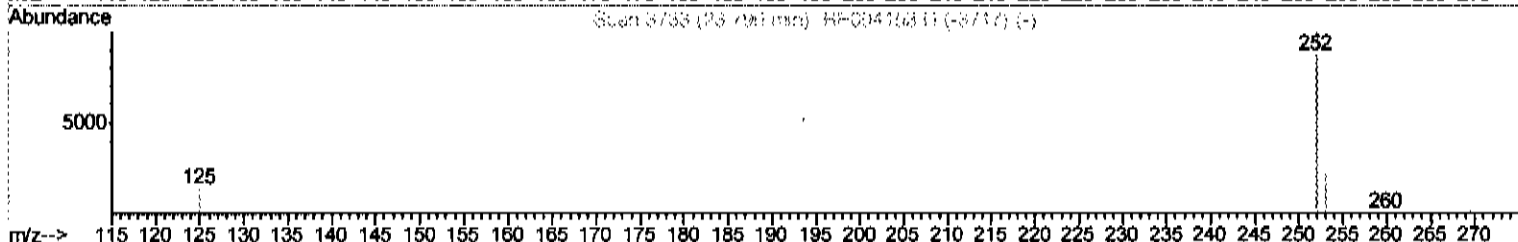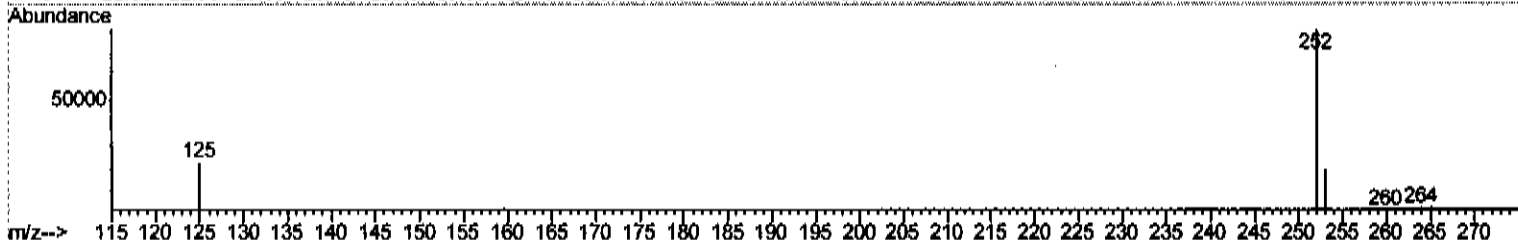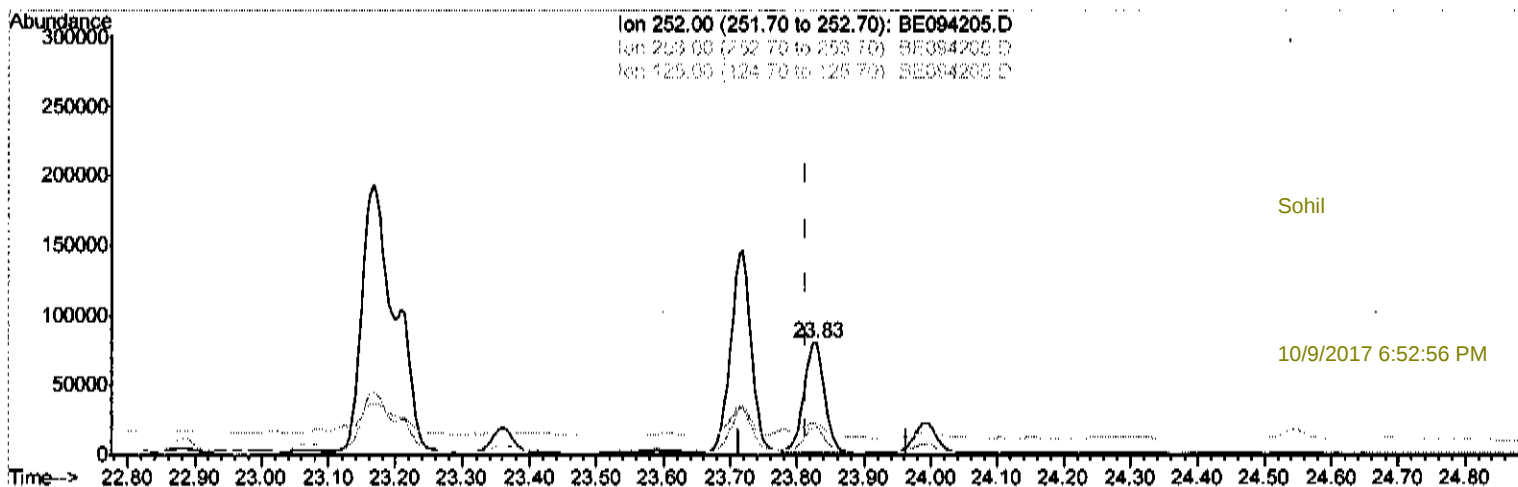

TIC: BE094205.D

(23) Benzo(a)pyrene (C)

23.828min (+0.014) 8.10ng/ul m

response 171848

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	24.78#
125.00	22.60	28.28#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

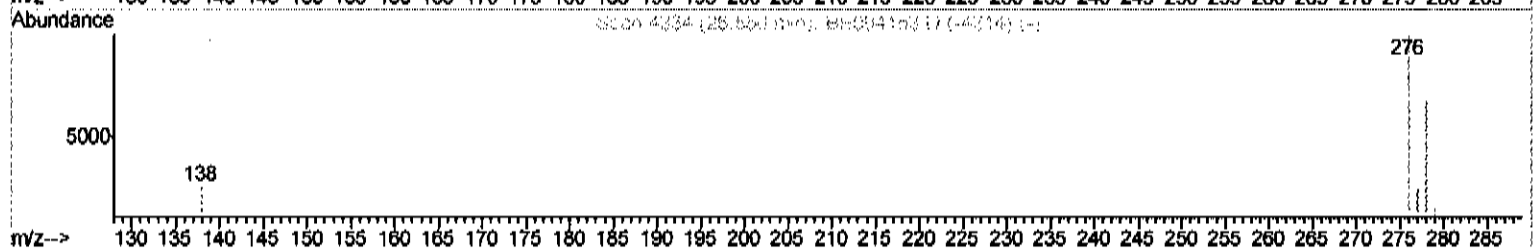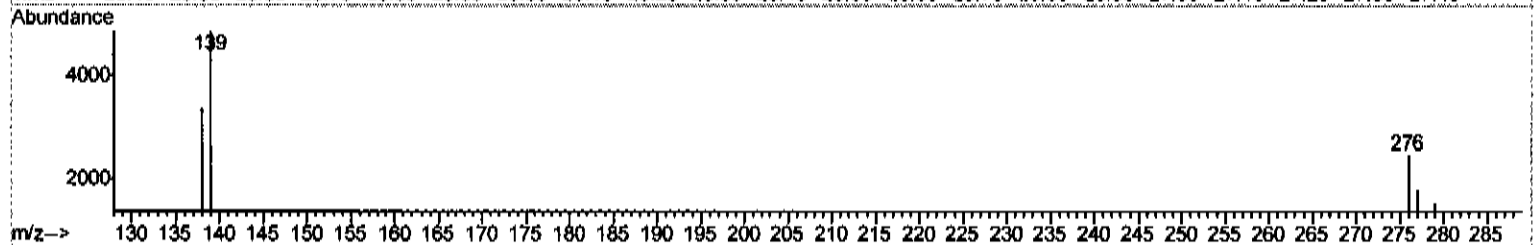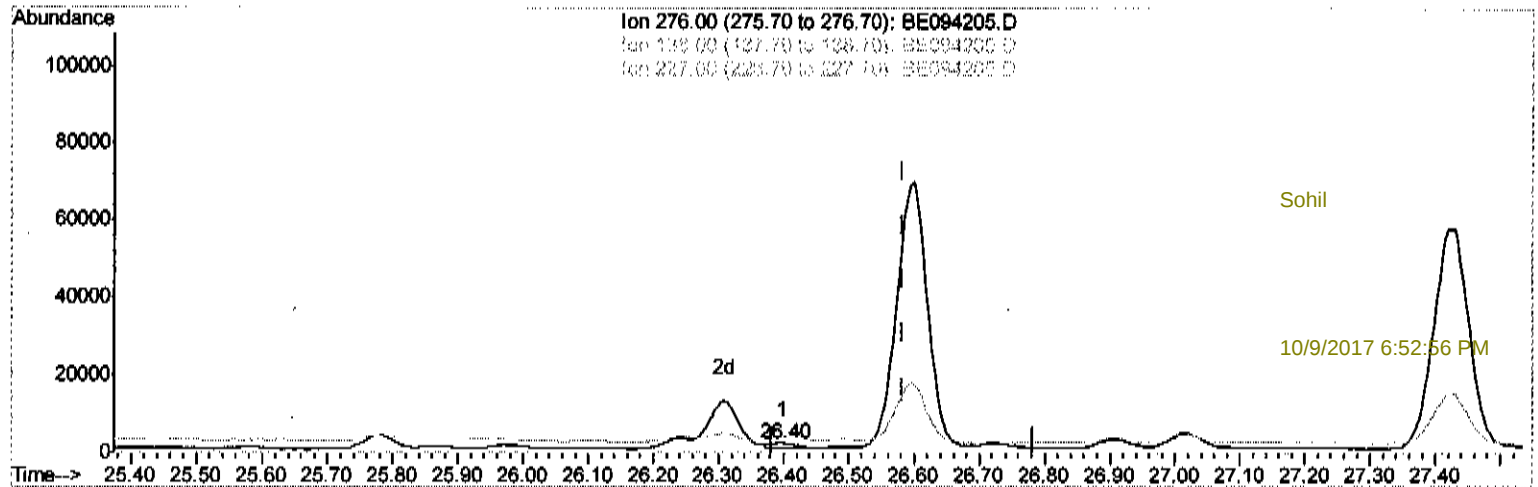

TIC: BE094205.D

(24) Indeno(1,2,3-cd)pyrene

26.399min (-0.164) 0.15ng/ul

SJ

response 3174

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	23.63#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : 15449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

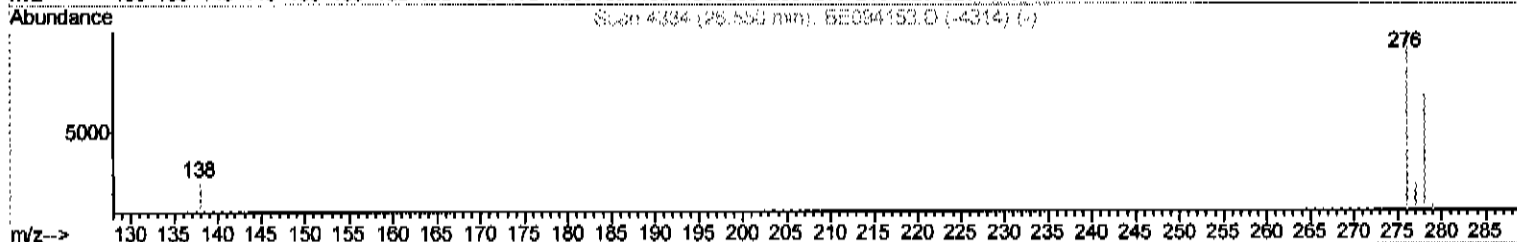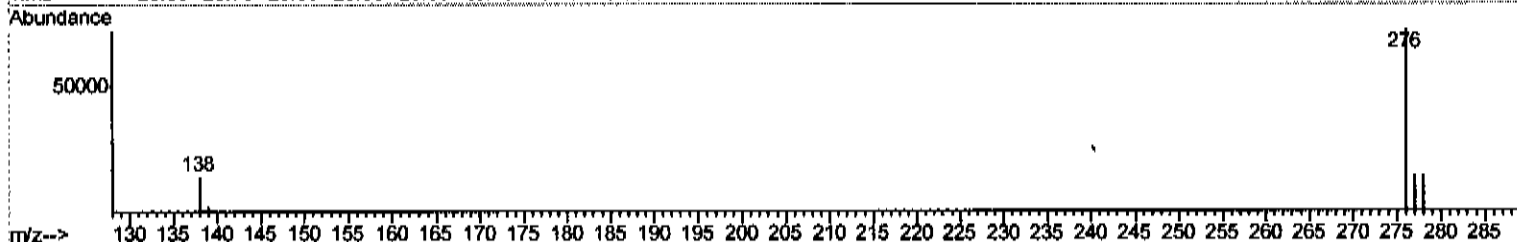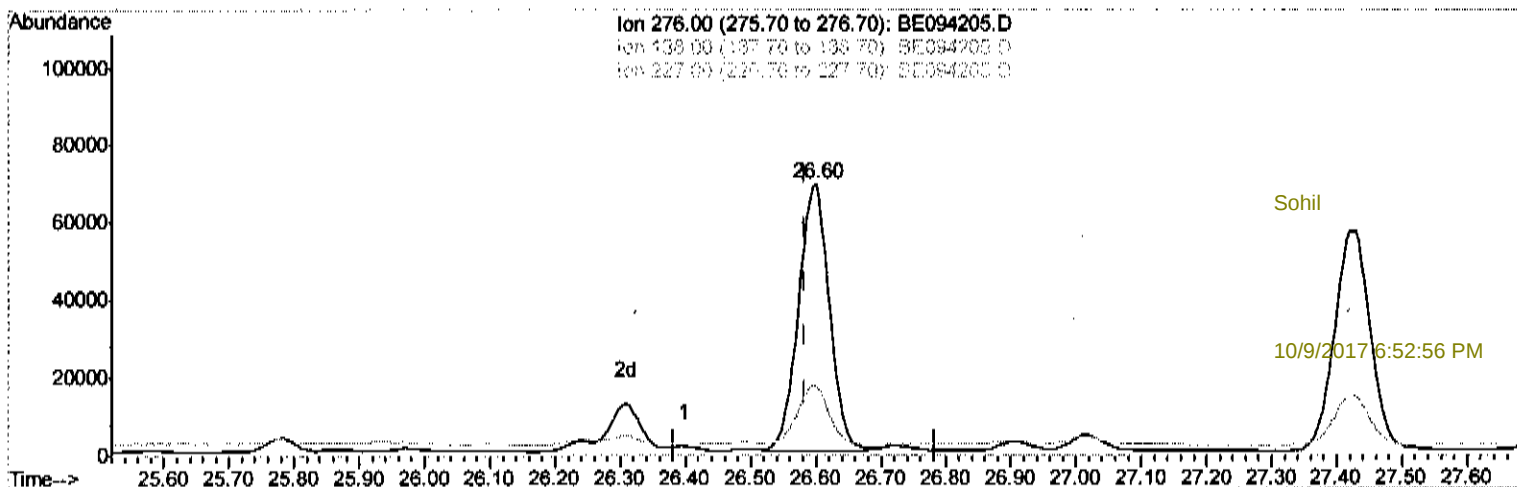

TIC: BE094205.D

(24) Indeno(1,2,3-cd)pyrene

26.600min (+0.017) 10.35ng/ul m

response 224695

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	0.33#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

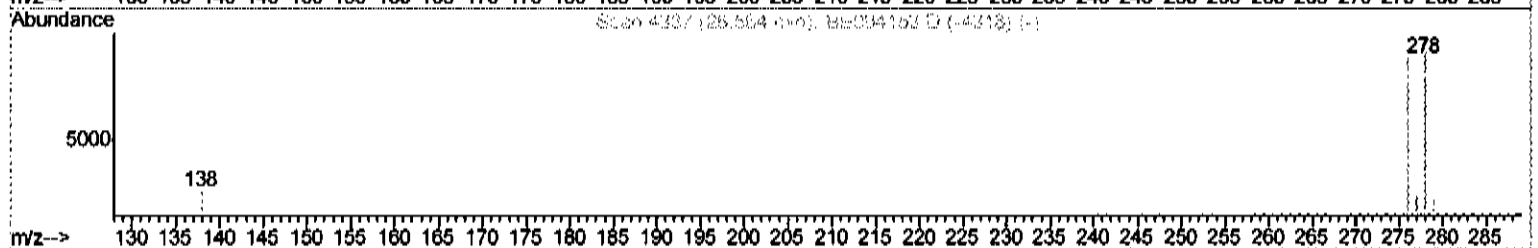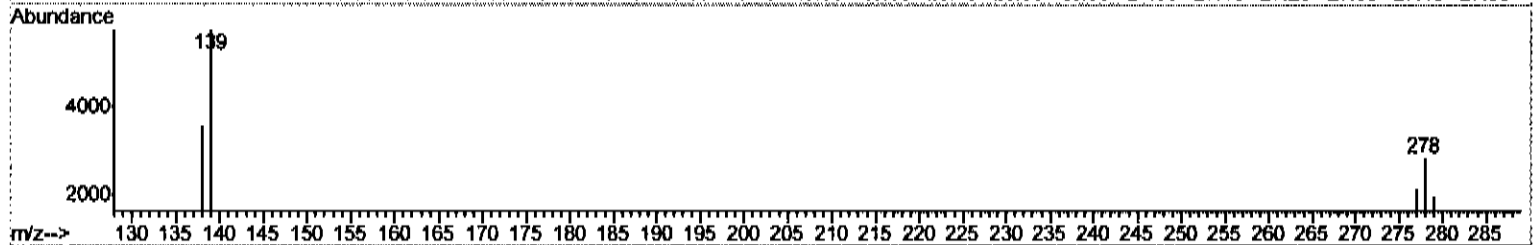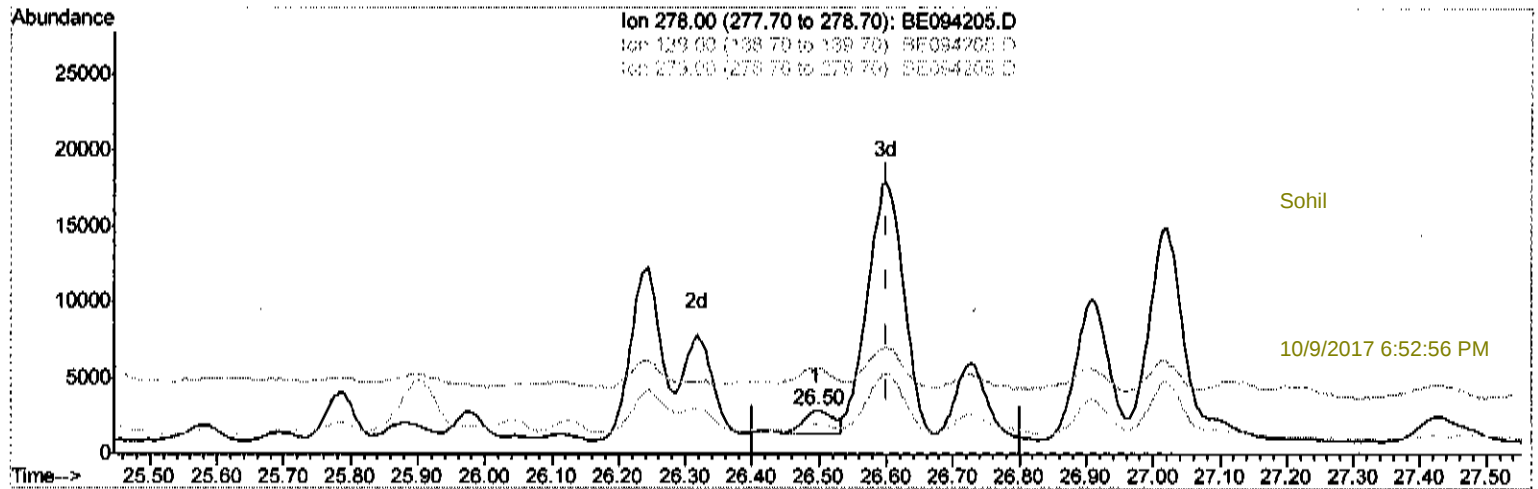

TIC: BE094205.D

(25) Dibenzo(a,h)anthracene

26.495min (-0.106) 0.25ng/ul

response 4486

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	199.83#
279.00	32.40	68.55#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

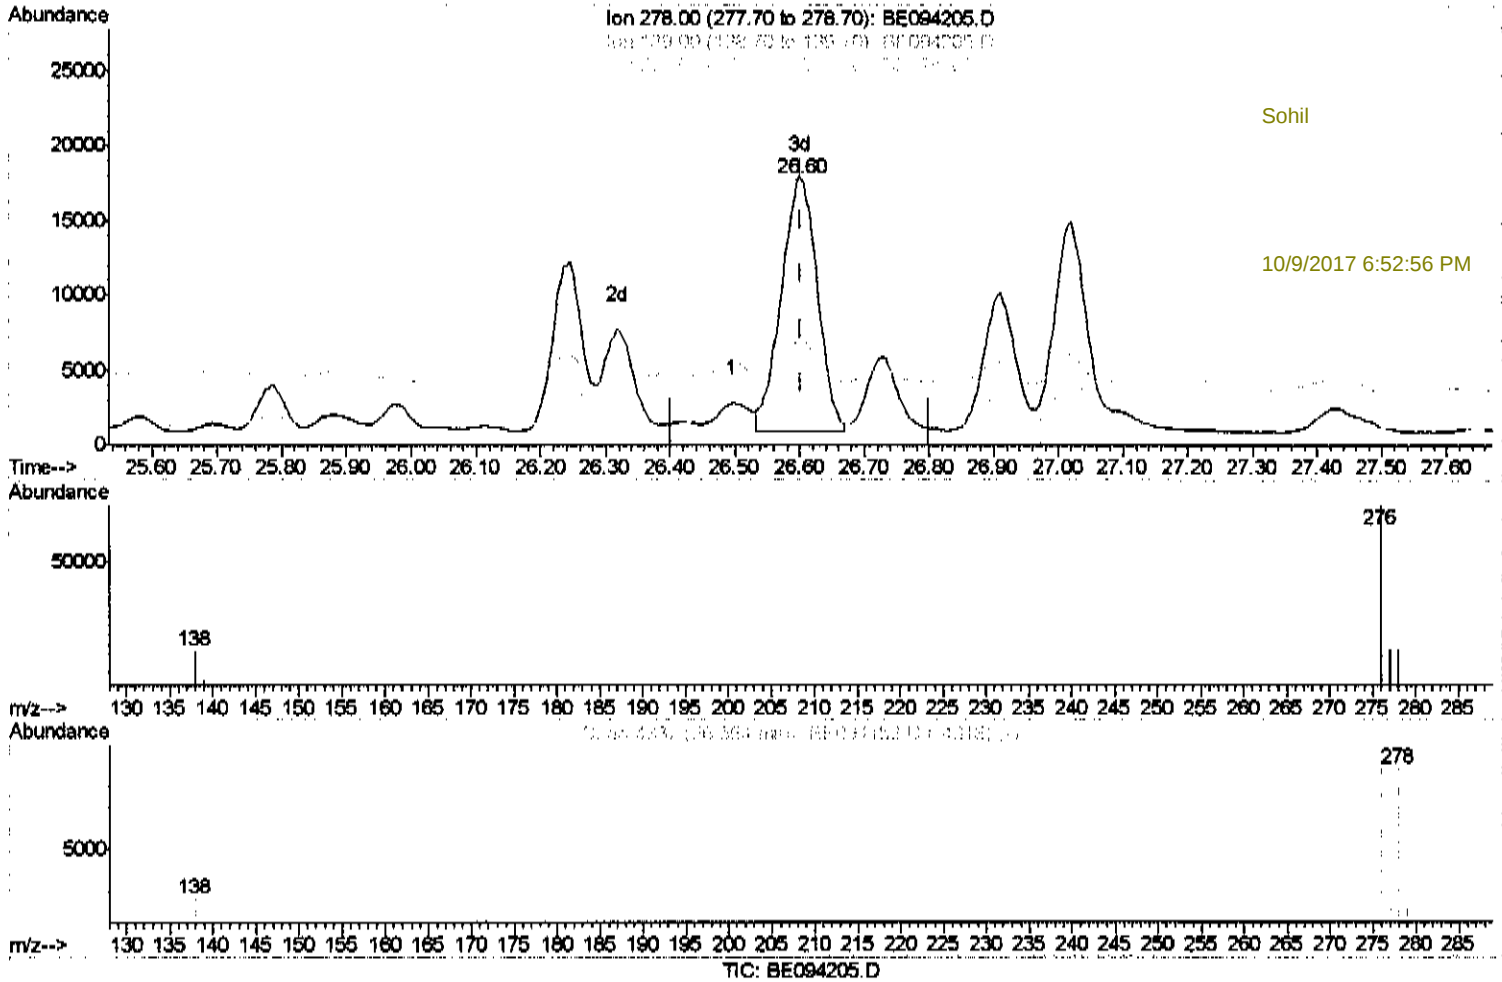

(25) Dibenzo(a,h)anthracene

26.600min (-0.001) 3.59ng/ul m

response 65431

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	39.28#
279.00	32.40	29.31
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 B-40(0-1)-092617

Manual Integrations
 APPROVED



Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

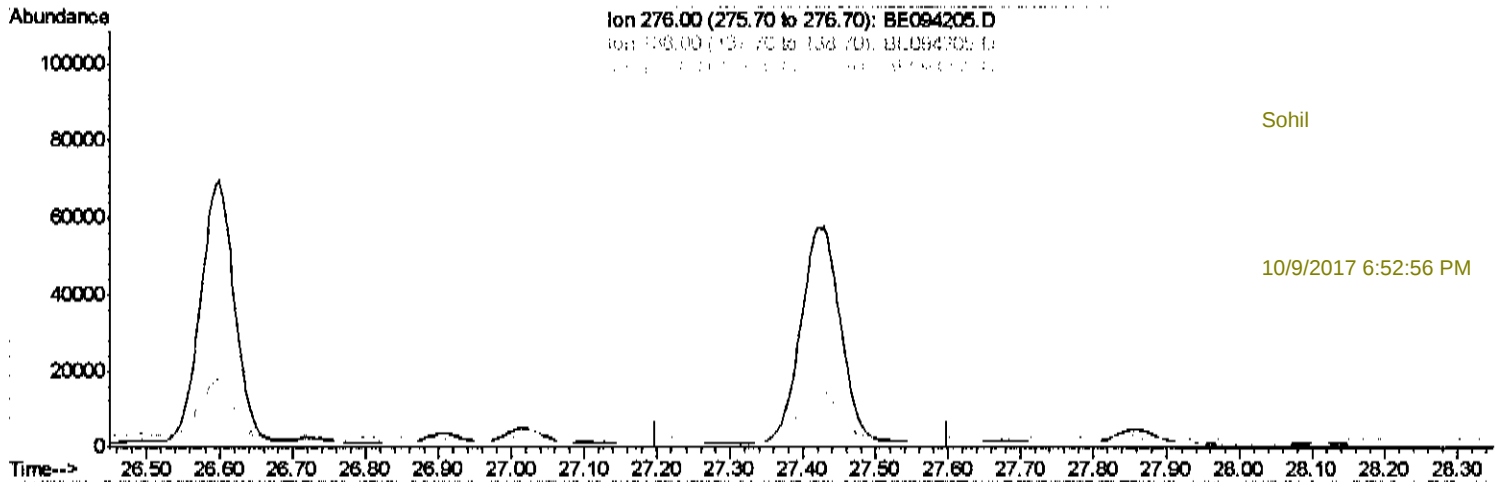

Sohil

10/9/2017 6:52:56 PM

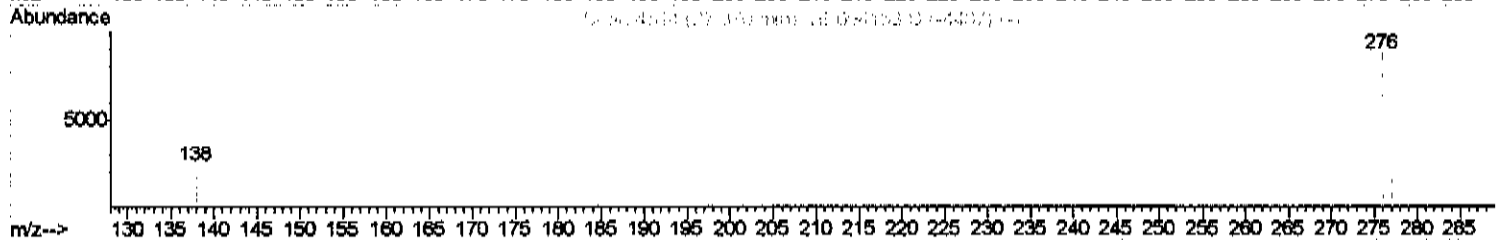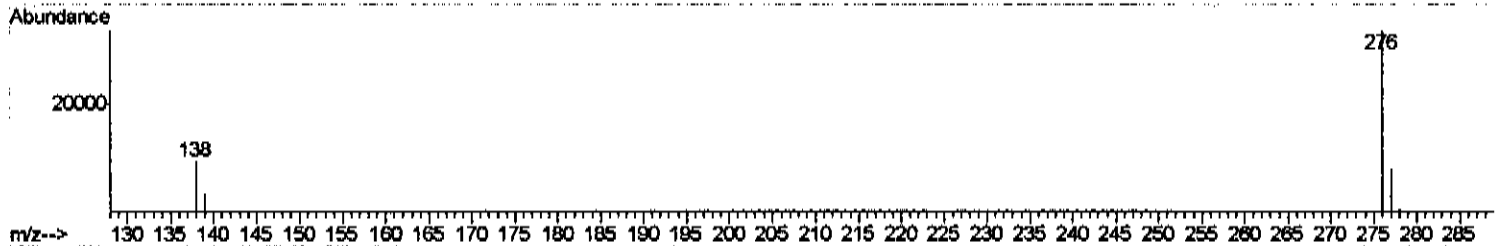

TIC: BE094205.D

(26) Benzo(g,h,i)perylene

27.399min (-27.399) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
138.00	27.30	0.00#
277.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
 Data File : BE094205.D
 Acq On : 7 Oct 2017 16:38
 Operator : SJ/JU
 Sample : I5449-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-40(0-1)-092617

Manual Integrations
 APPROVED

Sohil
 10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 01:38:22 2017
 Response via : Initial Calibration

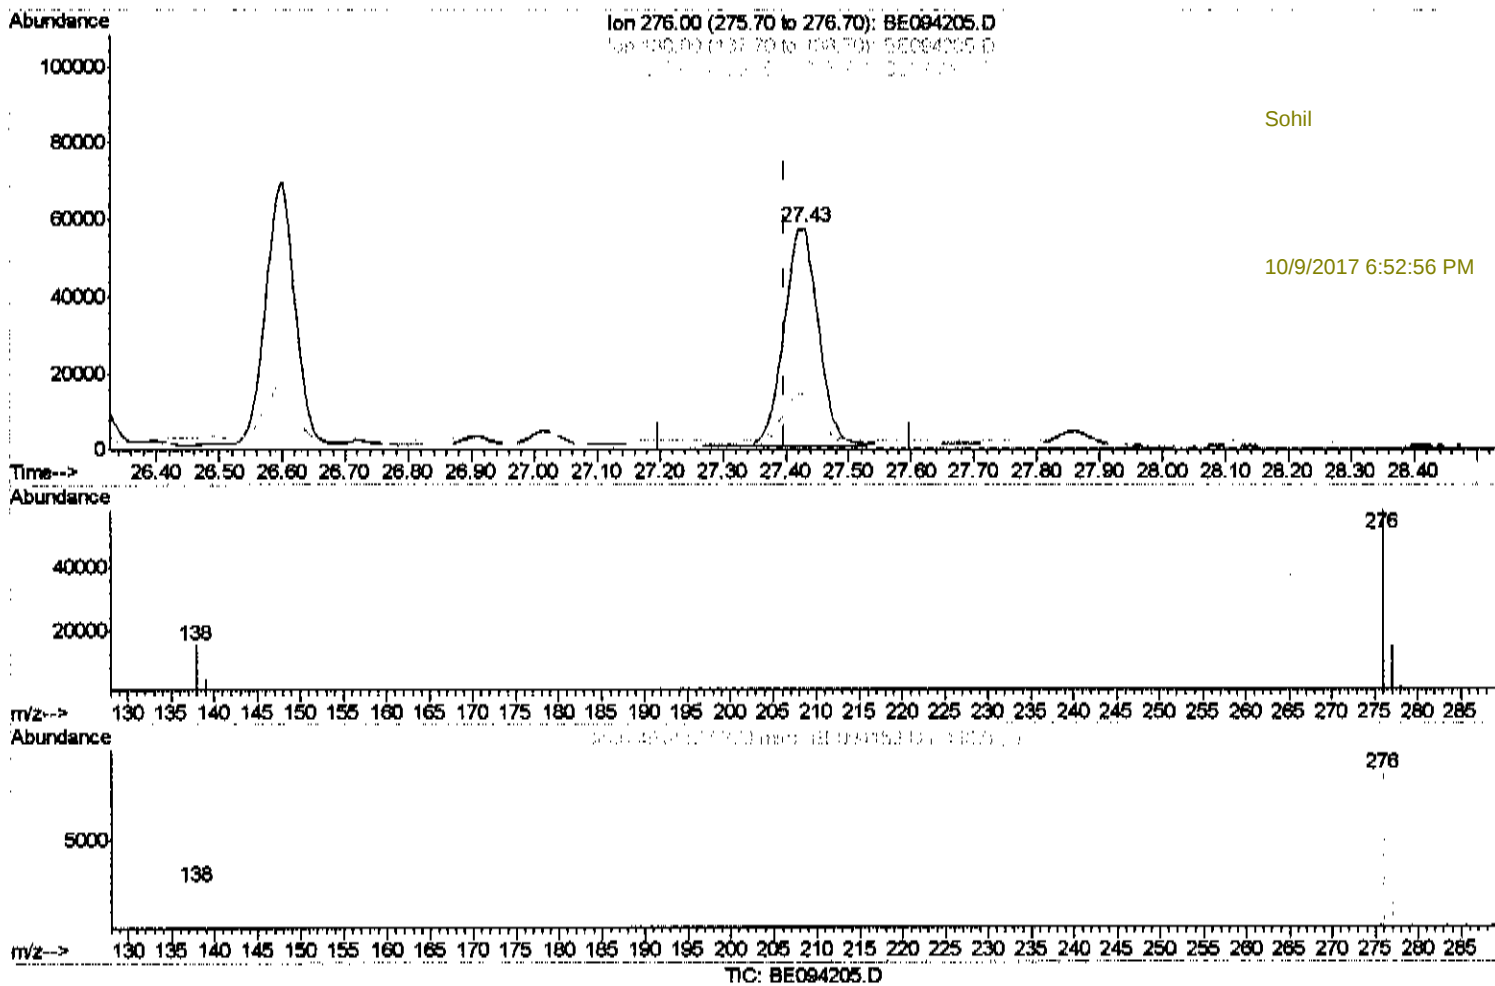

(26) Benzo(g,h,i)perylene

27.429min (+0.031) 11.59ng/ul m

response 216949

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	26.31
277.00	25.60	25.53
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampleId :
B-40(0-1)-092617

Data Path : Z:\HPCHEM1\BNA_E\Data\BE100717\
Data File : BE094205.D
Acq On : 7 Oct 2017 16:38
Operator : SJ/JU
Sample : I5449-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
10/9/2017 6:52:56 PM

Quant Time: Oct 08 03:22:31 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 01:38:22 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1556	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	8038	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.57	164	4958	0.40	ng/ul	0.05
10) Phenanthrene-d10	17.26	188	8381m	0.40	ng/ul	0.02
16) Chrysene-d12	21.41	240	9394m	0.40	ng/ul	0.00
20) Perylene-d12	23.94	264	7517m	0.40	ng/ul	0.00

Sohil

JU 10/9/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.33	152	2128m	0.17	ng/ul	0.04
14) Fluoranthene-d10	19.27	212	4323m	0.15	ng/ul	-0.01

10/9/2017 6:52:56 PM

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.74	128	39994	2.031	ng/ul#	95
7) Acenaphthylene	14.30	152	13836	0.716	ng/ul#	89
8) Acenaphthene	14.63	153	7654	0.481	ng/ul#	87
9) Fluorene	15.59	166	9016	0.484	ng/ul#	81
11) Pentachlorophenol	16.93	266	1143m	1.162	ng/ul	
12) Phenanthrene	17.29	178	373703m	17.063	ng/ul	
13) Anthracene	17.38	178	38482	1.807	ng/ul	95
15) Fluoranthene	19.30	202	578332m	20.097	ng/ul	
17) Pyrene	19.67	202	561446	21.481	ng/ul#	80
18) Benzo(a)anthracene	21.40	228	262453	10.531	ng/ul#	86
19) Chrysene	21.45	228	407718	14.167	ng/ul	95
21) Benzo(b)fluoranthene	23.17	252	506752m	24.817	ng/ul	
22) Benzo(k)fluoranthene	23.21	252	149127m	6.318	ng/ul	
23) Benzo(a)pyrene	23.83	252	171848m	8.099	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.60	276	224695m	10.352	ng/ul	
25) Dibenzo(a,h)anthracene	26.60	278	65431m	3.594	ng/ul	
26) Benzo(g,h,i)perylene	27.43	276	216949m	11.587	ng/ul	

JU 10/9/17

JU 10/9/17

JU 10/9/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed