
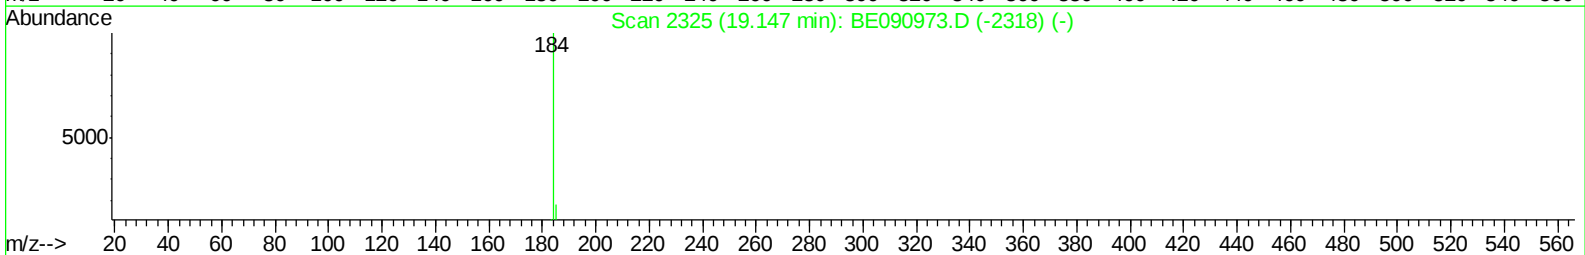
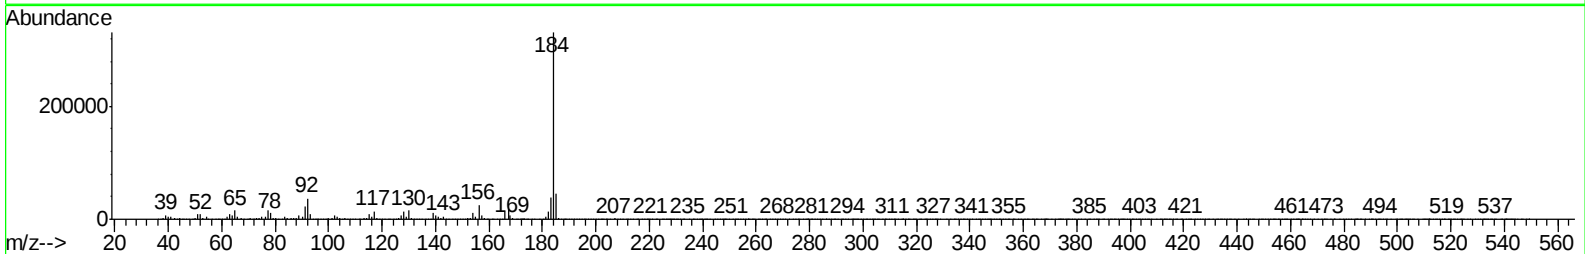


Data Path : Z:\HPCHEM1\BNA E\Data\BE100815\
Data File : BE090995.D
Acq On : 8 Oct 2015 8:49
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 01:32:17 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 17:11:43 2015
Response via : Initial Calibration

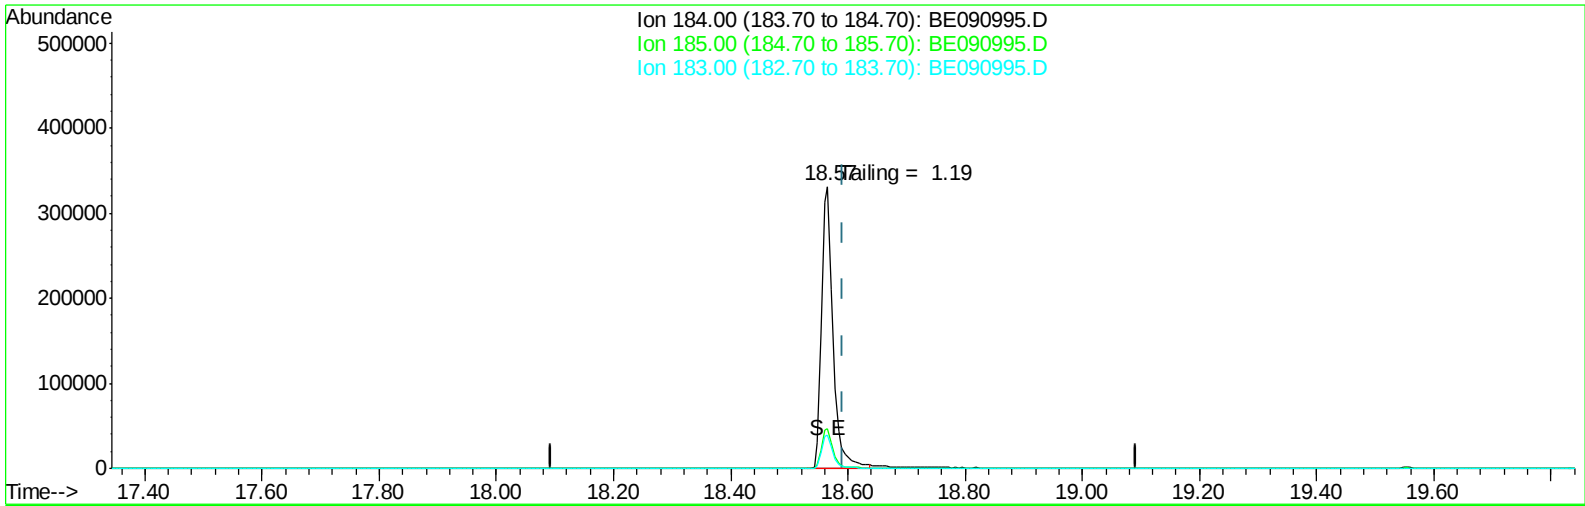

TIC: BE090995.D

(27) Benzidine




18.566min (-0.028) 554.70ng

response 462436

Ion	Exp%	Act%
184.00	100	100
185.00	27.90	13.93#
183.00	20.50	11.61#
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA E\Data\BE100815\  
Data File : BE090995.D  
Acq On    : 8 Oct 2015 8:49  
Operator  : UM/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Oct 09 01:32:17 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 17:11:43 2015
Response via : Initial Calibration

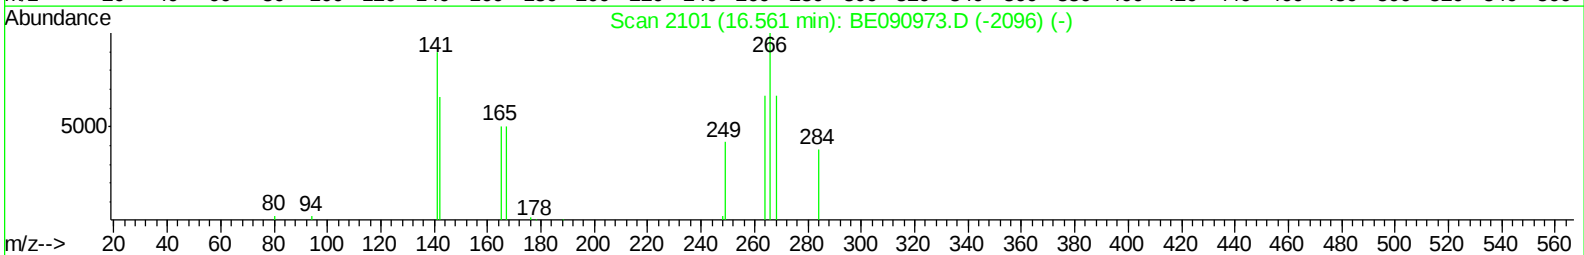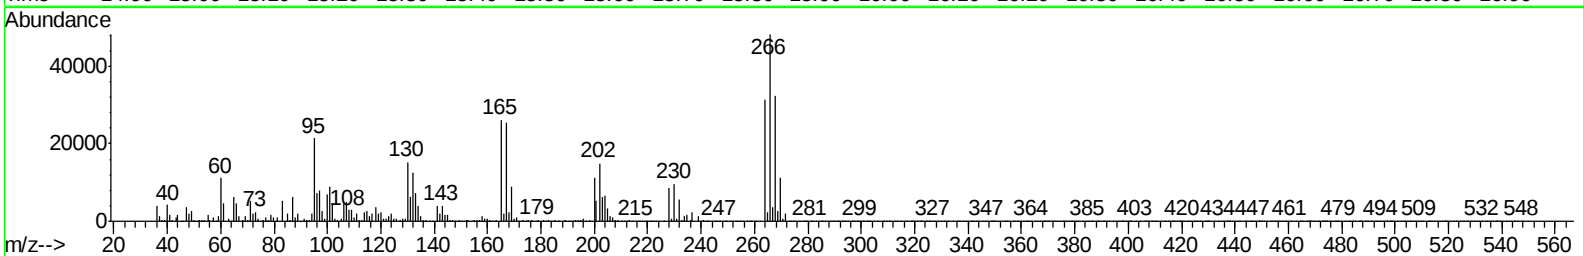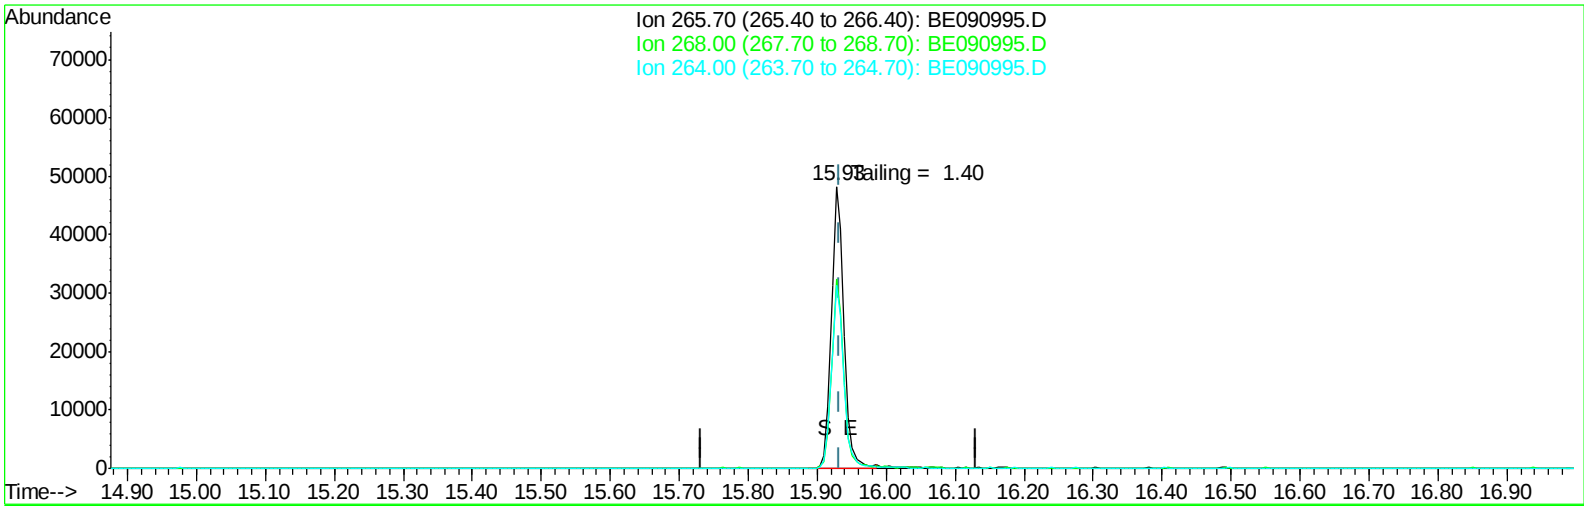

TIC: BE090995.D

(22) Pentachlorophenol
15.928min (-0.004) 611.71ng
response 61277

Ion	Exp%	Act%
265.70	100	100
268.00	72.70	67.08
264.00	70.30	65.05
0.00	0.00	0.00