


Data Path : Z:\HPCHEM1\BNA E\DATA\BE100815\
 Data File : BE090995.D
 Acq On : 8 Oct 2015 8:49
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 07 17:11:43 2015

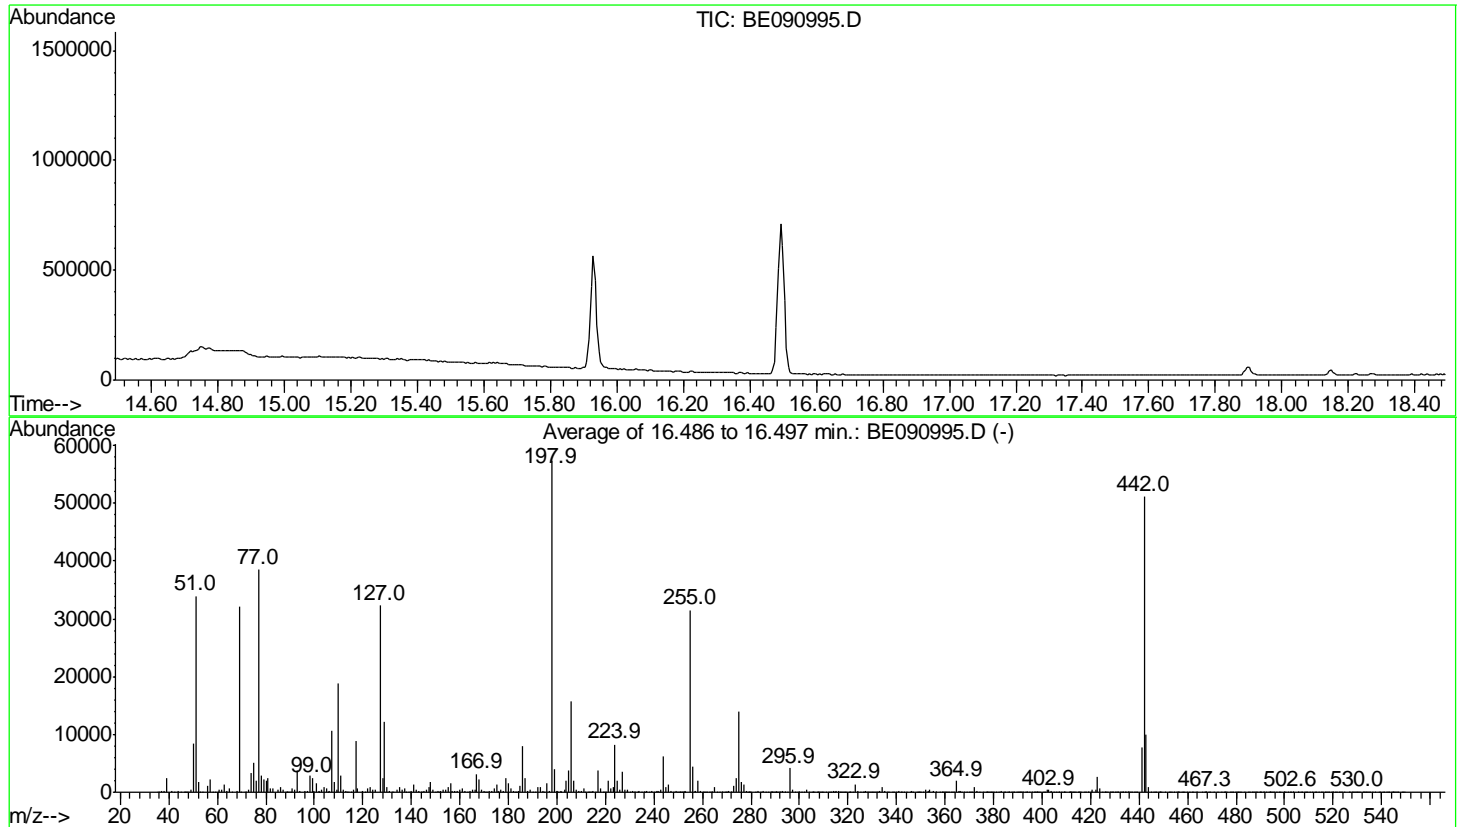

AutoFind: Scans 2365, 2366, 2367; Background Corrected with Scan 2358

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.2	33991	PASS
68	69	0.00	2	0.8	256	PASS
69	198	0.00	100	55.9	32072	PASS
70	69	0.00	2	0.3	101	PASS
127	198	10	80	56.4	32332	PASS
197	198	0.00	2	0.5	276	PASS
198	198	100	100	100.0	57369	PASS
199	198	5	9	7.0	4030	PASS
275	198	10	60	24.2	13876	PASS
365	198	1	100	3.3	1898	PASS
441	442	0.01	24	15.3	7838	PASS
442	198	50	100	89.1	51104	PASS
443	442	15	24	19.6	10030	PASS