

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
 Data File : BE094219.D
 Acq On : 9 Oct 2017 13:59
 Operator : SJ/JU
 Sample : PB102985BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 10 09:19:09 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 09:18:40 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1277	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	7024	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	4280	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.42	240	8532	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	602337	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3414	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	8585	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	1028	0.064	ng/ul#	24
17) Pyrene	19.64	202	1173	0.049	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094219.D
Acq On : 9 Oct 2017 13:59
Operator : SJ/JU
Sample : PB102985BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 10 09:19:09 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

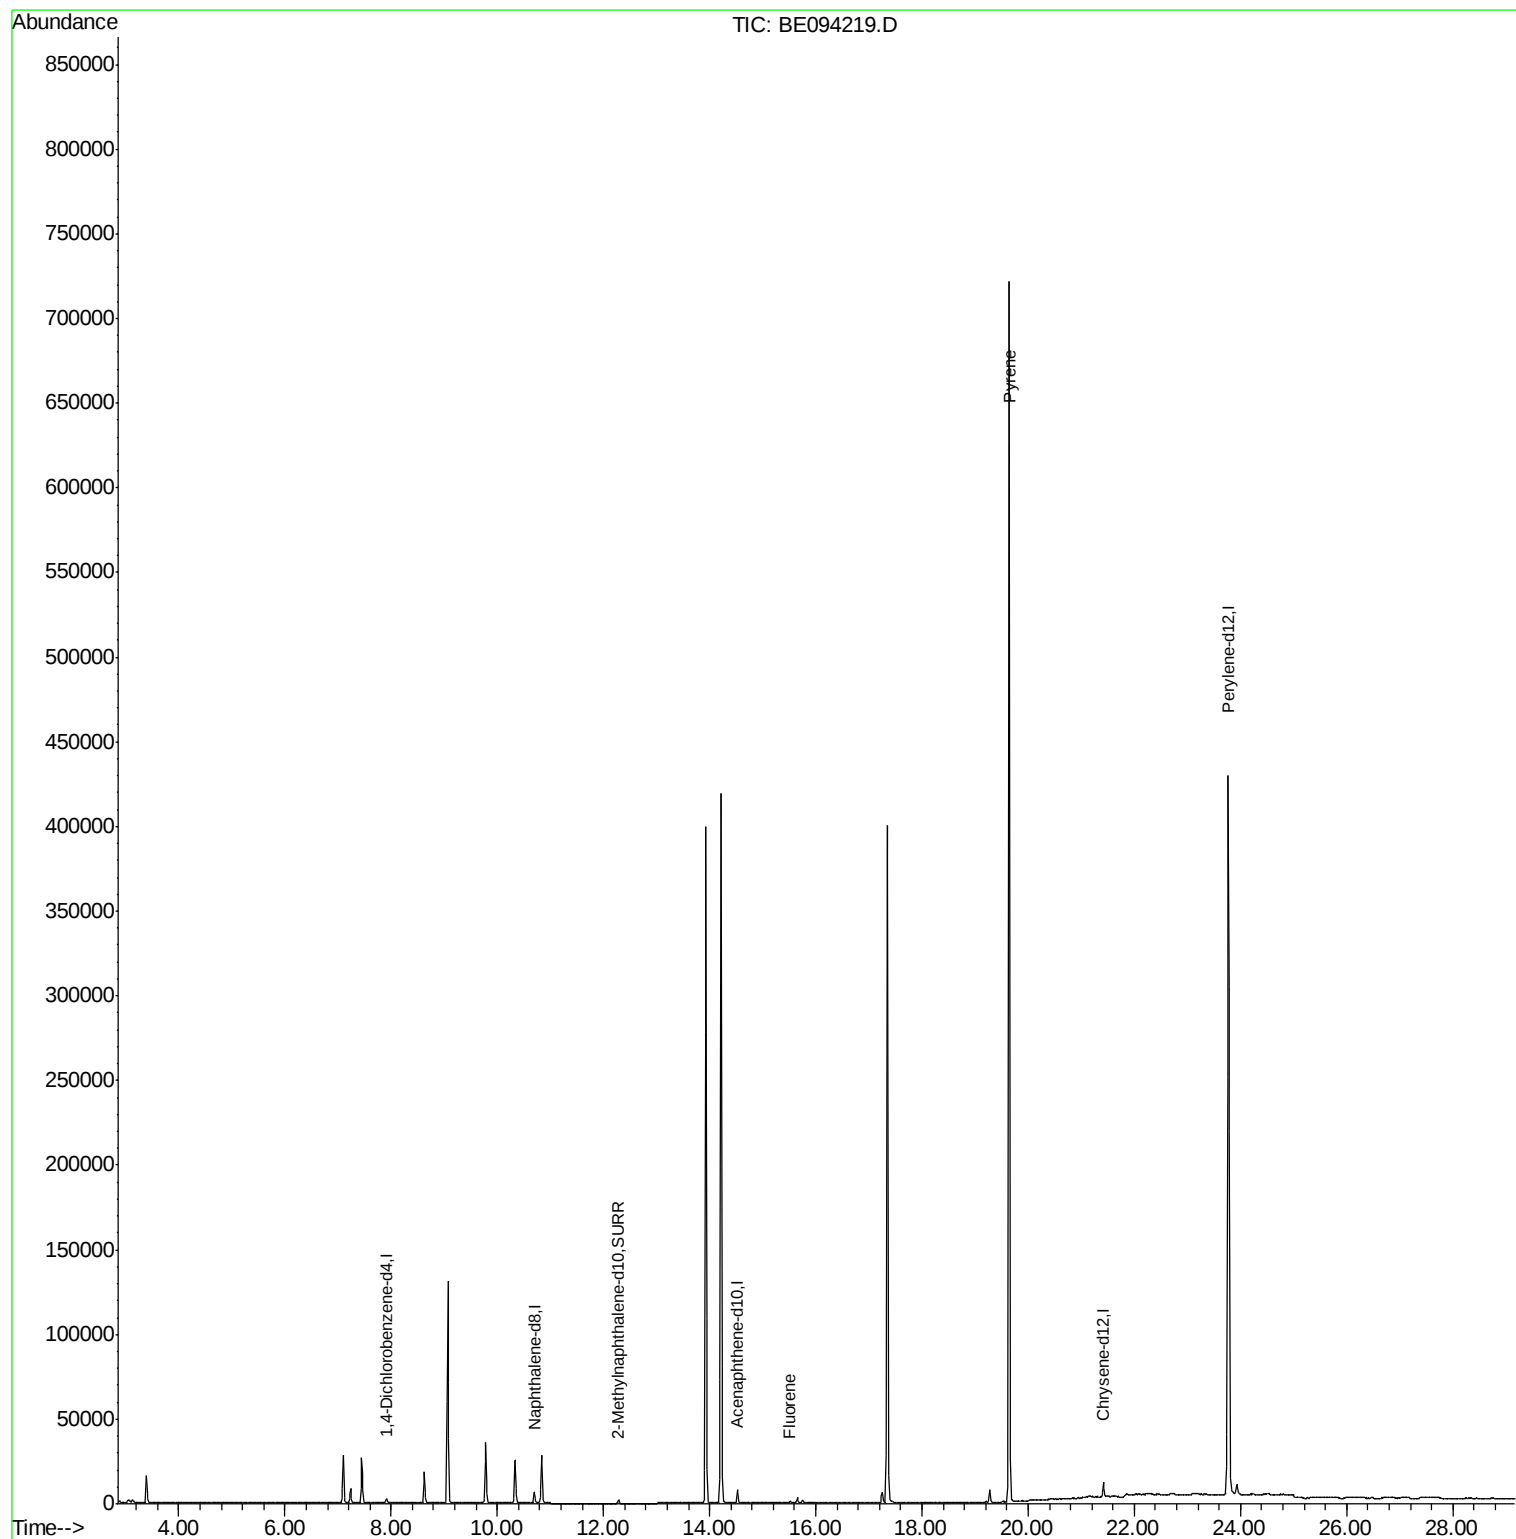

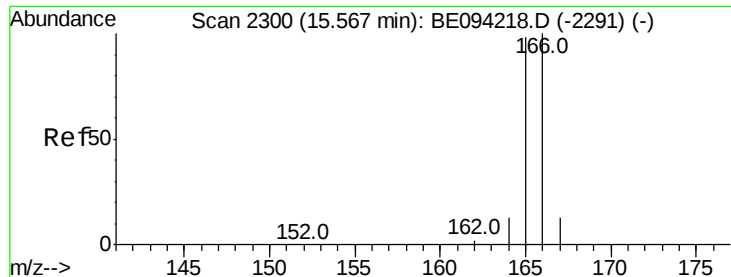

#9

Fluorene

Concen: 0.064 ng/ul

RT: 15.51 min Scan# 2292

Delta R.T. -0.05 min

Lab File: BE094219.D

Acq: 9 Oct 2017 13:59

Instrument :

BNA_E

ClientSampleId :


Tot Ion:166 Resp: 1028

Ion Ratio Lower Upper




166 100

165 13.4 73.4 110.2#

167 37.4 14.6 22.0#

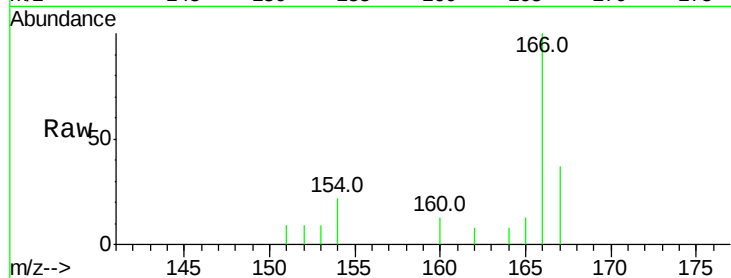

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

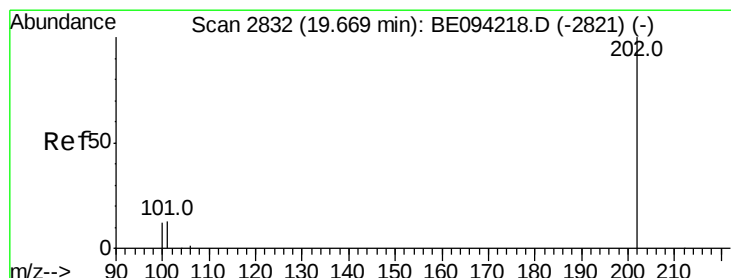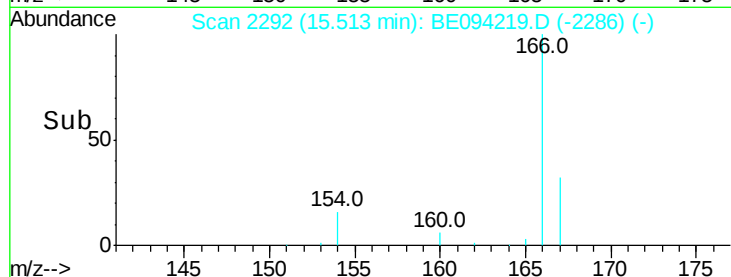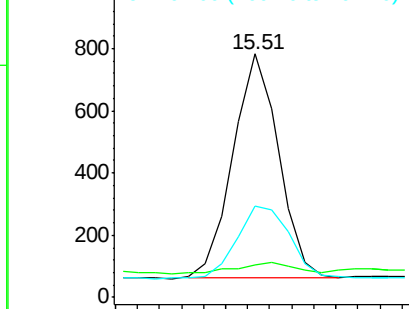

#17

Pyrene

Concen: 0.049 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.03 min

Lab File: BE094219.D

Acq: 9 Oct 2017 13:59


Tgt Ion:202 Resp: 1173

Ion Ratio Lower Upper

202 100

101 136.1 18.2 27.4#

100 730.0 15.6 23.4#

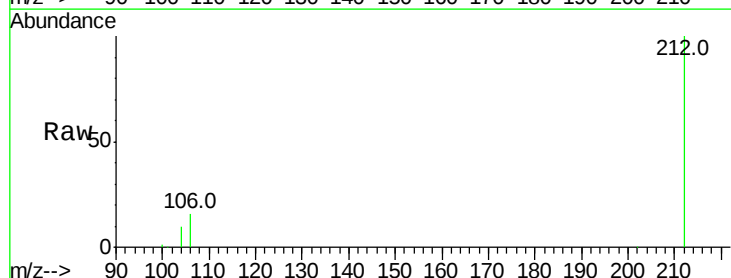

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

