

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
 Data File : BE094223.D
 Acq On : 9 Oct 2017 16:28
 Operator : SJ/JU
 Sample : I5522-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 10 09:20:13 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 09:18:40 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1269	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	7042	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	4259	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	10058	0.40	ng/ul	0.00
20) Perylene-d12	23.77	264	612779	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3110	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	8673	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
17) Pyrene	19.66	202	12087	0.432	ng/ul#	85
18) Benzo(a)anthracene	21.39	228	7022	0.263	ng/ul#	89
19) Chrysene	21.45	228	8912	0.289	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094223.D
Acq On : 9 Oct 2017 16:28
Operator : SJ/JU
Sample : I5522-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 10 09:20:13 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration




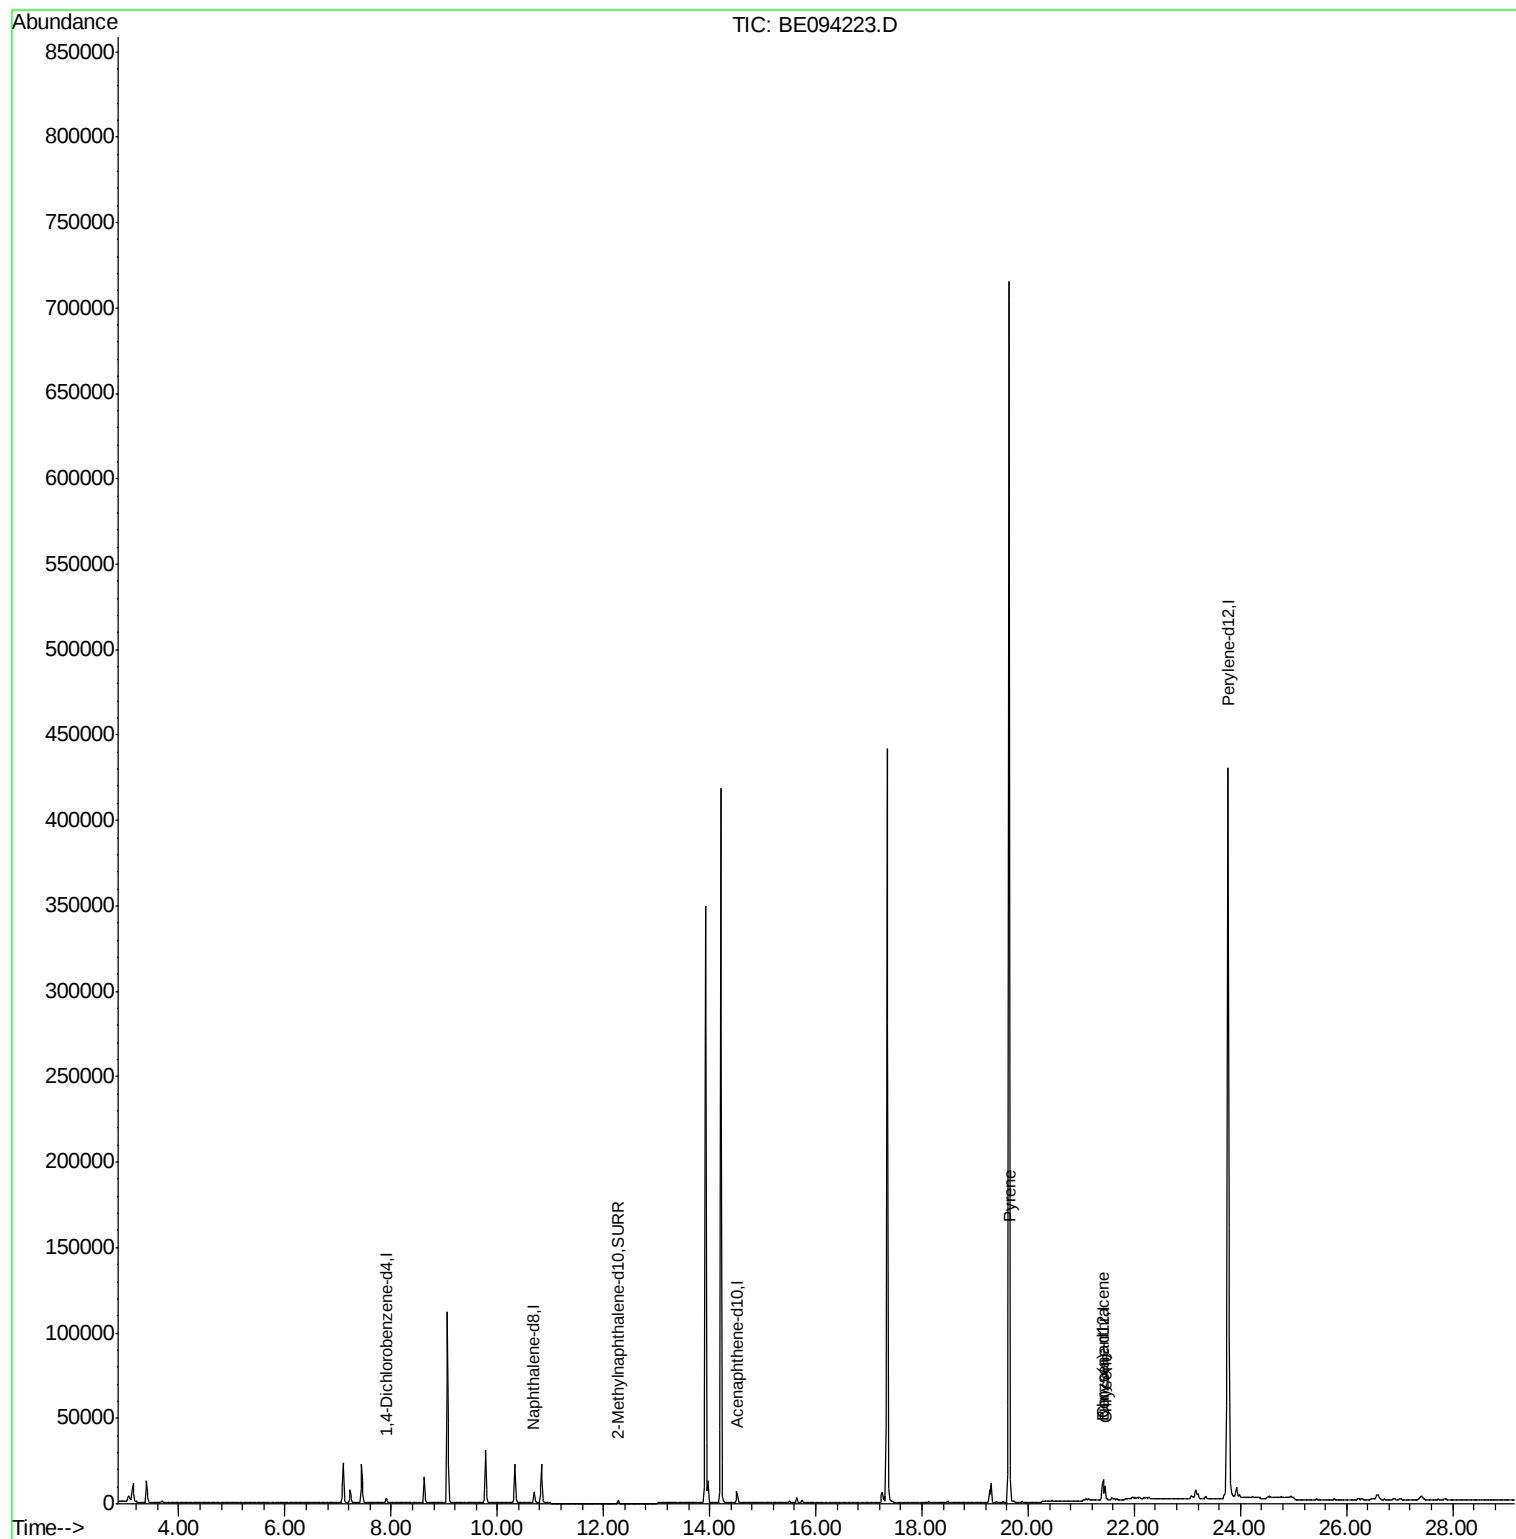


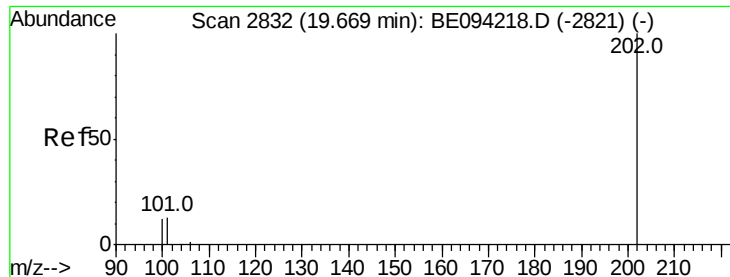

#17
Pvrene
Concen: 0.432 ng/ul
RT: 19.66 min Scan# 2831
Delta R.T. -0.01 min
Lab File: BE094223.D
Acq: 9 Oct 2017 16:28




Instrument :
BNA_E
ClientSampleId :




Tot Ion:202 Resp: 12087
Ion Ratio Lower Upper
202 100
101 14.9 18.2 27.4#
100 13.3 15.6 23.4#

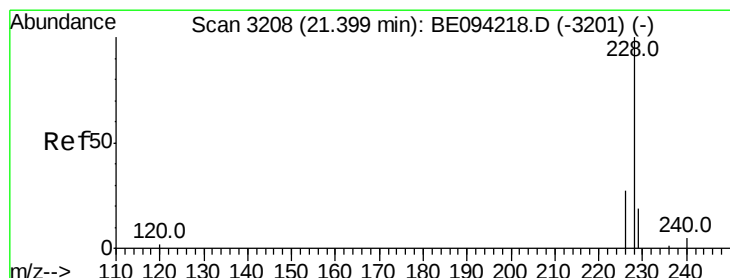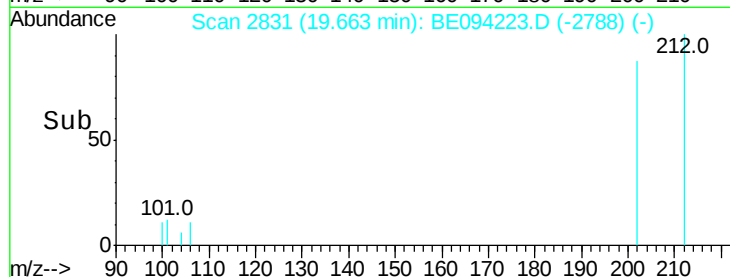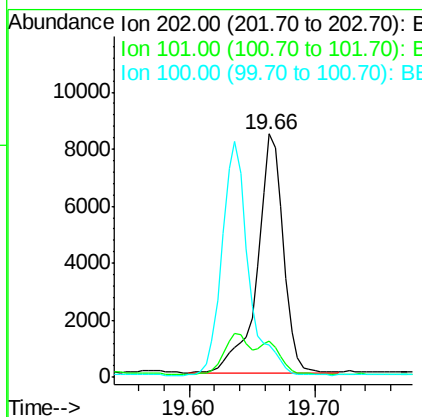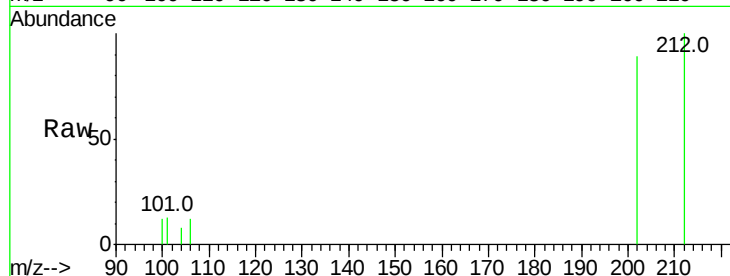

#18
Benzo(a)anthracene
Concen: 0.263 ng/ul
RT: 21.39 min Scan# 3208
Delta R.T. -0.00 min
Lab File: BE094223.D
Acq: 9 Oct 2017 16:28

Tgt Ion:228 Resp: 7022
Ion Ratio Lower Upper
228 100
229 28.8 22.8 34.2
226 32.7 17.0 25.6#

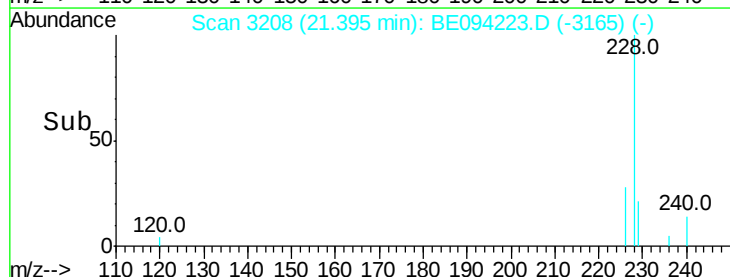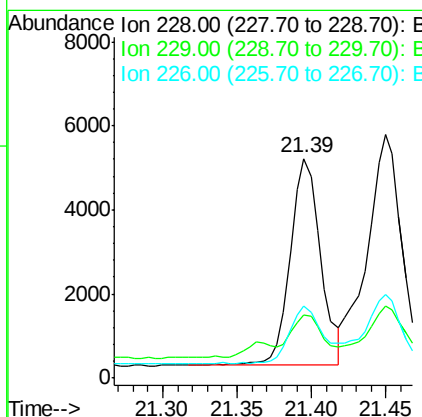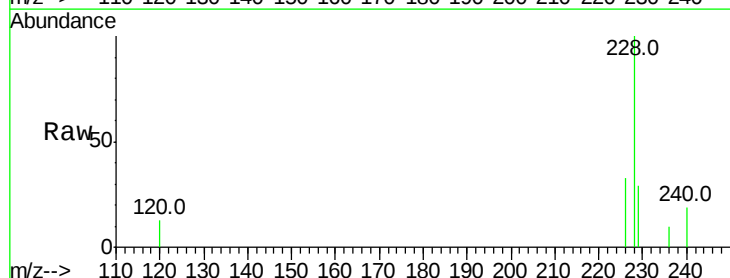

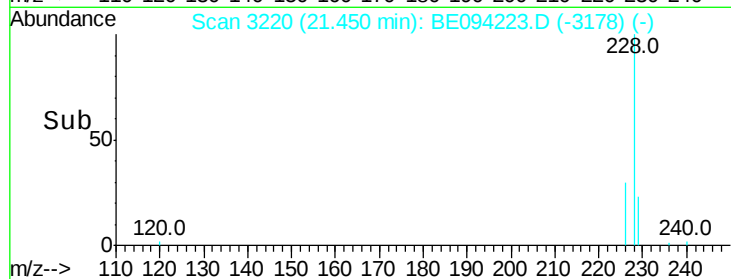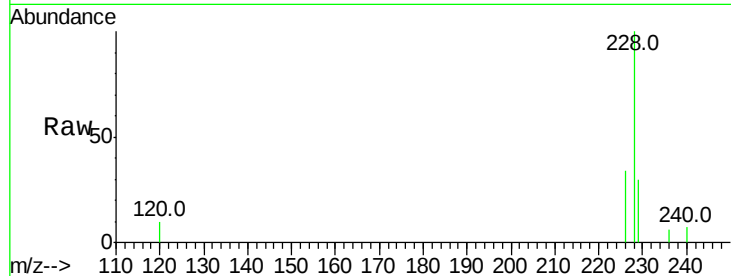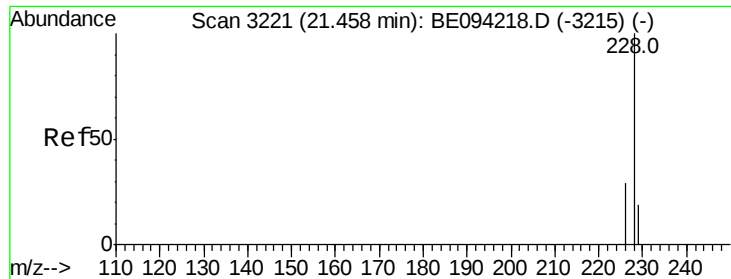

#19

Chrysene

Concen: 0.289 ng/ul

RT: 21.45 min Scan# 3220

Delta R.T. -0.01 min

Lab File: BE094223.D

Acq: 9 Oct 2017 16:28

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 8912

Ion Ratio Lower Upper

228 100

226 34.1 23.4 35.0

229 29.6 17.7 26.5#

