

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
 Data File : BE094236.D
 Acq On : 10 Oct 2017 00:31
 Operator : SJ/JU
 Sample : PB102994BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 10 08:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 04:05:38 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	2446	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	12938	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	7943	0.40	ng/ul	-0.02
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.41	240	16460	0.40	ng/ul	-0.01
20) Perylene-d12	23.76	264	1095423	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	6235	0.31	ng/ul	-0.02
14) Fluoranthene-d10	19.27	212	14744	0.00	ng/ul	-0.02
Target Compounds						
9) Fluorene	15.51	166	1783	0.06	ng/ul#	22
17) Pyrene	19.63	202	1946	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094236.D
Acq On : 10 Oct 2017 00:31
Operator : SJ/JU
Sample : PB102994BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 10 08:51:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 04:05:38 2017
Response via : Initial Calibration

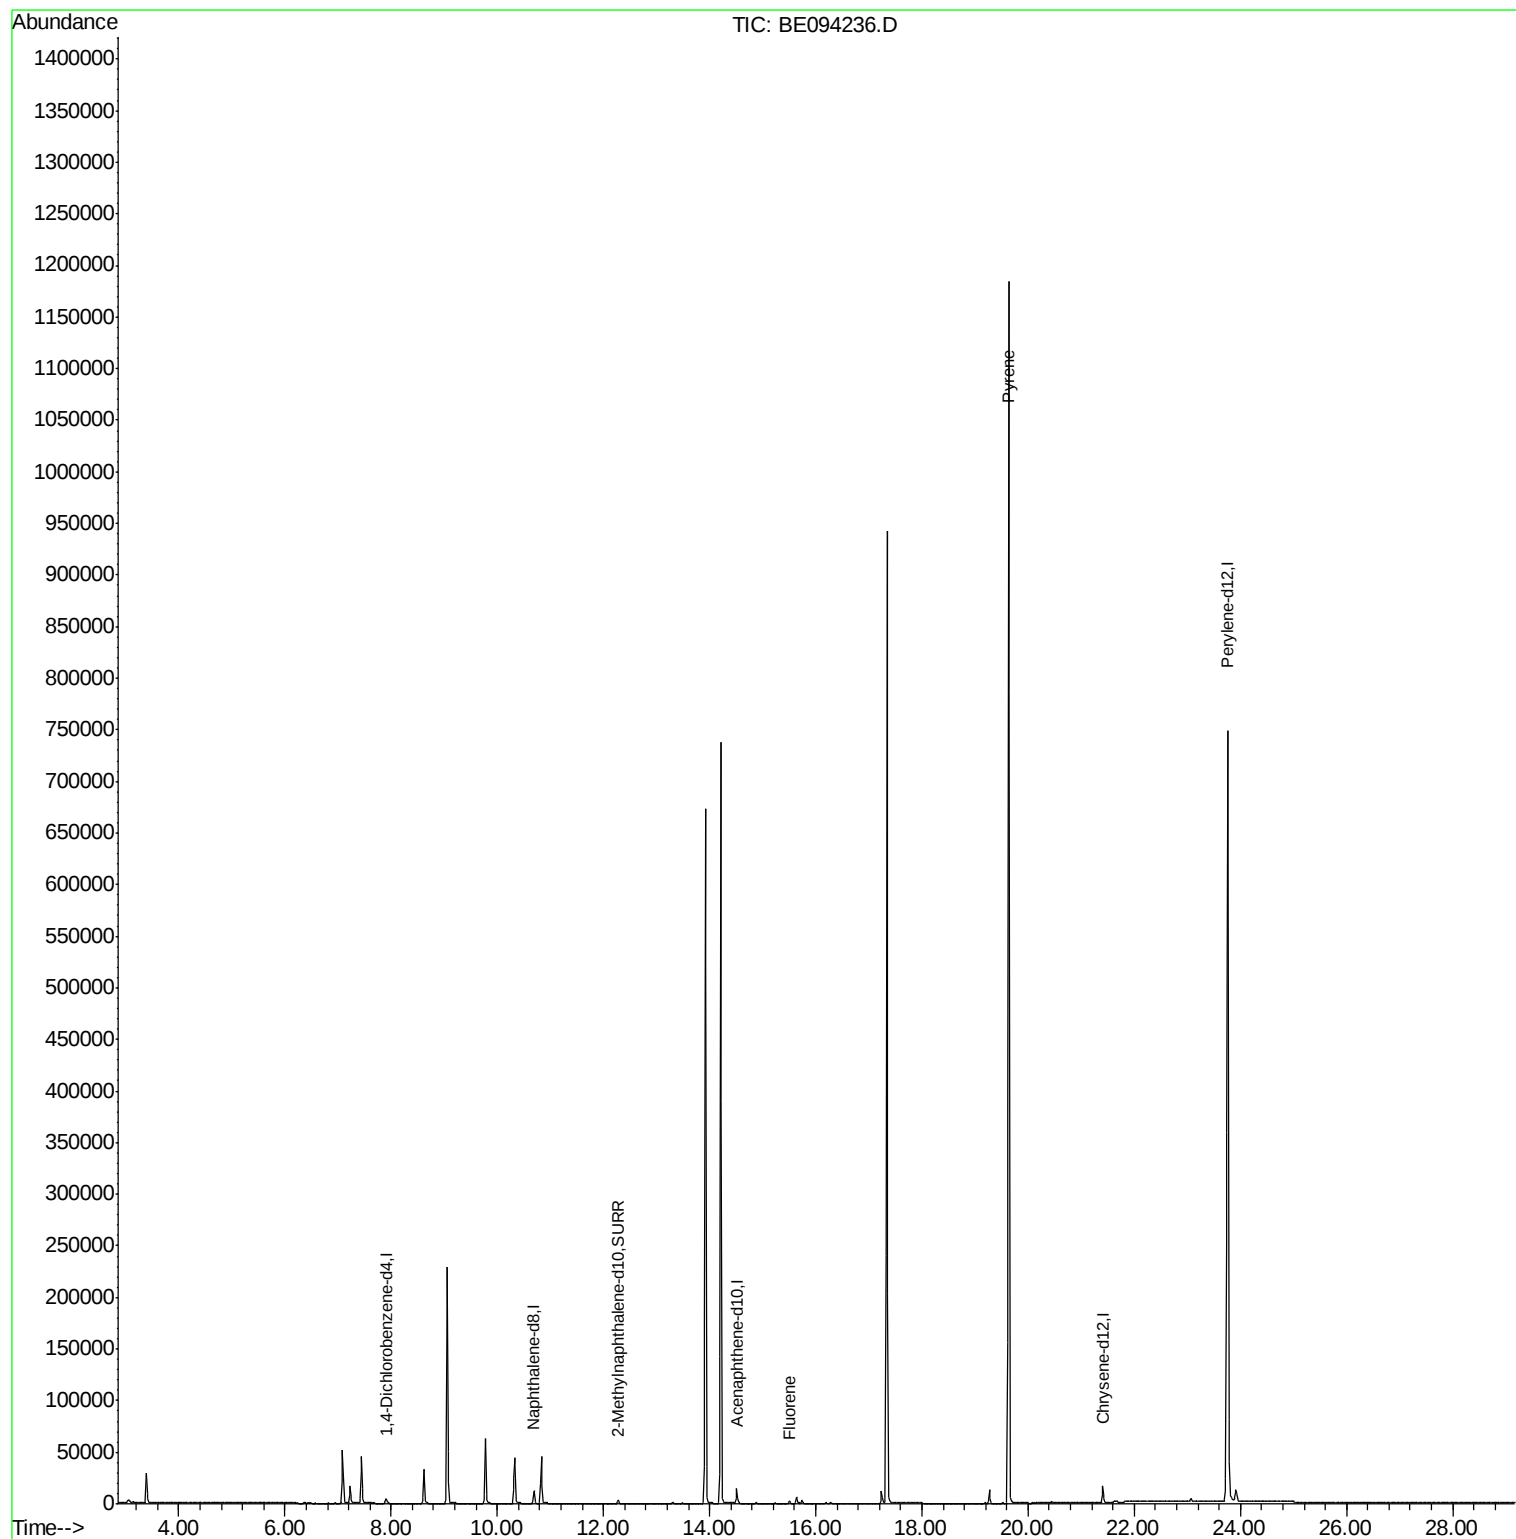

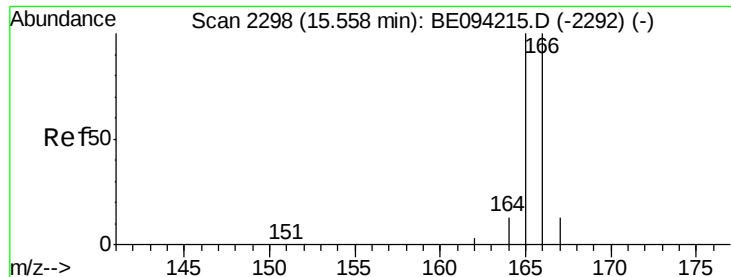

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.51 min Scan# 2292

Delta R.T. -0.08 min

Lab File: BE094236.D

Acq: 10 Oct 2017 00:31

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 1783

Ion Ratio Lower Upper

166 100

165 9.2 73.4 110.2#

167 34.4 14.6 22.0#

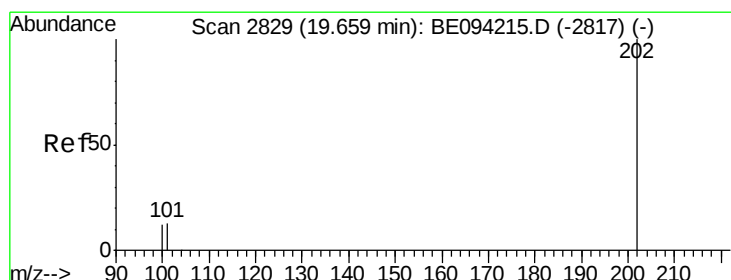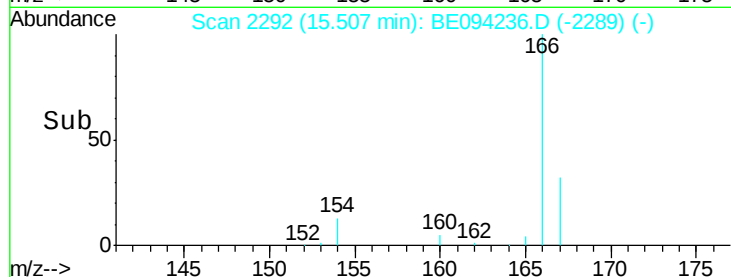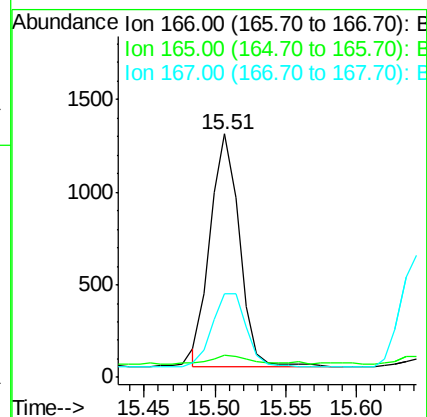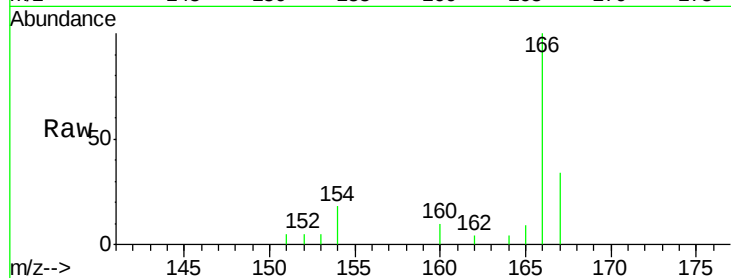

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.63 min Scan# 2824

Delta R.T. -0.04 min

Lab File: BE094236.D

Acq: 10 Oct 2017 00:31

Tgt Ion:202 Resp: 1946

Ion Ratio Lower Upper

202 100

101 170.6 18.2 27.4#

100 993.6 15.6 23.4#

