




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094219.D
Acq On : 9 Oct 2017 13:59
Operator : SJ/JU
Sample : PB102985BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK85

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:36 PM

Quant Time: Oct 10 09:19:09 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

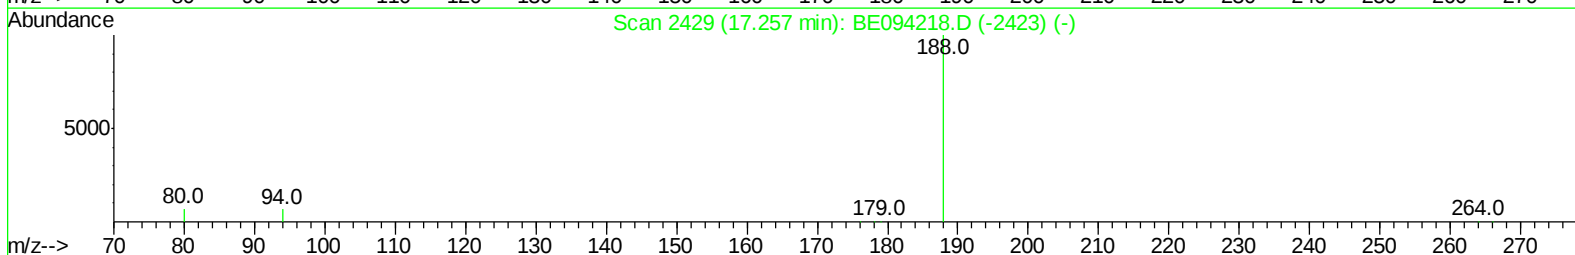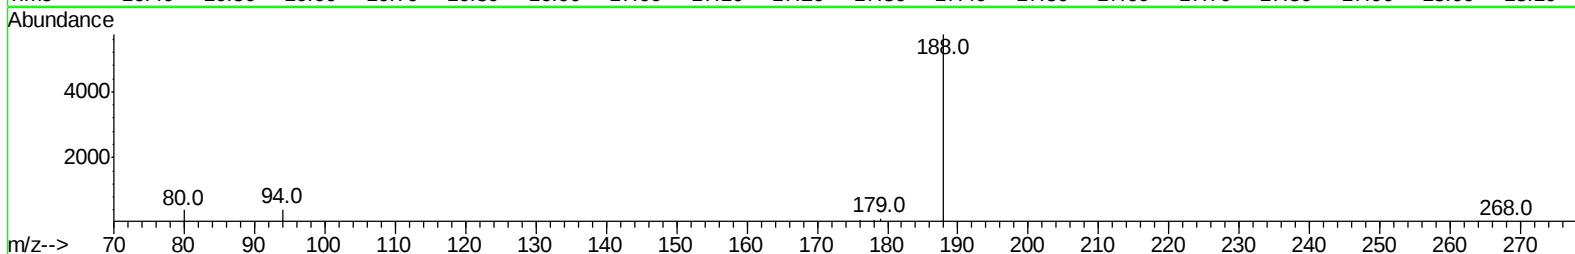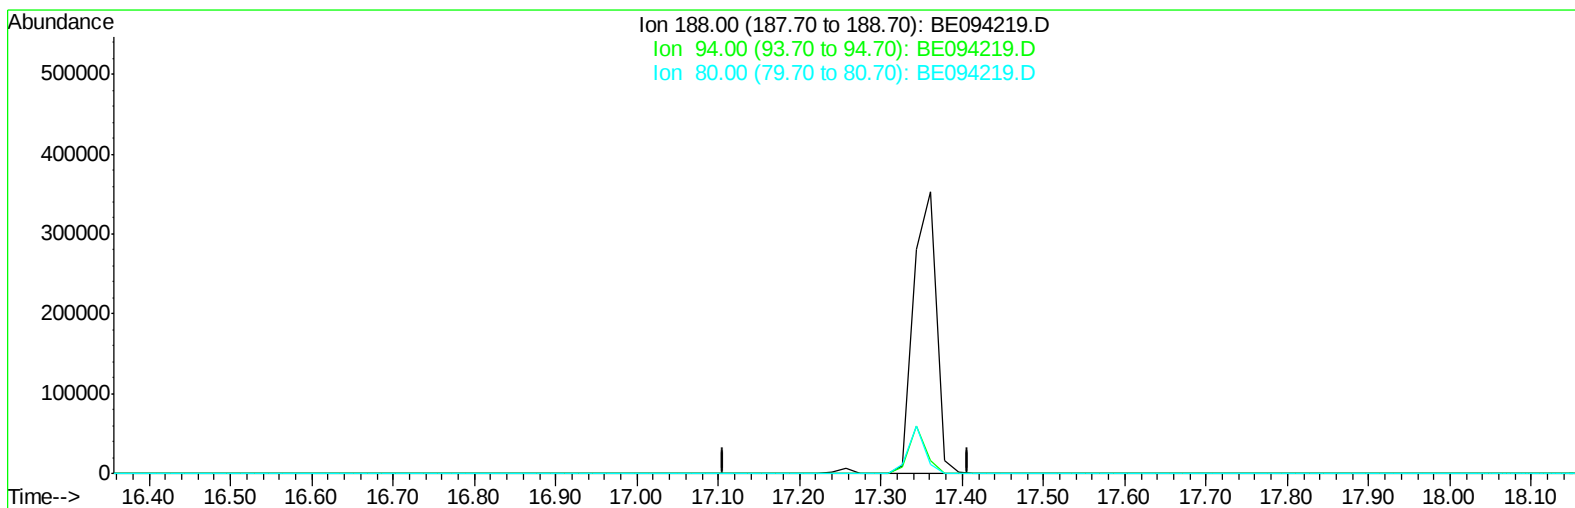

TIC: BE094219.D

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094219.D
Acq On : 9 Oct 2017 13:59
Operator : SJ/JU
Sample : PB102985BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK85

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:36 PM

Quant Time: Oct 10 09:19:09 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

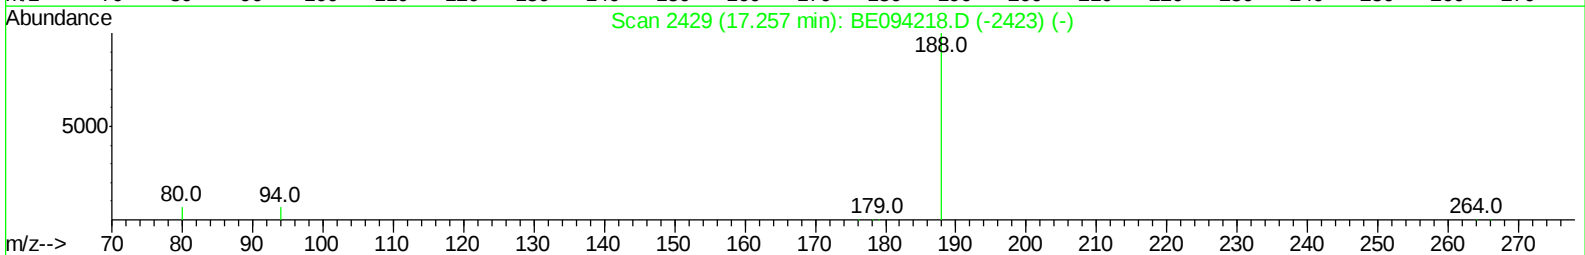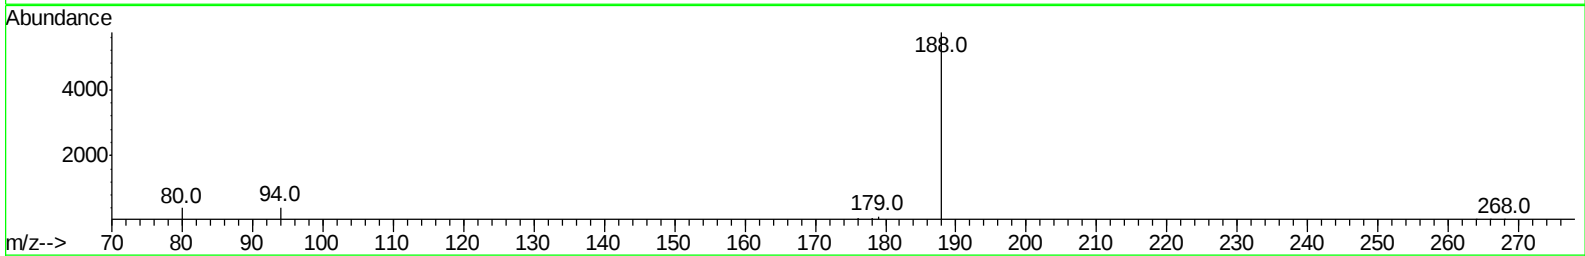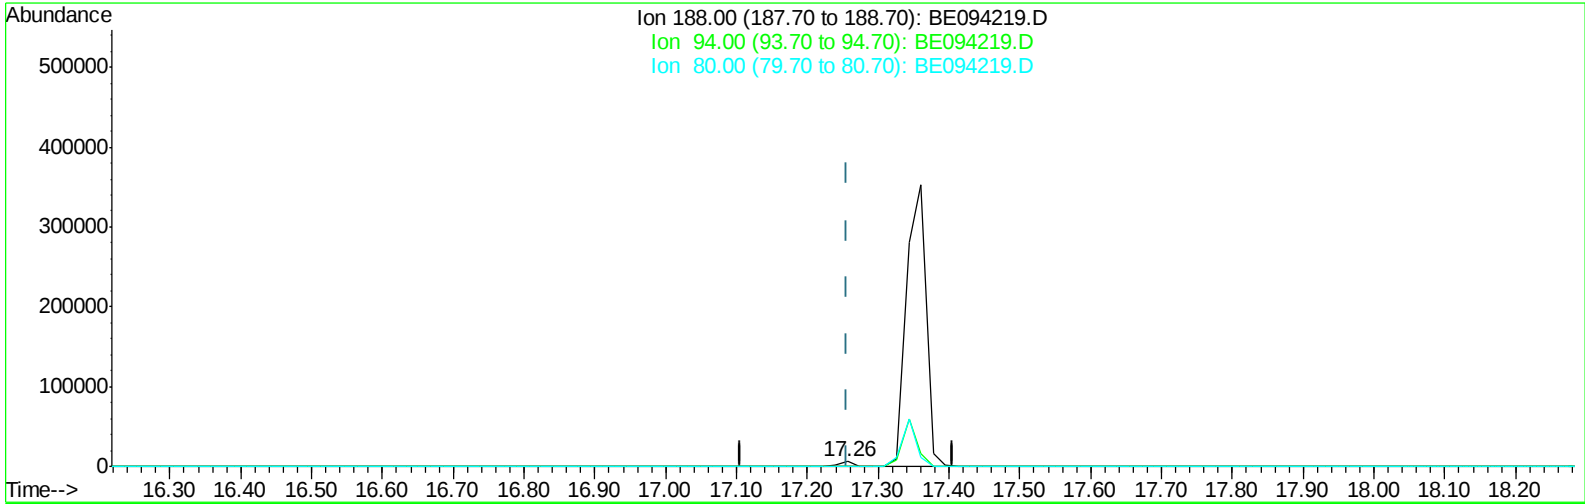

TIC: BE094219.D

(10) Phenanthrene-d10 (I)

17.256min (-0.001) 0.40ng/ul m

response 9028

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.53#
80.00	11.80	7.15#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094219.D
Acq On : 9 Oct 2017 13:59
Operator : SJ/JU
Sample : PB102985BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK85

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:36 PM

Quant Time: Oct 10 09:25:06 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

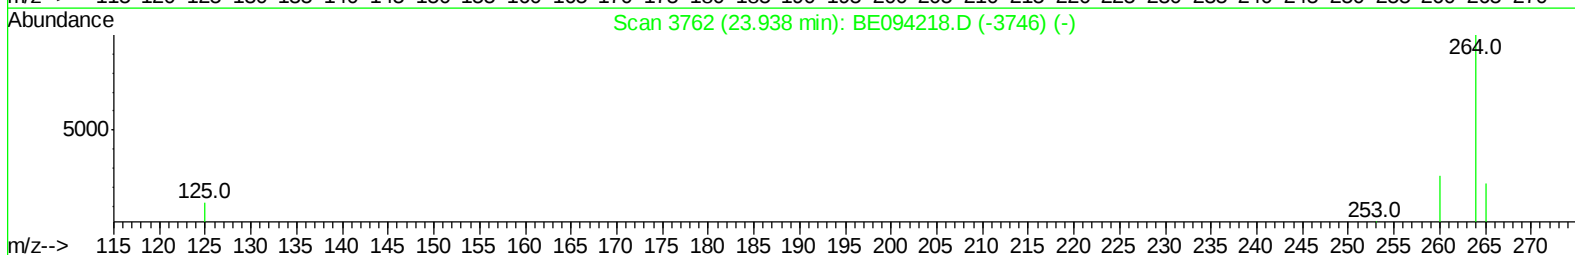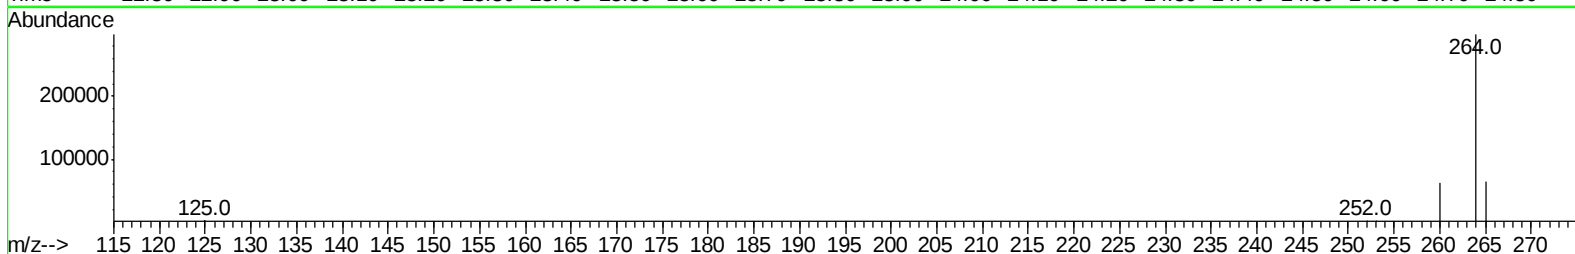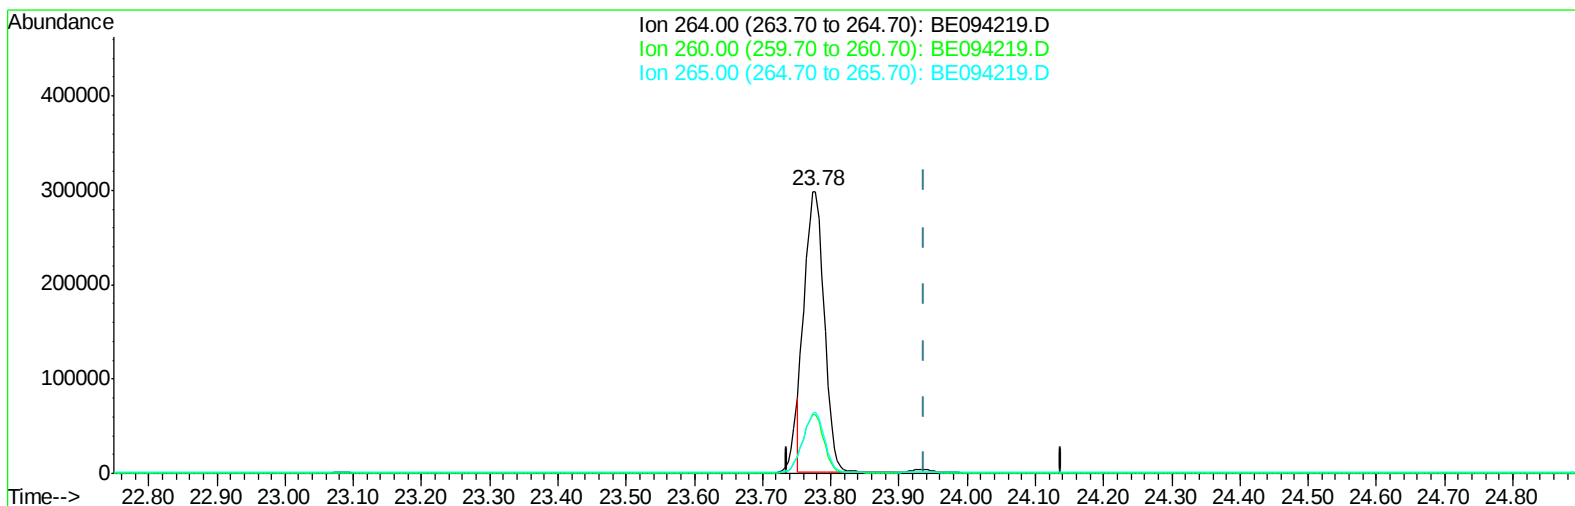

TIC: BE094219.D

(20) Perylene-d12 (I)

23.778min (-0.160) 0.40ng/ul

response 602337

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.74#
265.00	103.50	21.61#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094219.D
Acq On : 9 Oct 2017 13:59
Operator : SJ/JU
Sample : PB102985BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK85

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:36 PM

Quant Time: Oct 10 09:25:06 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

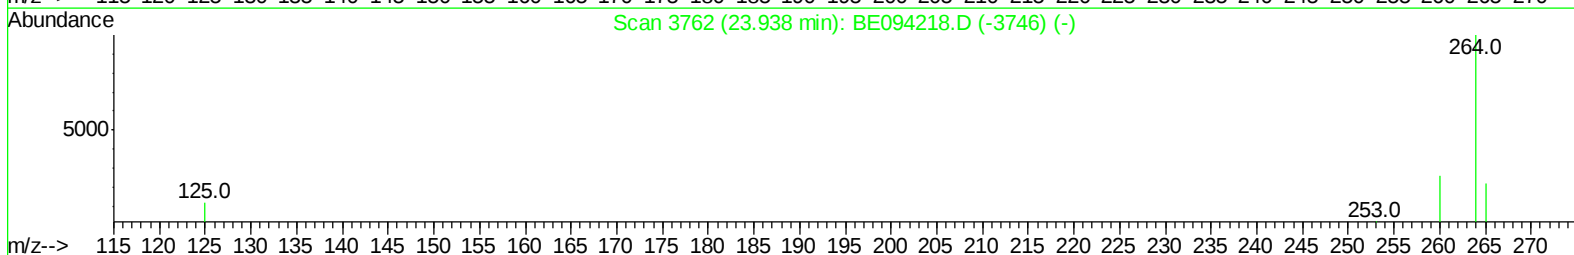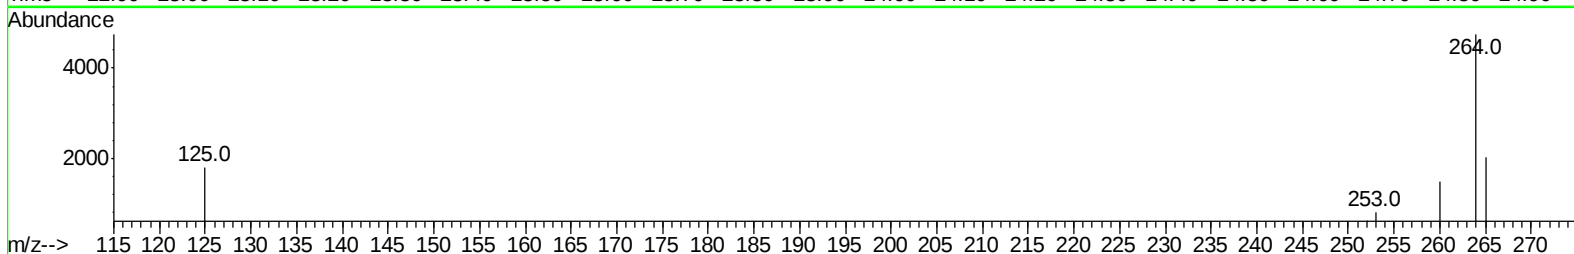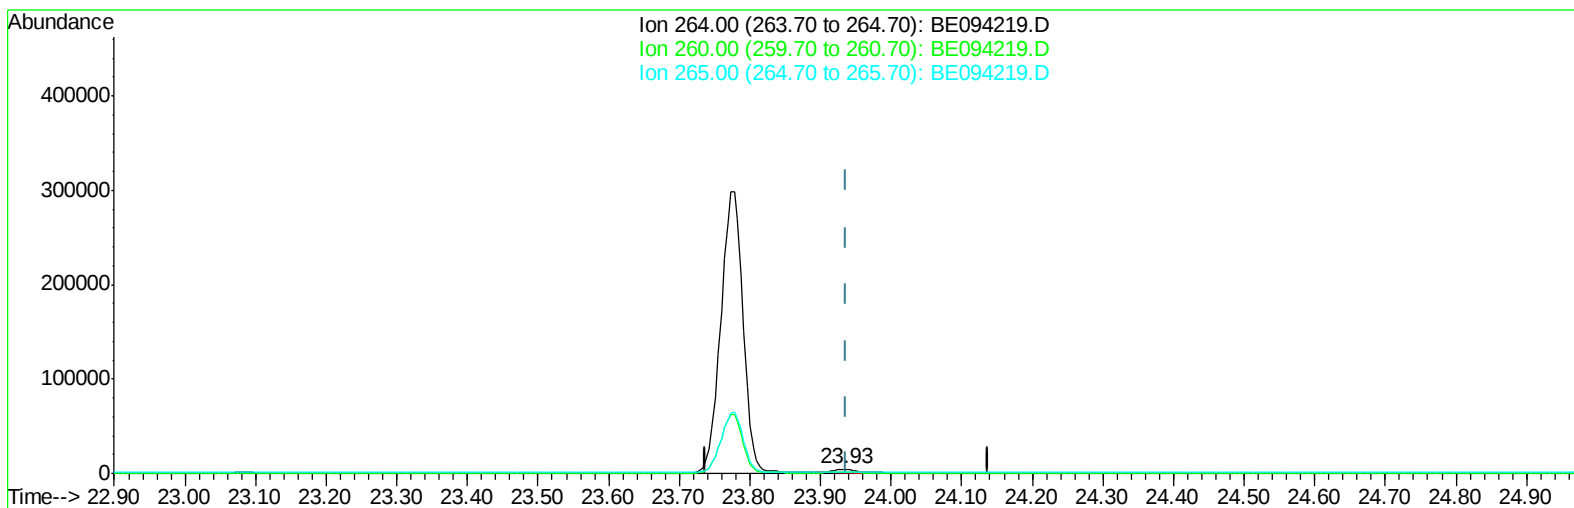

TIC: BE094219.D

(20) Perylene-d12 (I)

23.933min (-0.005) 0.40ng/ul m

response 8566

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	31.37
265.00	103.50	42.55#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
 Data File : BE094219.D
 Acq On : 9 Oct 2017 13:59
 Operator : SJ/JU
 Sample : PB102985BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK85

Manual Integrations
 APPROVED

Sohil
 10/10/2017 4:56:36 PM

Quant Time: Oct 10 09:26:20 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 09:18:40 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1277	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	7024	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	4280	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9028m	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	8532	0.40	ng/ul	0.00
20) Perylene-d12	23.93	264	8566m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3414	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	8585	0.28	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	1173	0.049	ng/ul#	Ovalue 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094219.D
Acq On : 9 Oct 2017 13:59
Operator : SJ/JU
Sample : PB102985BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK85

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:36 PM

Quant Time: Oct 10 09:26:20 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

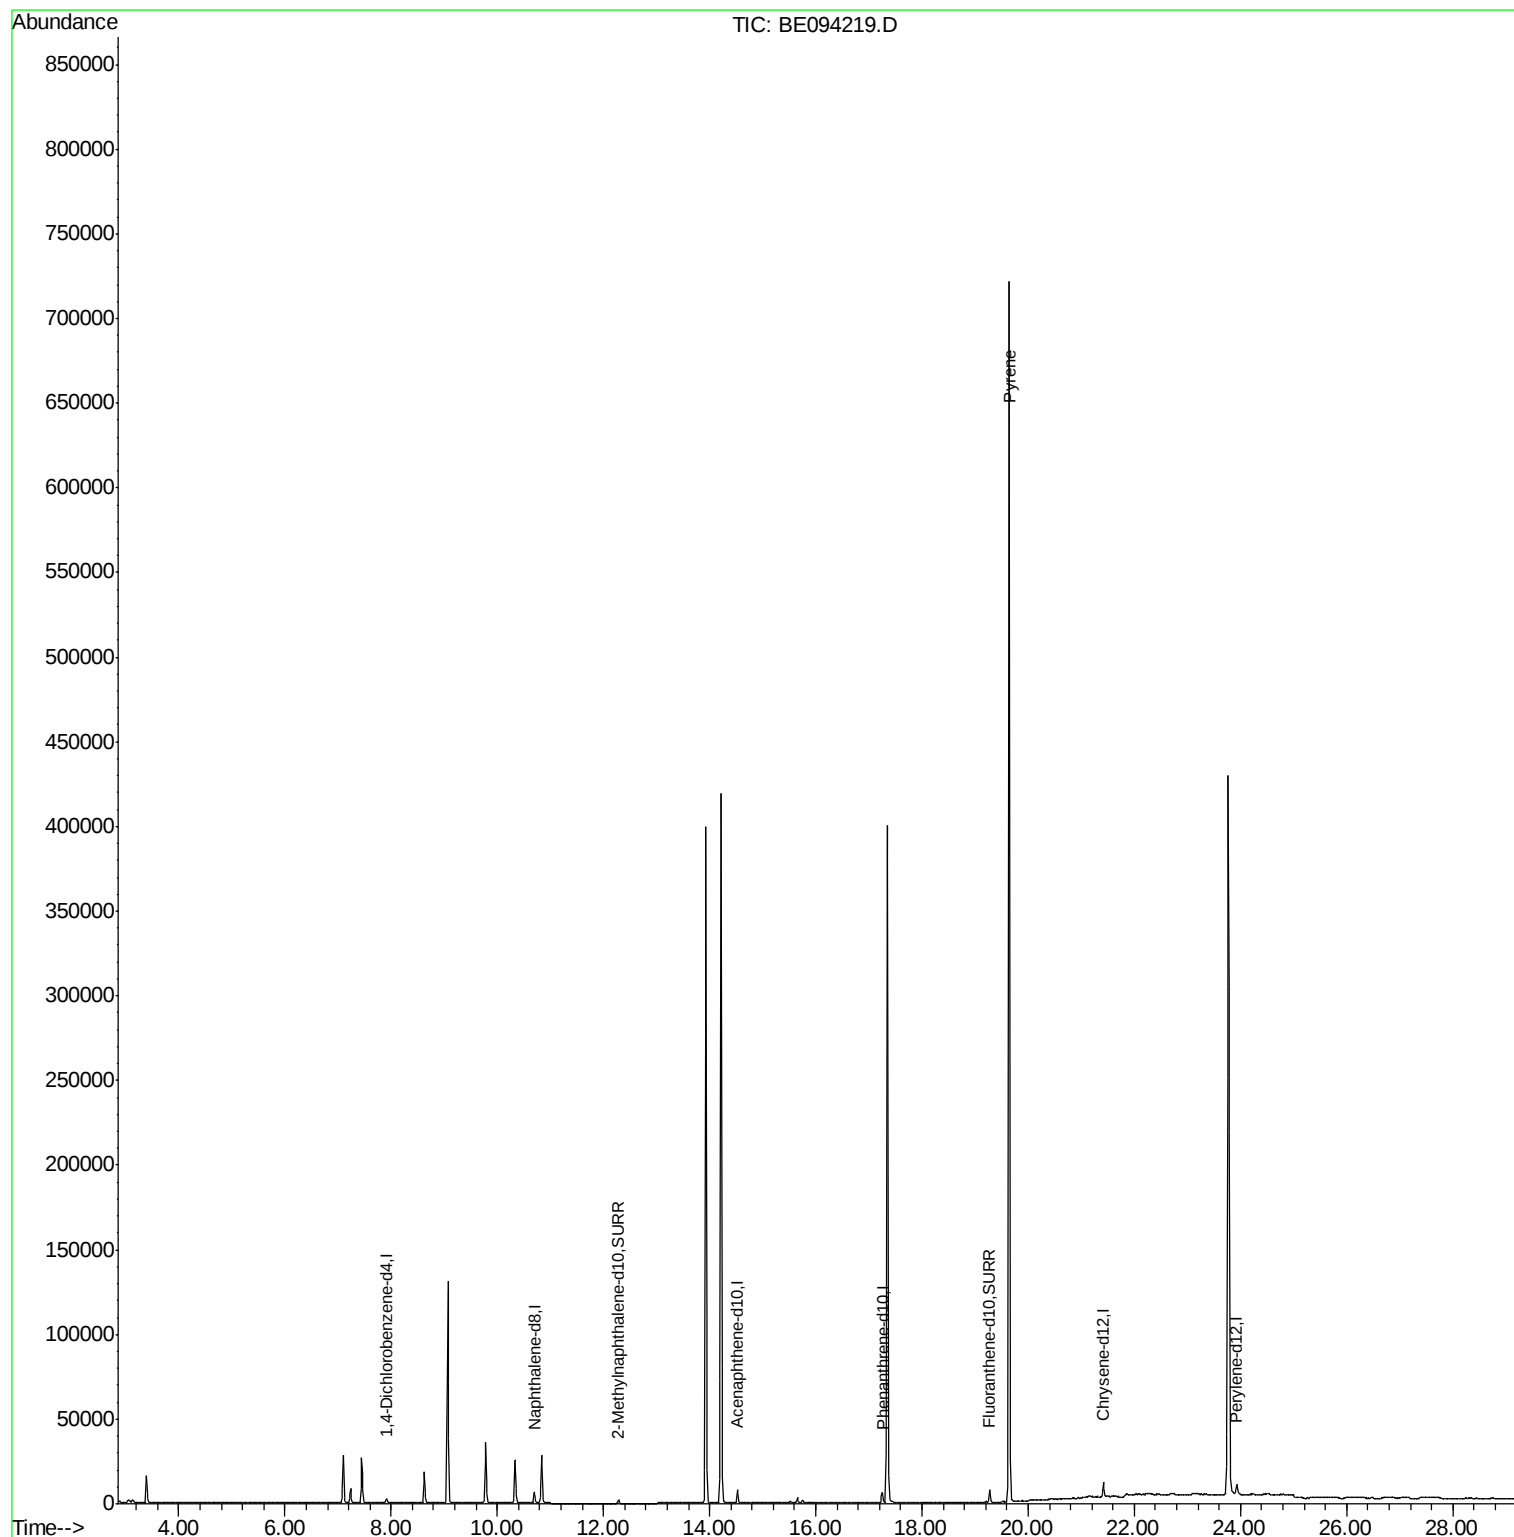

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
 Data File : BE094219.D
 Acq On : 9 Oct 2017 13:59
 Operator : SJ/JU
 Sample : PB102985BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK85

Manual Integrations
 APPROVED

Sohil
 10/10/2017 4:56:36 PM

Quant Time: Oct 10 09:27:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 09:18:40 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1277	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	7024	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	4280	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9028m	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	8532	0.40	ng/ul	0.00
20) Perylene-d12	23.93	264	8566m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3414	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	8585	0.28	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094219.D
Acq On : 9 Oct 2017 13:59
Operator : SJ/JU
Sample : PB102985BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK85

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:36 PM

Quant Time: Oct 10 09:27:24 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

