




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094220.D
Acq On : 9 Oct 2017 14:37
Operator : SJ/JU
Sample : PB102999BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK99

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:38 PM

Quant Time: Oct 10 09:19:21 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

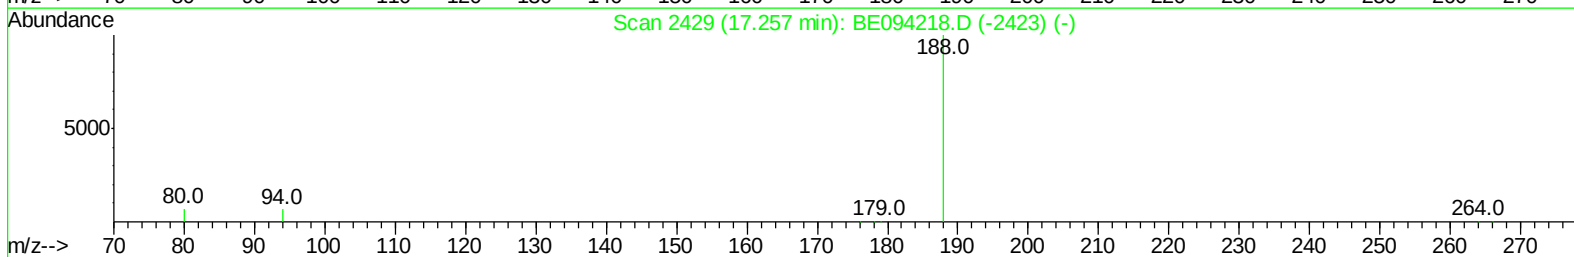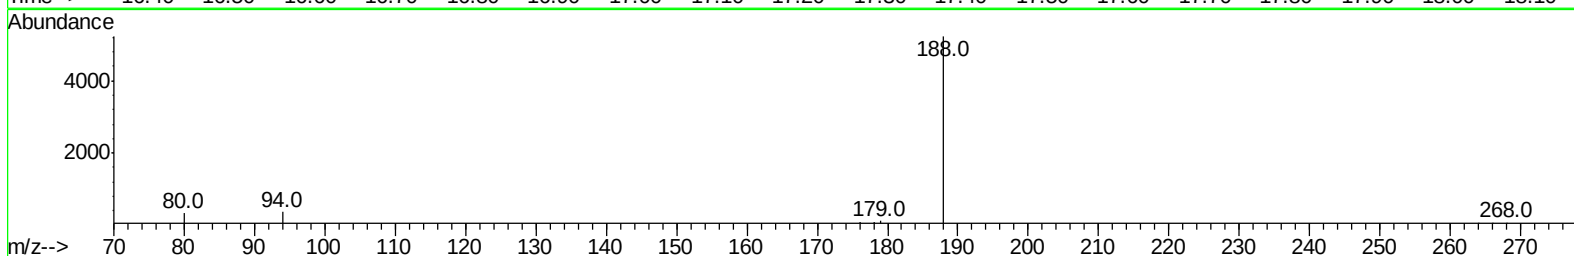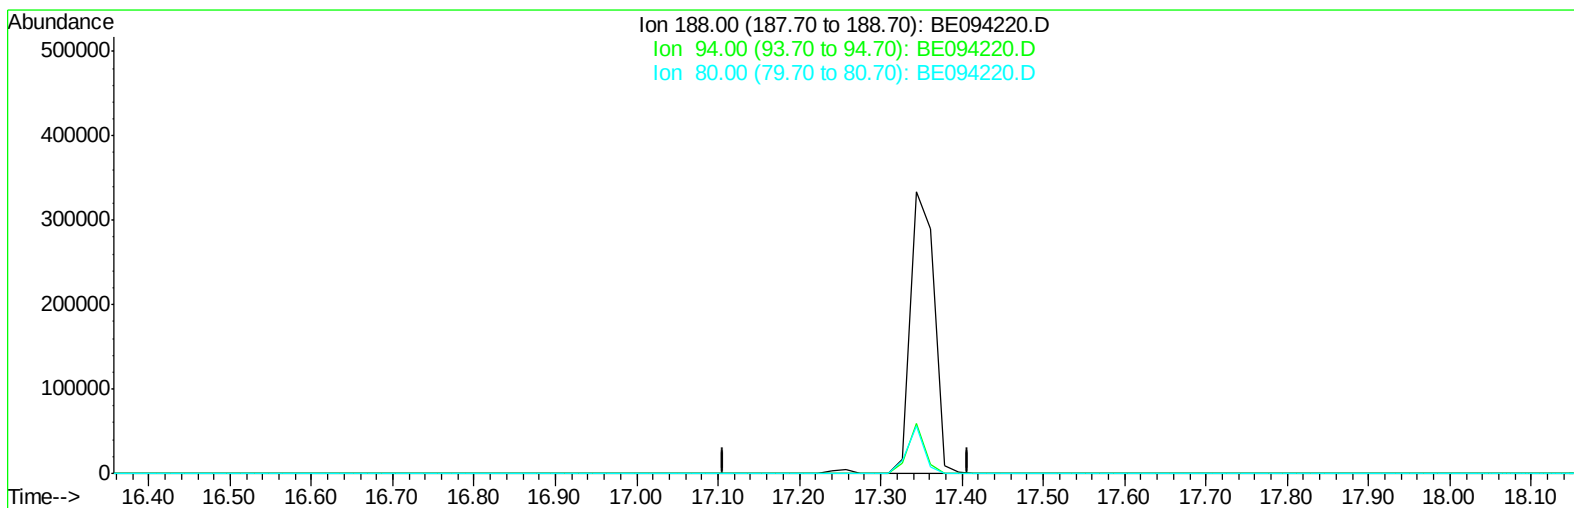

TIC: BE094220.D

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094220.D
Acq On : 9 Oct 2017 14:37
Operator : SJ/JU
Sample : PB102999BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK99

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:38 PM

Quant Time: Oct 10 09:19:21 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

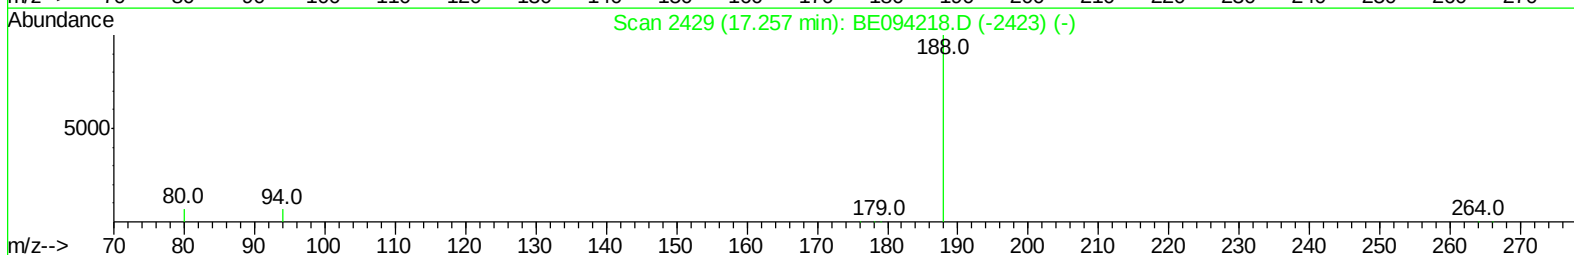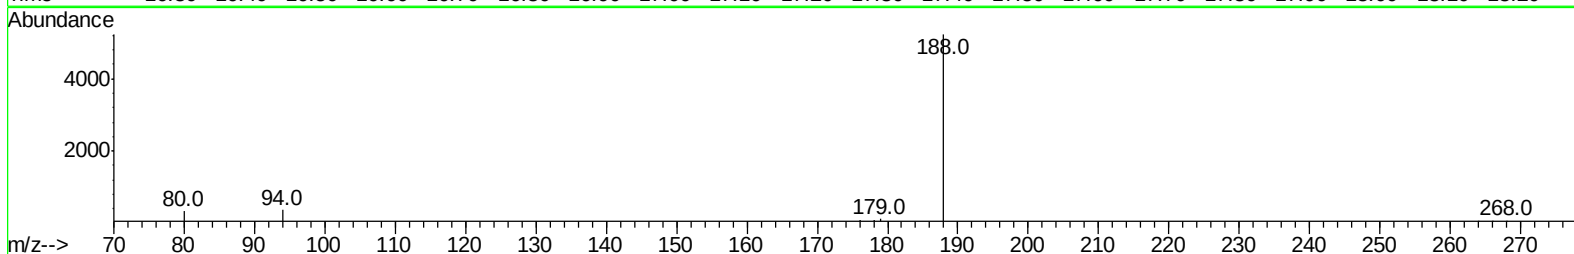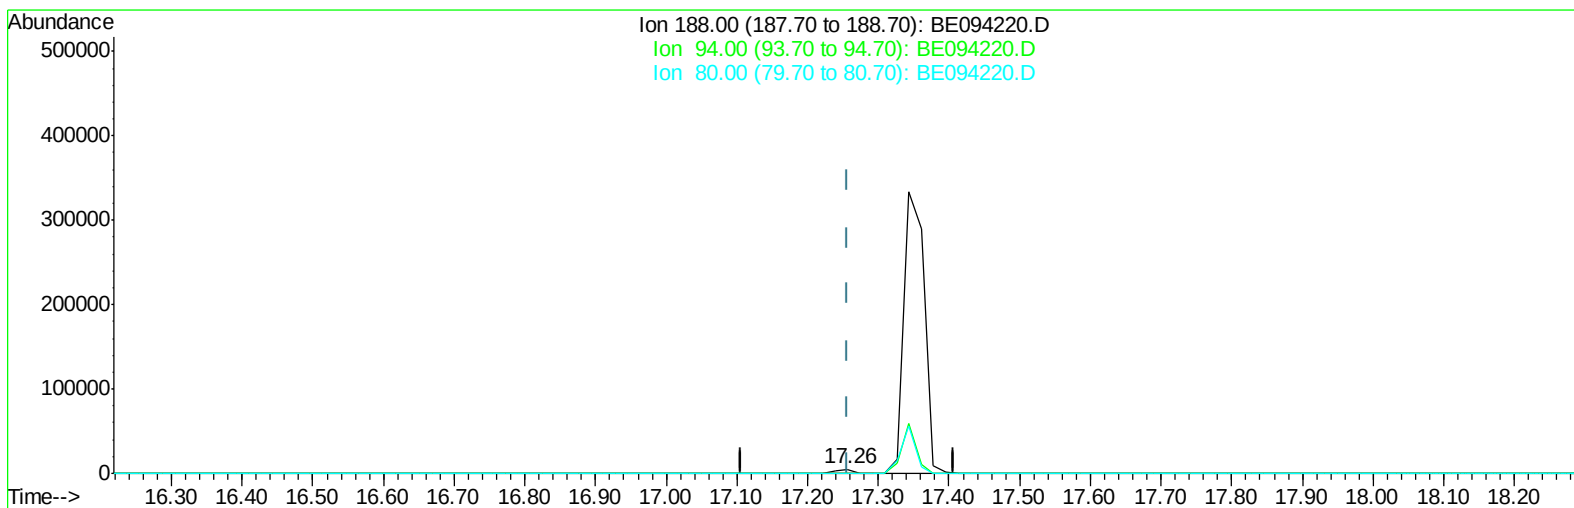

TIC: BE094220.D

(10) Phenanthrene-d10 (I)

17.257min (-0.000) 0.40ng/ul m

response 8736

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.87#
80.00	11.80	6.45#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094220.D
Acq On : 9 Oct 2017 14:37
Operator : SJ/JU
Sample : PB102999BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK99

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:38 PM

Quant Time: Oct 10 09:29:19 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

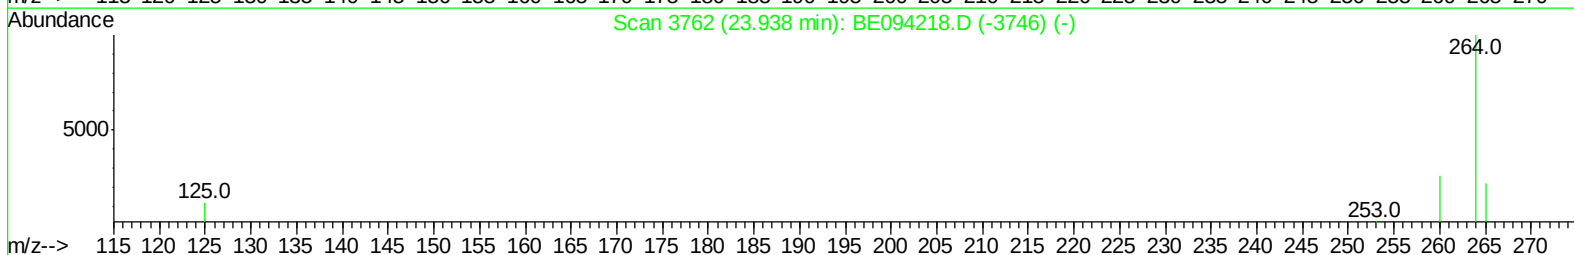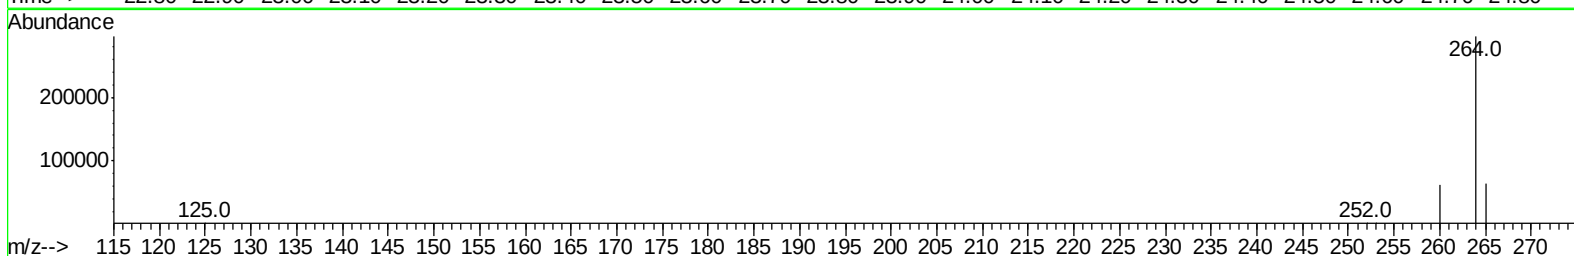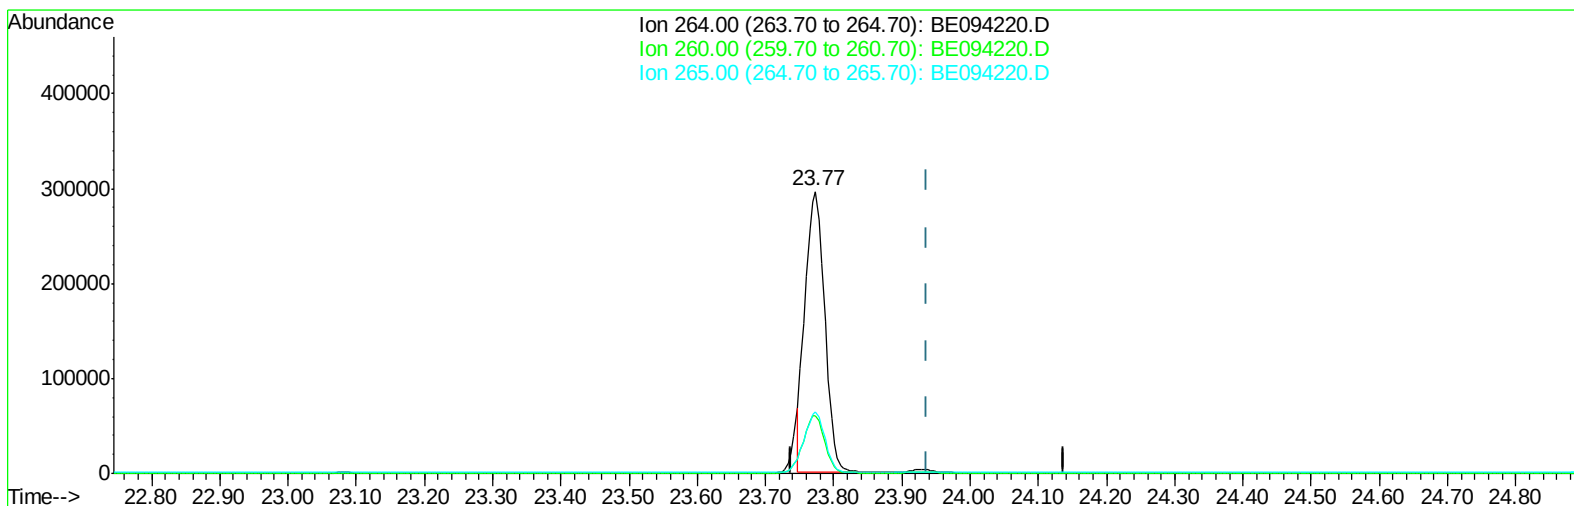

TIC: BE094220.D

(20) Perylene-d12 (I)

23.774min (-0.164) 0.40ng/ul

response 595094

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.66#
265.00	103.50	21.71#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094220.D
Acq On : 9 Oct 2017 14:37
Operator : SJ/JU
Sample : PB102999BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK99

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:38 PM

Quant Time: Oct 10 09:29:19 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

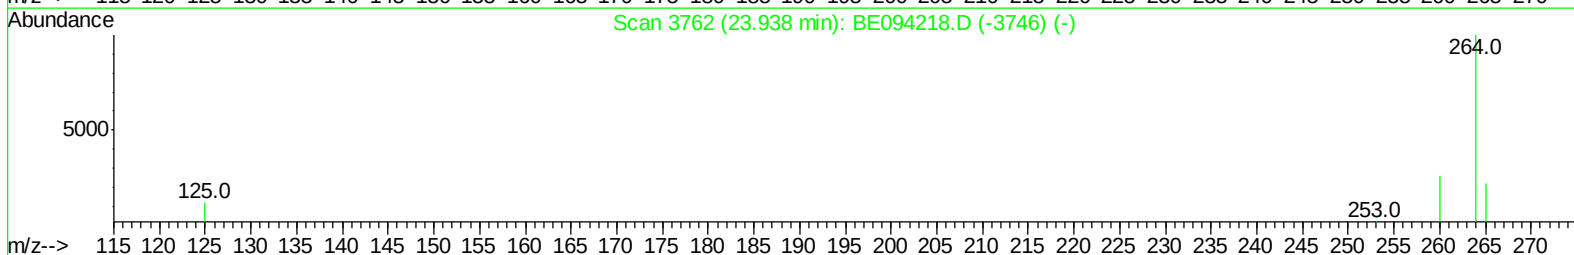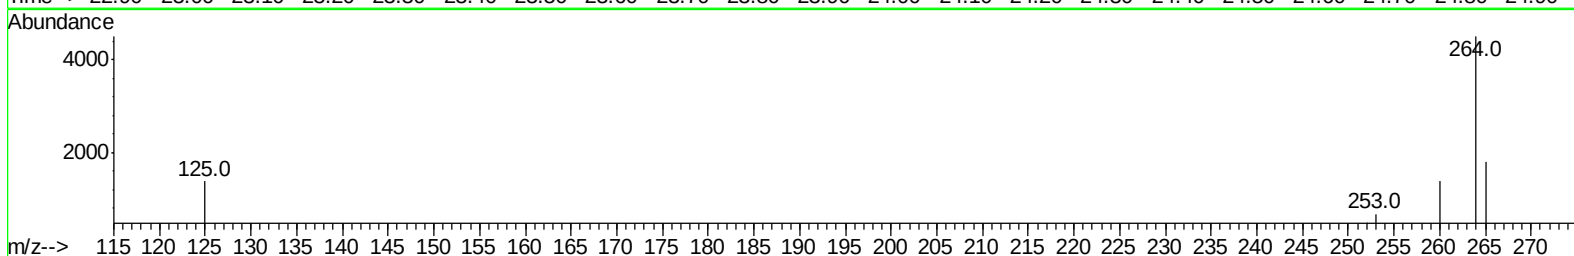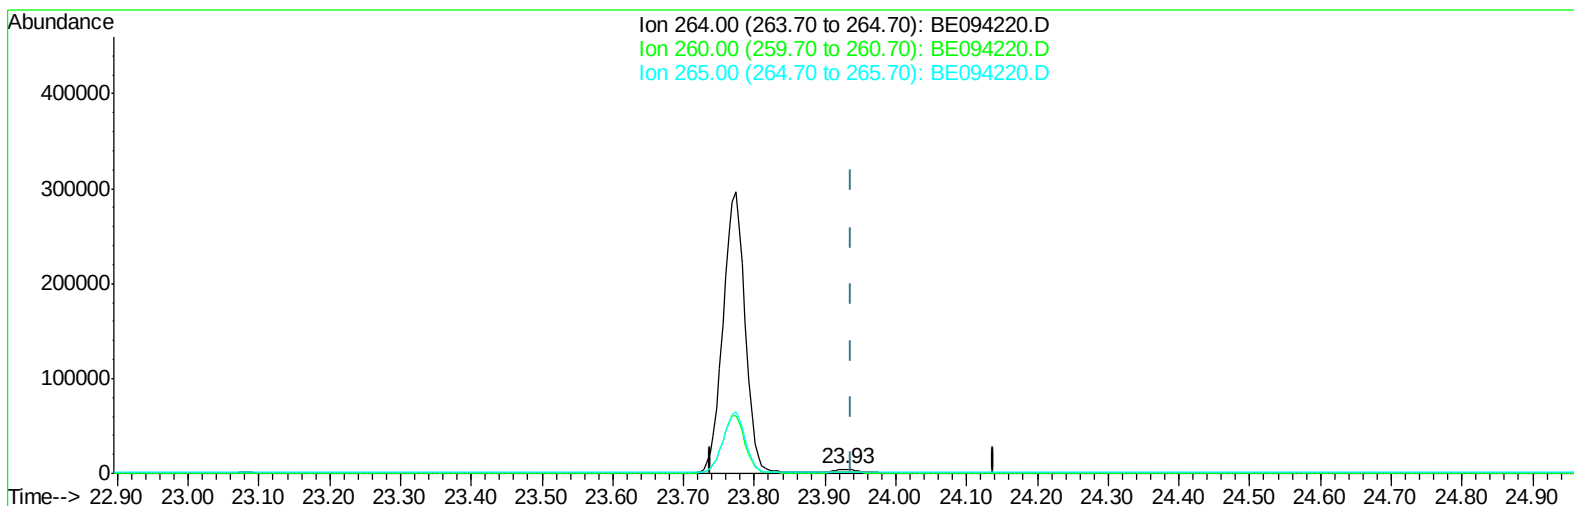

TIC: BE094220.D

(20) Perylene-d12 (I)

23.929min (-0.009) 0.40ng/ul m

response 7589

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.53
265.00	103.50	39.95#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094220.D
Acq On : 9 Oct 2017 14:37
Operator : SJ/JU
Sample : PB102999BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK99

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:38 PM

Quant Time: Oct 10 09:30:47 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1073	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	6201	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	3928	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	8736m	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	8279	0.40	ng/ul	0.00
20) Perylene-d12	23.93	264	7589m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3087	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	8441	0.29	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094220.D
Acq On : 9 Oct 2017 14:37
Operator : SJ/JU
Sample : PB102999BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK99

Manual Integrations
APPROVED

Sohil
10/10/2017 4:56:38 PM

Quant Time: Oct 10 09:30:47 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

