




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100917\
Data File : BE094221.D
Acq On : 9 Oct 2017 15:16
Operator : SJ/JU
Sample : I5695-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TWP-B-42

Manual Integrations
APPROVED

Sohil
10/11/2017 9:29:43 AM

Quant Time: Oct 10 16:19:21 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

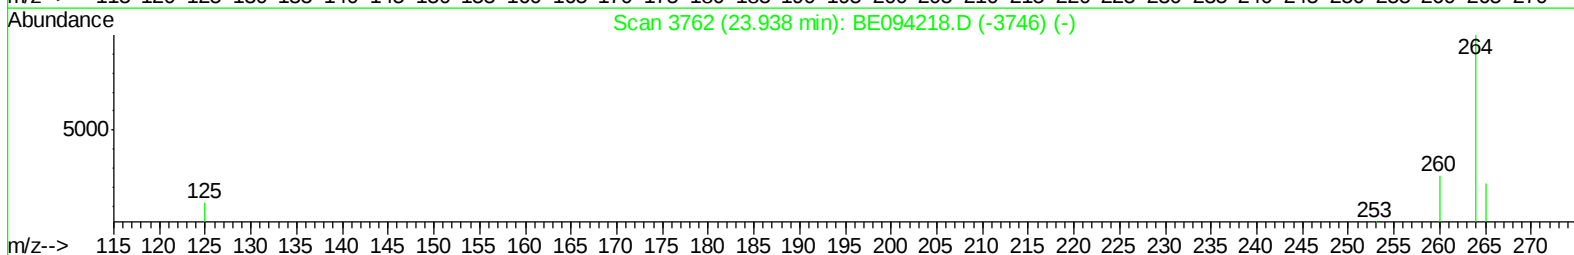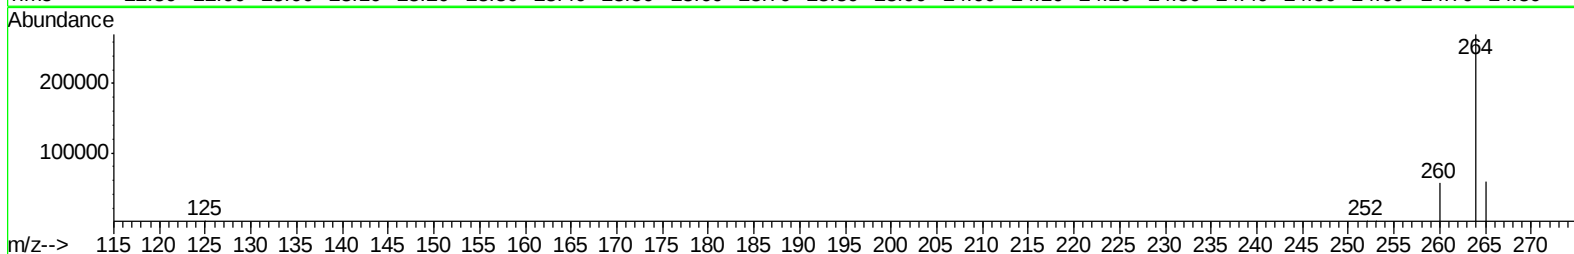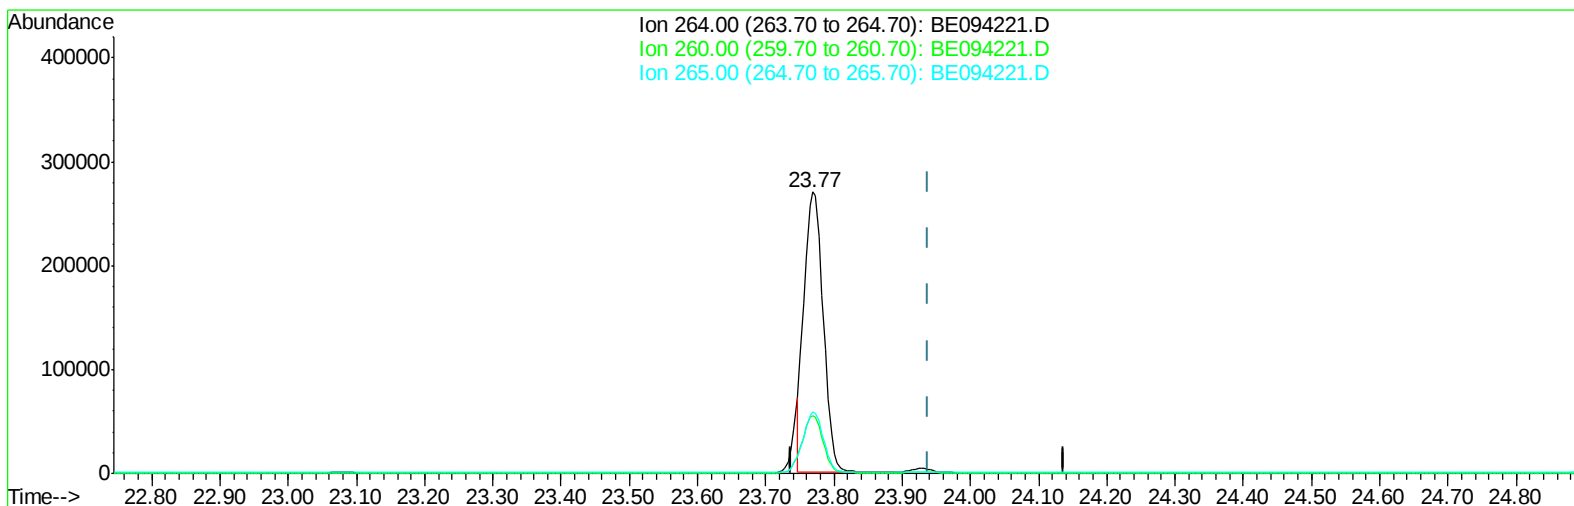

TIC: BE094221.D

(20) Perylene-d12 (I)

23.769min (-0.169) 0.40ng/ul

response 529493

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.59#
265.00	103.50	21.83#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE100917\
Data File : BE094221.D
Acq On : 9 Oct 2017 15:16
Operator : SJ/JU
Sample : I5695-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TWP-B-42

Manual Integrations
APPROVED

Sohil
10/11/2017 9:29:43 AM

Quant Time: Oct 10 16:19:21 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

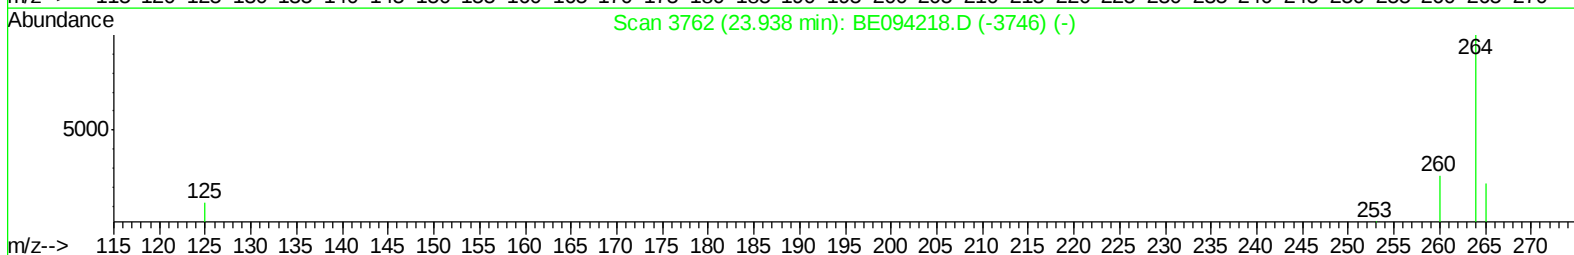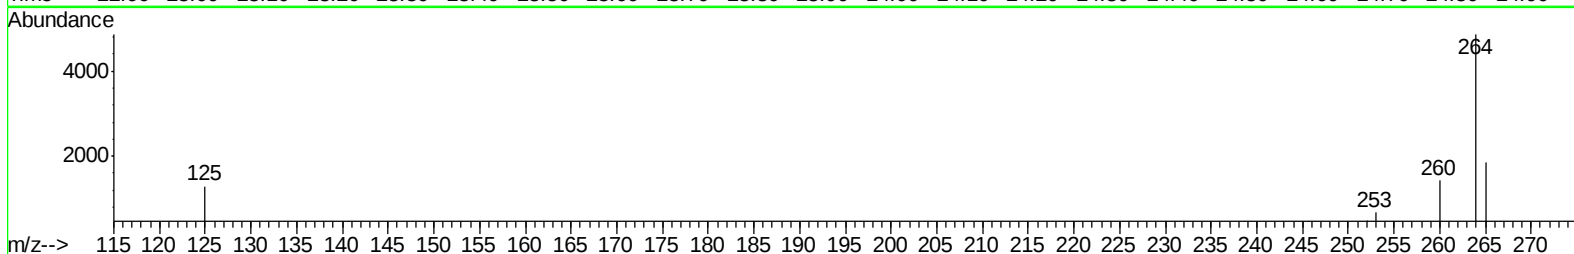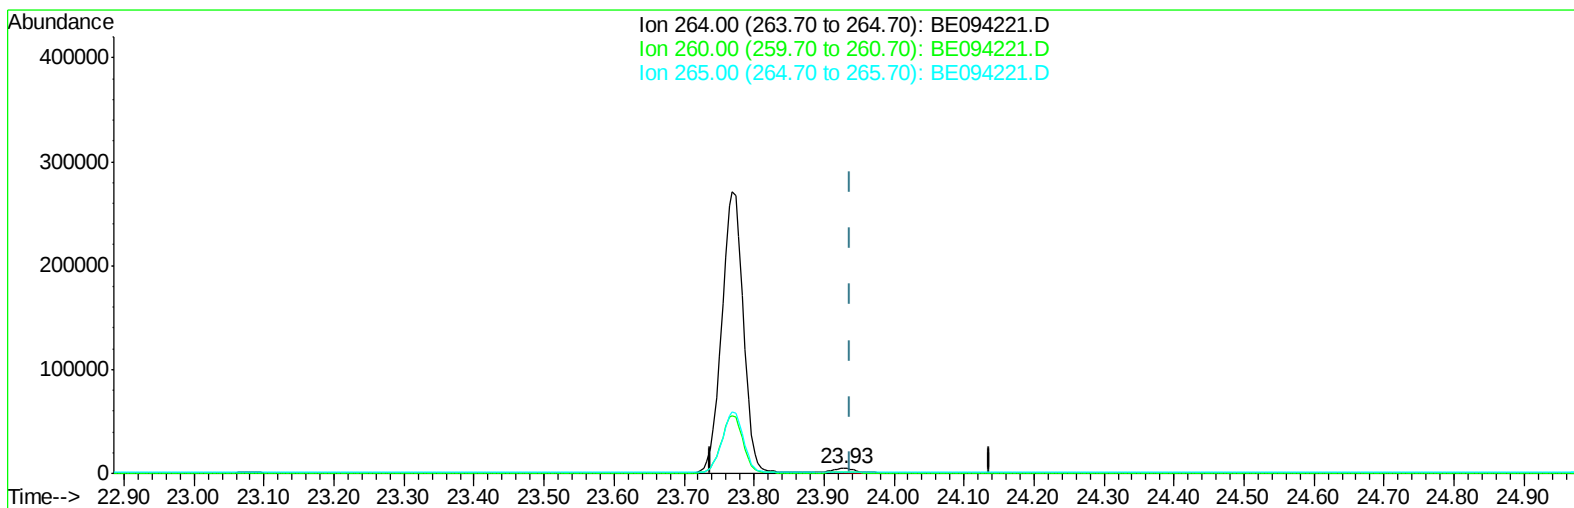

TIC: BE094221.D

(20) Perylene-d12 (I)

23.928min (-0.010) 0.40ng/ul m

response 8437

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	29.36
265.00	103.50	38.37#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE100917\
 Data File : BE094221.D
 Acq On : 9 Oct 2017 15:16
 Operator : SJ/JU
 Sample : I5695-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 TWP-B-42

Manual Integrations
 APPROVED

Sohil
 10/11/2017 9:29:43 AM

Quant Time: Oct 10 16:24:22 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 10 09:18:40 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1366	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	7440	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	6775	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9449	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	9065	0.40	ng/ul	0.00
20) Perylene-d12	23.93	264	8437m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3231	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	7880	0.25	ng/ul	0.00
Target Compounds				Qvalue		
8) Acenaphthene	14.58	153	3318	0.153	ng/ul	96
9) Fluorene	15.57	166	1776	0.070	ng/ul#	89
12) Phenanthrene	17.29	178	4131	0.167	ng/ul#	93
13) Anthracene	17.38	178	2029	0.084	ng/ul#	77
15) Fluoranthene	19.30	202	6172	0.190	ng/ul	83
17) Pyrene	19.66	202	6452	0.256	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE100917\
Data File : BE094221.D
Acq On : 9 Oct 2017 15:16
Operator : SJ/JU
Sample : I5695-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
TWP-B-42

Manual Integrations
APPROVED

Sohil
10/11/2017 9:29:43 AM

Quant Time: Oct 10 16:24:22 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 10 09:18:40 2017
Response via : Initial Calibration

