




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094236.D
Acq On : 10 Oct 2017 00:31
Operator : SJ/JU
Sample : PB102994BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK94

Manual Integrations
APPROVED

Sohil
10/10/2017 4:58:18 PM

Quant Time: Oct 10 08:51:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 04:05:38 2017
Response via : Initial Calibration

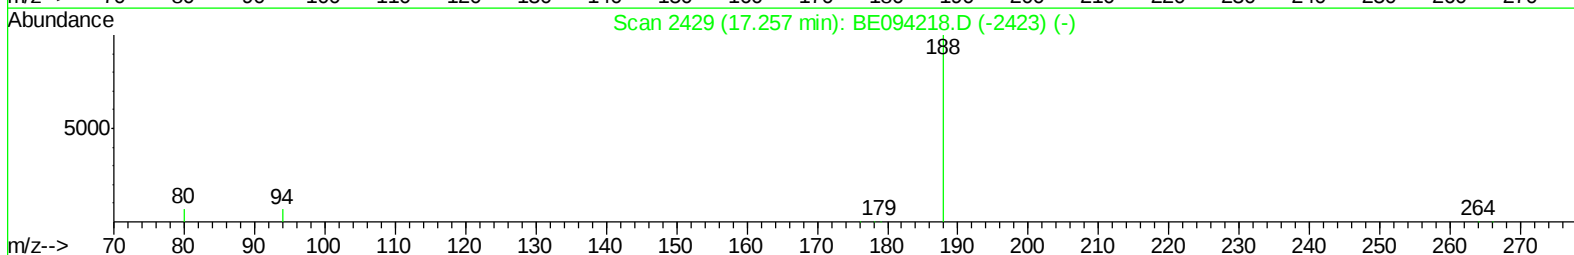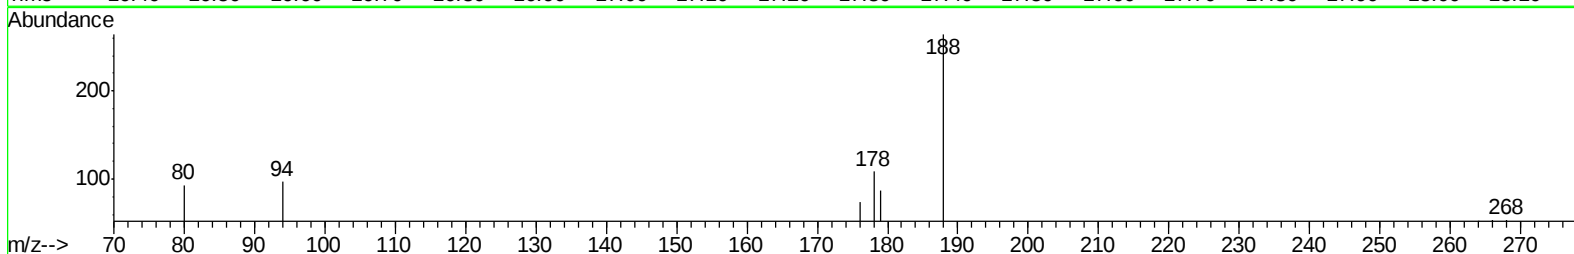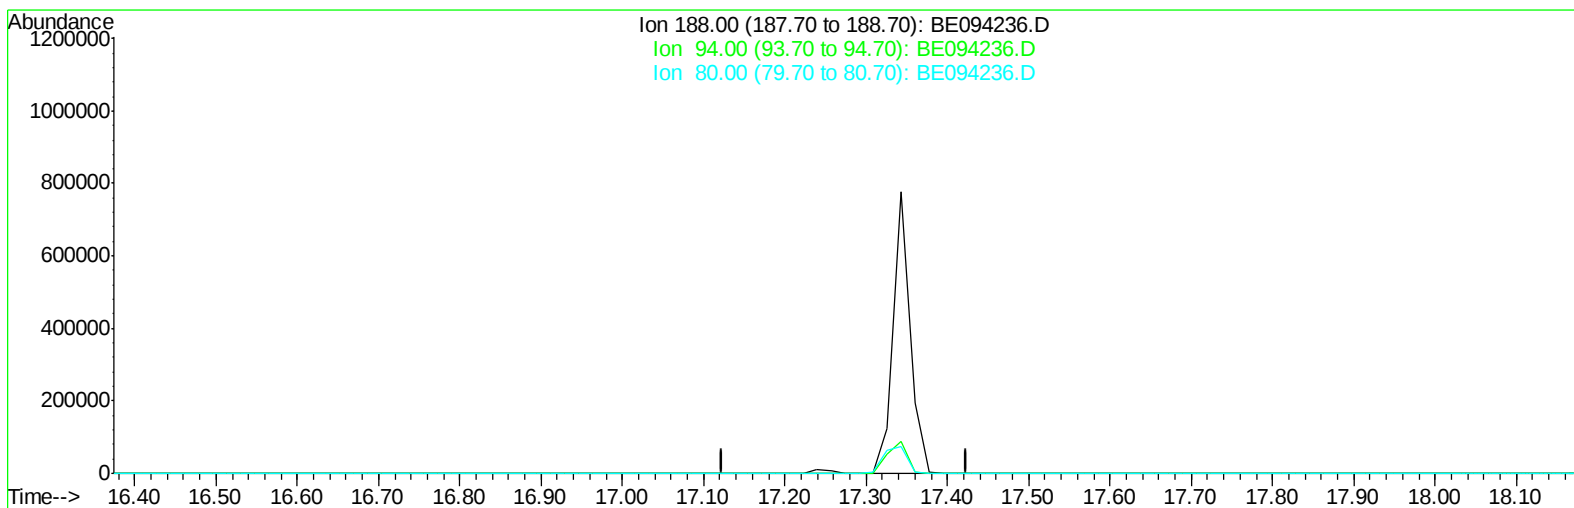

TIC: BE094236.D

(10) Phenanthrene-d10 (I)

17.274min (-17.274) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094236.D
Acq On : 10 Oct 2017 00:31
Operator : SJ/JU
Sample : PB102994BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK94

Manual Integrations
APPROVED

Sohil
10/10/2017 4:58:18 PM

Quant Time: Oct 10 08:51:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 04:05:38 2017
Response via : Initial Calibration

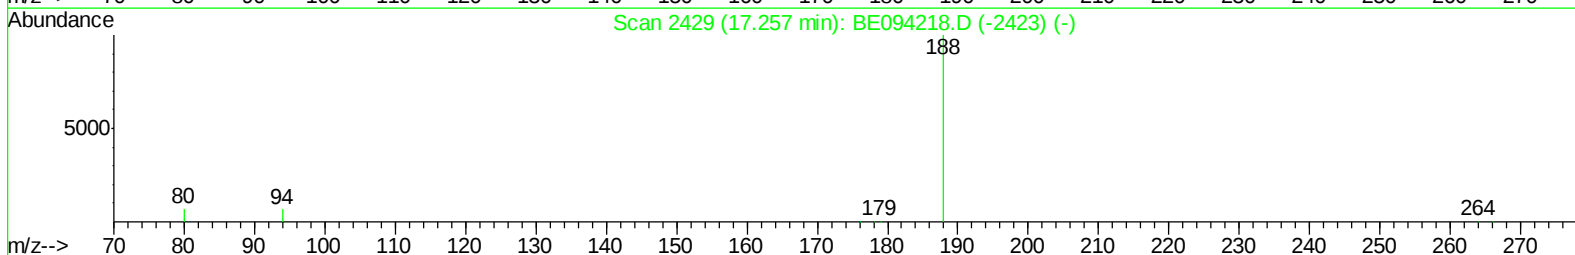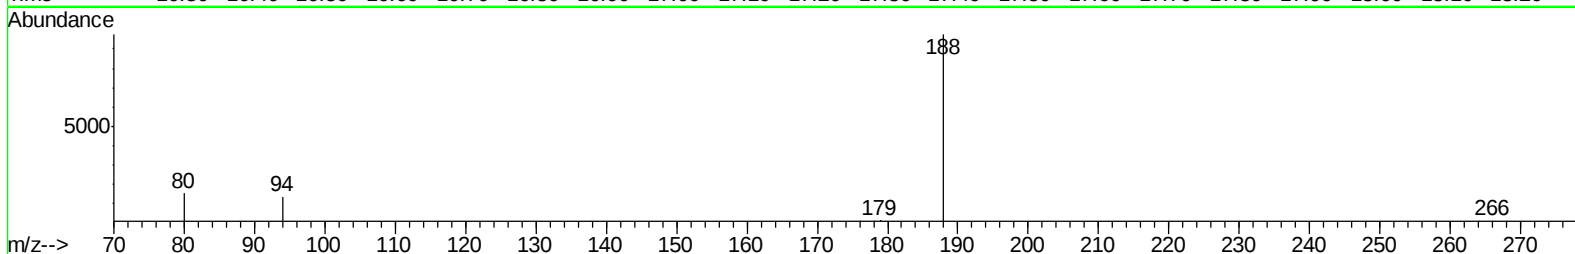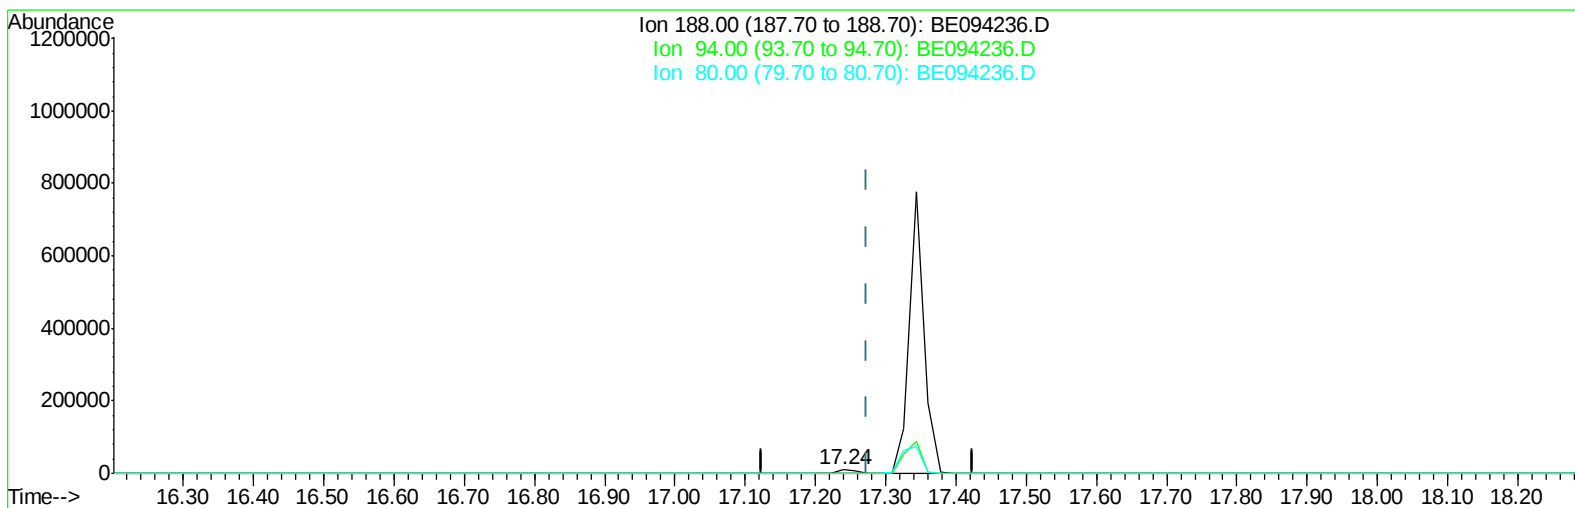

TIC: BE094236.D

(10) Phenanthrene-d10 (I)

17.240min (-0.034) 0.40ng/ul m

response 16934

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.62#
80.00	11.80	15.20#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094236.D
Acq On : 10 Oct 2017 00:31
Operator : SJ/JU
Sample : PB102994BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK94

Manual Integrations
APPROVED

Sohil
10/10/2017 4:58:18 PM

Quant Time: Oct 10 10:07:51 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 04:05:38 2017
Response via : Initial Calibration

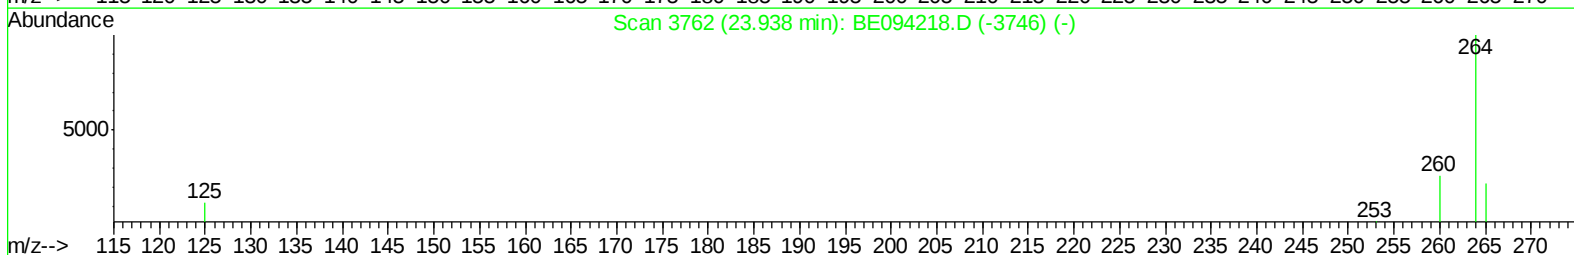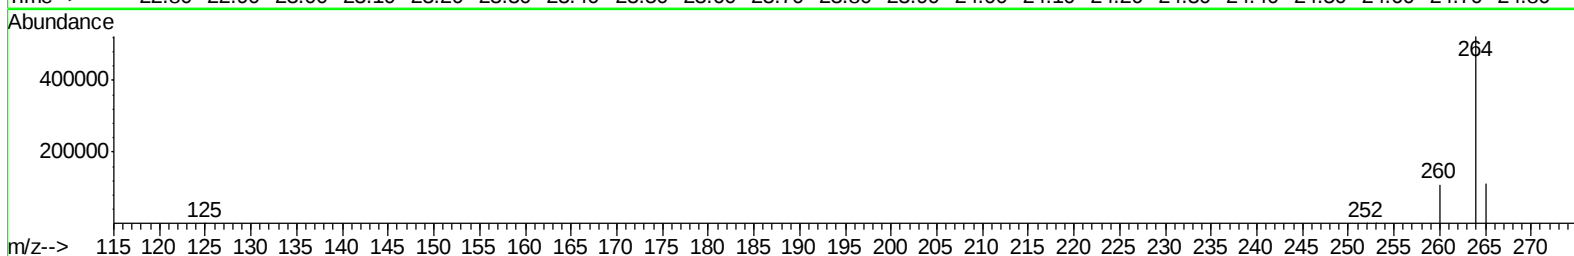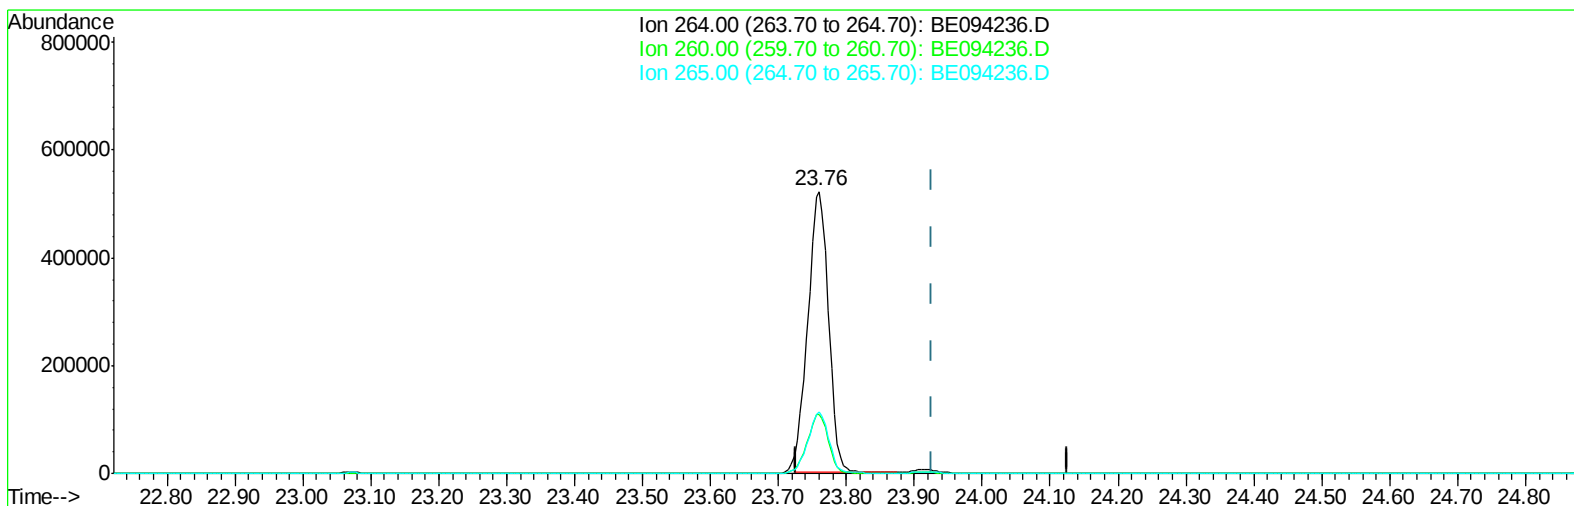

TIC: BE094236.D

(20) Perylene-d12 (I)

23.760min (-0.167) 0.40ng/ul

response 1095423

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.85#
265.00	103.50	21.68#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094236.D
Acq On : 10 Oct 2017 00:31
Operator : SJ/JU
Sample : PB102994BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK94

Manual Integrations
APPROVED

Sohil
10/10/2017 4:58:18 PM

Quant Time: Oct 10 10:07:51 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 04:05:38 2017
Response via : Initial Calibration

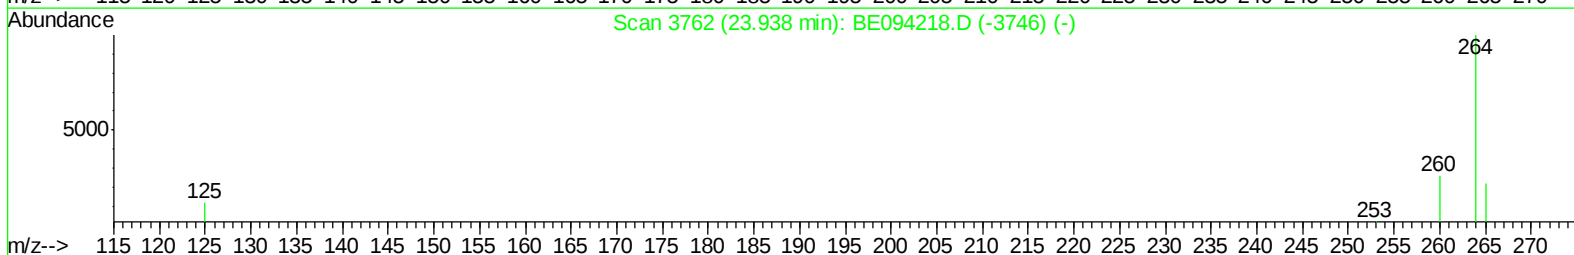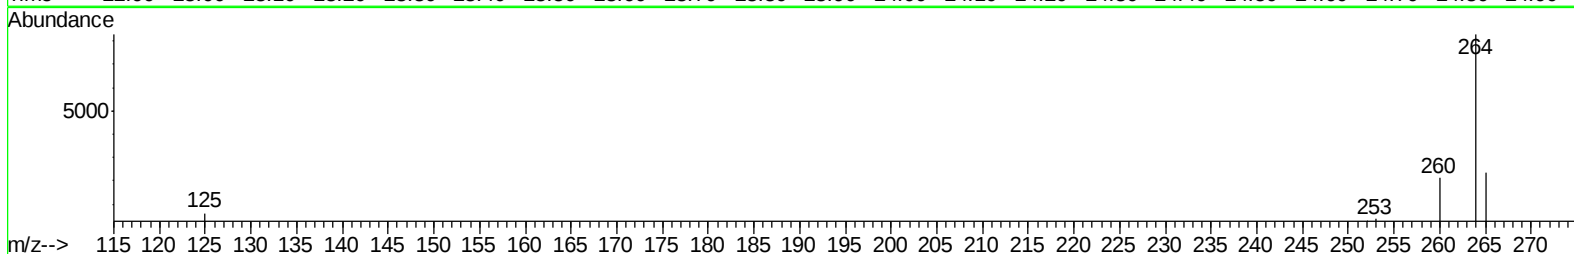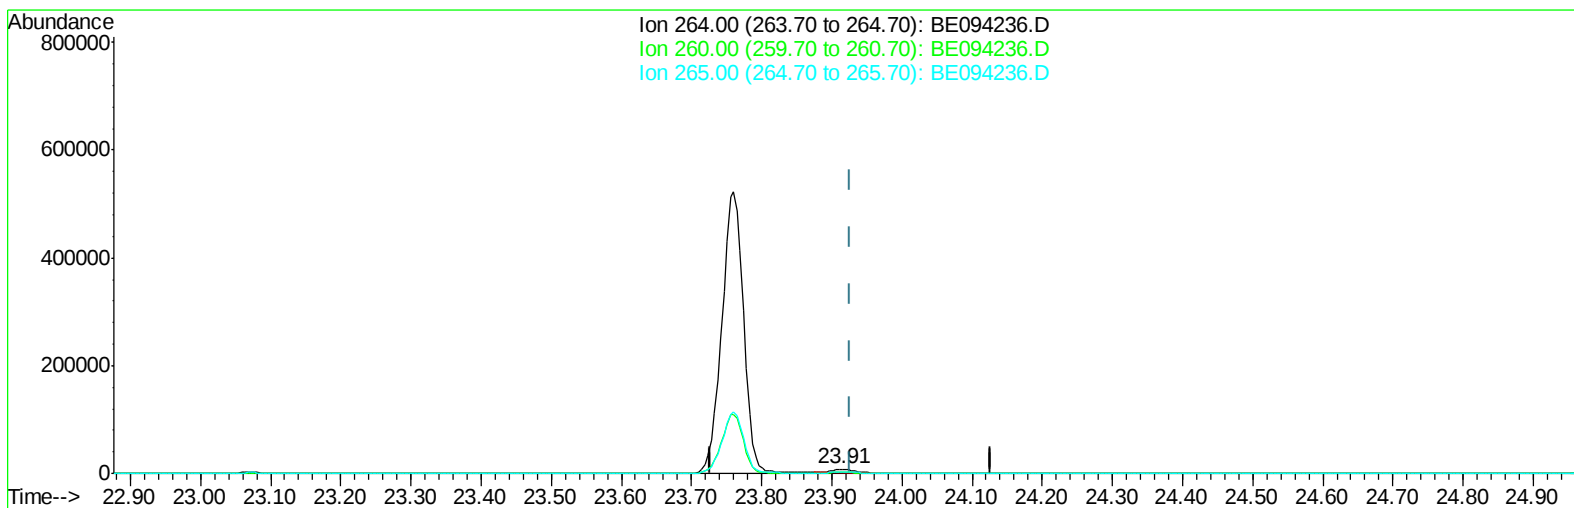

TIC: BE094236.D

(20) Perylene-d12 (I)

23.915min (-0.013) 0.40ng/ul m

response 15157

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.58
265.00	103.50	28.47#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
 Data File : BE094236.D
 Acq On : 10 Oct 2017 00:31
 Operator : SJ/JU
 Sample : PB102994BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK94

Manual Integrations
 APPROVED

Sohil
 10/10/2017 4:58:18 PM

Quant Time: Oct 10 10:09:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 09 04:05:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	2446	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	12938	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	7943	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.24	188	16934m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.41	240	16460	0.40	ng/ul	-0.01
20) Perylene-d12	23.91	264	15157m	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.27	152	6235	0.31	ng/ul	-0.02
14) Fluoranthene-d10	19.27	212	14744	0.26	ng/ul	-0.02

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE100917\
Data File : BE094236.D
Acq On : 10 Oct 2017 00:31
Operator : SJ/JU
Sample : PB102994BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK94

Manual Integrations
APPROVED

Sohil
10/10/2017 4:58:18 PM

Quant Time: Oct 10 10:09:34 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 09 04:05:38 2017
Response via : Initial Calibration

