

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\
 Data File : BE094257.D
 Acq On : 10 Oct 2017 18:48
 Operator : SJ/JU
 Sample : I5522-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 11 07:32:27 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 07:23:41 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1964	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	10215	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	5680	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	11807	0.40	ng/ul	-0.02
16) Chrysene-d12	21.41	240	12158	0.40	ng/ul	0.00
20) Perylene-d12	23.92	264	13438	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	5289	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	12076	0.31	ng/ul	0.00
Target Compounds				Ovalue		
12) Phenanthrene	17.29	178	2185	0.071	ng/ul	96
13) Anthracene	17.29	178	2153	0.072	ng/ul	98
15) Fluoranthene	19.30	202	5900	0.146	ng/ul	85
17) Pyrene	19.66	202	5944	0.176	ng/ul#	87
18) Benzo(a)anthracene	21.40	228	2511	0.078	ng/ul#	87
19) Chrysene	21.45	228	3494	0.094	ng/ul#	87
21) Benzo(b)fluoranthene	23.15	252	6230	0.171	ng/ul	86
22) Benzo(k)fluoranthene	23.15	252	6230	0.148	ng/ul#	84
23) Benzo(a)pyrene	23.81	252	2651	0.070	ng/ul#	77
24) Indeno(1,2,3-cd)pyrene	26.58	276	2206	0.057	ng/ul#	81
26) Benzo(g,h,i)perylene	27.40	276	1877	0.056	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\
Data File : BE094257.D
Acq On : 10 Oct 2017 18:48
Operator : SJ/JU
Sample : I5522-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 11 07:32:27 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 07:23:41 2017
Response via : Initial Calibration

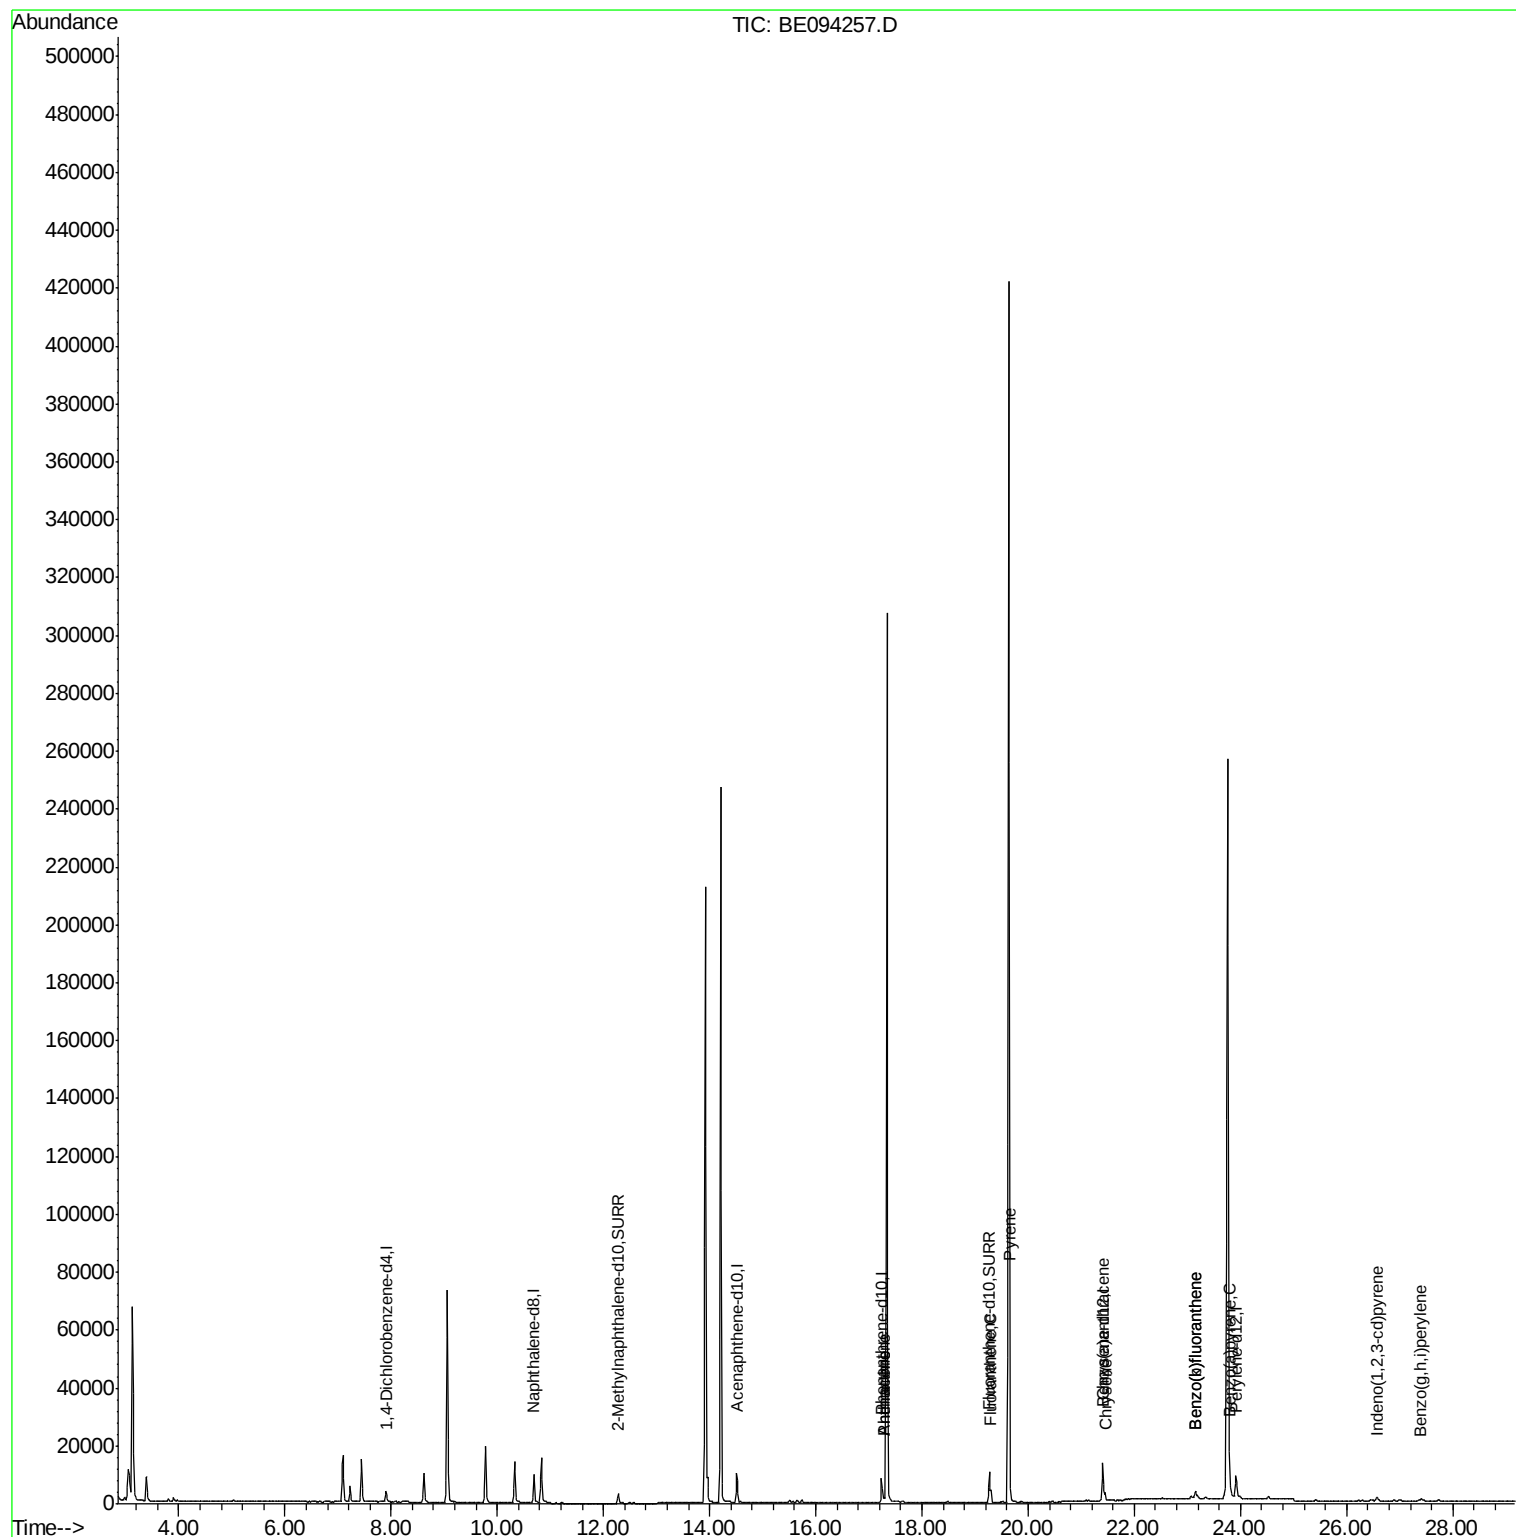

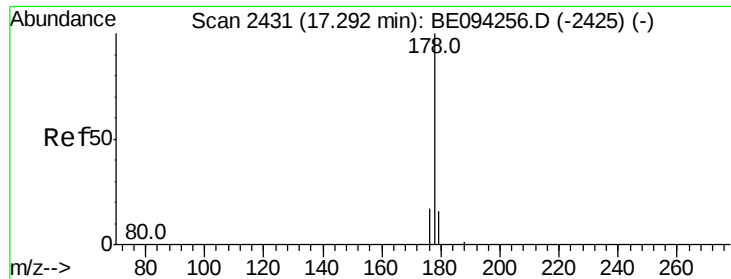

#12

Phenanthrene

Concen: 0.071 ng/ul

RT: 17.29 min Scan# 2431

Delta R.T. -0.00 min

Lab File: BE094257.D

Acq: 10 Oct 2017 18:48

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 2185

Ion Ratio Lower Upper

178 100

179 22.2 18.4 27.6




176 20.1 13.6 20.4

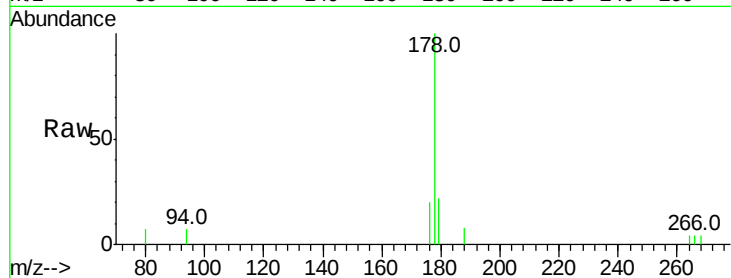

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

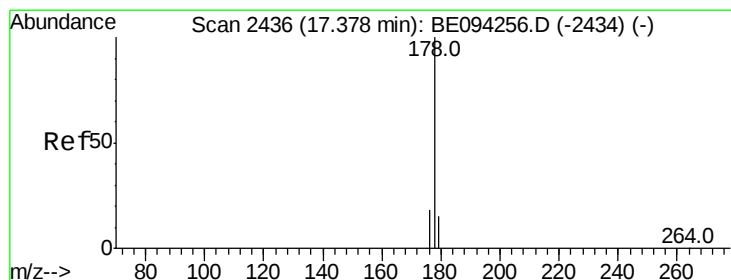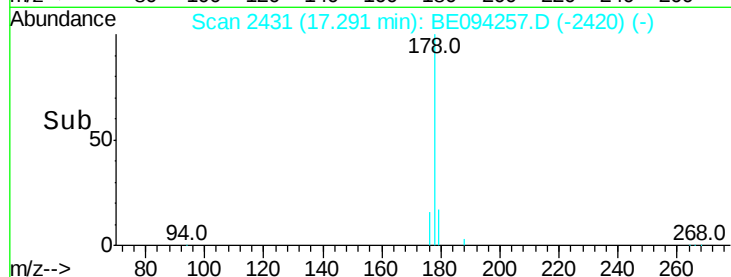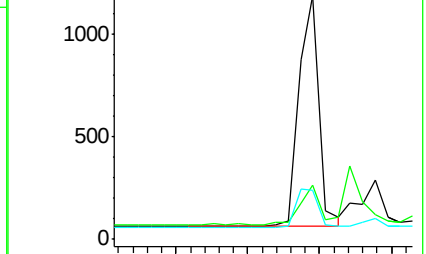

#13

Anthracene

Concen: 0.072 ng/ul

RT: 17.29 min Scan# 2431

Delta R.T. -0.09 min

Lab File: BE094257.D

Acq: 10 Oct 2017 18:48


Tgt Ion:178 Resp: 2153

Ion Ratio Lower Upper

178 100

179 22.2 18.1 27.1



176 20.1 14.7 22.1

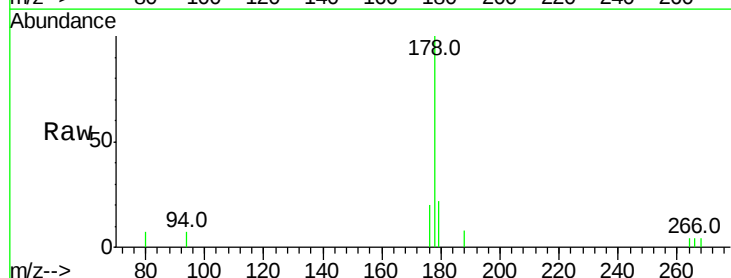


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



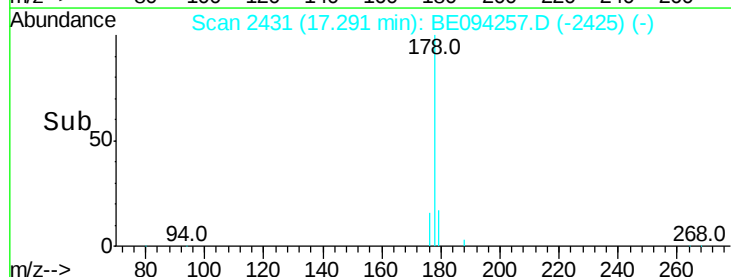
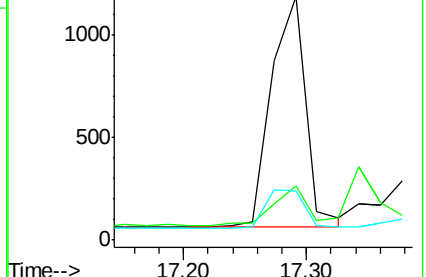


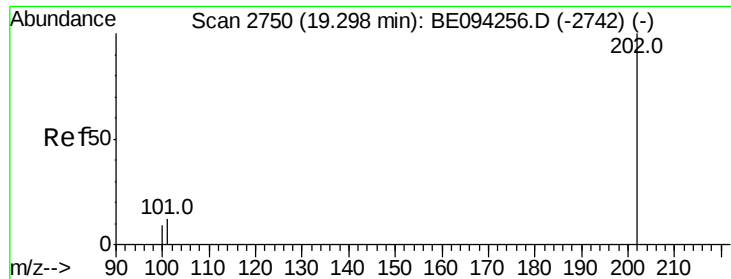

#15
Fluoranthene
Concen: 0.146 ng/ul
RT: 19.30 min Scan# 2751
Delta R.T. 0.00 min
Lab File: BE094257.D
Acq: 10 Oct 2017 18:48




Instrument :
BNA_E
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
202	100		
101	13.4	0.0	30.3
100	10.8	0.0	39.5

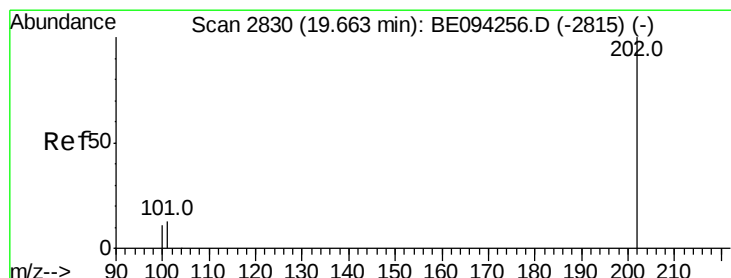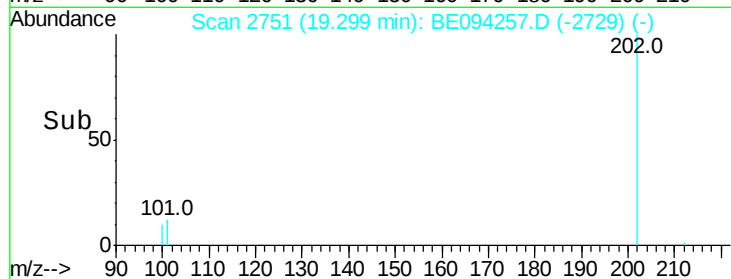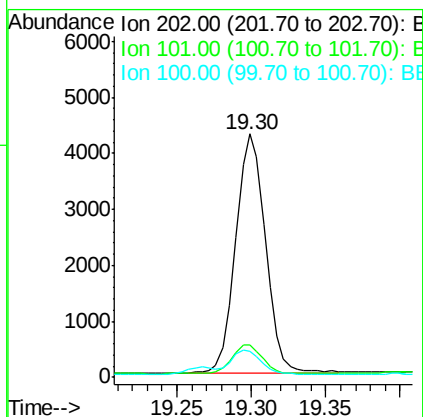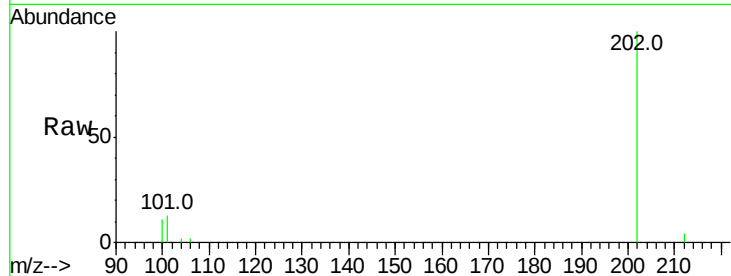

#17
Pyrene
Concen: 0.176 ng/ul
RT: 19.66 min Scan# 2830
Delta R.T. -0.00 min
Lab File: BE094257.D
Acq: 10 Oct 2017 18:48

Tgt Ion	Ratio	Lower	Upper
202	100		
101	16.0	18.2	27.4#
100	14.1	15.6	23.4#

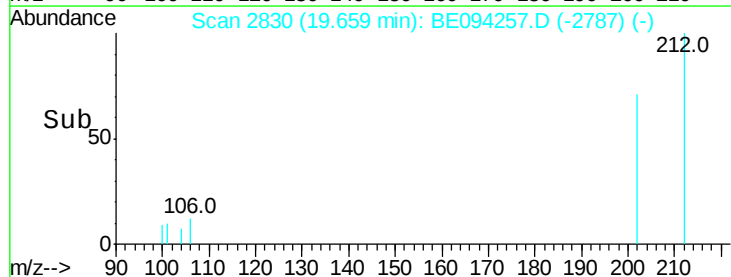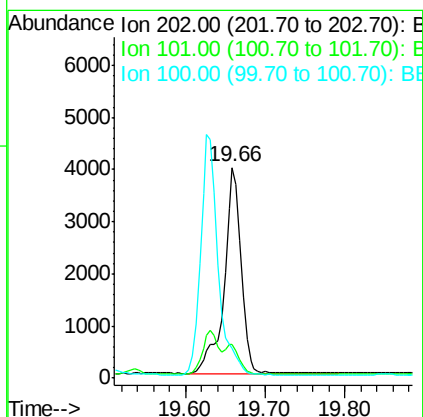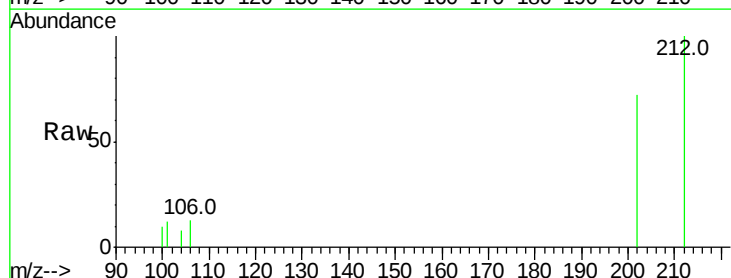

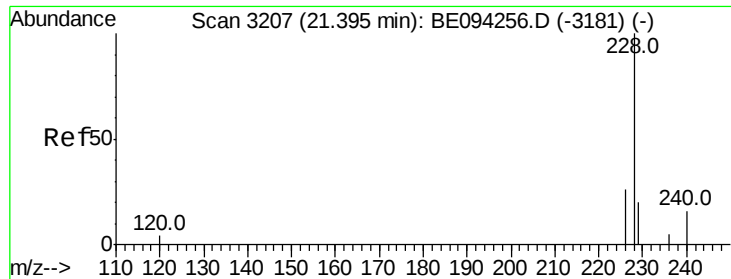

#18

Benzo(a)anthracene

Concen: 0.078 ng/ul

RT: 21.40 min Scan# 3208

Delta R.T. 0.00 min

Lab File: BE094257.D

Acq: 10 Oct 2017 18:48

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 2511

Ion Ratio Lower Upper




228 100

229 30.5 22.8 34.2

226 33.4 17.0 25.6#

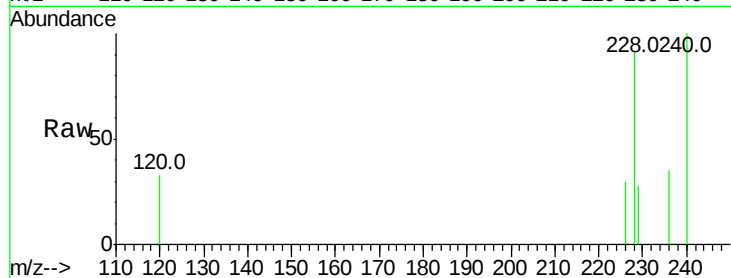

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

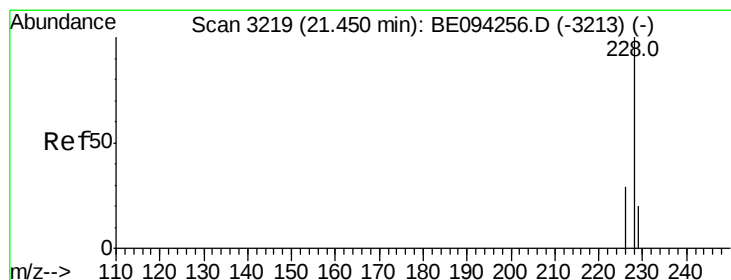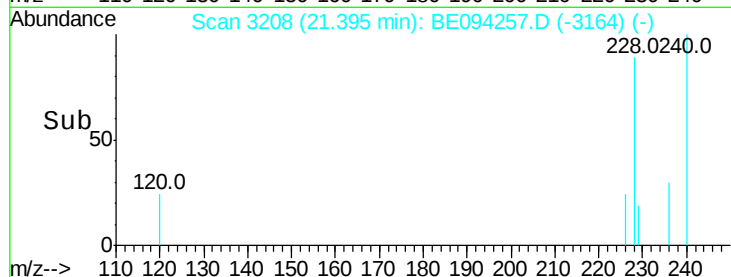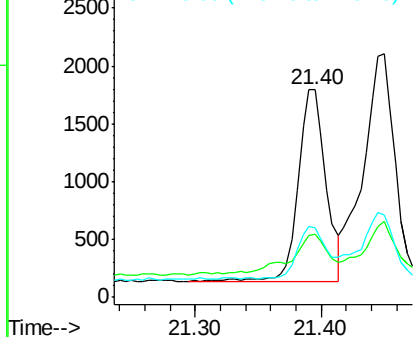

#19

Chrysene

Concen: 0.094 ng/ul

RT: 21.45 min Scan# 3220

Delta R.T. 0.00 min

Lab File: BE094257.D

Acq: 10 Oct 2017 18:48


Tgt Ion:228 Resp: 3494

Ion Ratio Lower Upper



228 100


226 34.0 23.4 35.0

229 31.0 17.7 26.5#

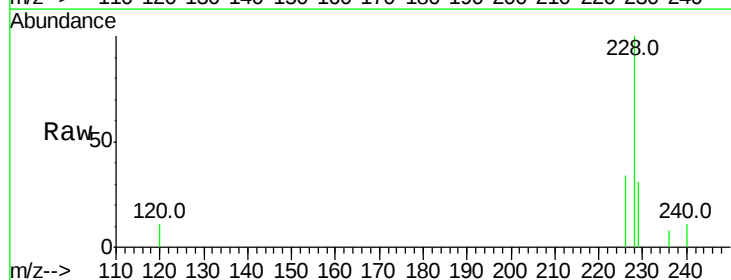

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

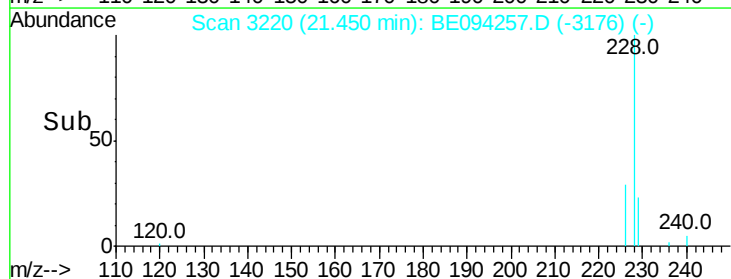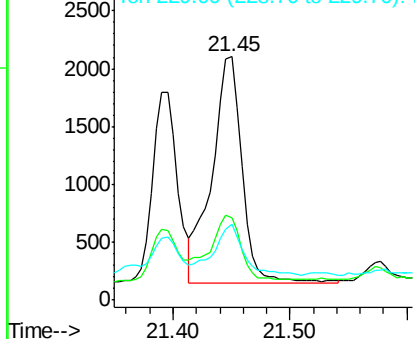

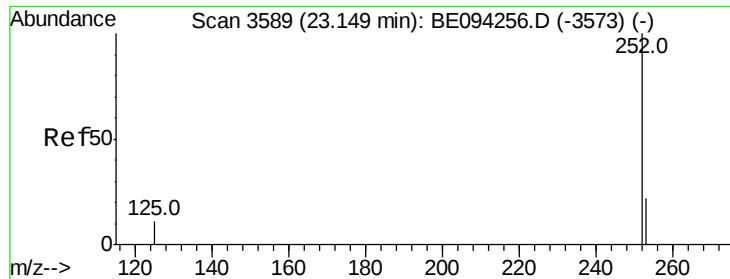

#21

Benzo(b)fluoranthene

Concen: 0.171 ng/ul

RT: 23.15 min Scan# 3590

Delta R.T. 0.00 min

Lab File: BE094257.D

Acq: 10 Oct 2017 18:48

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 6230

Ion Ratio Lower Upper




252 100

253 34.7 0.0 64.2

125 31.1 0.0 35.0

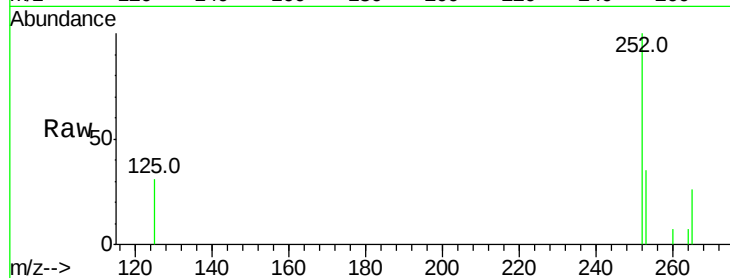

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

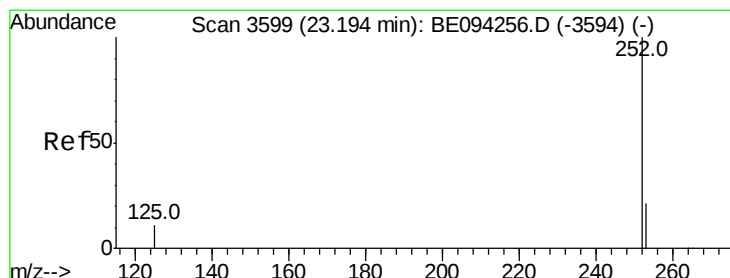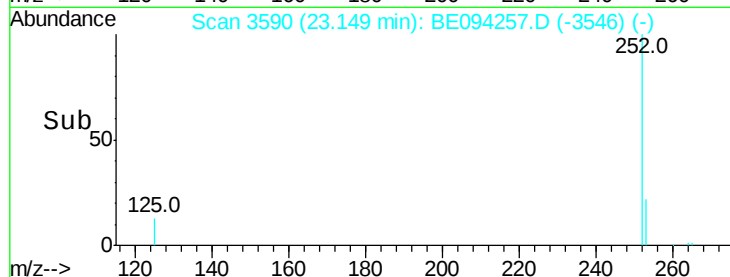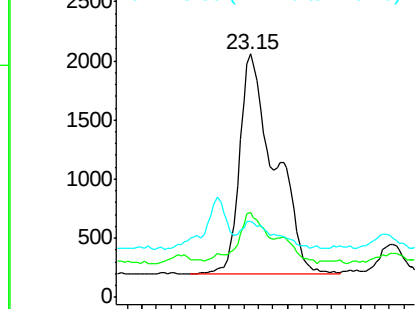

#22

Benzo(k)fluoranthene

Concen: 0.148 ng/ul

RT: 23.15 min Scan# 3590

Delta R.T. -0.05 min

Lab File: BE094257.D

Acq: 10 Oct 2017 18:48


Tgt Ion:252 Resp: 6230

Ion Ratio Lower Upper



252 100


253 34.7 24.5 36.7

125 31.1 13.7 20.5#

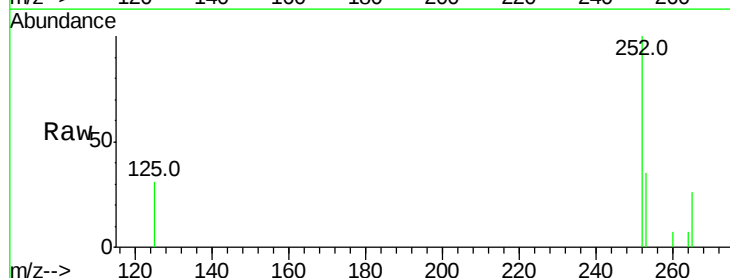

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

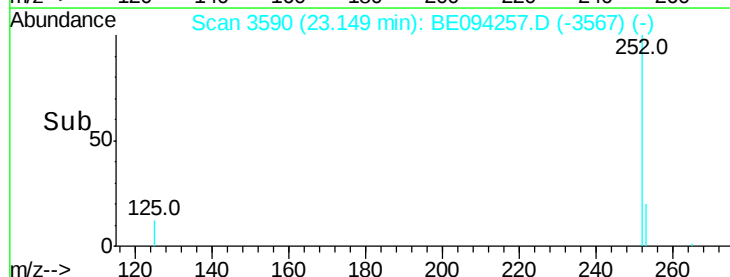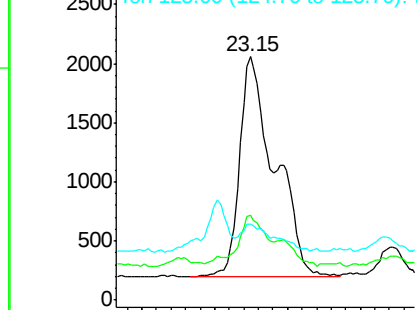

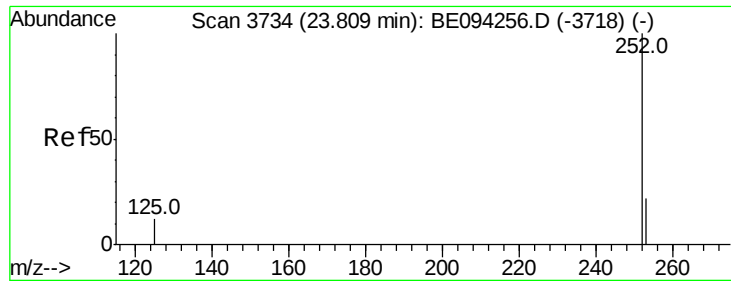

#23

Benzo(a)pyrene

Concen: 0.070 ng/u1

RT: 23.81 min Scan# 3735

Delta R.T. 0.00 min

Lab File: BE094257.D

Acq: 10 Oct 2017 18:48

Instrument :

BNA_E

ClientSampleId :





Tot Ion:252 Resp: 2651

Ion Ratio Lower Upper

252 100

253 41.0 28.5 42.7

125 43.7 18.1 27.1#

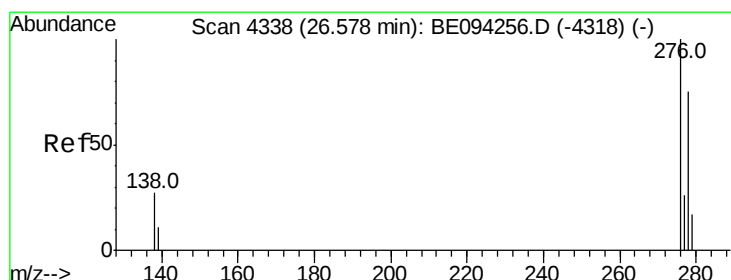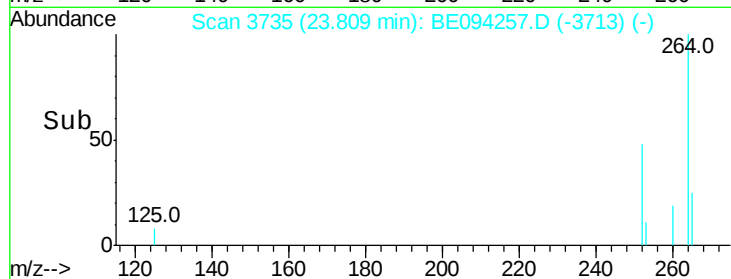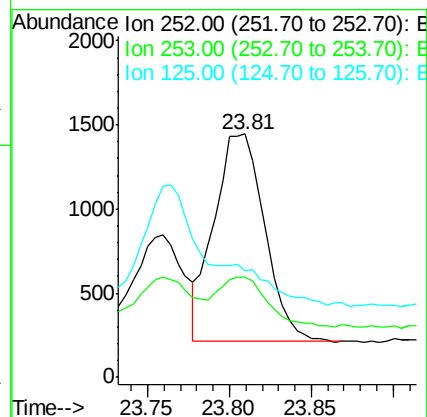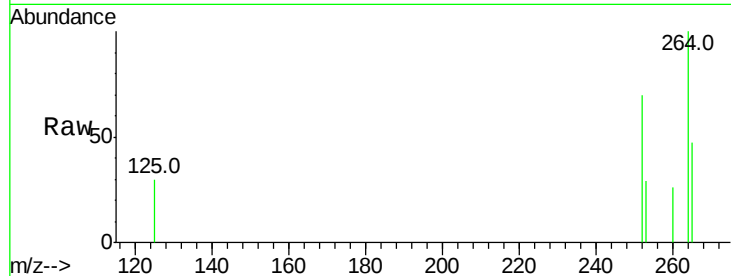

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.057 ng/u1

RT: 26.58 min Scan# 4339

Delta R.T. -0.00 min

Lab File: BE094257.D

Acq: 10 Oct 2017 18:48




Tgt Ion:276 Resp: 2206


Ion Ratio Lower Upper

276 100

138 25.3 28.0 42.0#

227 0.0 8.0 12.0#

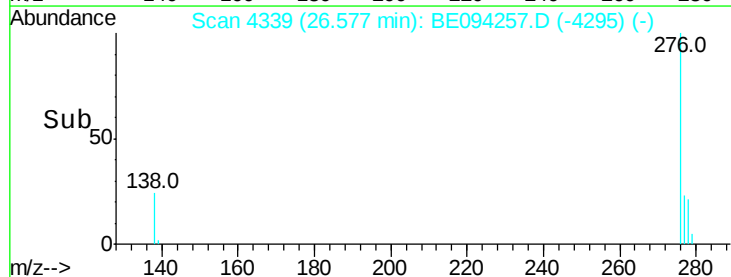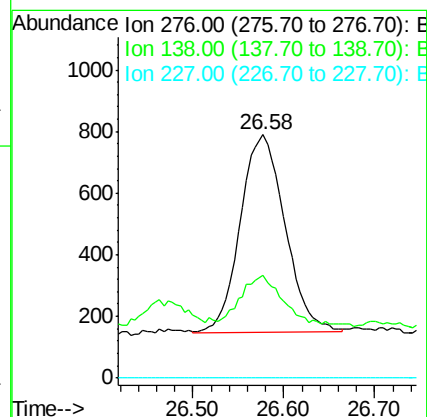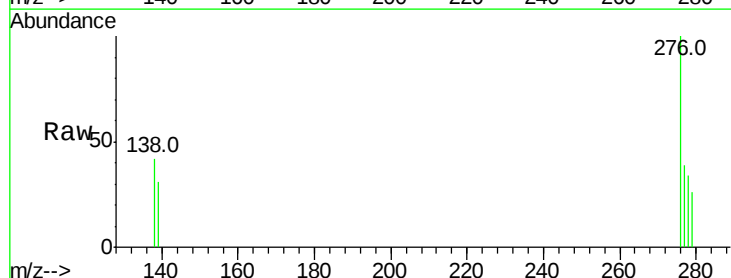

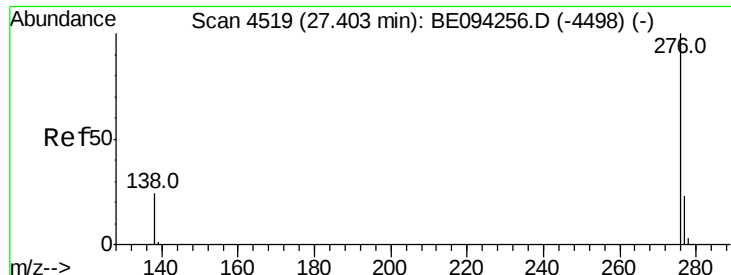

#26

Benzo(a,h,i)perylene

Concen: 0.056 ng/ul

RT: 27.40 min Scan# 4519

Delta R.T. -0.01 min


Lab File: BE094257.D

Acq: 10 Oct 2017 18:48

Instrument :

BNA_E

ClientSampleId :

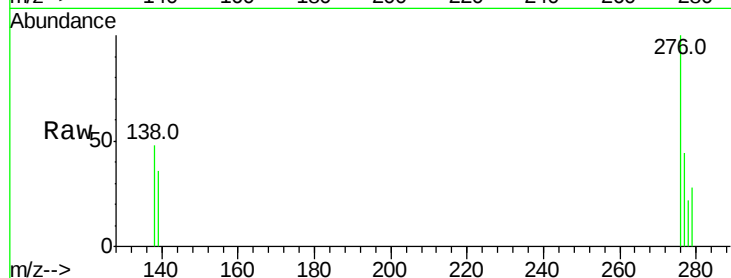


Tot Ion:276 Resp: 1877

Ion Ratio Lower Upper

276 100

138 47.8 21.8 32.8#

277 43.9 20.5 30.7#

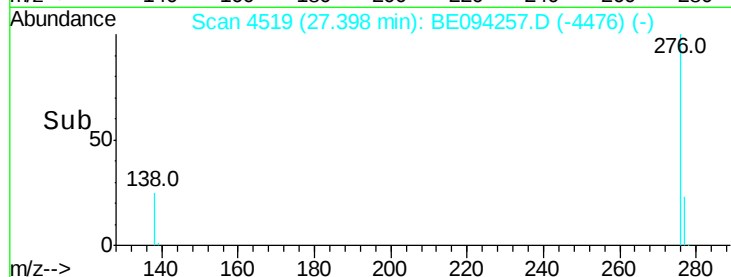

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

