

Quantitation Report (QT Reviewed)


Instrument :  
BNA\_E  
ClientSampled :  
C0AD6

Manual Integrations  
APPROVED

Sohil  
10/11/2017 7:19:41 PM

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
Data File : BE094252.D  
Acq On : 10 Oct 2017 13:42  
Operator : SJ/JU  
Sample : I5522-07  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Oct 11 06:58:58 2017  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 11 06:34:16 2017  
Response via : Initial Calibration

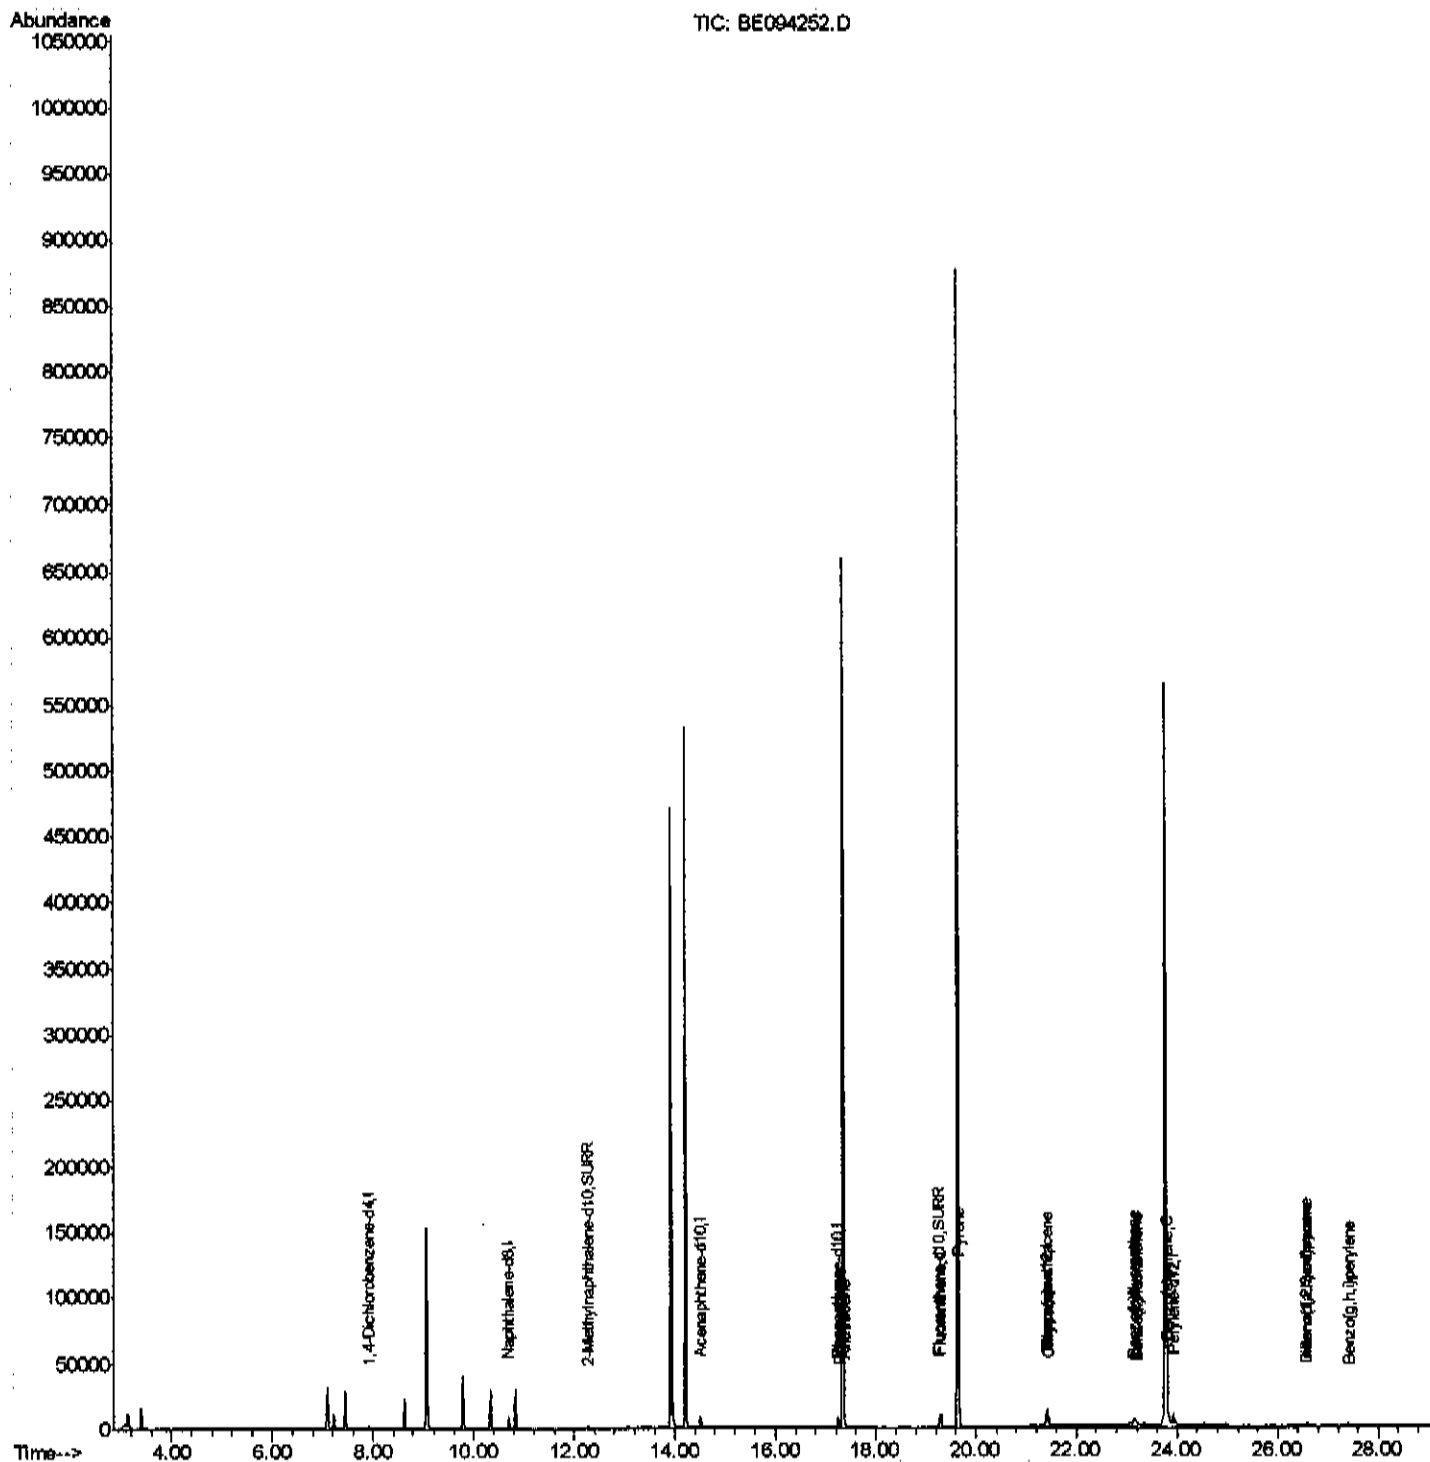

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:37:41 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

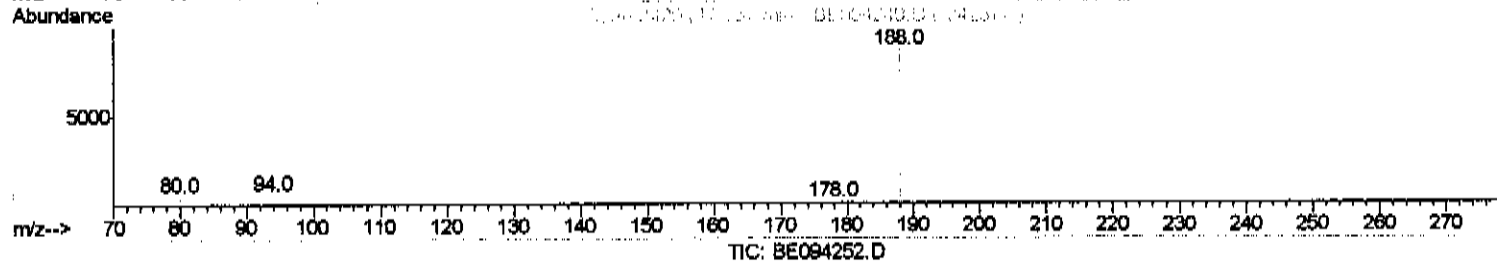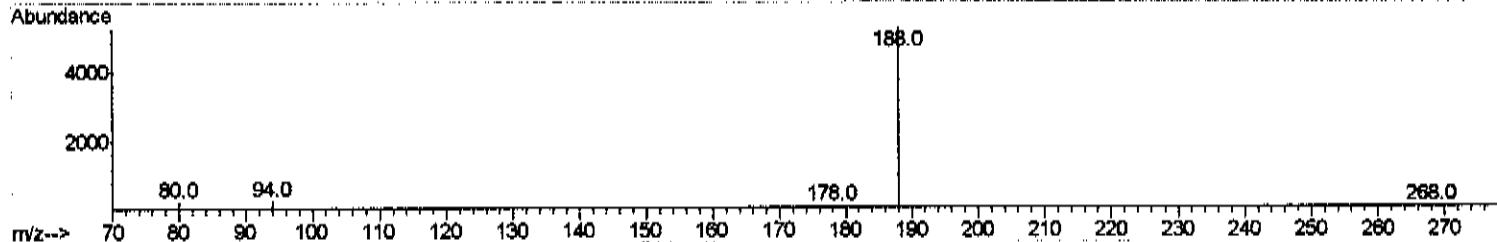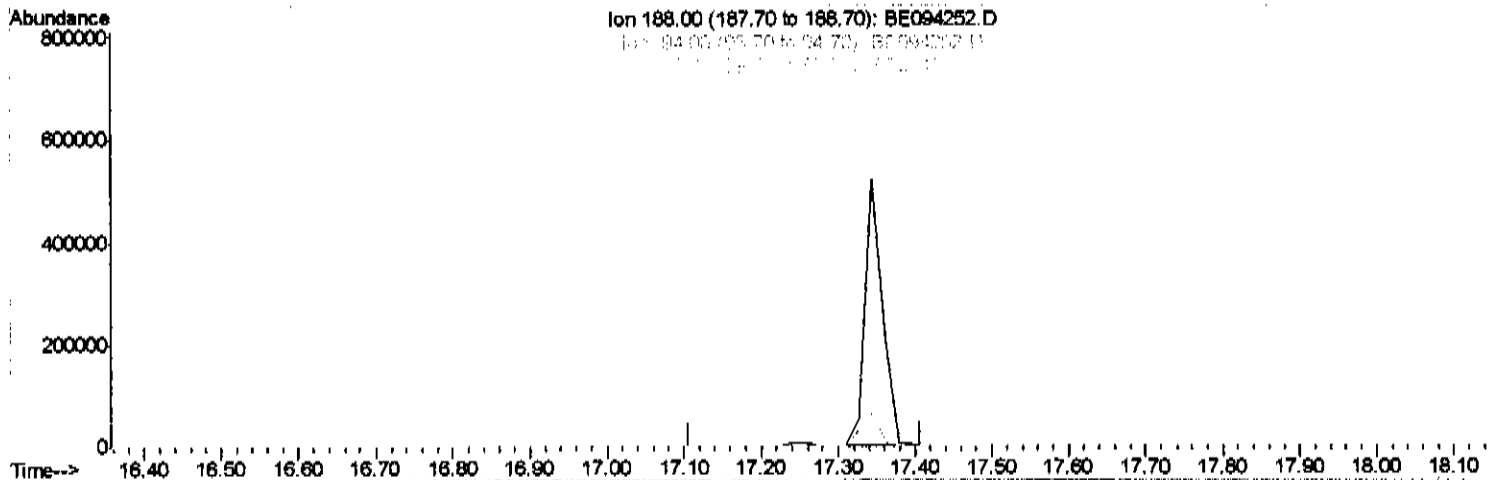

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 188.00 | 100   | 0.00  |
| 94.00  | 11.00 | 0.00# |
| 80.00  | 11.80 | 0.00# |
| 0.00   | 0.00  | 0.00  |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:37:41 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

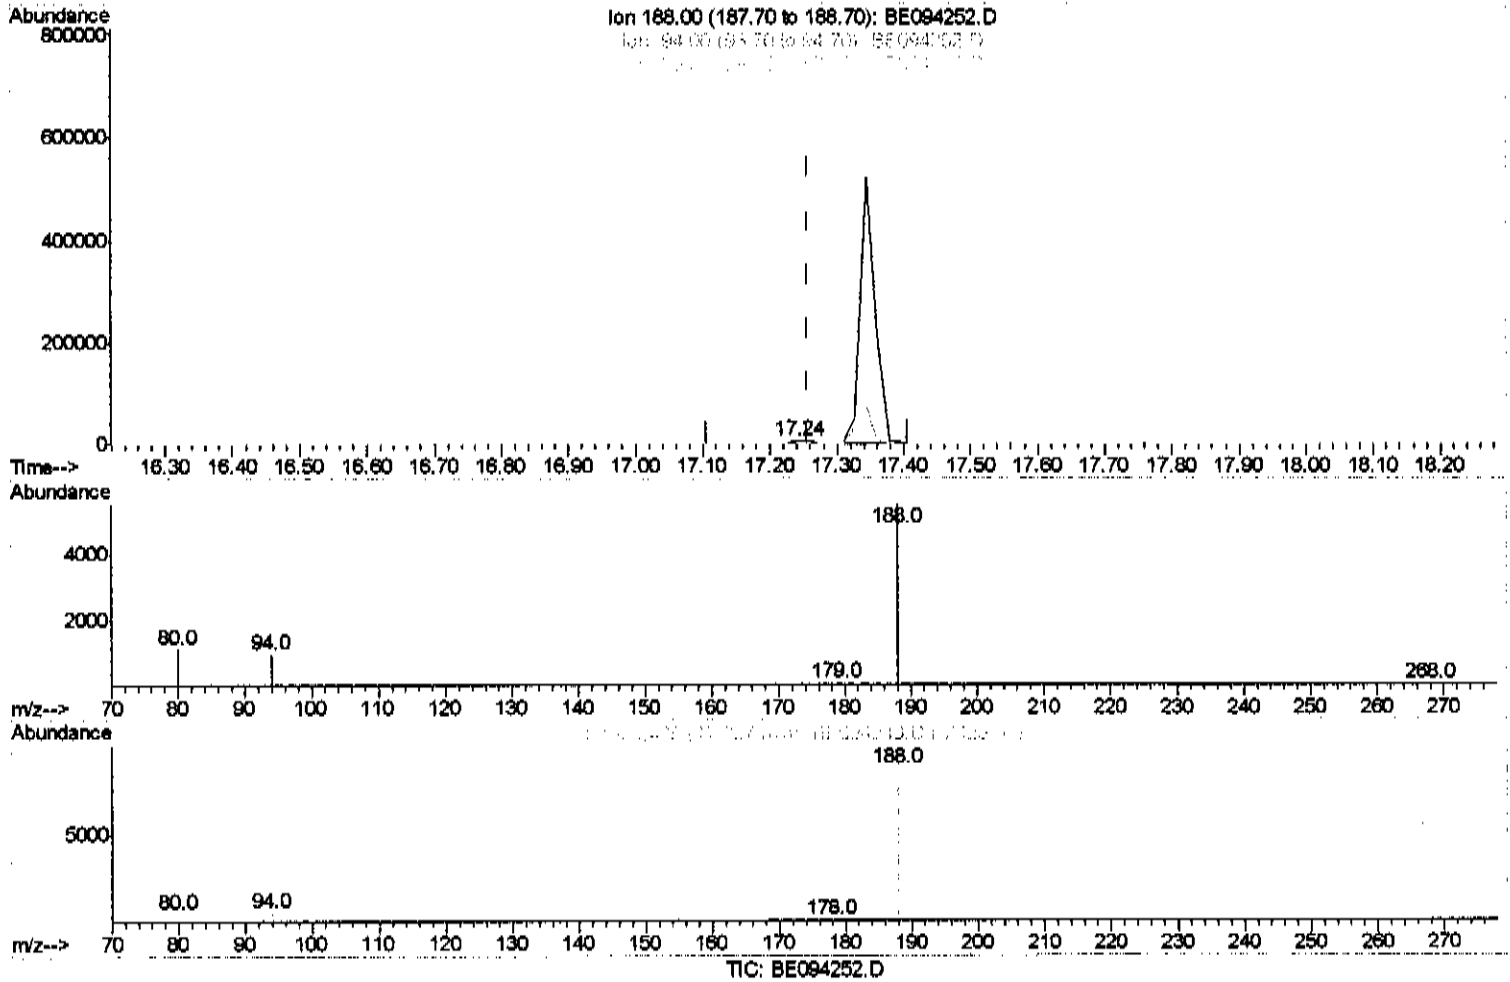

(10) Phenanthrene-d10 (I)

17.240min (-0.017) 0.40ng/ul m

response 11474

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 188.00 | 100   | 100    |
| 94.00  | 11.00 | 18.06% |
| 80.00  | 11.80 | 21.07% |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:54:57 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 OLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

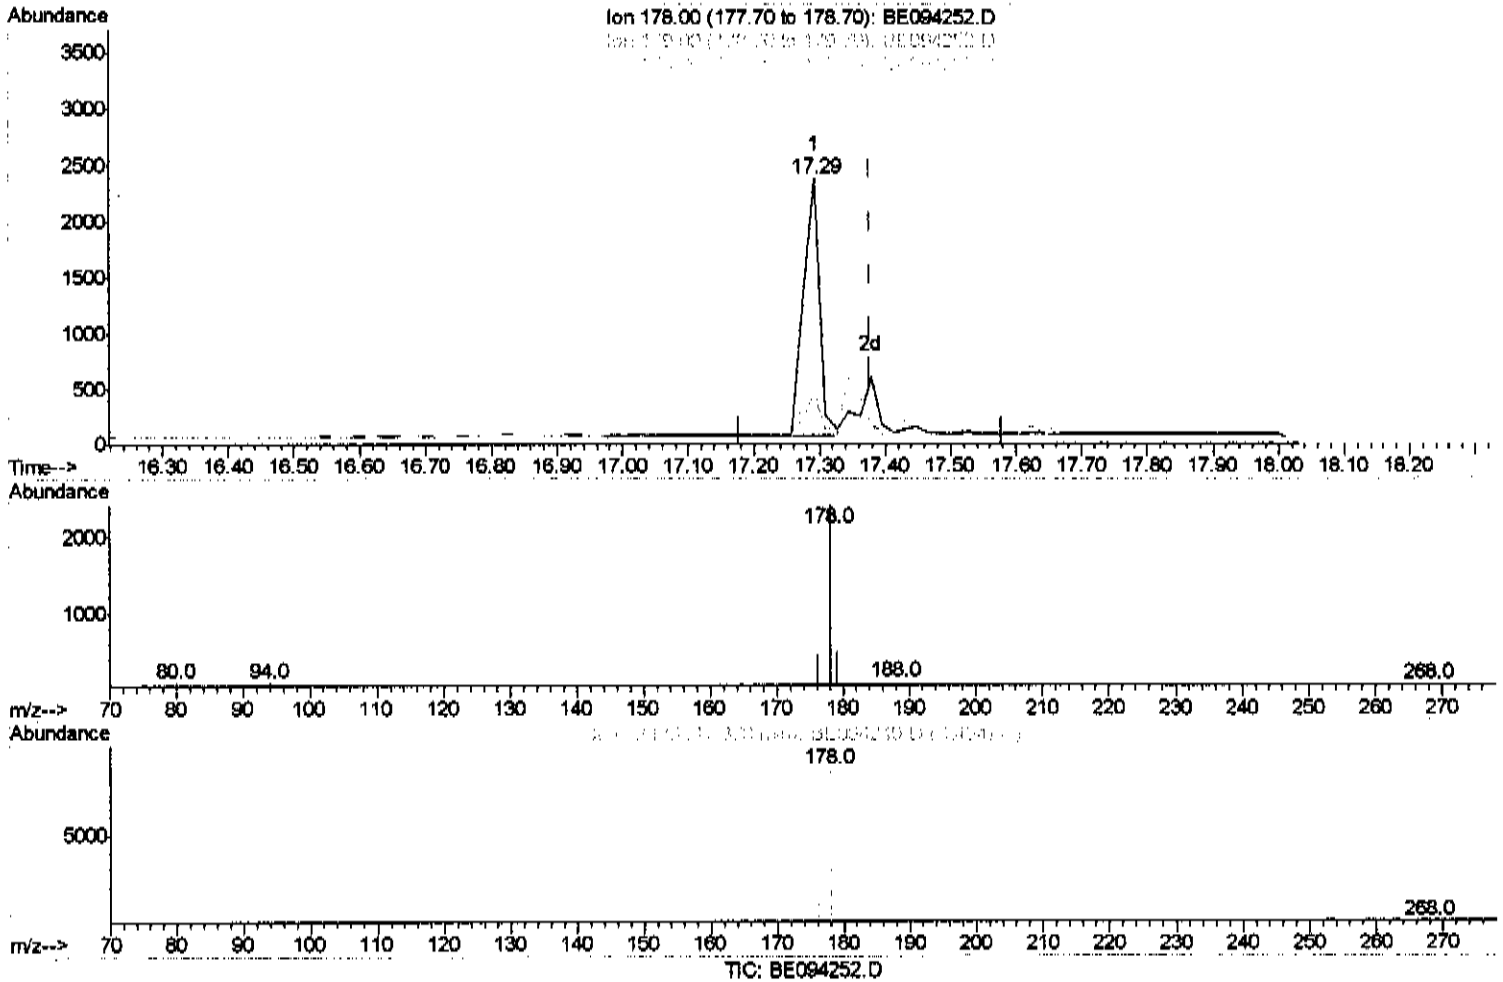

(13) Anthracene

17.292min (-0.087) 0.14ng/ul

response 4037

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 178.00 | 100   | 100   |
| 179.00 | 22.60 | 19.92 |
| 176.00 | 18.40 | 19.05 |
| 0.00   | 0.00  | 0.00  |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:54:57 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

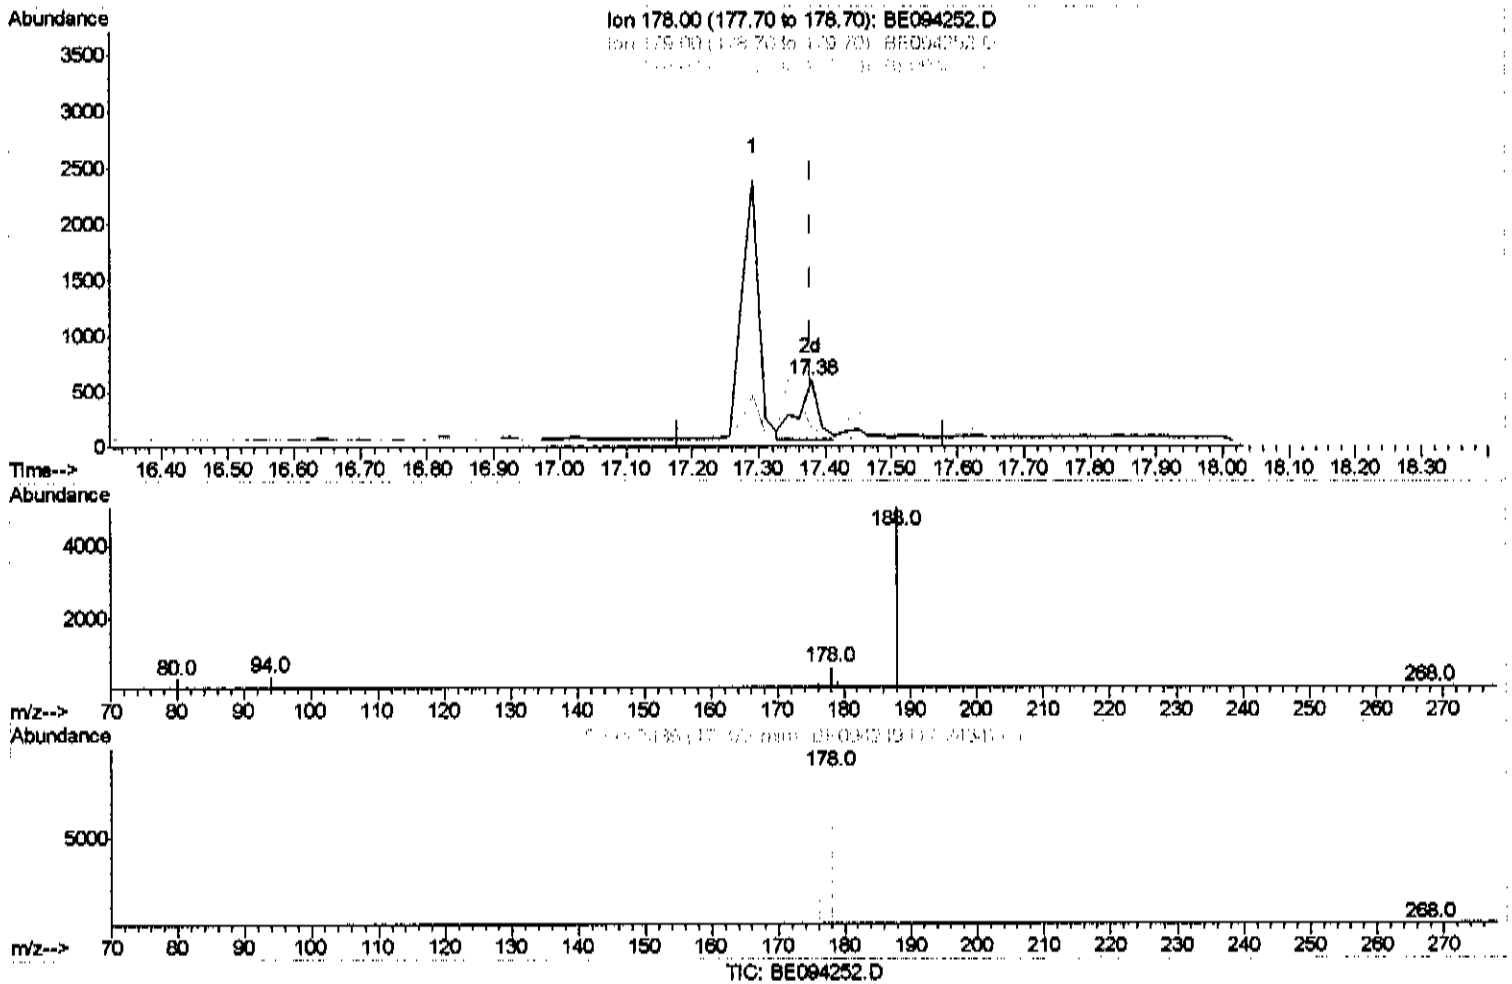

(13) Anthracene

17.378min (+0.000) 0.04ng/ul m

response 1155

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 178.00 | 100   | 100    |
| 179.00 | 22.60 | 29.44# |
| 176.00 | 18.40 | 27.30# |
| 0.00   | 0.00  | 0.00   |

*JU 10/11/17*

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:54:57 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

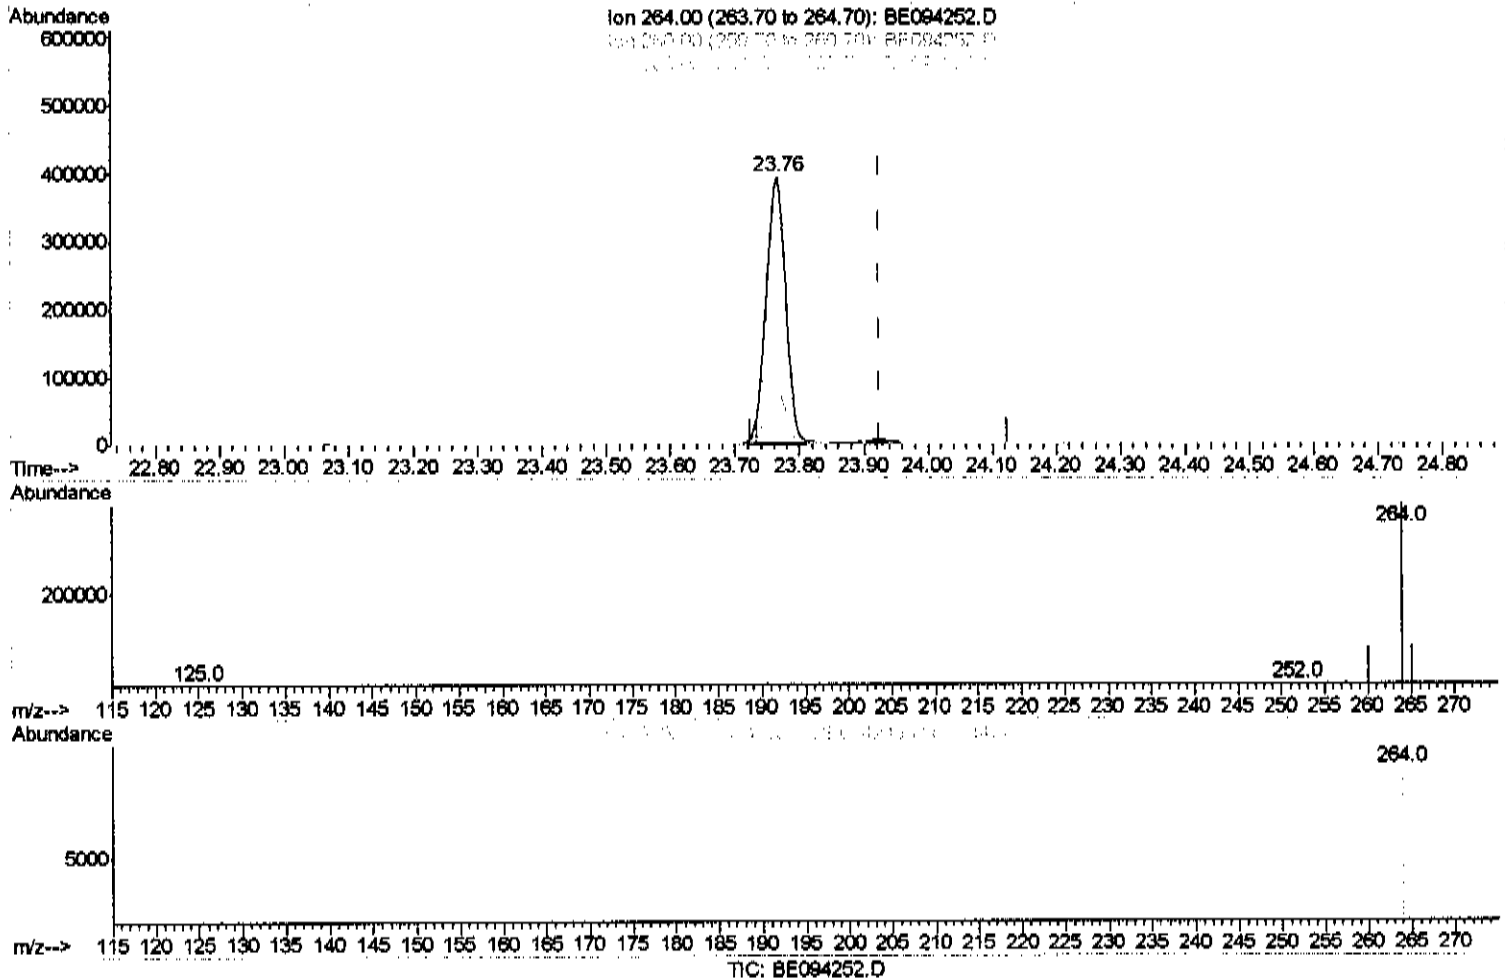

(20) Perylene-d12 (I)

23.764min (-0.160) 0.40ng/ul

response 809309

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100    | 100    |
| 260.00 | 30.10  | 21.00# |
| 266.00 | 103.50 | 21.60# |
| 0.00   | 0.00   | 0.00   |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:54:57 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 OLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

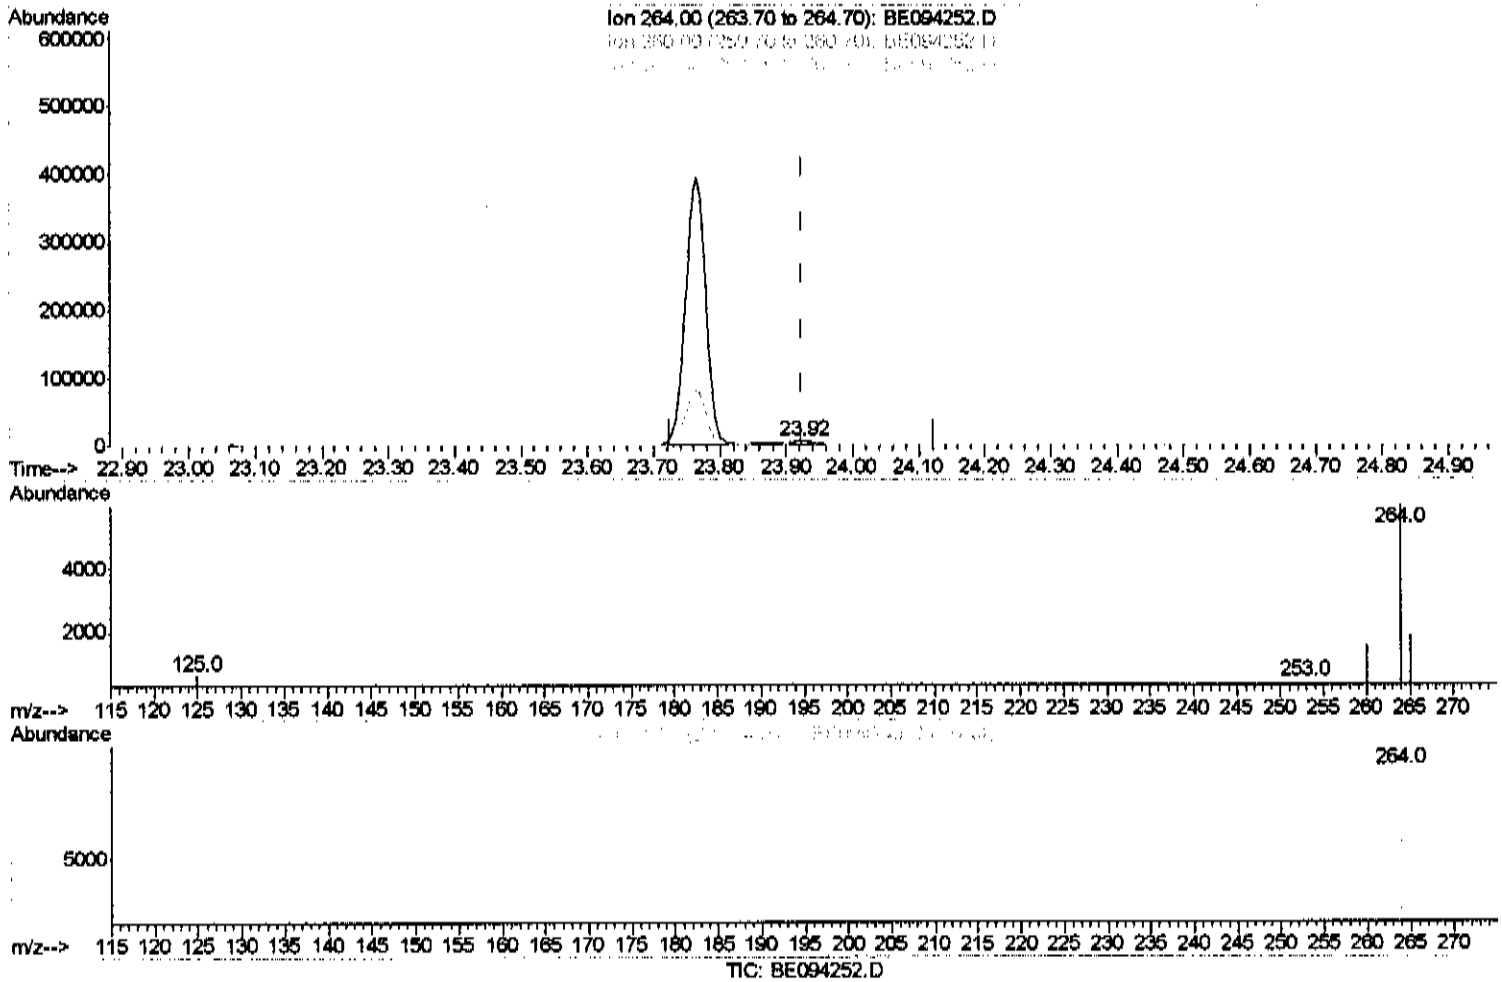

(20) Perylene-d12 (I)

23.924min (-0.000) 0.40ng/ul m

response 11593

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100    | 100    |
| 260.00 | 30.10  | 26.21  |
| 265.00 | 103.50 | 31.56% |
| 0.00   | 0.00   | 0.00   |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

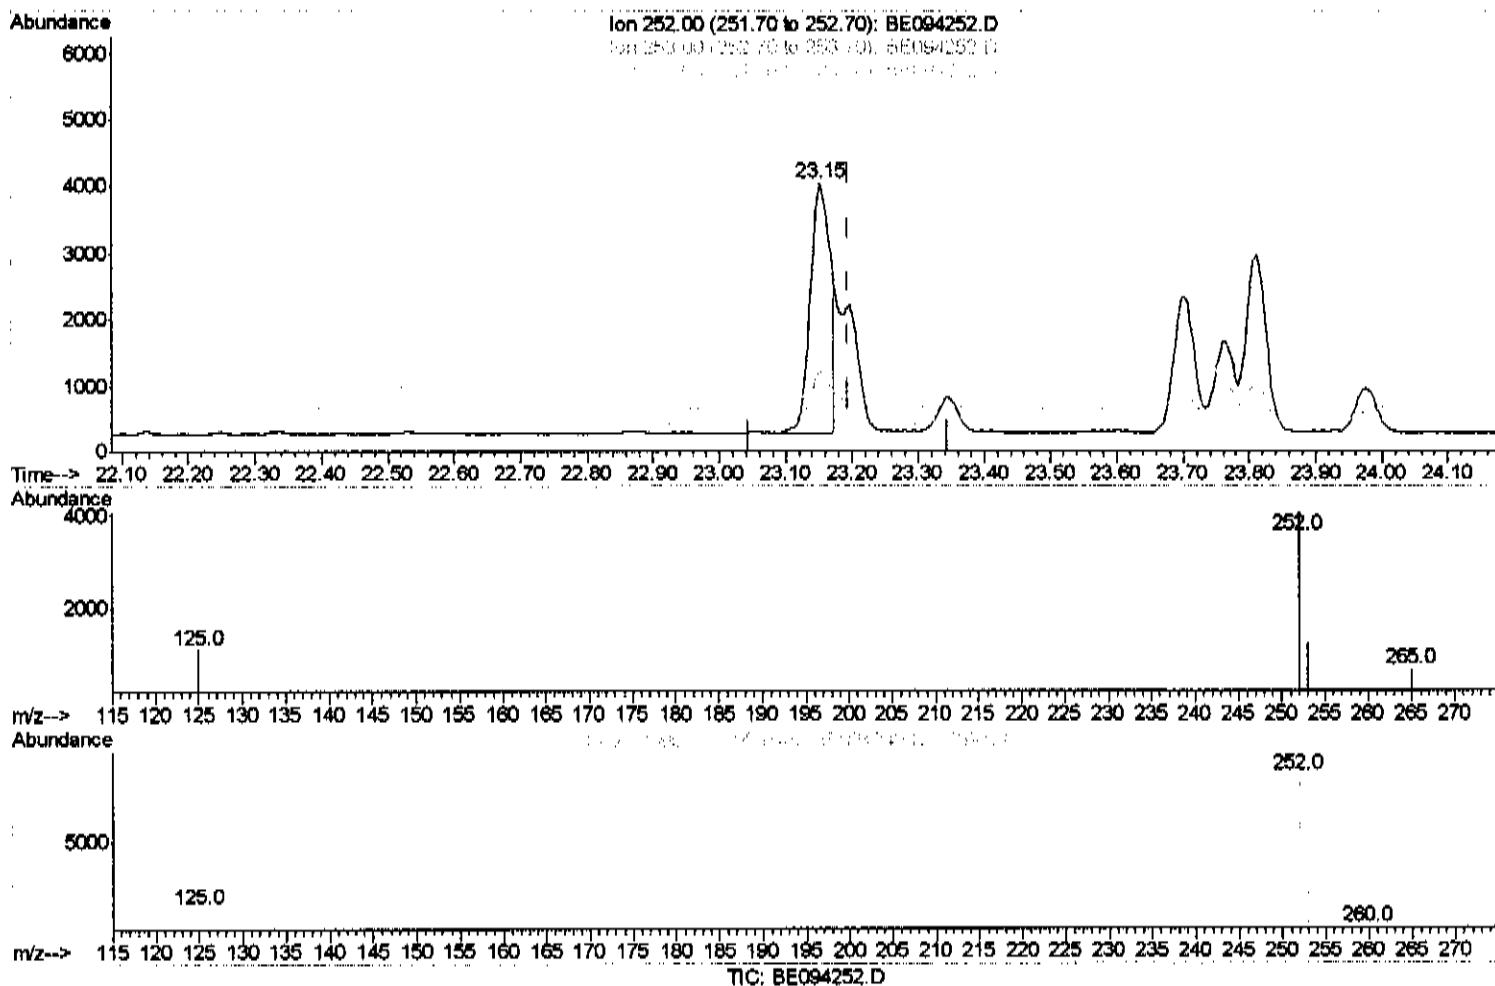

(22) Benzo(k)fluoranthene

23.150min (-0.046) 0.22ng/ul

response 8049

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 30.60 | 29.95  |
| 125.00 | 17.10 | 26.88# |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

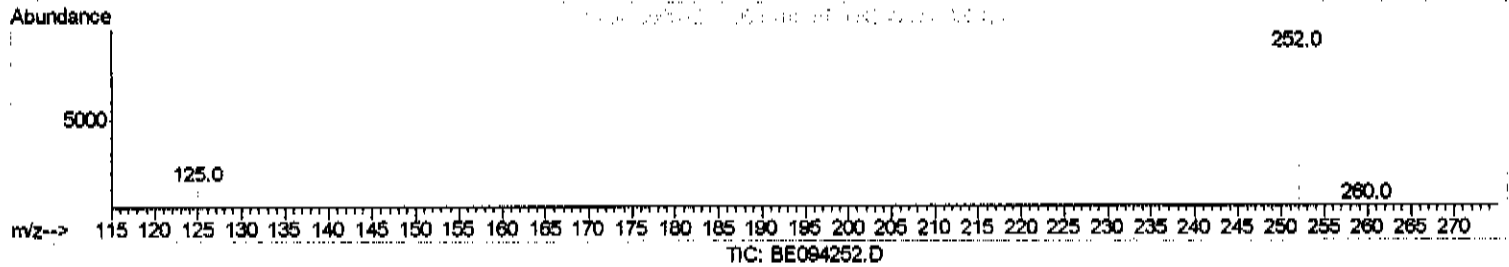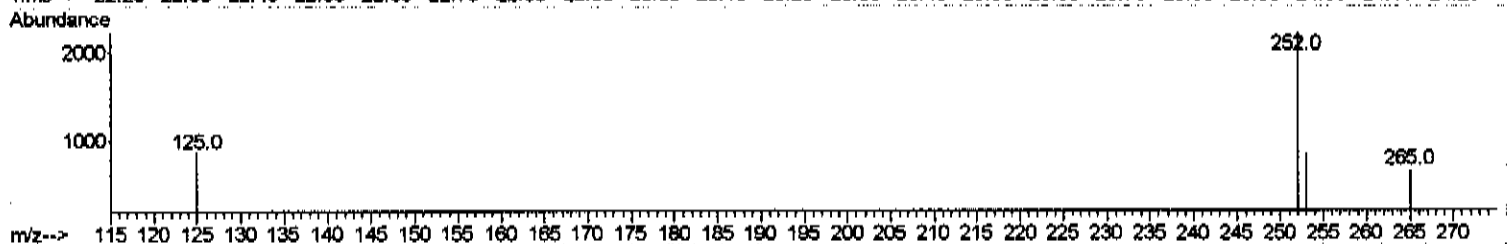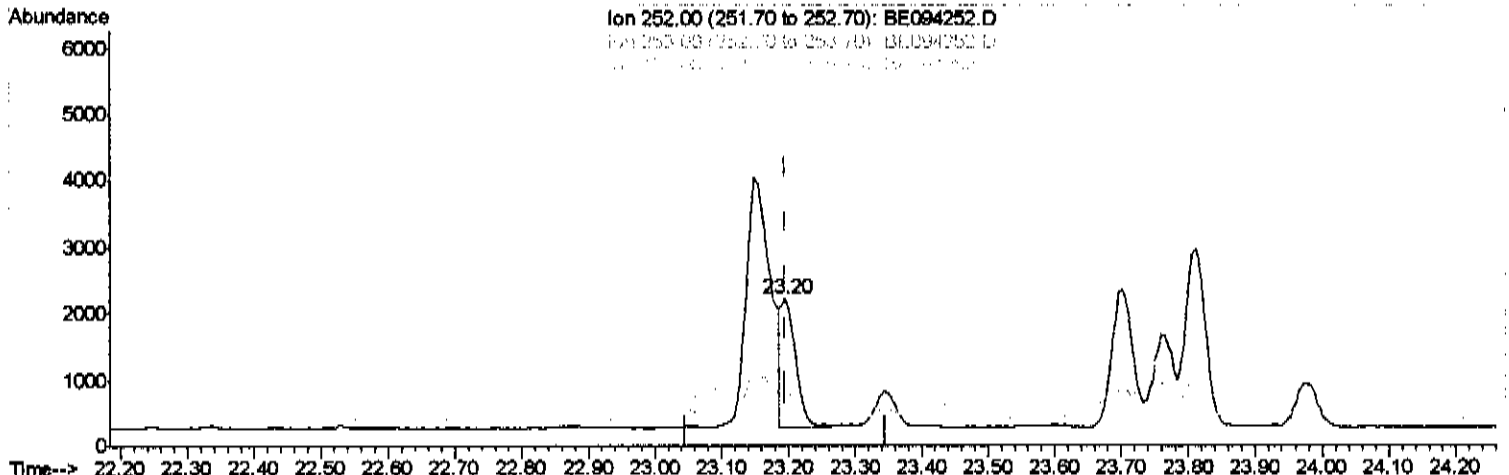

(22) Benzo(k)fluoranthene

23.195min (-0.000) 0.08ng/ul m

response 2944

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 30.60 | 37.38# |
| 125.00 | 17.10 | 38.78# |
| 0.00   | 0.00  | 0.00   |

*Handwritten signature:* JU 10/11/17

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acc On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

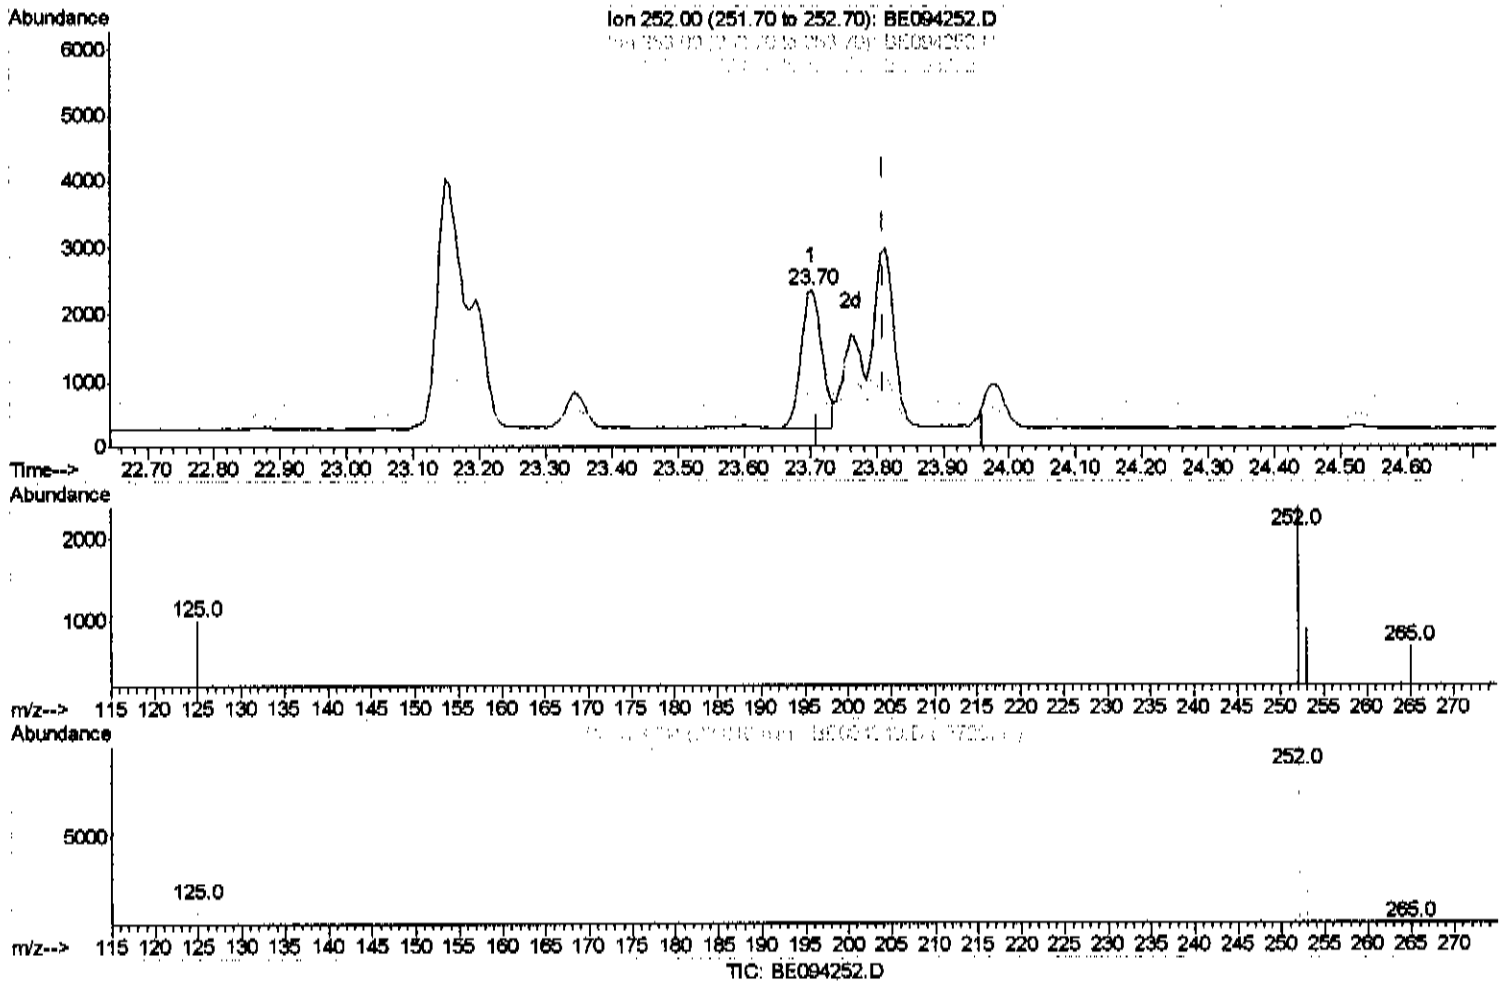

(23) Benzo(a)pyrene (C)

23.701min (-0.110) 0.14ng/ul

response 4805

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 35.60 | 37.47  |
| 125.00 | 22.60 | 42.17# |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

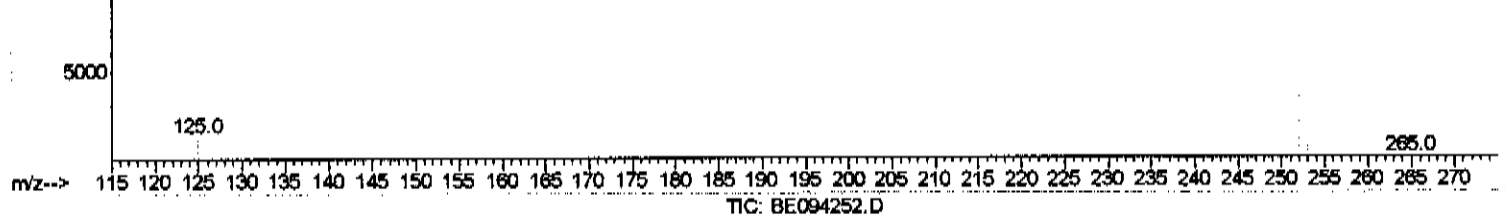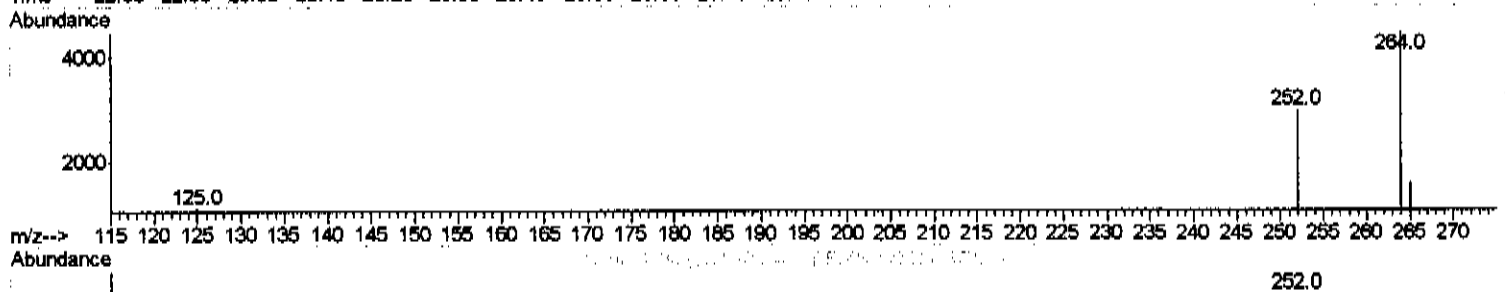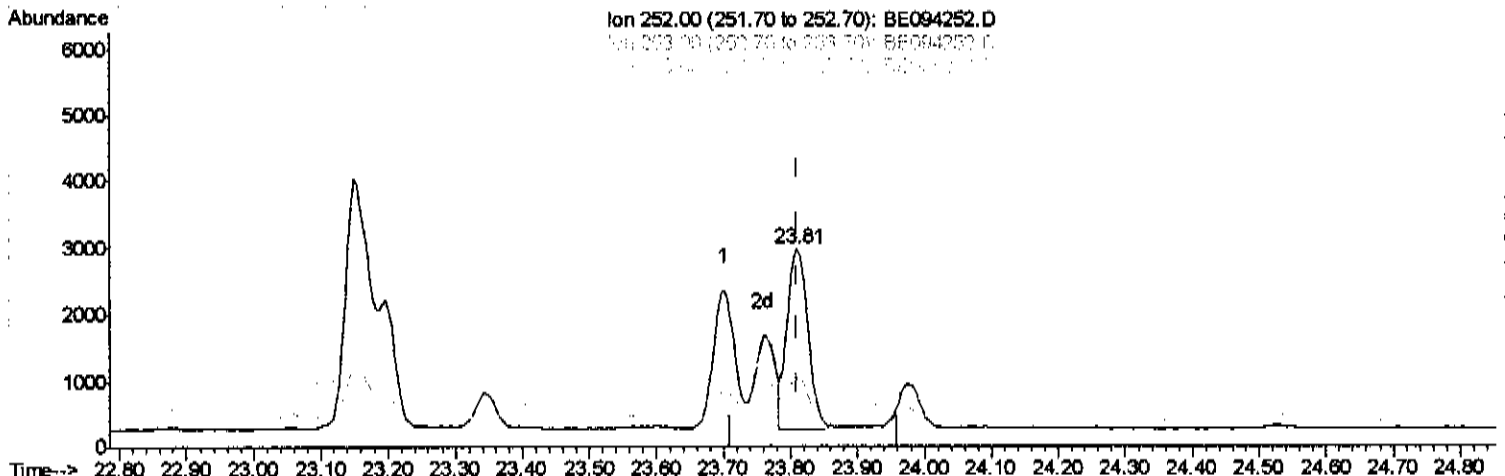

(23) Benzo(a)pyrene (C)

23.810min (-0.000) 0.18ng/ul m<sub>g</sub> 10/11/17  
 response 5753

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 35.60 | 34.41  |
| 125.00 | 22.60 | 36.55# |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

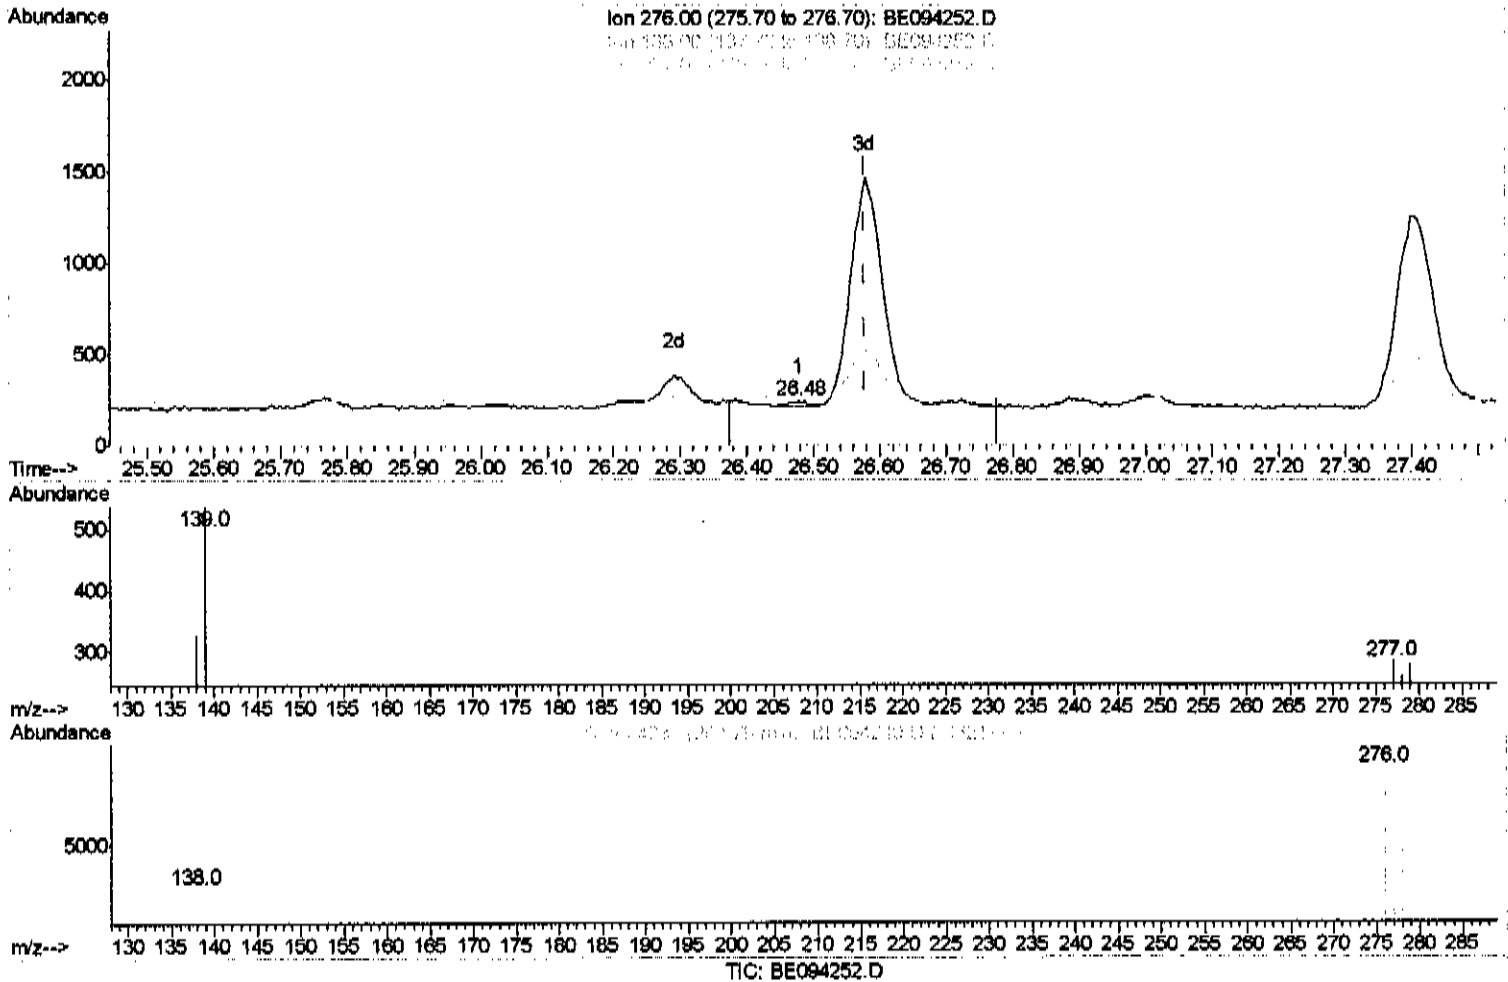

(24) Indeno(1,2,3-cd)pyrene

26.478min (-0.100) 0.00ng/ul

response 64

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 276.00 | 100   | 100     |
| 138.00 | 35.00 | 250.00% |
| 227.00 | 10.00 | 0.00%   |
| 0.00   | 0.00  | 0.00    |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

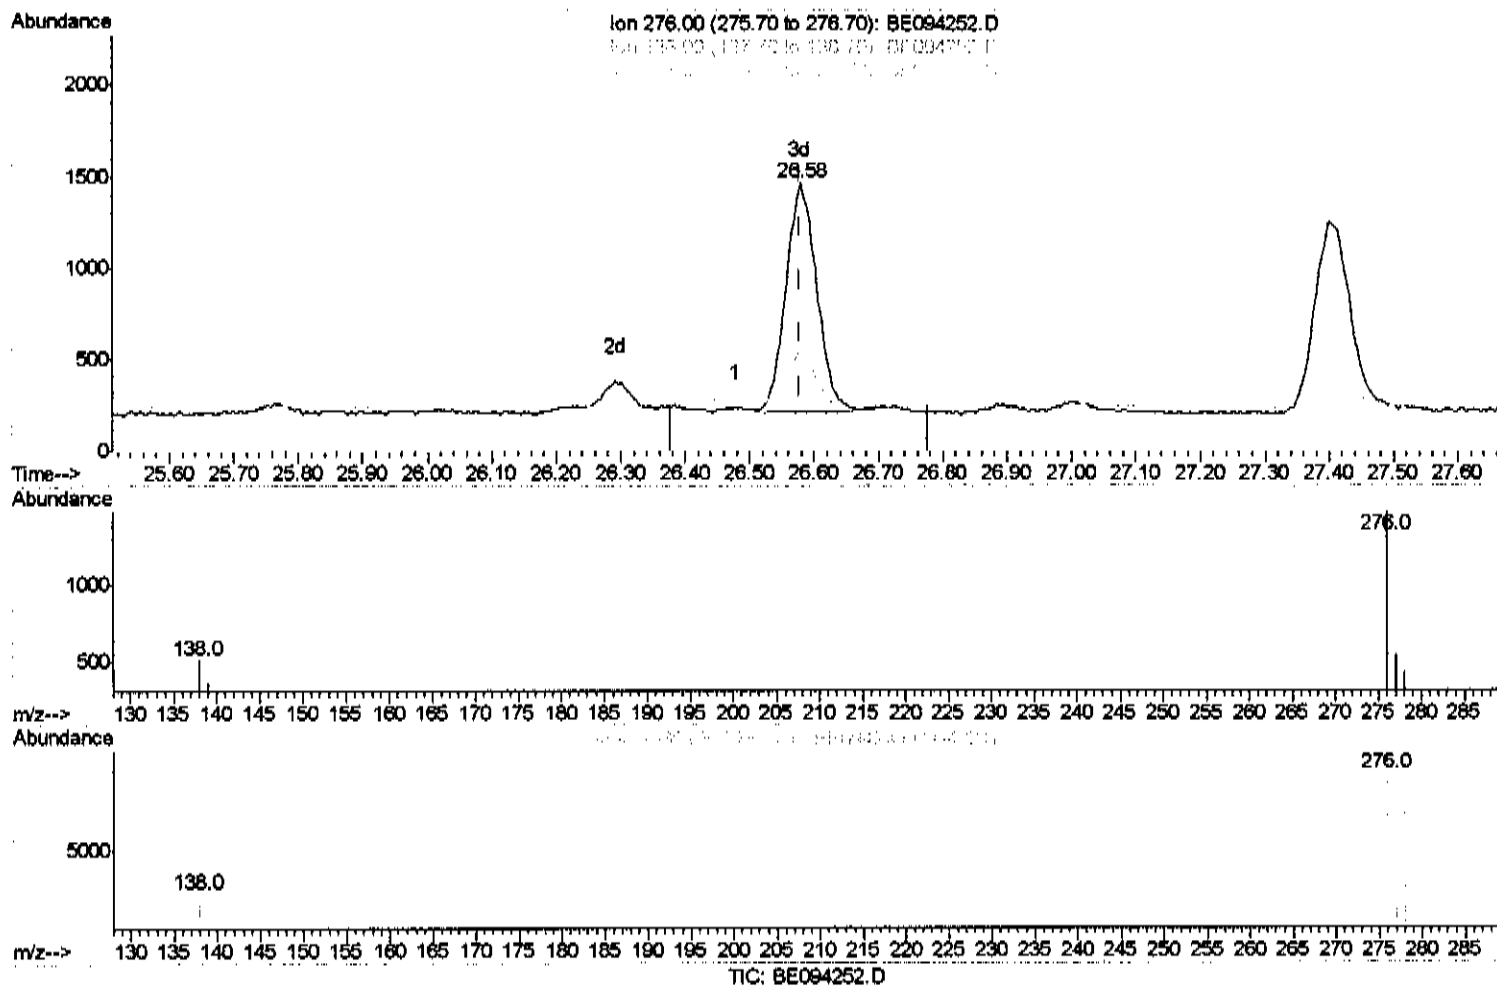

(24) Indeno(1,2,3-cd)pyrene

26.578min (+0.000) 0.12ng/ul m

response 4166

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 276.00 | 100   | 100   |
| 138.00 | 35.00 | 5.04# |
| 227.00 | 10.00 | 0.00# |
| 0.00   | 0.00  | 0.00  |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 OLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

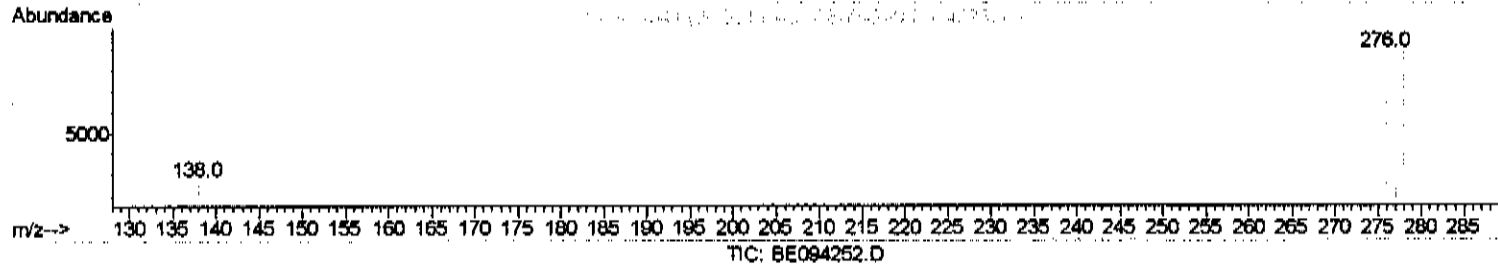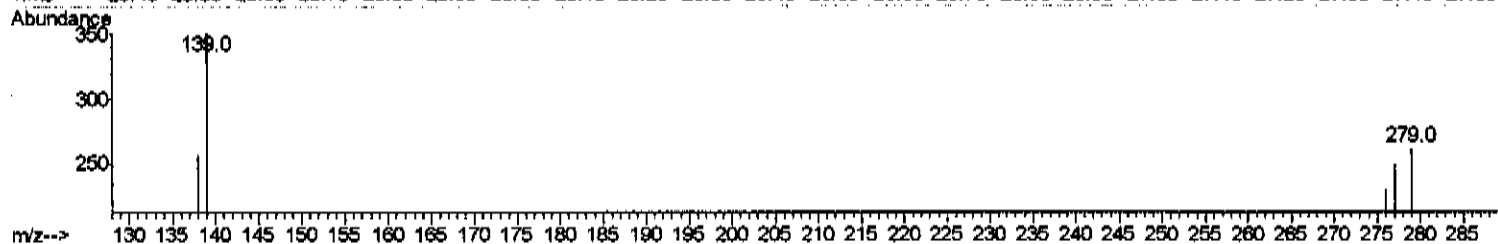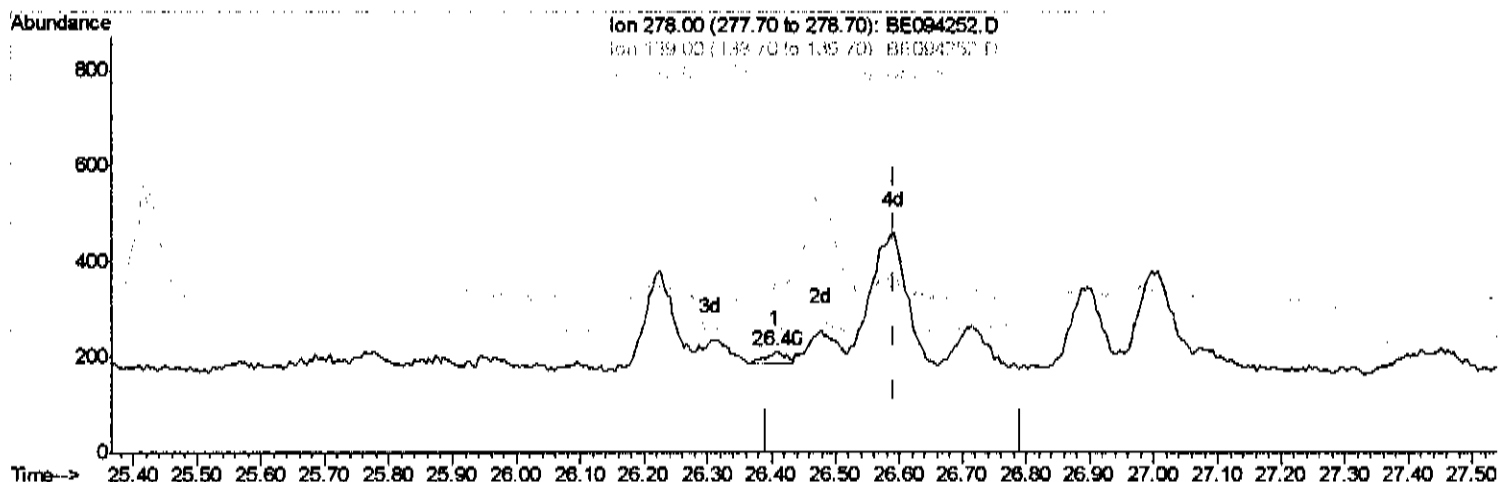

(25) Dibenzo(a,h)anthracene

26.405min (-0.187) 0.00ng/ul

response 56

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 278.00 | 100   | 100     |
| 139.00 | 21.70 | 165.57# |
| 279.00 | 32.40 | 123.58# |
| 0.00   | 0.00  | 0.00    |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

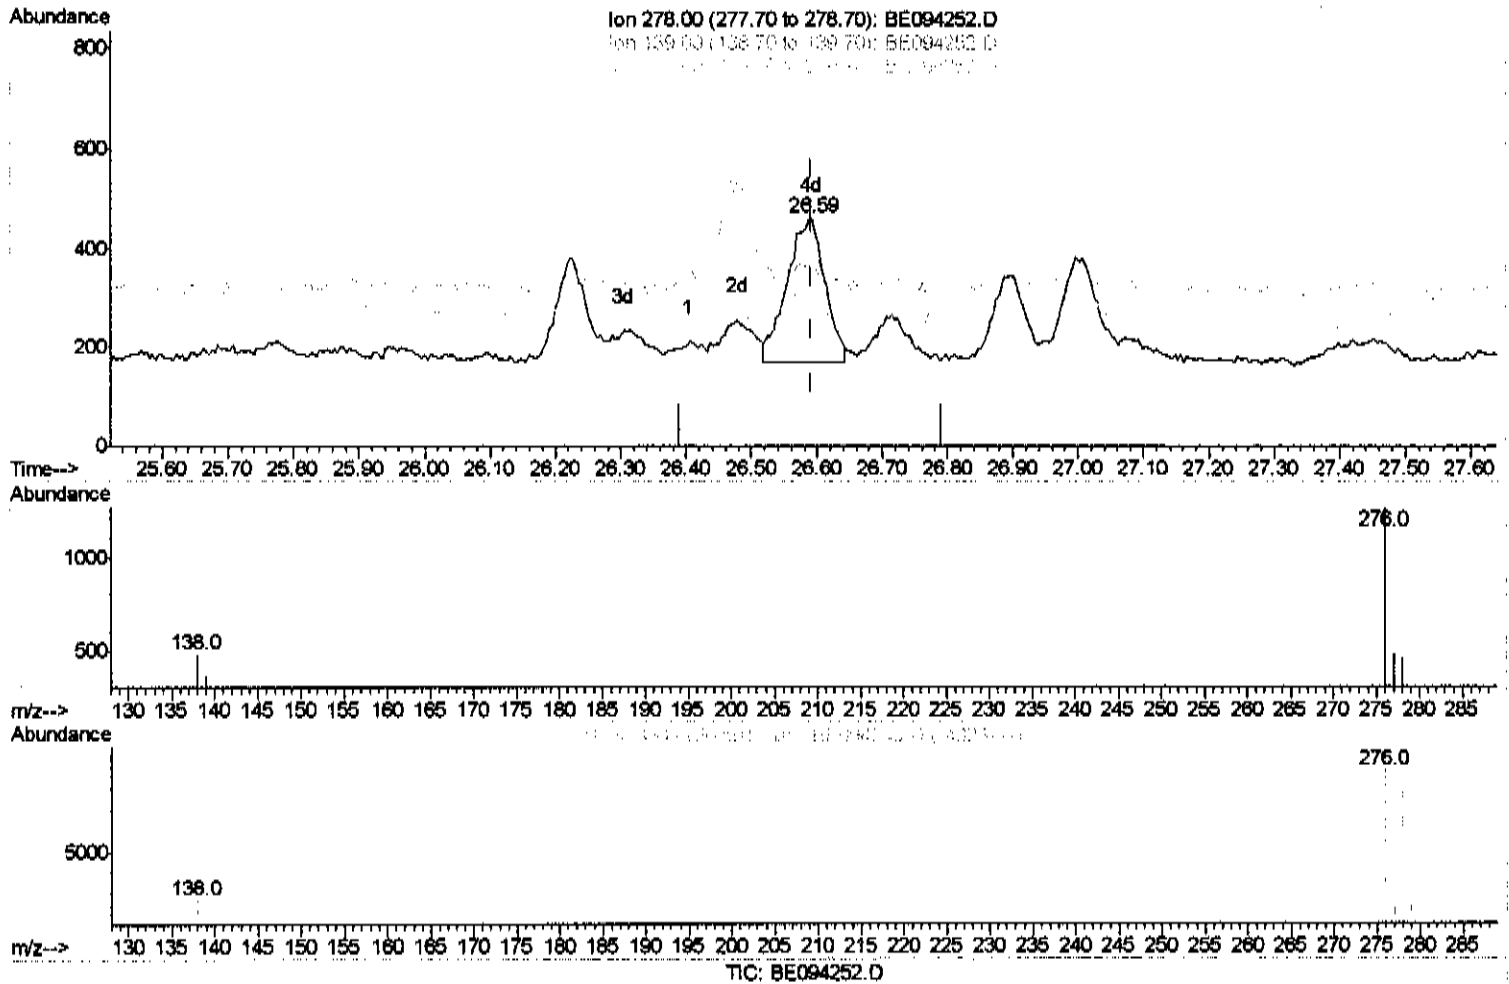

(25) Dibenzo(a,h)anthracene

26.591min (+0.000) 0.04ng/ul m

response 1178

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 278.00 | 100   | 100    |
| 139.00 | 21.70 | 80.26% |
| 279.00 | 32.40 | 65.73% |
| 0.00   | 0.00  | 0.00   |

# Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

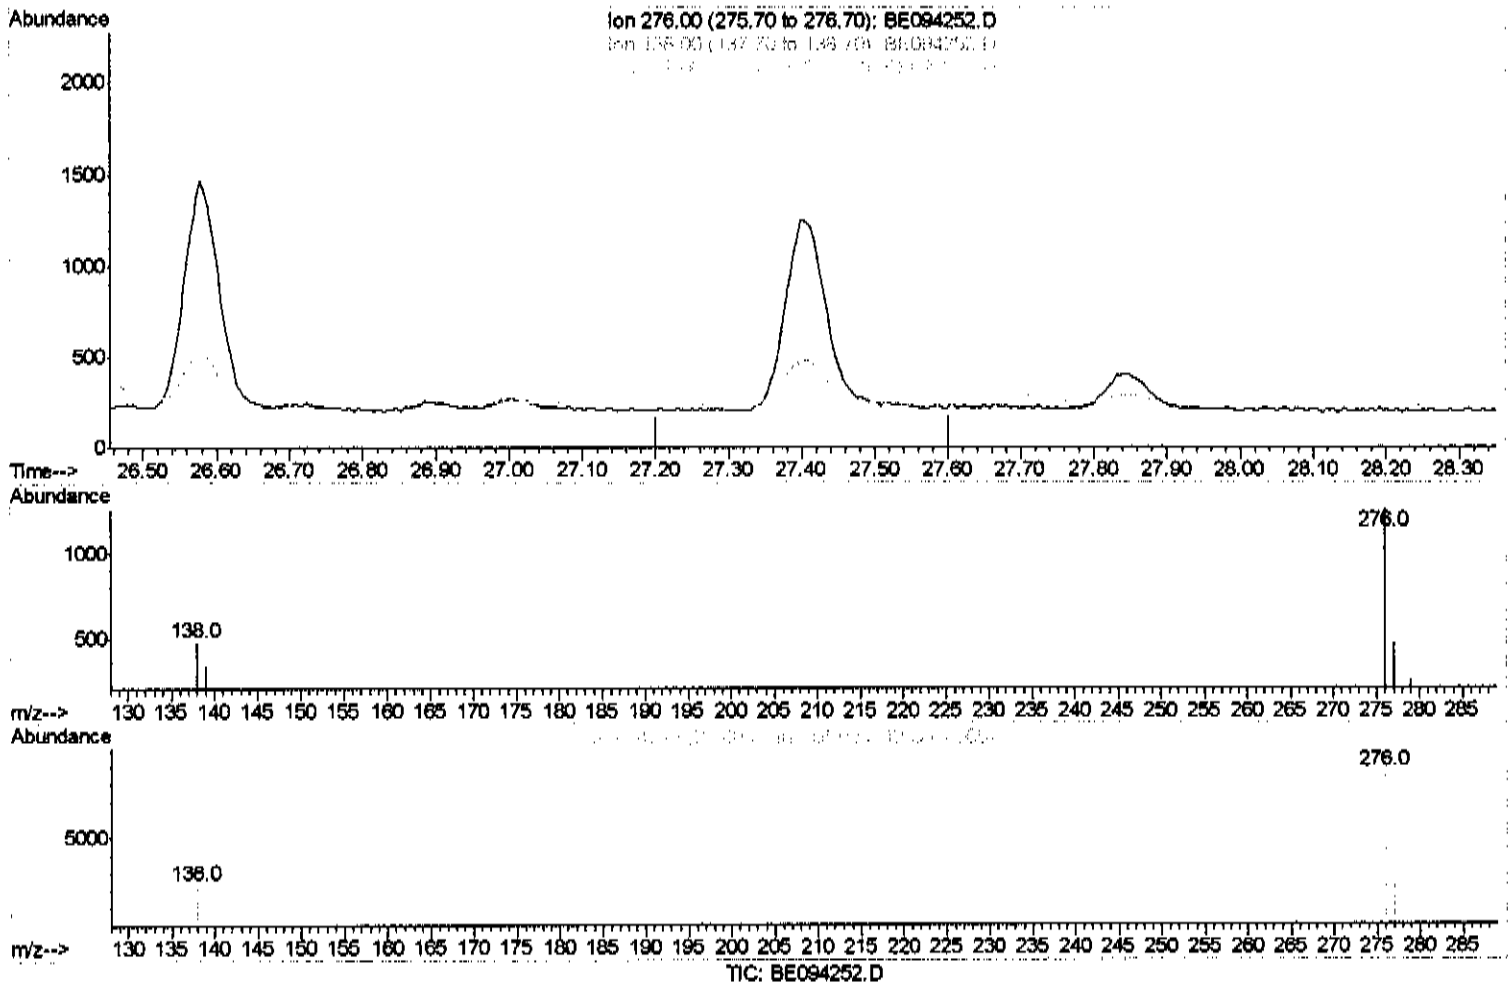

(26) Benzo(g,h,i)perylene

27.403min (-27.403) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 276.00 | 100   | 0.00  |
| 138.00 | 27.30 | 0.00# |
| 277.00 | 25.60 | 0.00# |
| 0.00   | 0.00  | 0.00  |

# Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
 Data File : BE094252.D  
 Acq On : 10 Oct 2017 13:42  
 Operator : SJ/JU  
 Sample : I5522-07  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampled :  
 C0AD6

Manual Integrations  
 APPROVED

Sohil  
 10/11/2017 7:19:41 PM

Quant Time: Oct 11 06:56:21 2017  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 11 06:34:16 2017  
 Response via : Initial Calibration

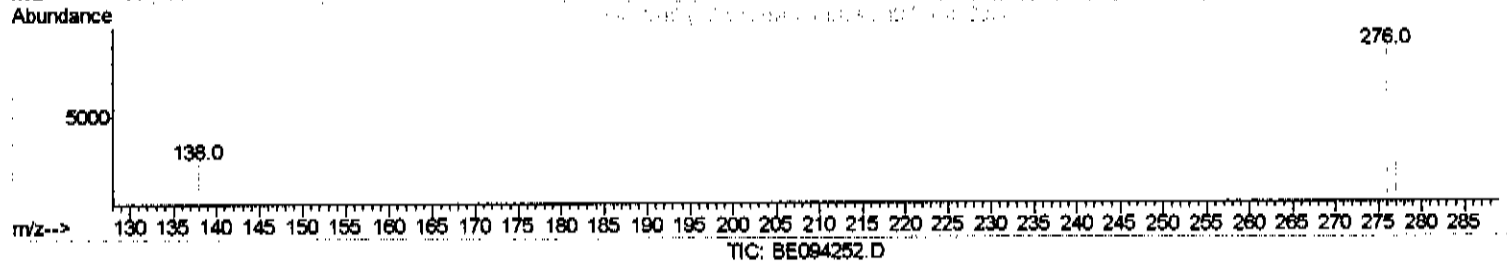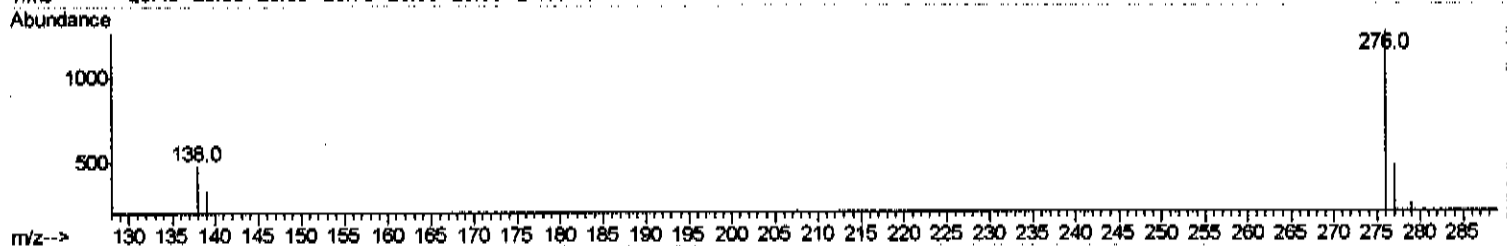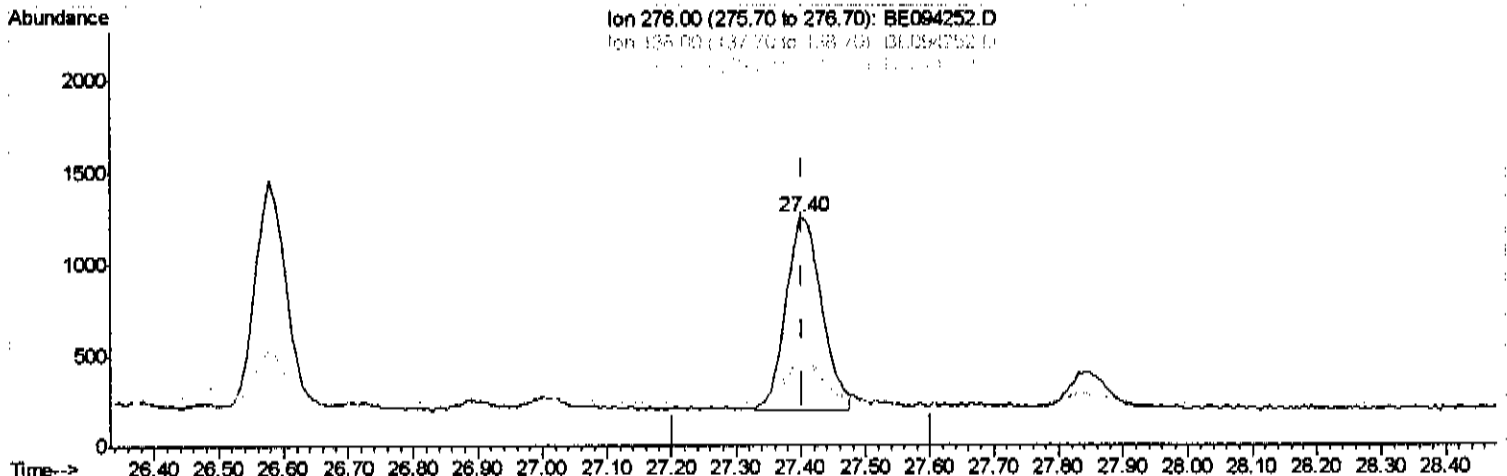

(26) Benzo(g,h,i)perylene

27.403min (+0.000) 0.14ng/ul m

response 4121

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 276.00 | 100   | 100    |
| 138.00 | 27.30 | 37.96# |
| 277.00 | 25.60 | 37.24# |
| 0.00   | 0.00  | 0.00   |

Quantitation Report (QT Reviewed)

Instrument :  
BNA\_E  
ClientSampleId :  
C0AD6

Manual Integrations  
APPROVED

Sohil  
10/11/2017 7:19:41 PM

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101017\  
Data File : BE094252.D  
Acq On : 10 Oct 2017 13:42  
Operator : SJ/JU  
Sample : I5522-07  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Oct 11 06:58:58 2017  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 11 06:34:16 2017  
Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.91  | 152  | 1796     | 0.40 | ng/ul | 0.00     |
| 2) Naphthalene-d8         | 10.69 | 136  | 9273     | 0.40 | ng/ul | 0.00     |
| 6) Acenaphthene-d10       | 14.51 | 164  | 5612     | 0.40 | ng/ul | 0.00     |
| 10) Phenanthrene-d10      | 17.24 | 188  | 11474m   | 0.40 | ng/ul | -0.02    |
| 16) Chrysene-d12          | 21.41 | 240  | 11550    | 0.40 | ng/ul | 0.00     |
| 20) Perylene-d12          | 23.92 | 264  | 11593m   | 0.40 | ng/ul | 0.00     |

JU 10/11/17  
JU 10/11/17

| System Monitoring Compounds | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|-----------------------------|-------|------|----------|------|-------|----------|
| 4) 2-Methylnaphthalene-d10  | 12.28 | 152  | 4205     | 0.29 | ng/ul | 0.00     |
| 14) Fluoranthene-d10        | 19.27 | 212  | 11024    | 0.29 | ng/ul | 0.00     |

| Target Compounds           | R.T.  | QIon | Response | Conc  | Units  | Ovalue |
|----------------------------|-------|------|----------|-------|--------|--------|
| 12) Phenanthrene           | 17.29 | 178  | 4057     | 0.135 | ng/ul  | 94     |
| 13) Anthracene             | 17.38 | 178  | 1155m    | 0.040 | ng/ul  | 85     |
| 15) Fluoranthene           | 19.30 | 202  | 11933    | 0.303 | ng/ul  | 83     |
| 17) Pyrene                 | 19.66 | 202  | 12209    | 0.380 | ng/ul# | 90     |
| 18) Benzo(a)anthracene     | 21.39 | 228  | 4988     | 0.163 | ng/ul# | 90     |
| 19) Chrysene               | 21.45 | 228  | 6597     | 0.186 | ng/ul# | 90     |
| 21) Benzo(b)fluoranthene   | 23.15 | 252  | 8573     | 0.272 | ng/ul  | 90     |
| 22) Benzo(k)fluoranthene   | 23.20 | 252  | 2944m    | 0.081 | ng/ul  |        |
| 23) Benzo(a)pyrene         | 23.81 | 252  | 5753m    | 0.176 | ng/ul  |        |
| 24) Indeno(1,2,3-cd)pyrene | 26.58 | 276  | 4166m    | 0.124 | ng/ul  |        |
| 25) Dibenzo(a,h)anthracene | 26.59 | 278  | 1178m    | 0.042 | ng/ul  |        |
| 26) Benzo(g,h,i)perylene   | 27.40 | 276  | 4121m    | 0.143 | ng/ul  |        |

JU 10/11/17  
JU 10/11/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed