

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101117\
 Data File : BE094282.D
 Acq On : 11 Oct 2017 16:46
 Operator : SJ/JU
 Sample : I5490-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 12 07:35:10 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 12 07:31:23 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1772	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	9130	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	5441	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.41	240	11267	0.40	ng/ul	0.00
20) Perylene-d12	23.76	264	735594	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	4295	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	10175	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
17) Pyrene	19.66	202	1484	0.047	ng/ul#	95
18) Benzo(a)anthracene	21.39	228	834	0.028	ng/ul#	60
19) Chrysene	21.44	228	943	0.027	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101117\
Data File : BE094282.D
Acq On : 11 Oct 2017 16:46
Operator : SJ/JU
Sample : I5490-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 12 07:35:10 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 07:31:23 2017
Response via : Initial Calibration




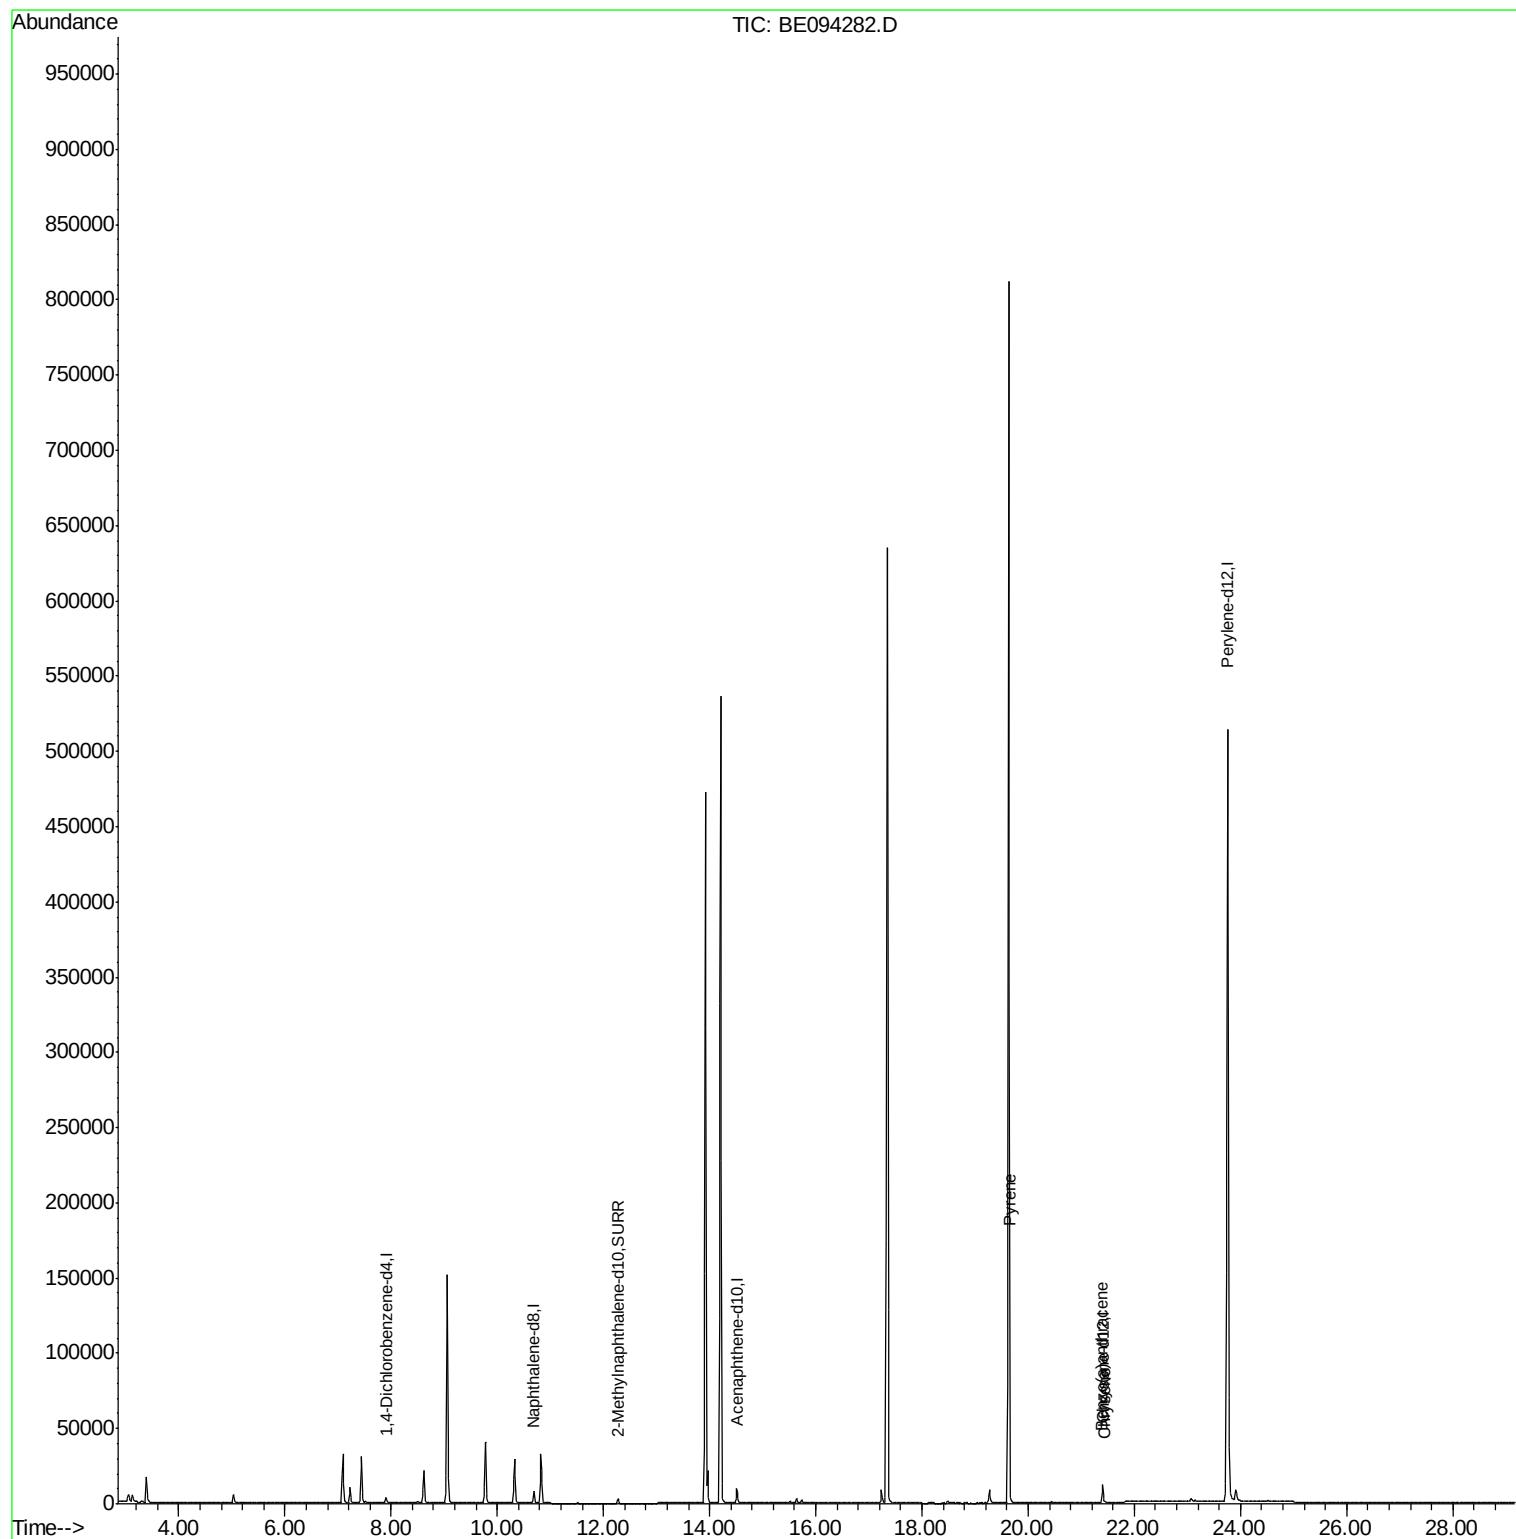


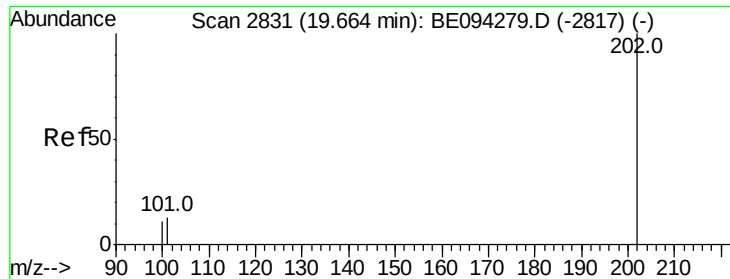

#17
Pvrene
Concen: 0.047 ng/ul
RT: 19.66 min Scan# 2829
Delta R.T. -0.01 min
Lab File: BE094282.D
Acq: 11 Oct 2017 16:46




Instrument :
BNA_E
ClientSampleId :




Tot Ion:202 Resp: 1484
Ion Ratio Lower Upper
202 100
101 22.2 18.2 27.4
100 23.8 15.6 23.4#

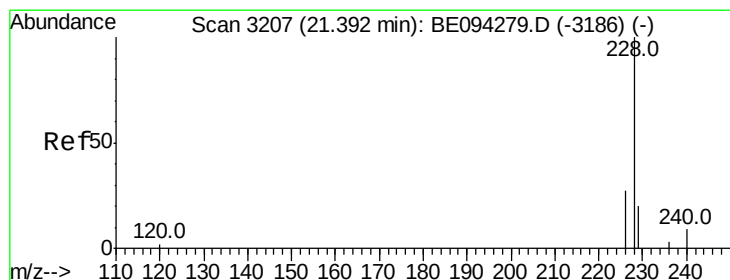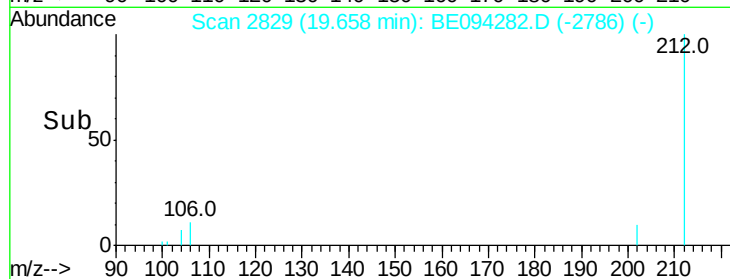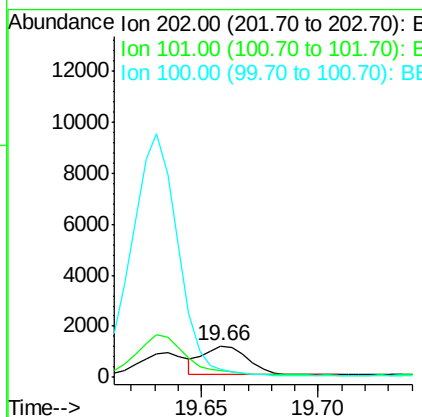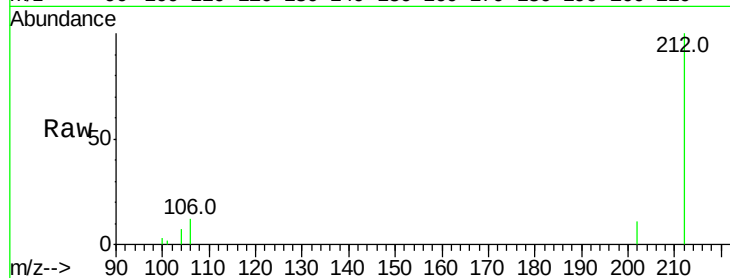

#18
Benzo(a)anthracene
Concen: 0.028 ng/ul
RT: 21.39 min Scan# 3206
Delta R.T. -0.00 min
Lab File: BE094282.D
Acq: 11 Oct 2017 16:46

Tgt Ion:228 Resp: 834
Ion Ratio Lower Upper
228 100
229 44.2 22.8 34.2#
226 46.6 17.0 25.6#

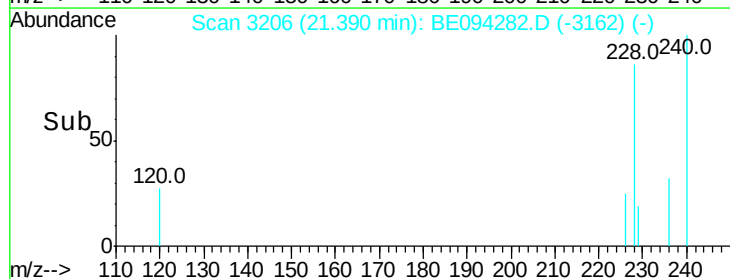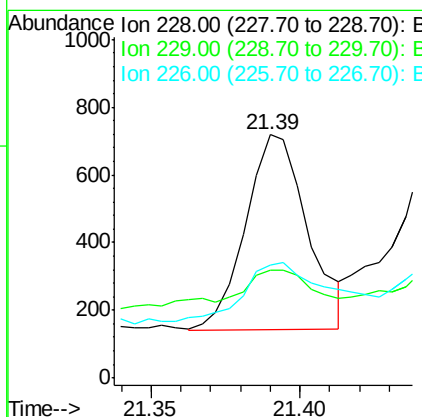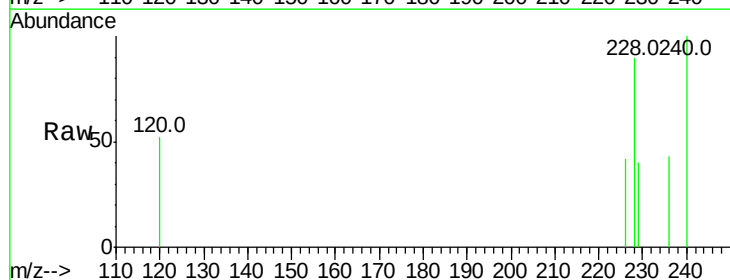

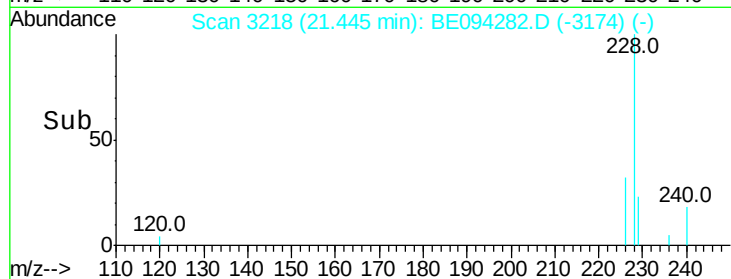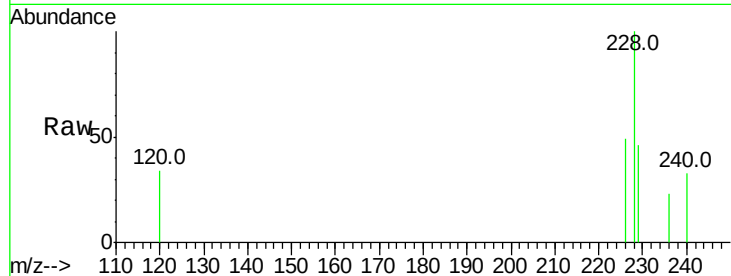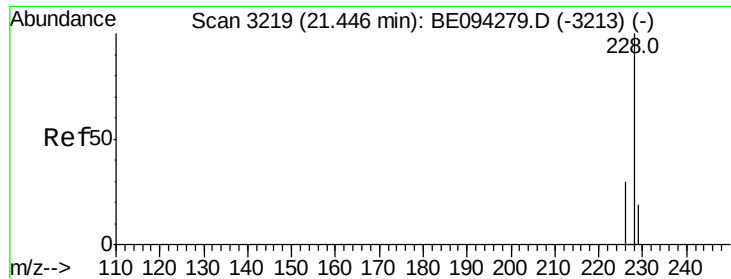

#19

Chrysene

Concen: 0.027 ng/ul

RT: 21.44 min Scan# 3218

Delta R.T. -0.00 min

Lab File: BE094282.D

Acq: 11 Oct 2017 16:46

Instrument :

BNA_E

ClientSampleId :

Tot Ion:228 Resp: 943

Ion Ratio Lower Upper

228 100

226 48.6 23.4 35.0#

229 45.5 17.7 26.5#

