




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101117\
Data File : BE094301.D
Acq On : 12 Oct 2017 4:27
Operator : SJ/JU
Sample : PB102872BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK72

Manual Integrations
APPROVED

Sohil
10/13/2017 12:06:06 PM

Quant Time: Oct 12 08:58:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 08:55:52 2017
Response via : Initial Calibration

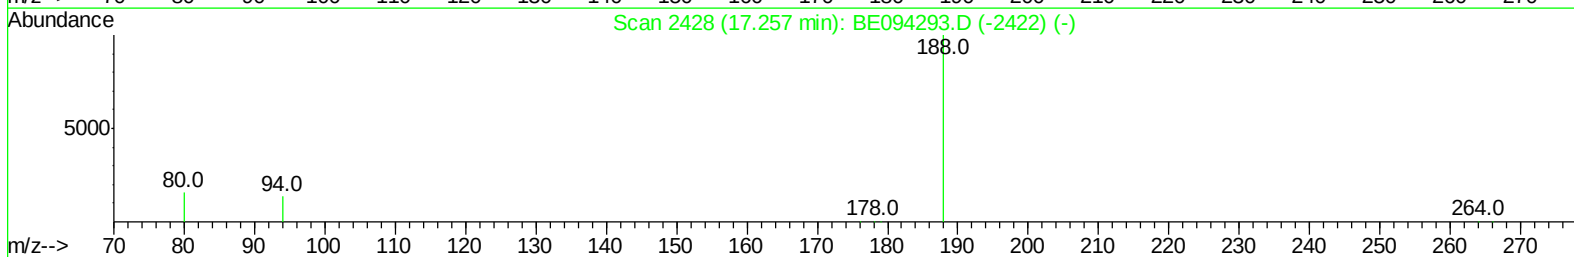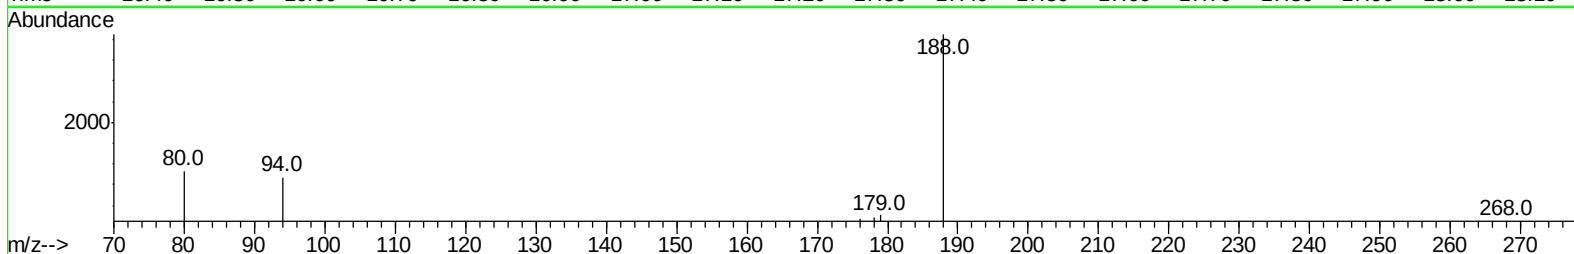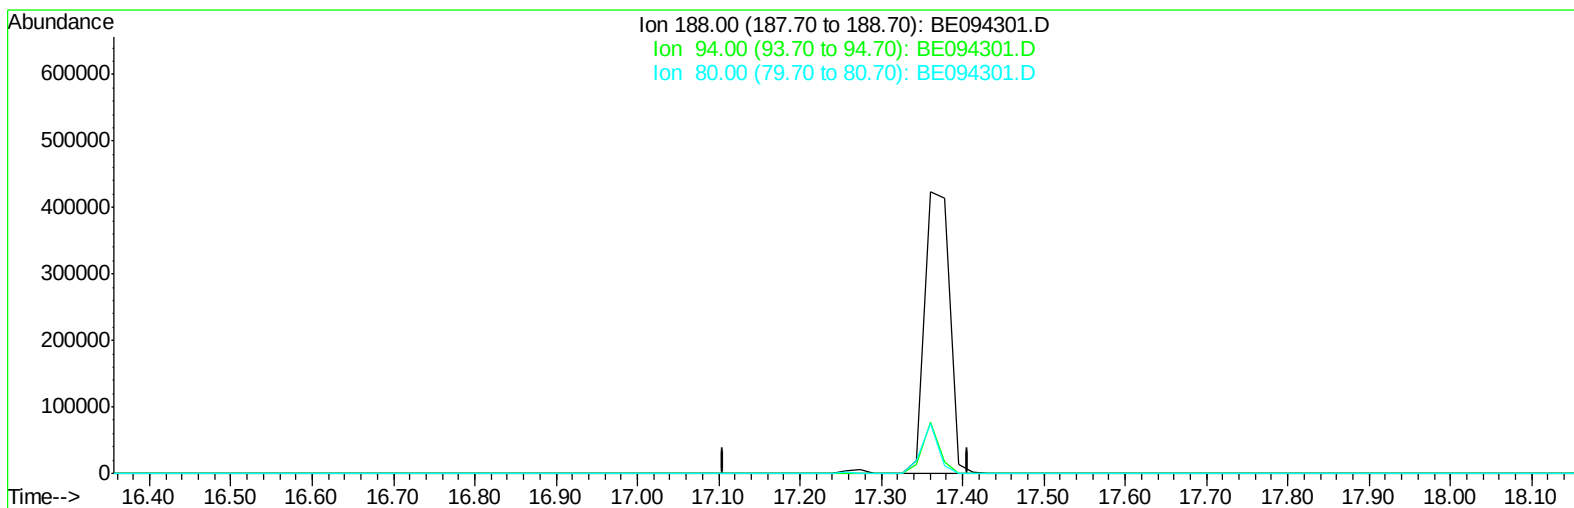

TIC: BE094301.D

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101117\
Data File : BE094301.D
Acq On : 12 Oct 2017 4:27
Operator : SJ/JU
Sample : PB102872BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK72

Manual Integrations
APPROVED

Sohil
10/13/2017 12:06:06 PM

Quant Time: Oct 12 08:58:57 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 08:55:52 2017
Response via : Initial Calibration

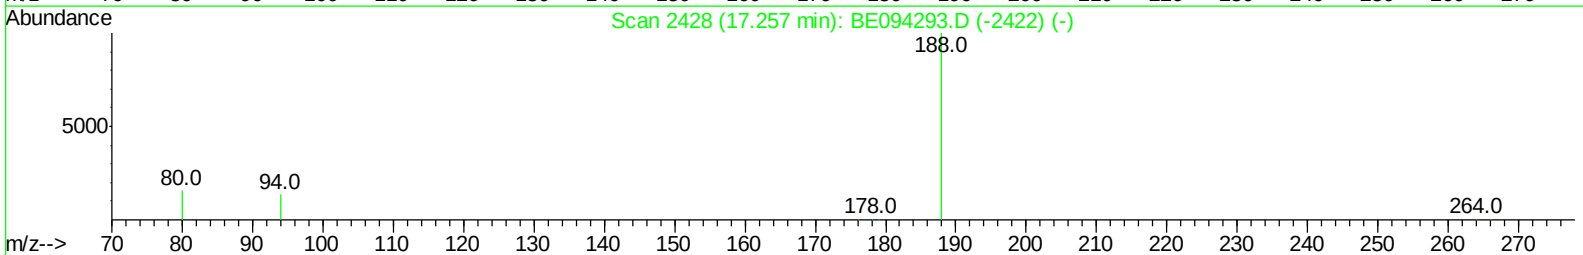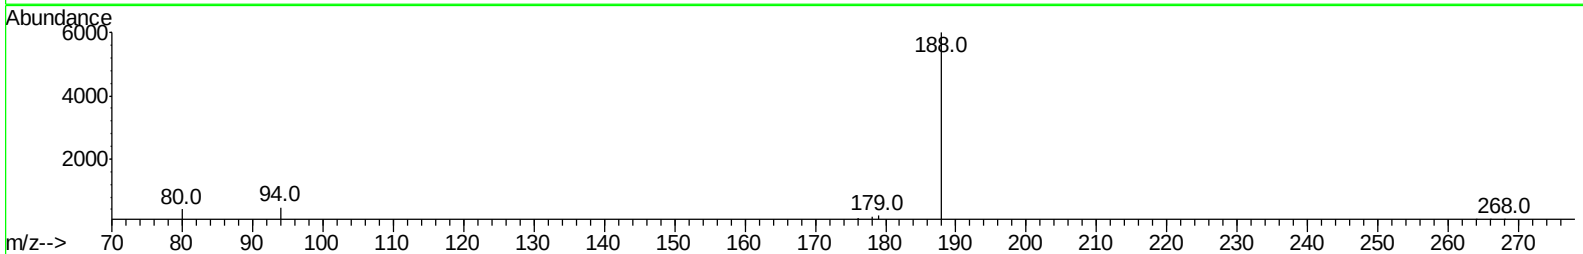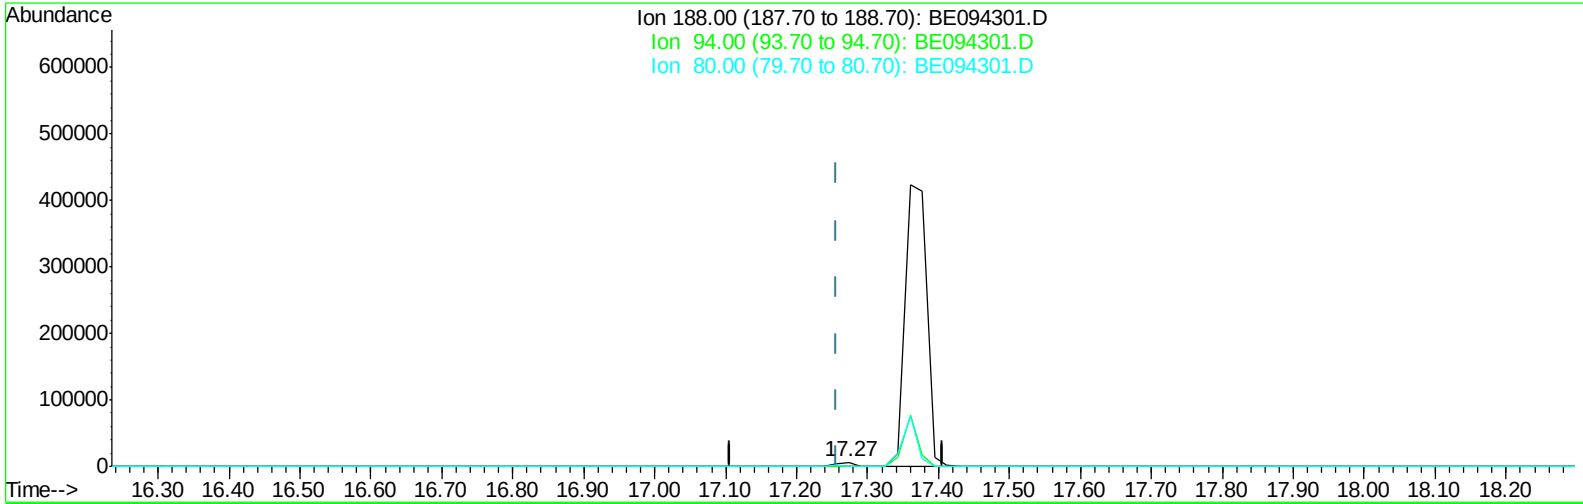

TIC: BE094301.D

(10) Phenanthrene-d10 (I)

17.273min (+0.017) 0.40ng/ul m

response 10684

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.84#
80.00	11.80	6.87#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101117\
Data File : BE094301.D
Acq On : 12 Oct 2017 4:27
Operator : SJ/JU
Sample : PB102872BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK72

Manual Integrations
APPROVED

Sohil
10/13/2017 12:06:06 PM

Quant Time: Oct 12 09:30:14 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 08:55:52 2017
Response via : Initial Calibration

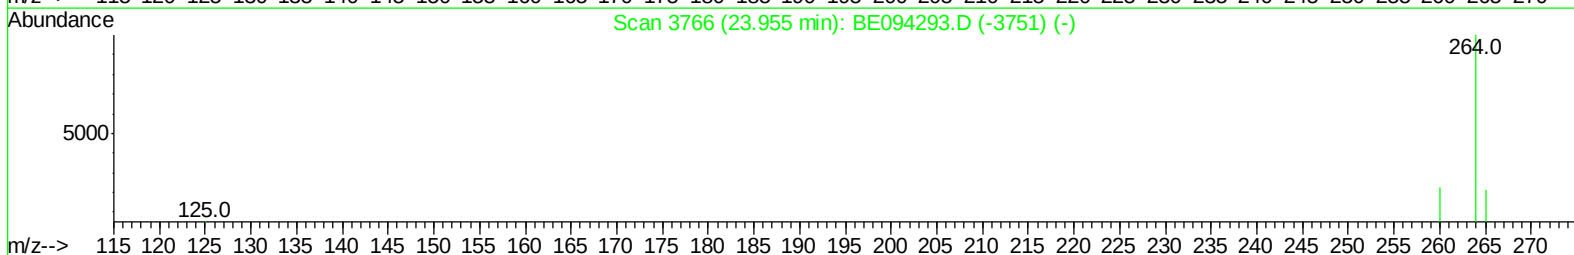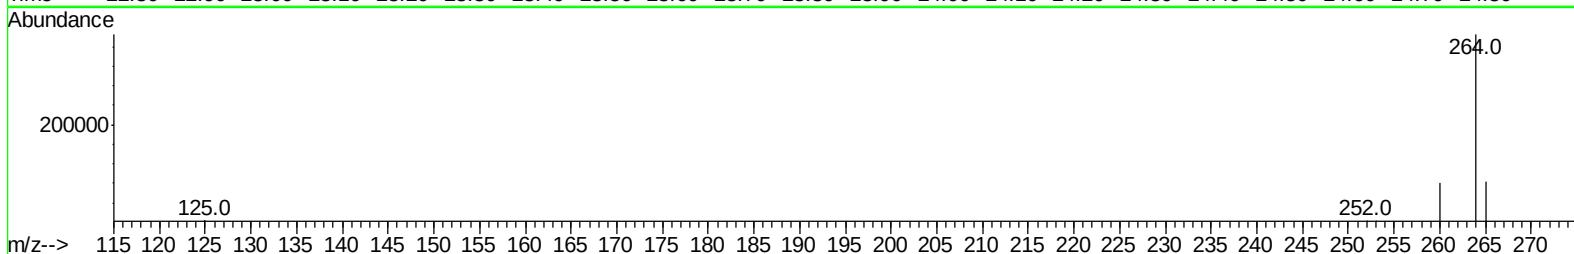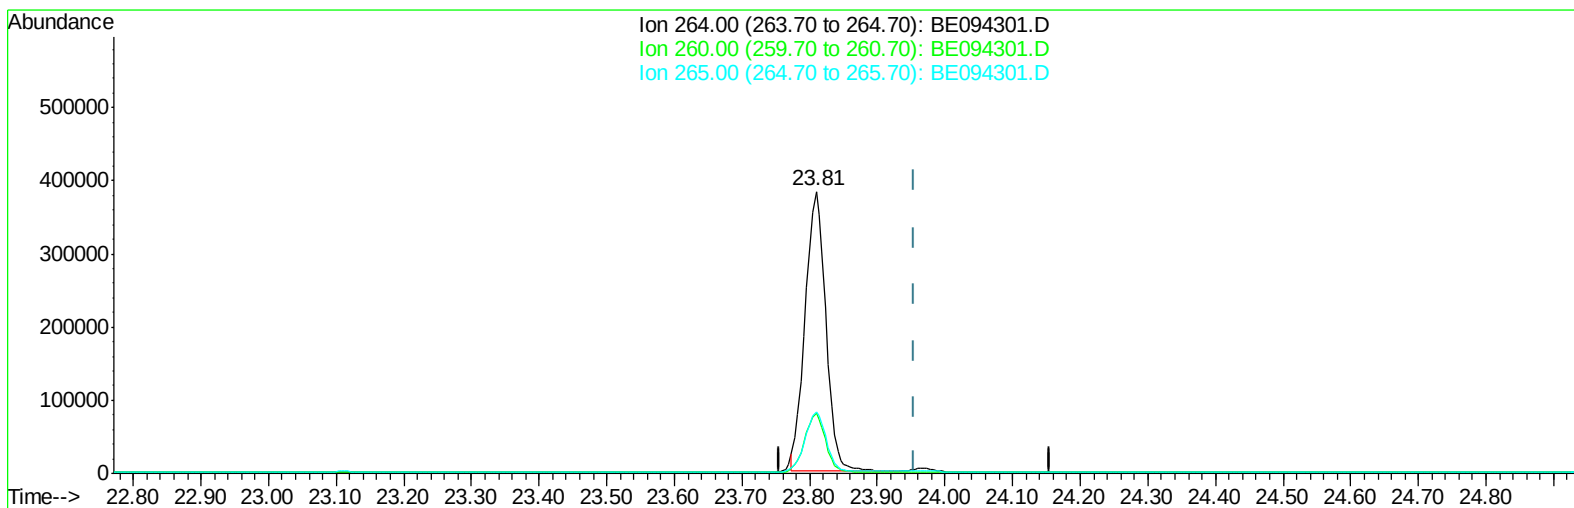

TIC: BE094301.D

(20) Perylene-d12 (I)

23.810min (-0.146) 0.40ng/ul

response 810159

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.18#
265.00	103.50	21.81#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE101117\
Data File : BE094301.D
Acq On : 12 Oct 2017 4:27
Operator : SJ/JU
Sample : PB102872BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK72

Manual Integrations
APPROVED

Sohil
10/13/2017 12:06:06 PM

Quant Time: Oct 12 09:30:14 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 08:55:52 2017
Response via : Initial Calibration

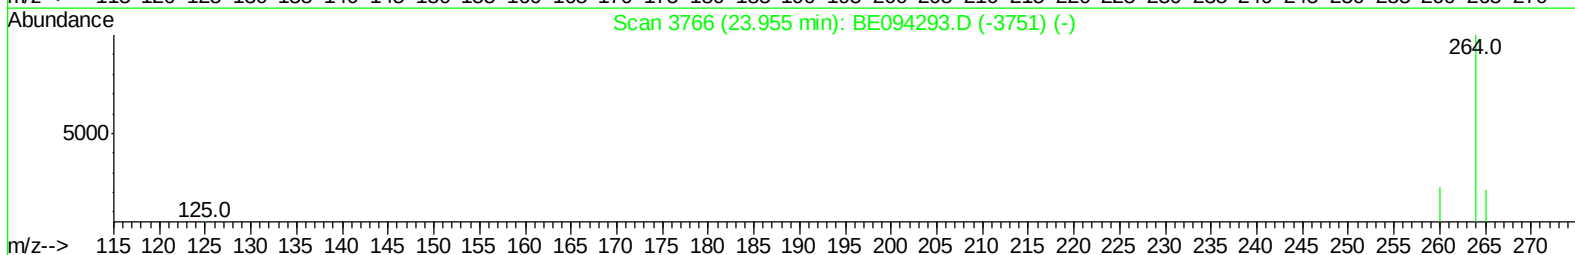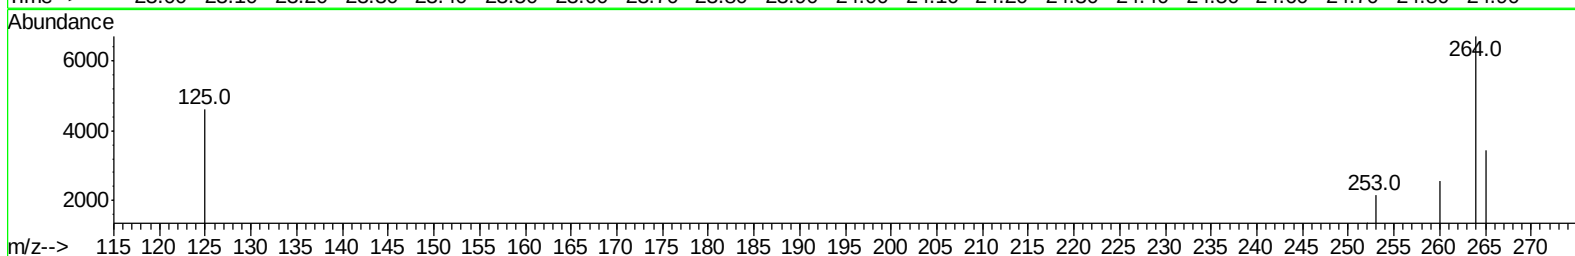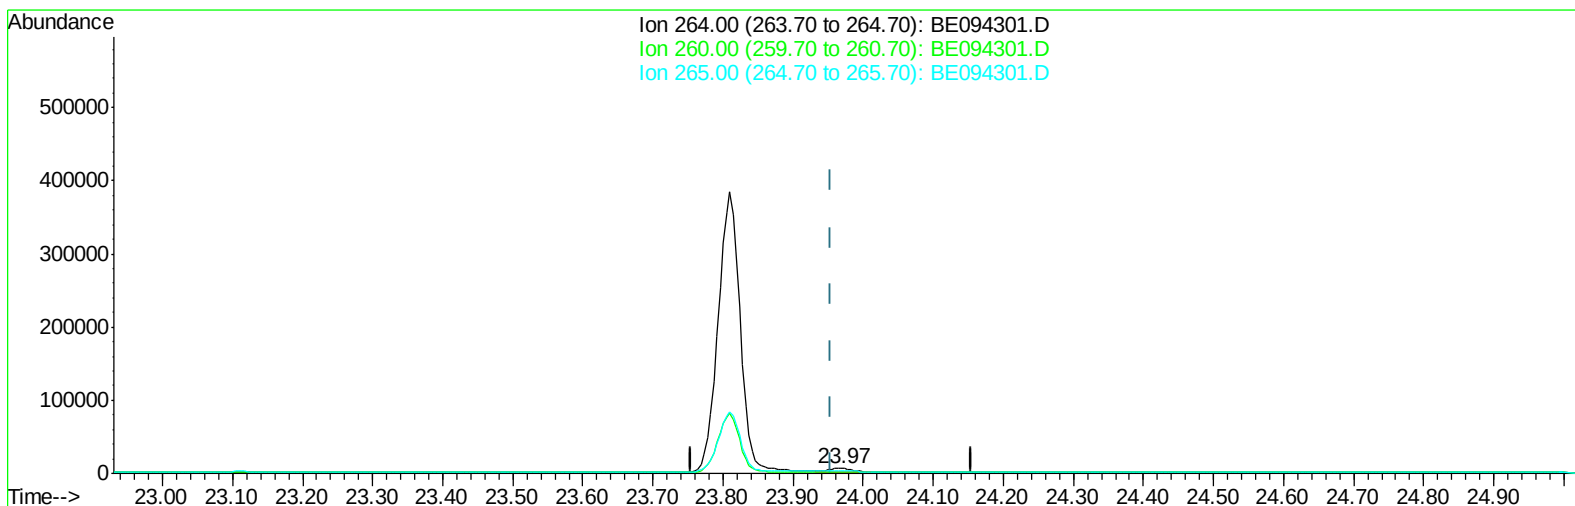

TIC: BE094301.D

(20) Perylene-d12 (I)

23.969min (+0.013) 0.40ng/ul m

response 12781

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	38.22#
265.00	103.50	51.40#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101117\
 Data File : BE094301.D
 Acq On : 12 Oct 2017 4:27
 Operator : SJ/JU
 Sample : PB102872BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK72

Manual Integrations
 APPROVED

Sohil
 10/13/2017 12:06:06 PM

Quant Time: Oct 12 09:31:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 12 08:55:52 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	1826	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	9117	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	5277	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.27	188	10684m	0.40	ng/ul	0.02
16) Chrysene-d12	21.44	240	10213	0.40	ng/ul	0.00
20) Perylene-d12	23.97	264	12781m	0.40	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	5324	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	11694	0.33	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101117\
Data File : BE094301.D
Acq On : 12 Oct 2017 4:27
Operator : SJ/JU
Sample : PB102872BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK72

Manual Integrations
APPROVED

Sohil
10/13/2017 12:06:06 PM

Quant Time: Oct 12 09:31:24 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 08:55:52 2017
Response via : Initial Calibration

