

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101215\
 Data File : BE091005.D
 Acq On : 12 Oct 2015 21:43
 Operator : UM/IZ
 Sample : SSTD3.272
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTD3.272

Quant Time: Oct 13 07:19:37 2015
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE101215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 13 07:04:09 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	4220	0.40	ng/ul	0.00
2) Naphthalene-d8	9.63	136	20148	0.40	ng/ul	0.00
6) Acenaphthene-d10	13.45	164	10467	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.17	188	25667	0.40	ng/ul	0.00
16) Chrysene-d12	20.32	240	32779	0.40	ng/ul	0.00
20) Perylene-d12	22.24	264	32173	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul	
14) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
11) Pentachlorophenol	15.93	266	12666	6.63	ng/ul	Ovalue 91




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE101215\
Data File : BE091005.D
Acq On : 12 Oct 2015 21:43
Operator : UM/IZ
Sample : SSTD3.272
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTD3.272

Quant Time: Oct 13 07:19:37 2015
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM02.2-EPA-SIM-BE101215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 13 07:04:09 2015
Response via : Initial Calibration

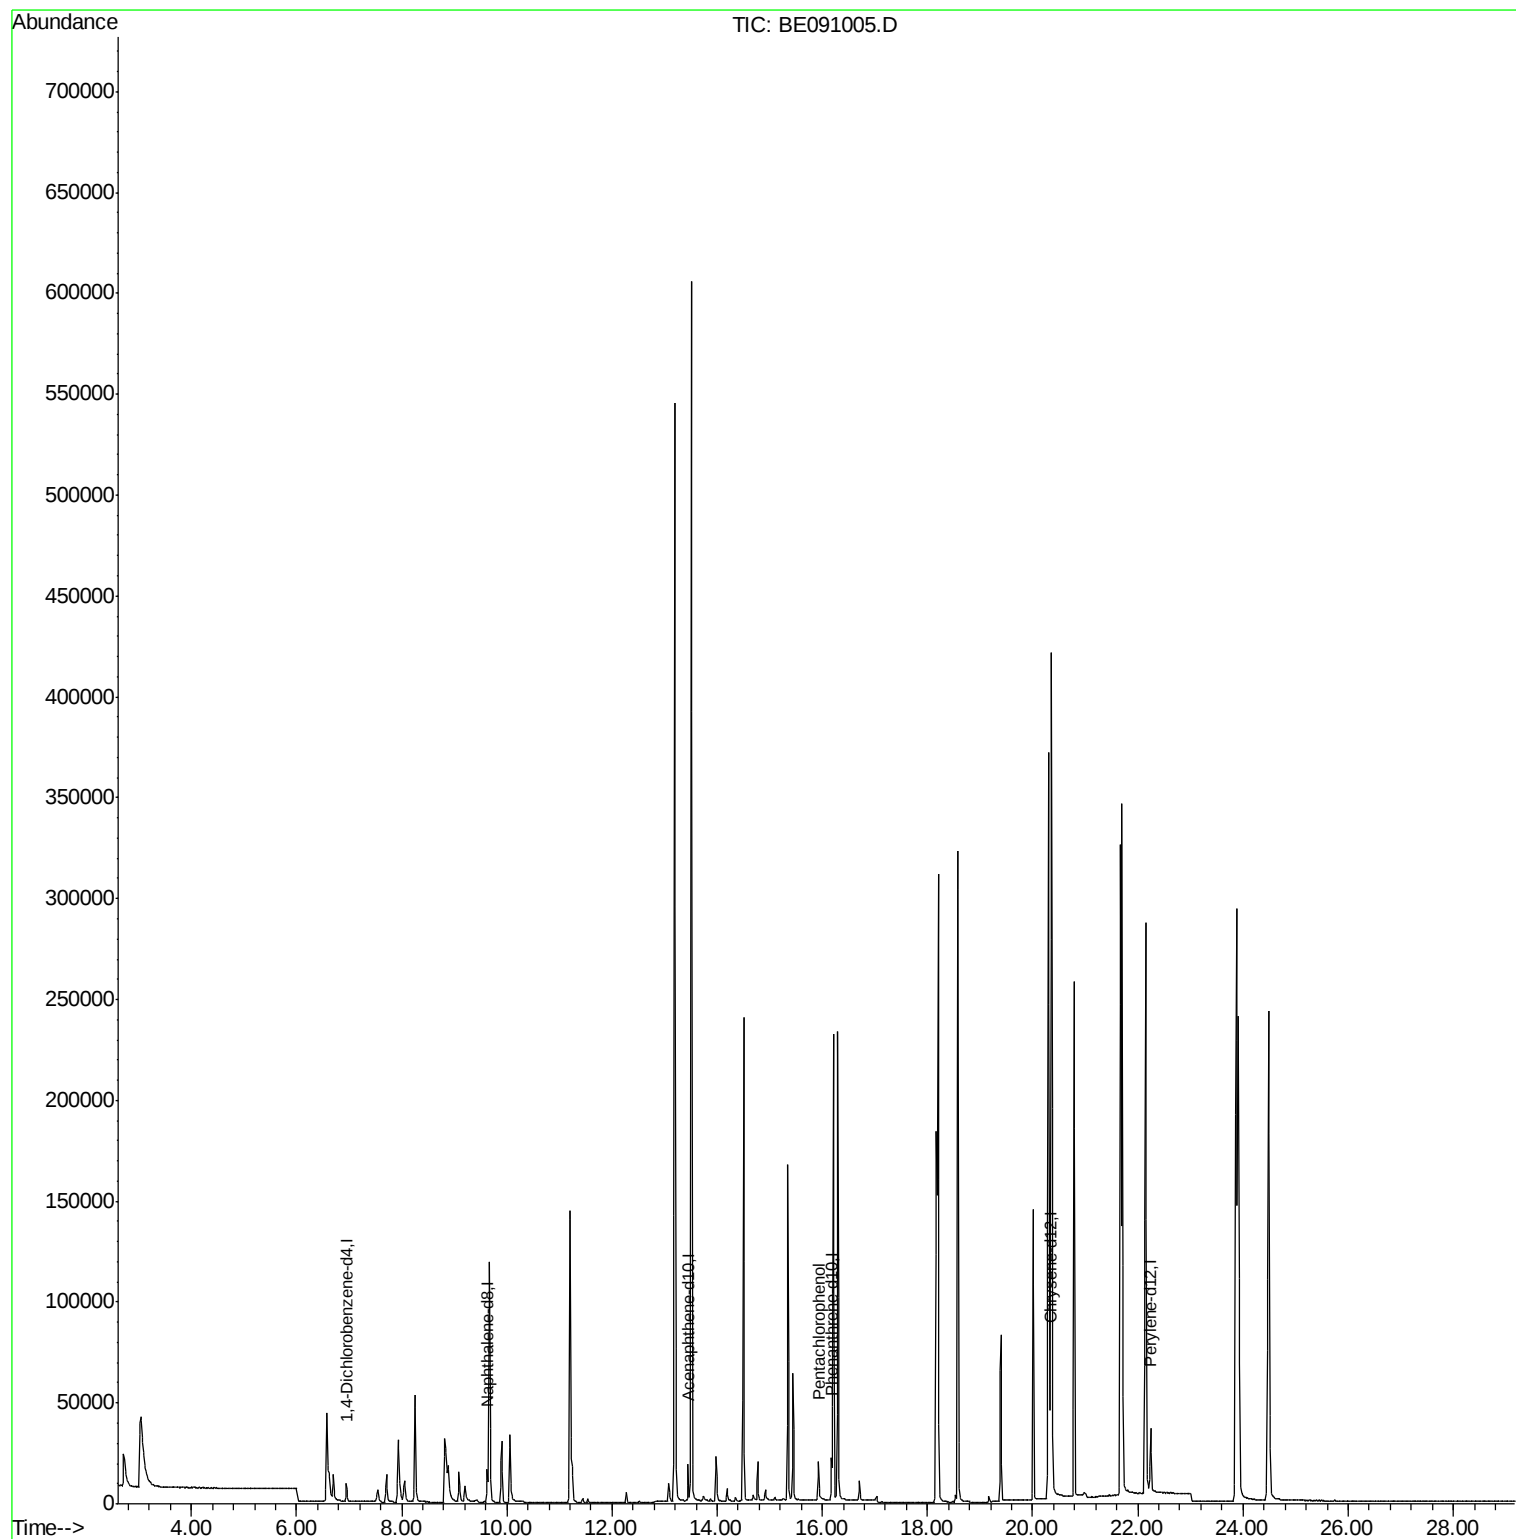

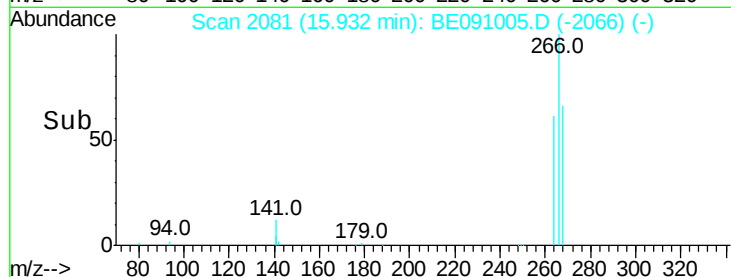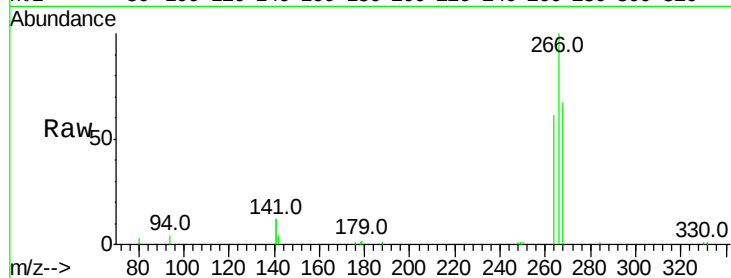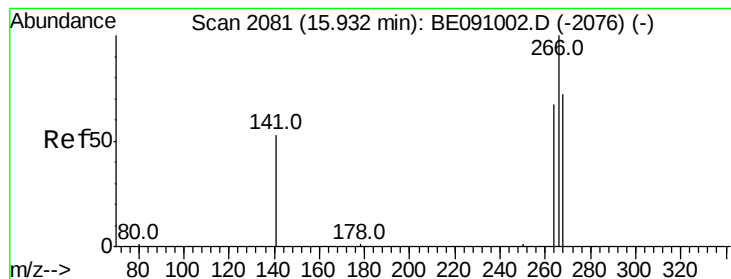

#11

Pentachlorophenol

Concen: 6.63 ng/ul

RT: 15.93 min Scan# 2081

Delta R.T. -0.00 min

Lab File: BE091005.D

Acq: 12 Oct 2015 21:43

Instrument :

BNA_E

ClientSampleId :

SSTD3.272

Tot Ion:266 Resp: 12666

Ion Ratio Lower Upper

266 100

264 62.2 56.5 84.7

268 64.5 56.6 84.8

