
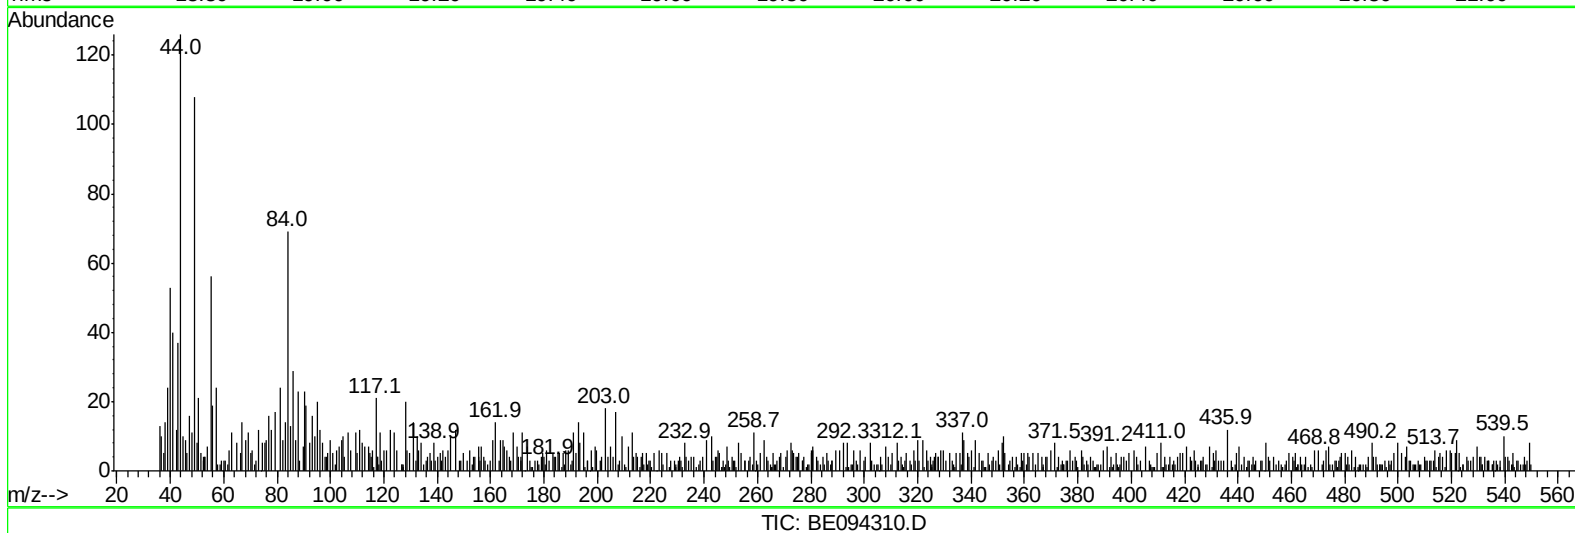


Data Path : Z:\HPCHEM1\BNA E\Data\BE101217\
 Data File : BE094310.D
 Acq On : 12 Oct 2017 11:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 23:57:31 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 11 16:25:21 2017
 Response via : Initial Calibration

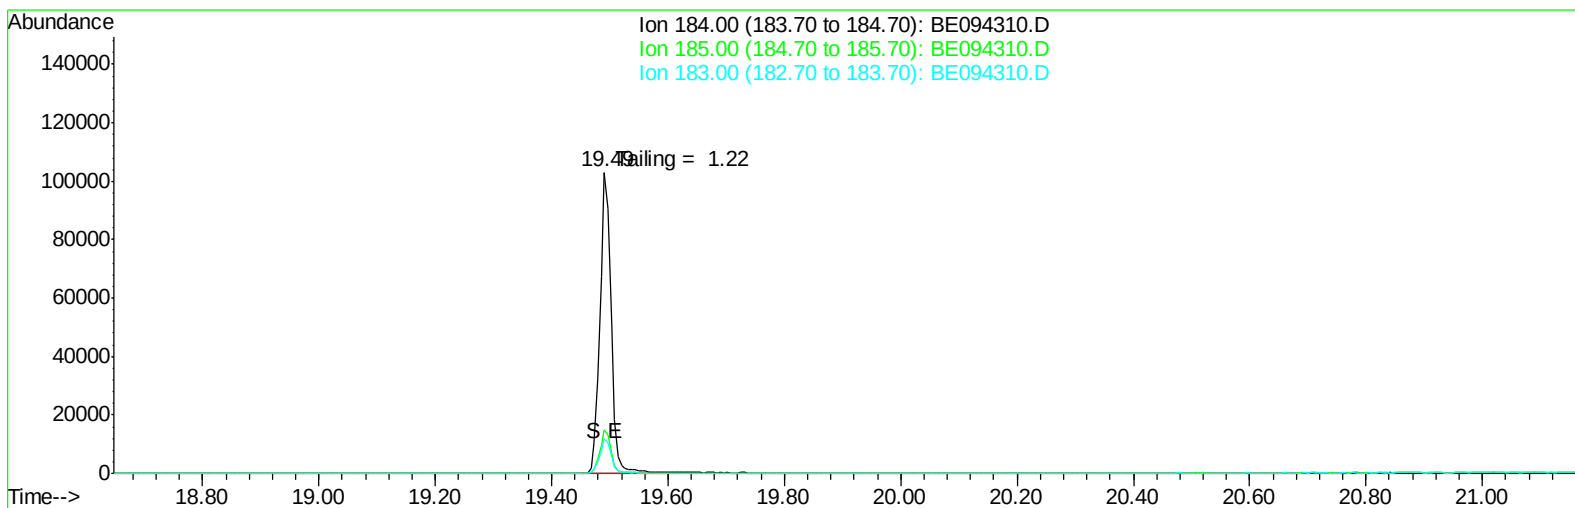

TIC: BE094310.D

(76) Benzidine



12.693min (-0.017) 15.02ng

response 5

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	62.50#
183.00	11.60	62.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE101217\
Data File : BE094310.D
Acq On : 12 Oct 2017 11:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 23:57:31 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

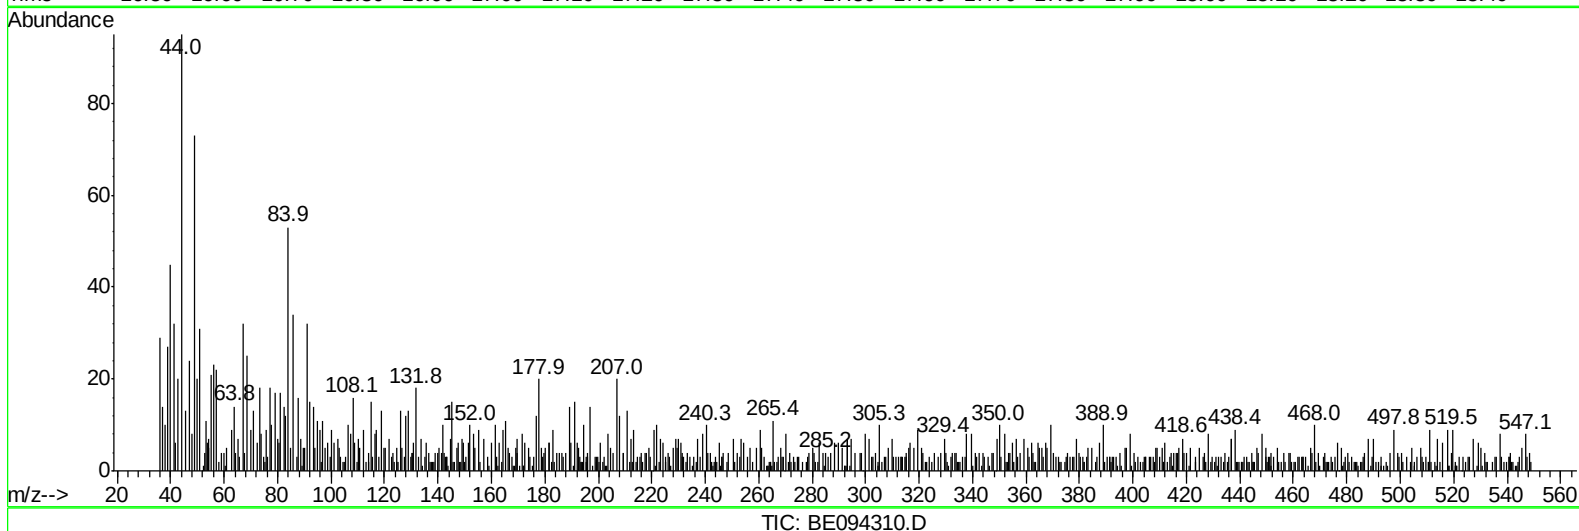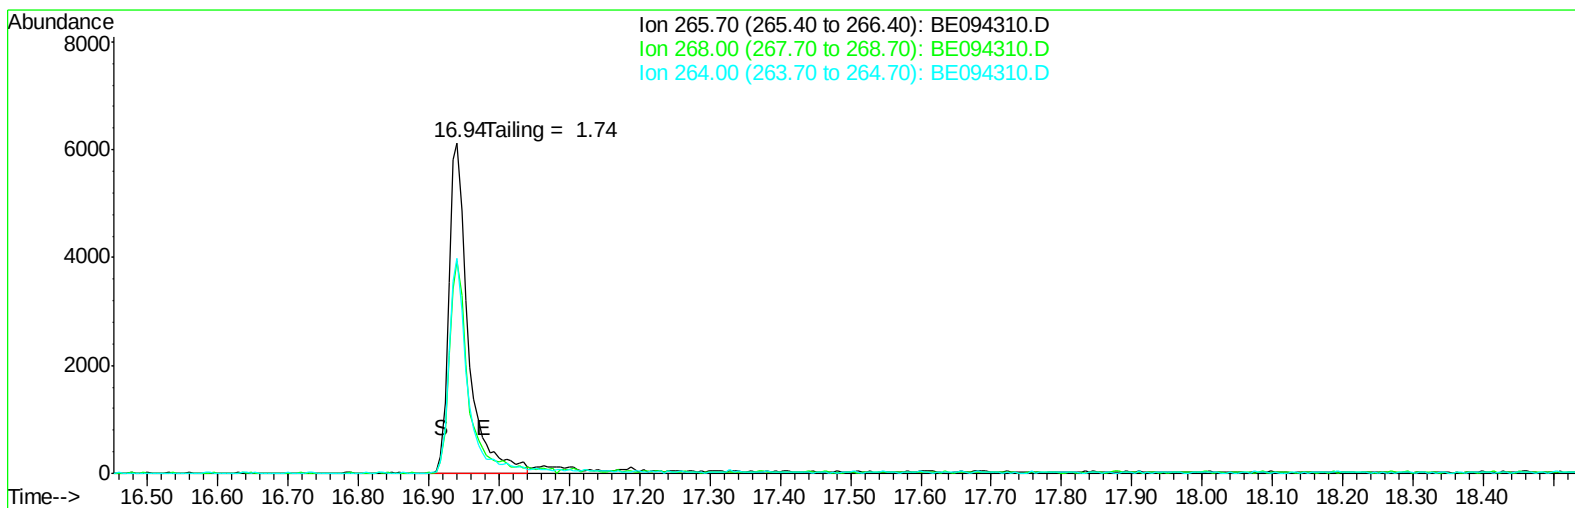

(69) Pentachlorophenol (C)

11.430min (+0.249) 43.03ng

response 7

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.54
264.00	61.90	53.85
0.00	0.00	0.00