

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
 Data File : BE094321.D
 Acq On : 13 Oct 2017 12:41
 Operator : SJ/JU
 Sample : PB102983BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 14 02:18:01 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 02:15:10 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1252	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	5862	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	3690	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.43	240	10740	0.40	ng/ul	0.00
20) Perylene-d12	23.80	264	643440	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	2711	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	8359	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.52	166	839	0.060	ng/ul#	21
17) Pyrene	19.65	202	1314	0.044	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094321.D
Acq On : 13 Oct 2017 12:41
Operator : SJ/JU
Sample : PB102983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 14 02:18:01 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:15:10 2017
Response via : Initial Calibration

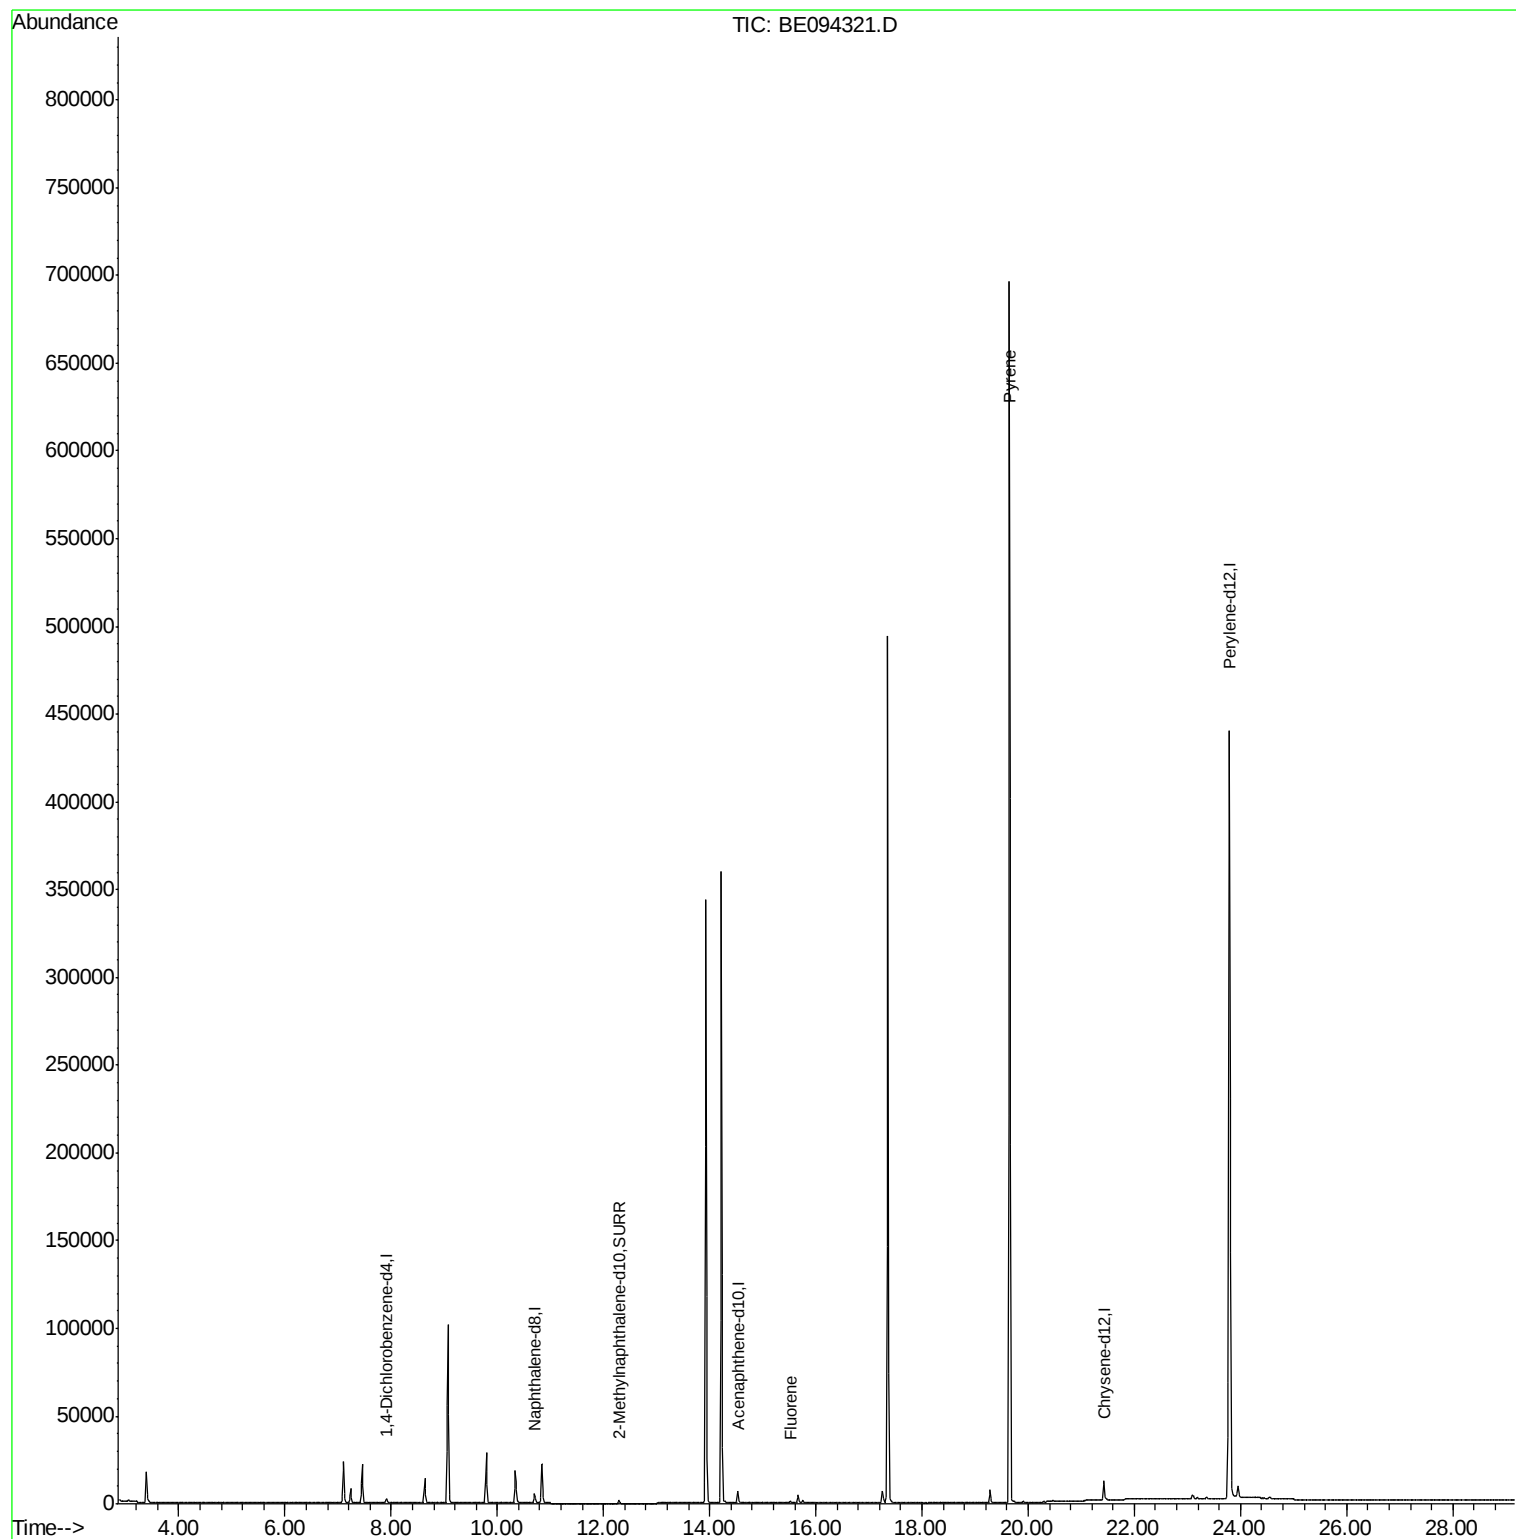

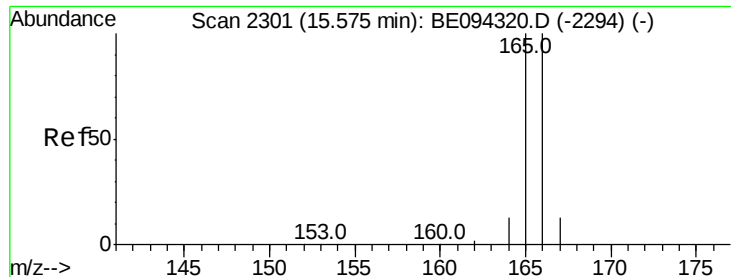

#9

Fluorene

Concen: 0.060 ng/ul

RT: 15.52 min Scan# 2294

Delta R.T. -0.05 min

Lab File: BE094321.D

Acq: 13 Oct 2017 12:41

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 839

Ion Ratio Lower Upper

166 100

165 14.8 73.4 110.2#

167 48.3 14.6 22.0#

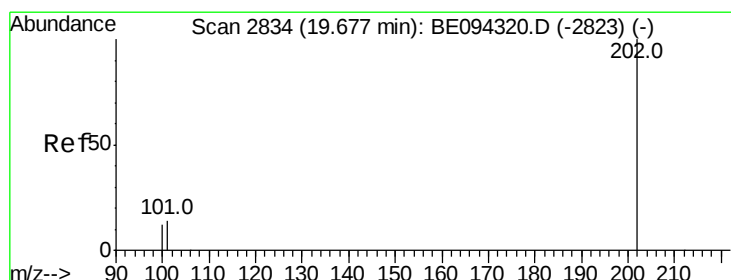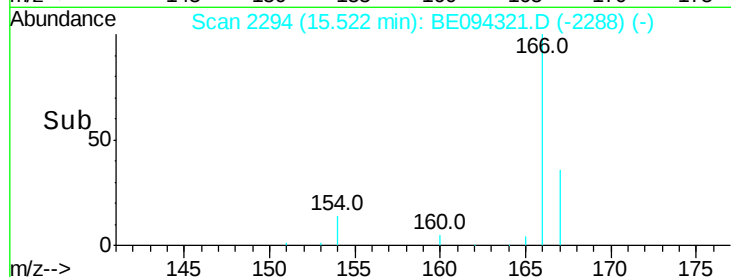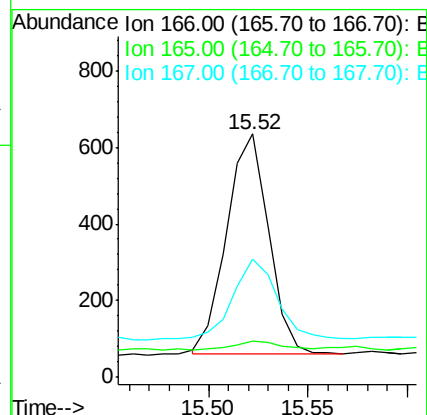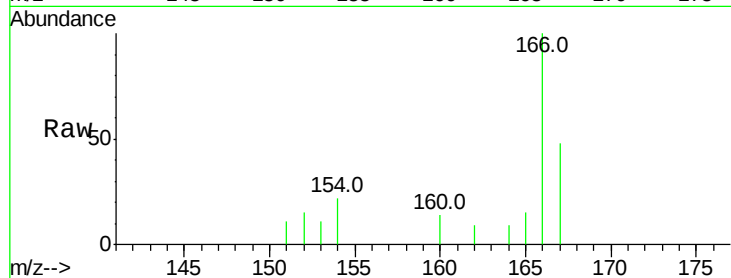

#17

Pyrene

Concen: 0.044 ng/ul

RT: 19.65 min Scan# 2828

Delta R.T. -0.03 min

Lab File: BE094321.D

Acq: 13 Oct 2017 12:41

Tgt Ion:202 Resp: 1314

Ion Ratio Lower Upper

202 100

101 155.1 18.2 27.4#

100 852.4 15.6 23.4#

