




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094321.D
Acq On : 13 Oct 2017 12:41
Operator : SJ/JU
Sample : PB102983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK83

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:34 PM

Quant Time: Oct 14 02:18:01 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:15:10 2017
Response via : Initial Calibration

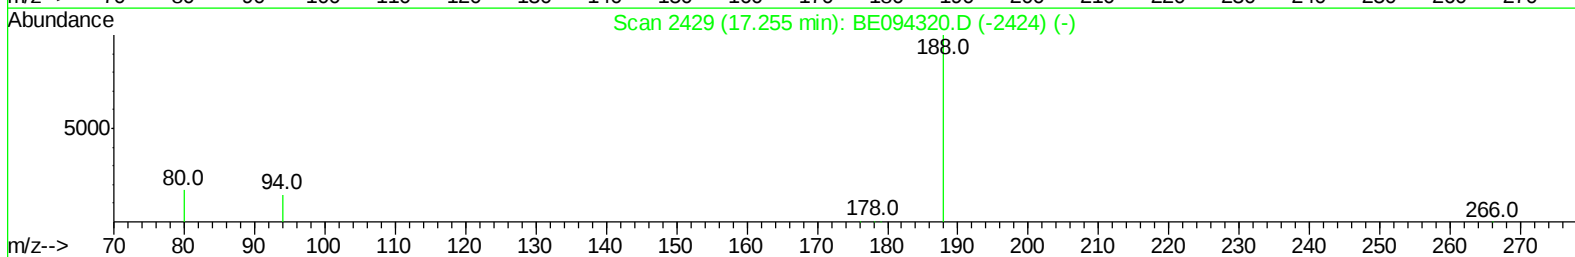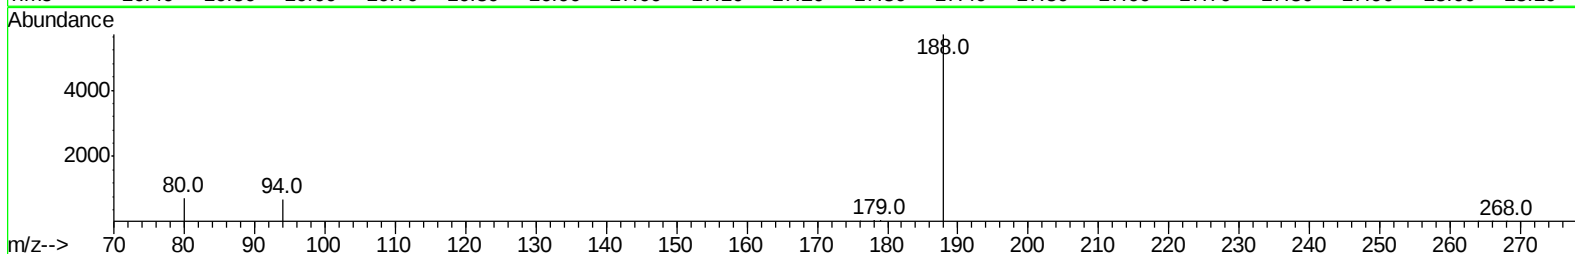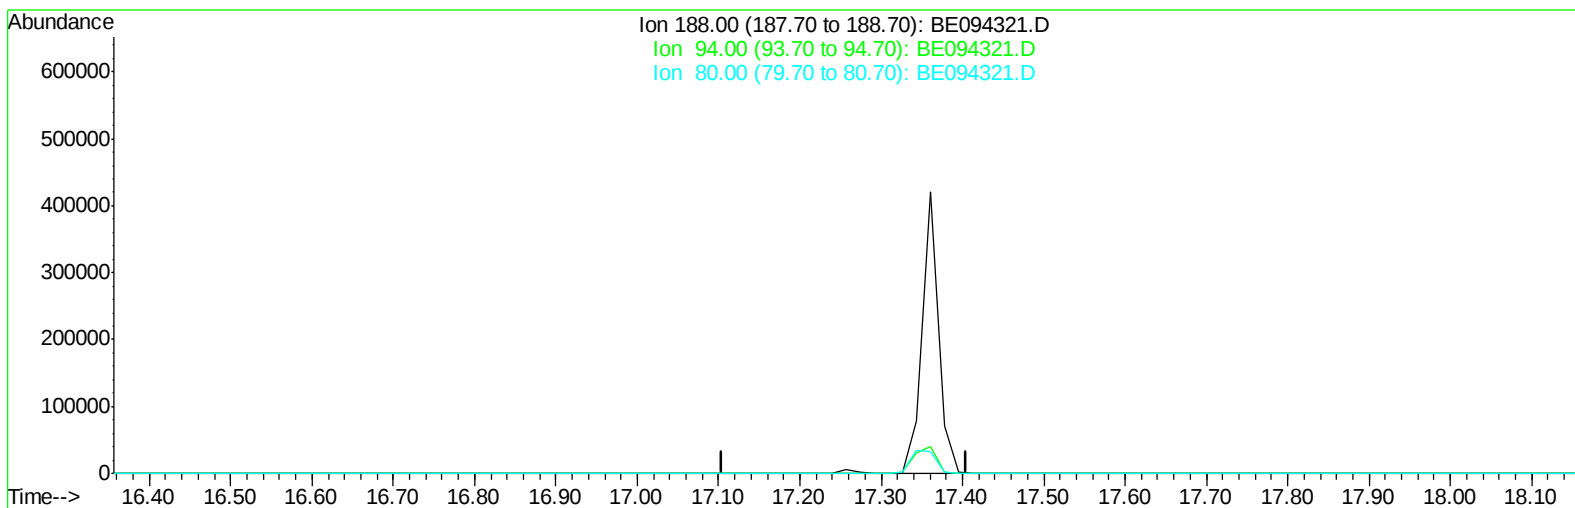

TIC: BE094321.D

(10) Phenanthrene-d10 (I)

17.255min (-17.255) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094321.D
Acq On : 13 Oct 2017 12:41
Operator : SJ/JU
Sample : PB102983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK83

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:34 PM

Quant Time: Oct 14 02:18:01 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:15:10 2017
Response via : Initial Calibration

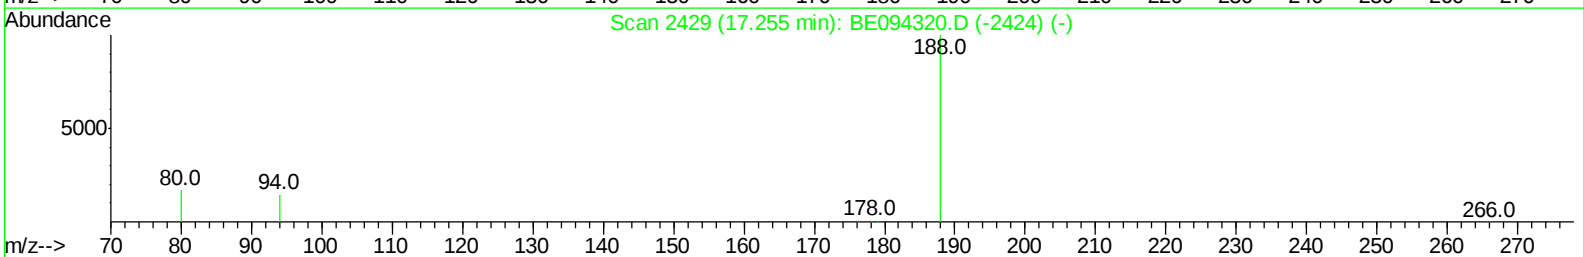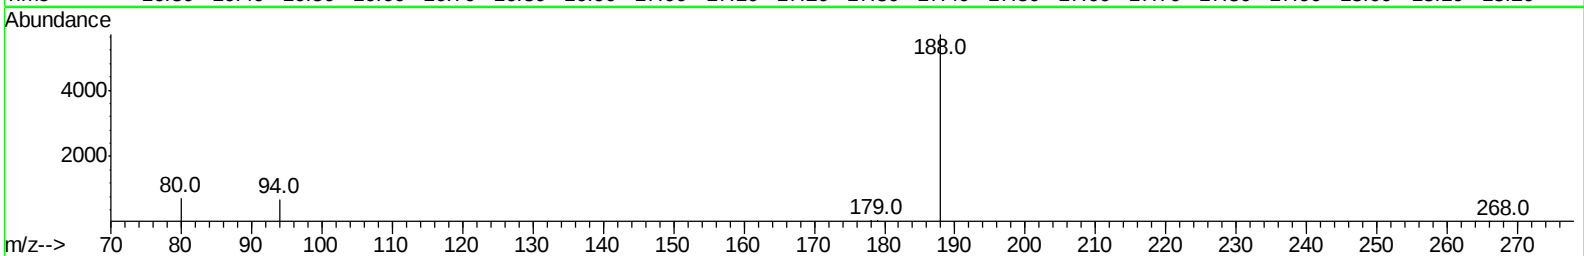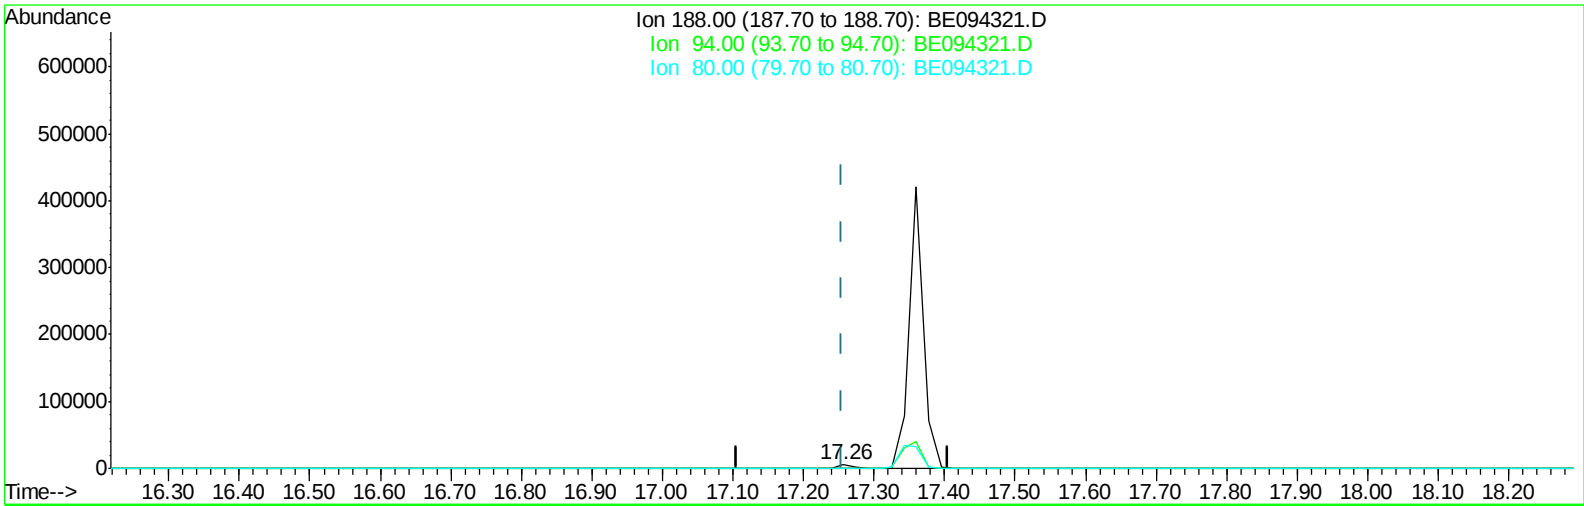

TIC: BE094321.D

(10) Phenanthrene-d10 (I)

17.256min (+0.001) 0.40ng/ul m

response 9065

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.64
80.00	11.80	13.12
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094321.D
Acq On : 13 Oct 2017 12:41
Operator : SJ/JU
Sample : PB102983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK83

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:34 PM

Quant Time: Oct 14 02:22:23 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:15:10 2017
Response via : Initial Calibration

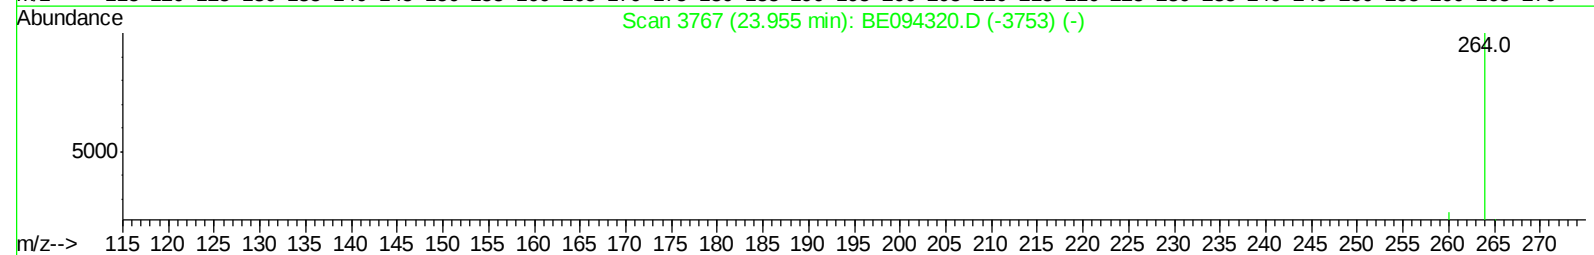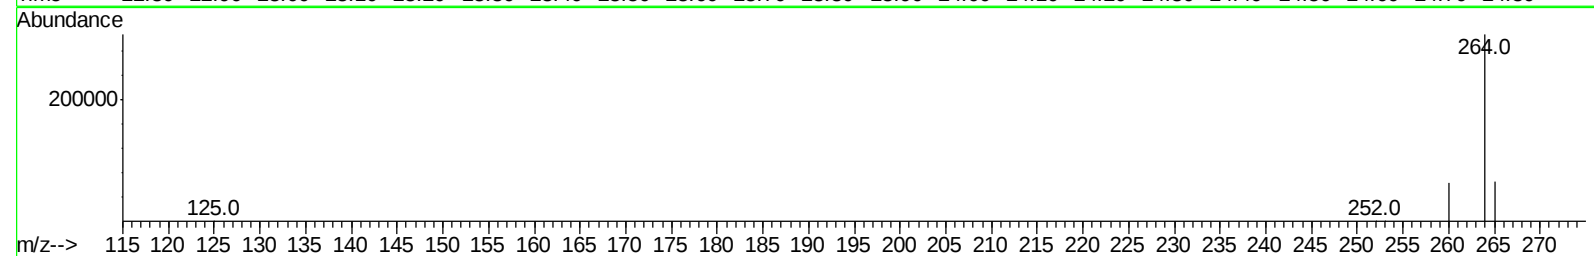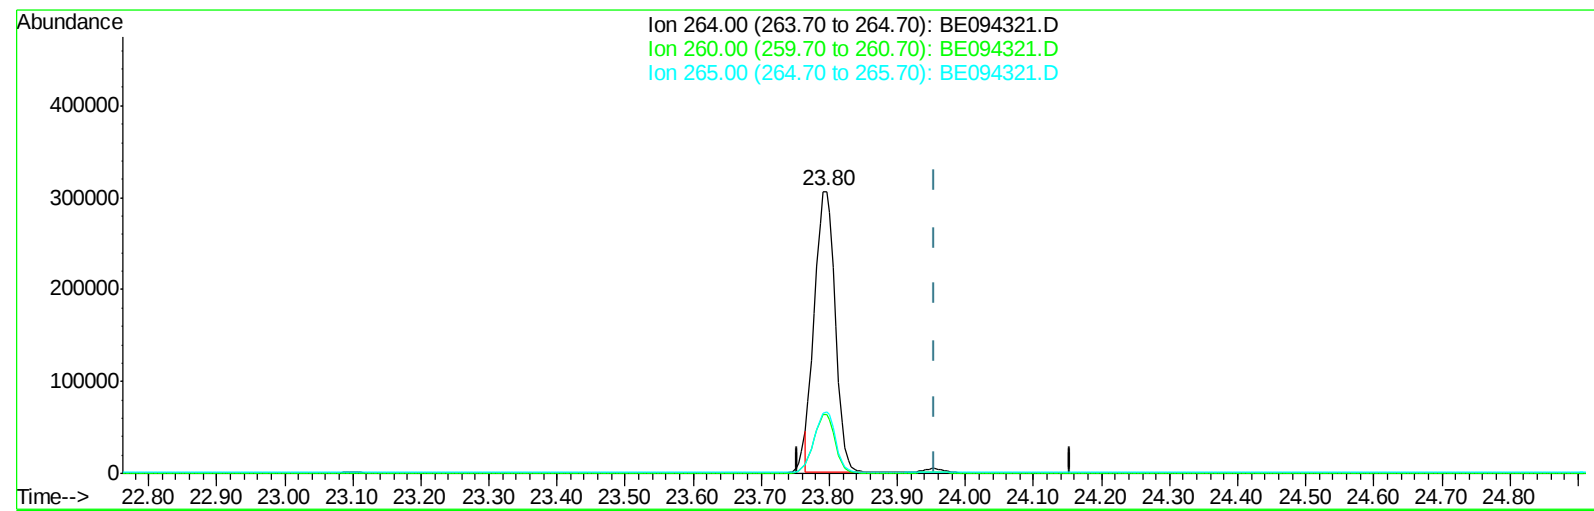

TIC: BE094321.D

(20) Perylene-d12 (I)

23.796min (-0.159) 0.40ng/ul

response 643440

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.86#
265.00	103.50	21.74#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094321.D
Acq On : 13 Oct 2017 12:41
Operator : SJ/JU
Sample : PB102983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK83

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:34 PM

Quant Time: Oct 14 02:22:23 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:15:10 2017
Response via : Initial Calibration

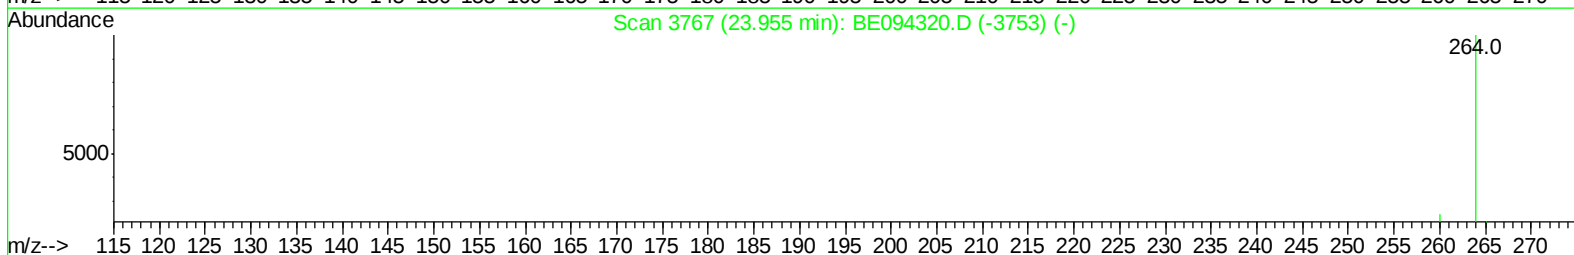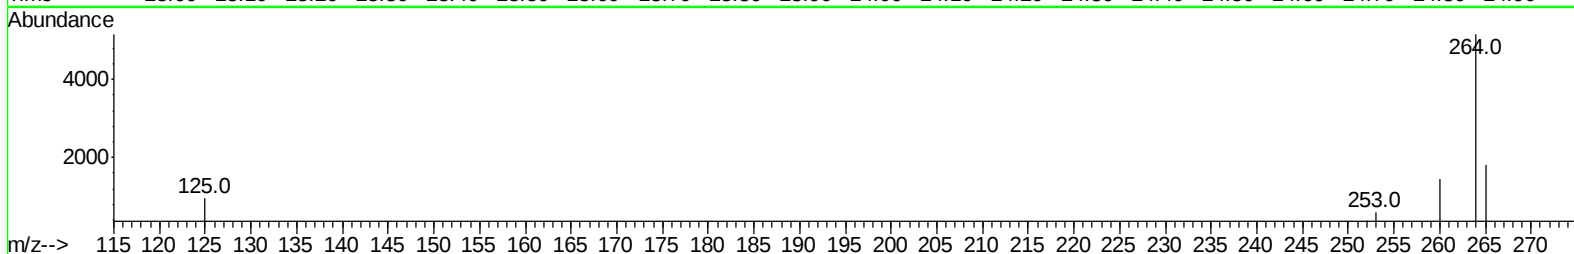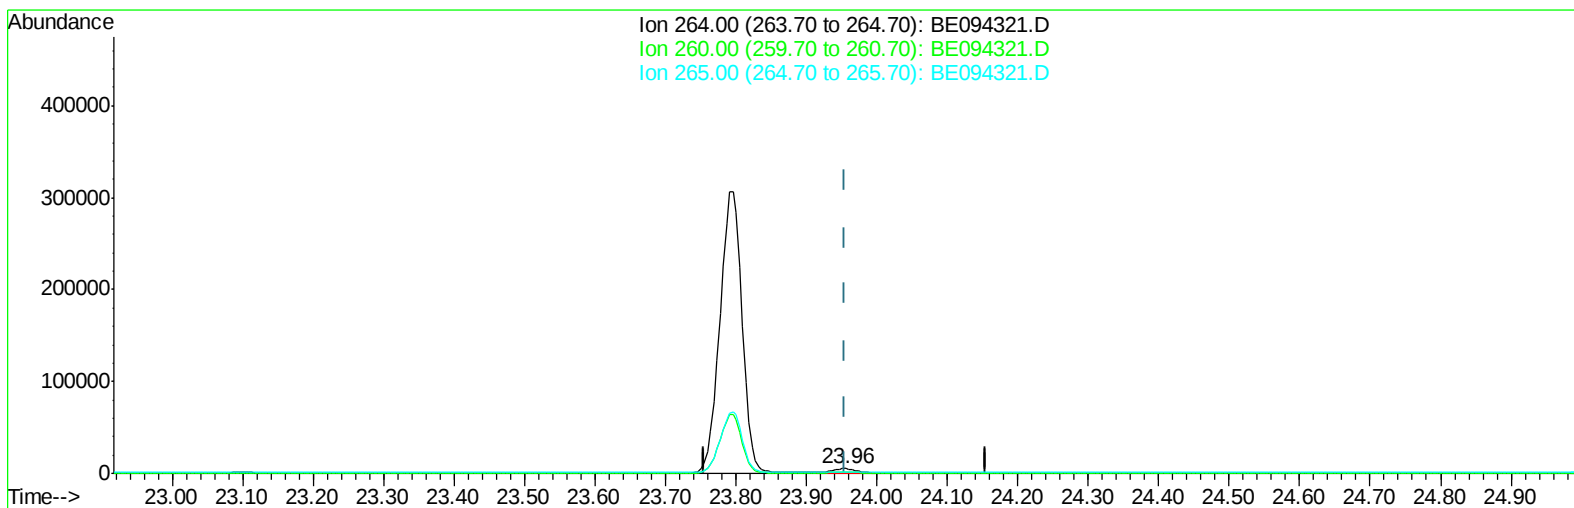

TIC: BE094321.D

(20) Perylene-d12 (I)

23.955min (+0.000) 0.40ng/ul m

response 9886

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	28.43
265.00	103.50	35.20#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
 Data File : BE094321.D
 Acq On : 13 Oct 2017 12:41
 Operator : SJ/JU
 Sample : PB102983BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK83

Manual Integrations
 APPROVED

Sohil
 10/16/2017 8:22:34 PM

Quant Time: Oct 14 02:23:15 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 02:15:10 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1252	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	5862	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.53	164	3690	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	9065m	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	10740	0.40	ng/ul	0.00
20) Perylene-d12	23.96	264	9886m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	2711	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	8359	0.28	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094321.D
Acq On : 13 Oct 2017 12:41
Operator : SJ/JU
Sample : PB102983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK83

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:34 PM

Quant Time: Oct 14 02:23:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 02:15:10 2017
Response via : Initial Calibration

