




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094333.D
Acq On : 13 Oct 2017 21:14
Operator : SJ/JU
Sample : I5568-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-75(1-3)-092917

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:57 PM

Quant Time: Oct 14 04:01:49 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 03:57:24 2017
Response via : Initial Calibration

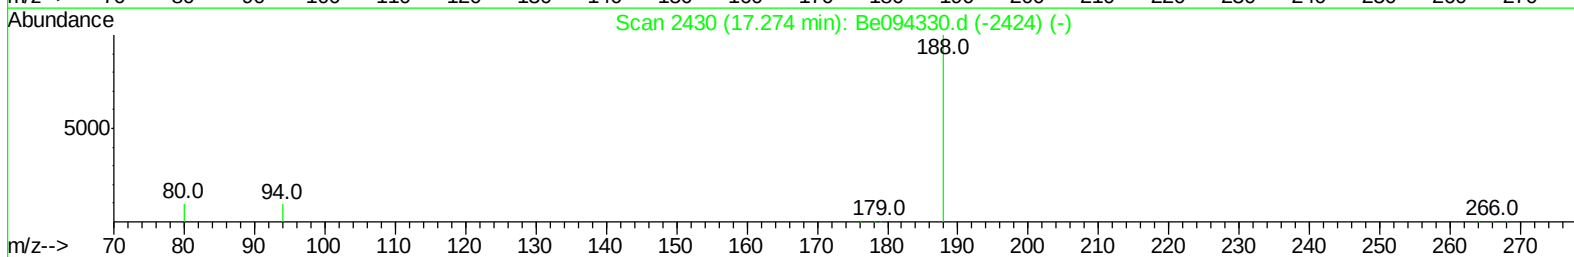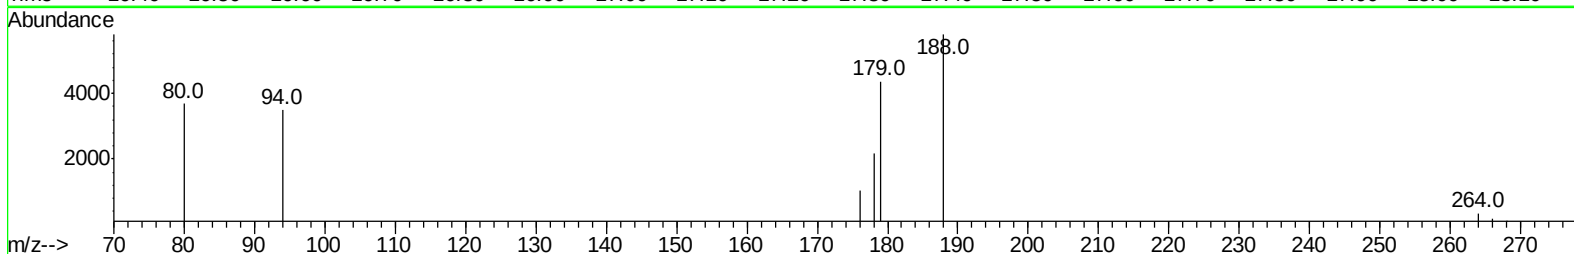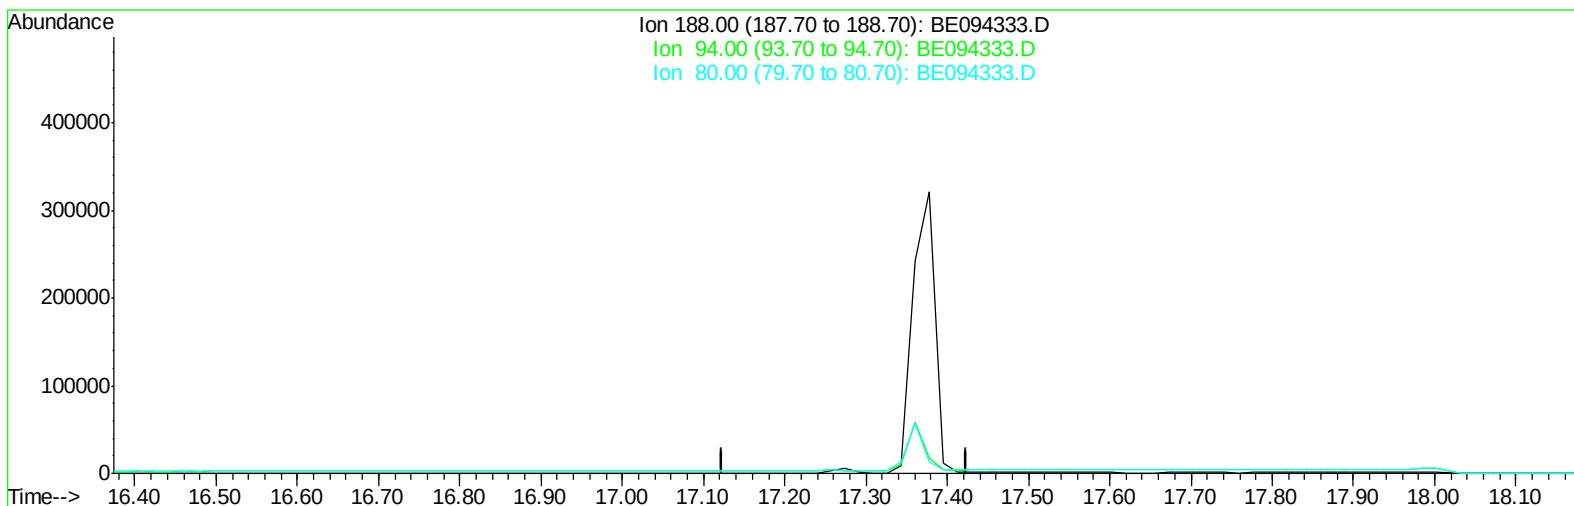

TIC: BE094333.D

(10) Phenanthrene-d10 (I)

17.274min (-17.274) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094333.D
Acq On : 13 Oct 2017 21:14
Operator : SJ/JU
Sample : I5568-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-75(1-3)-092917

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:57 PM

Quant Time: Oct 14 04:01:49 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 03:57:24 2017
Response via : Initial Calibration

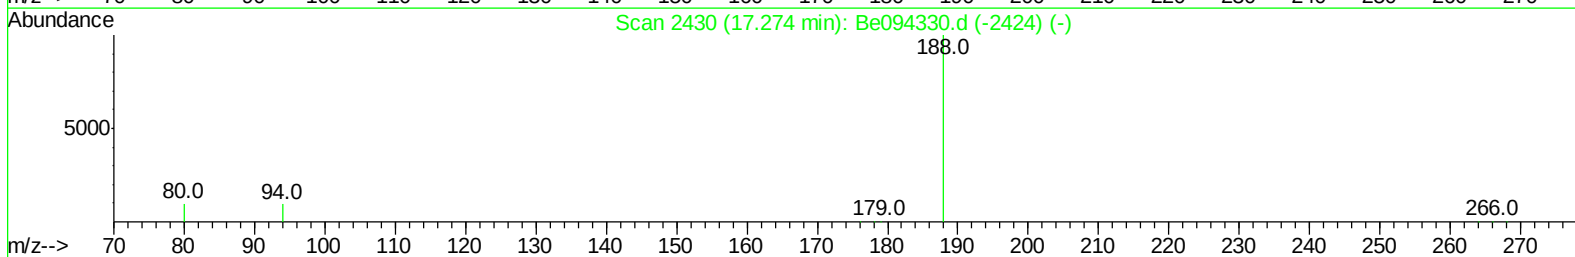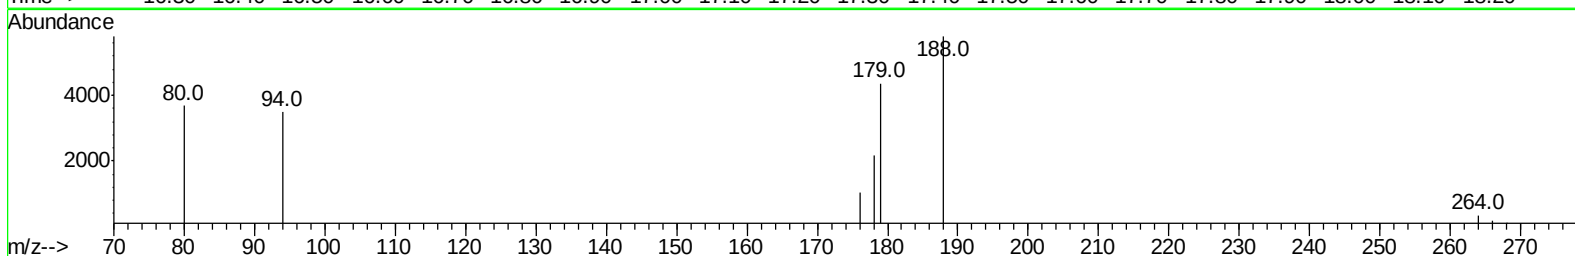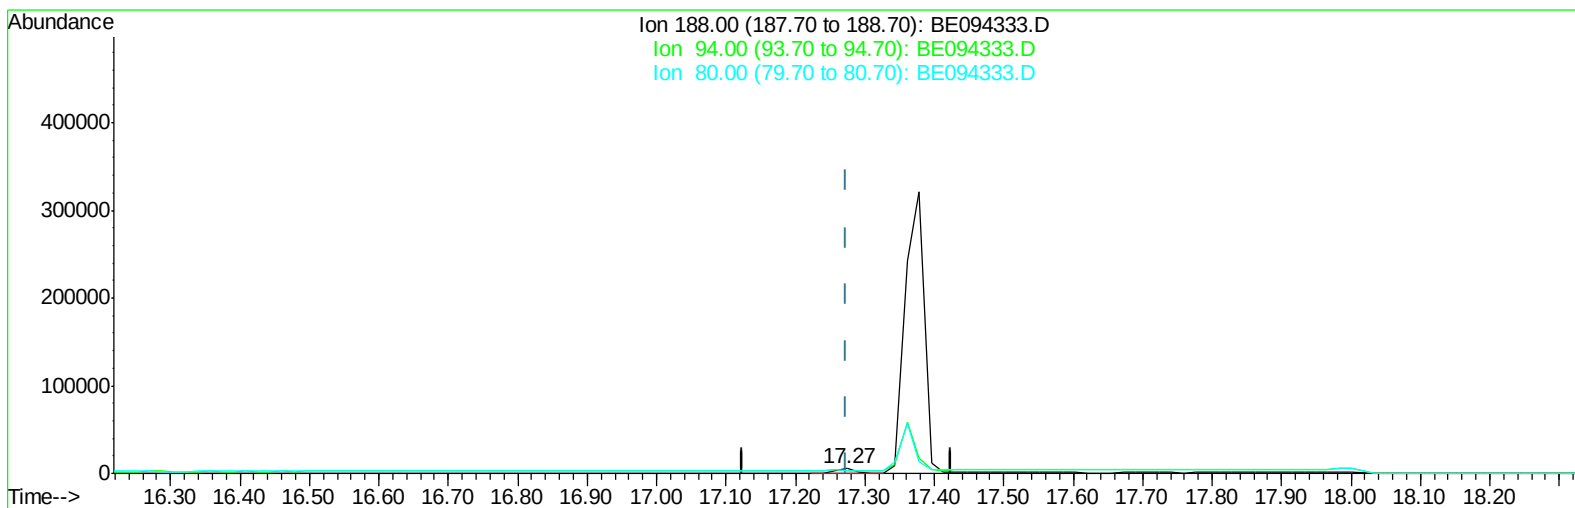

TIC: BE094333.D

(10) Phenanthrene-d10 (I)

17.274min (+0.000) 0.40ng/ul m

response 11440

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	60.42#
80.00	11.80	63.61#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094333.D
Acq On : 13 Oct 2017 21:14
Operator : SJ/JU
Sample : I5568-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-75(1-3)-092917

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:57 PM

Quant Time: Oct 14 04:16:25 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 03:57:24 2017
Response via : Initial Calibration

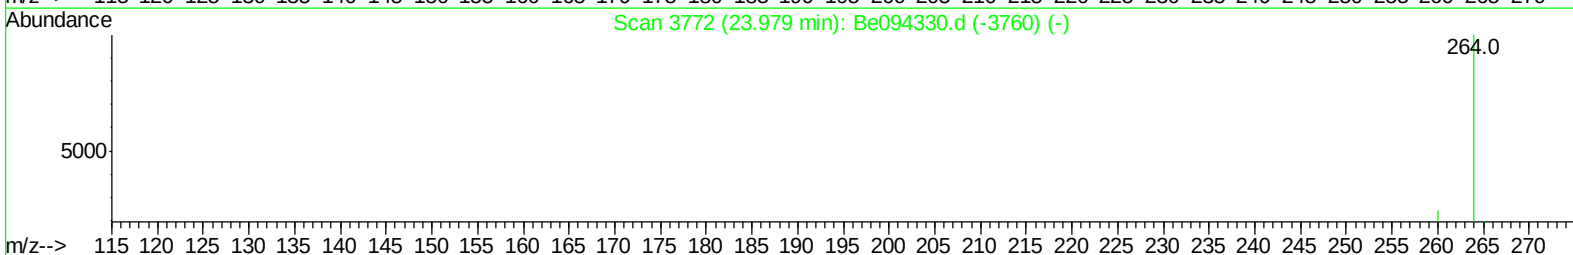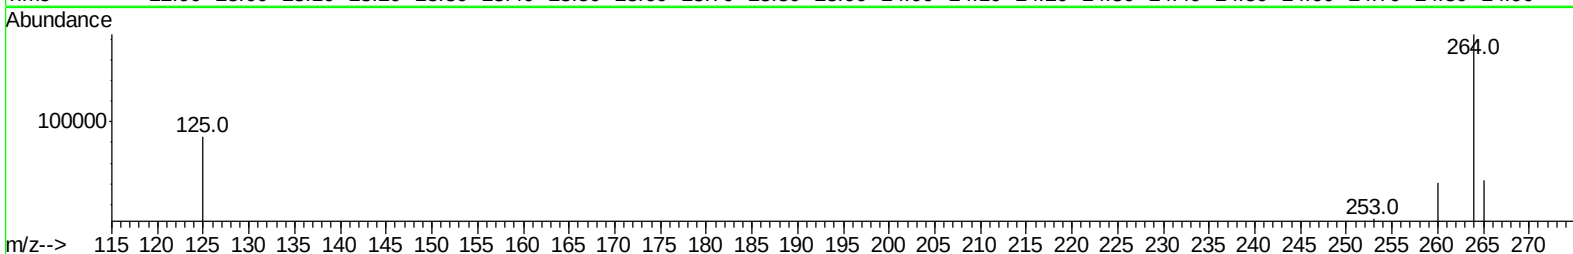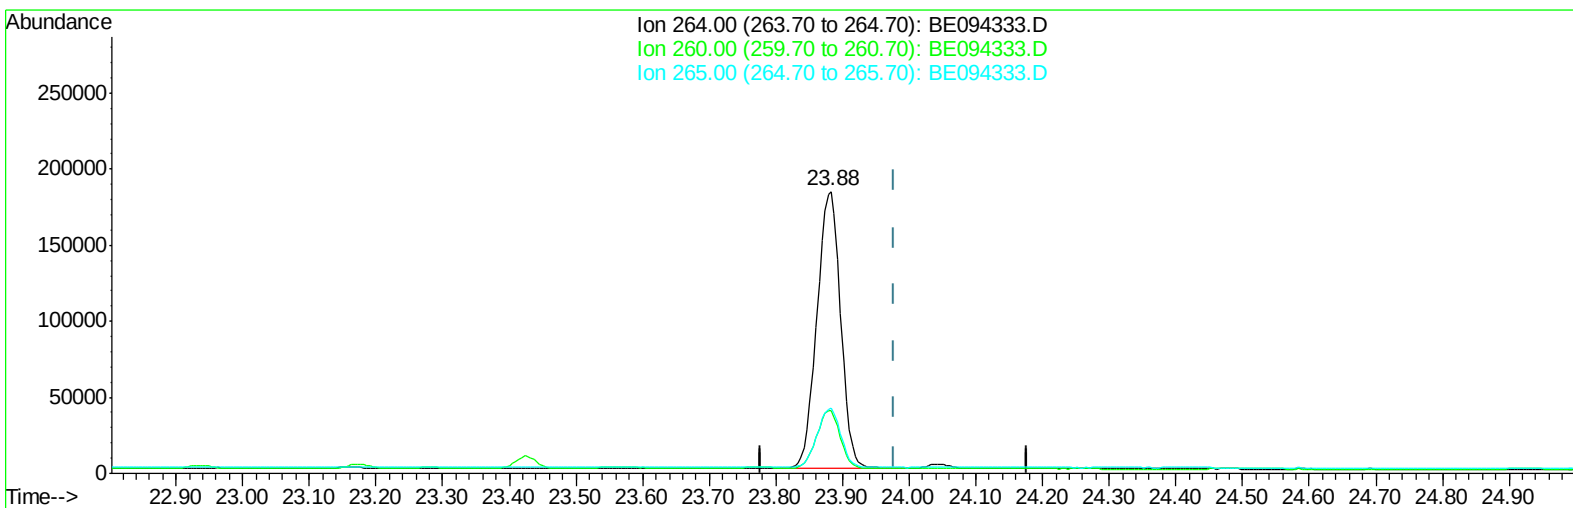

TIC: BE094333.D

(20) Perylene-d12 (I)

23.883min (-0.096) 0.40ng/ul

response 448342

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.11#
265.00	103.50	23.23#
0.00	0.00	0.00




Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094333.D
Acq On : 13 Oct 2017 21:14
Operator : SJ/JU
Sample : I5568-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-75(1-3)-092917

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:57 PM

Quant Time: Oct 14 04:16:25 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 03:57:24 2017
Response via : Initial Calibration

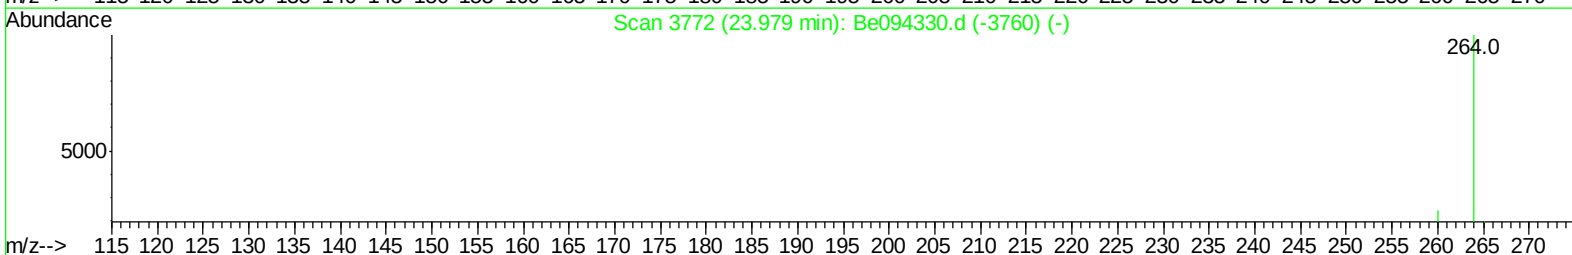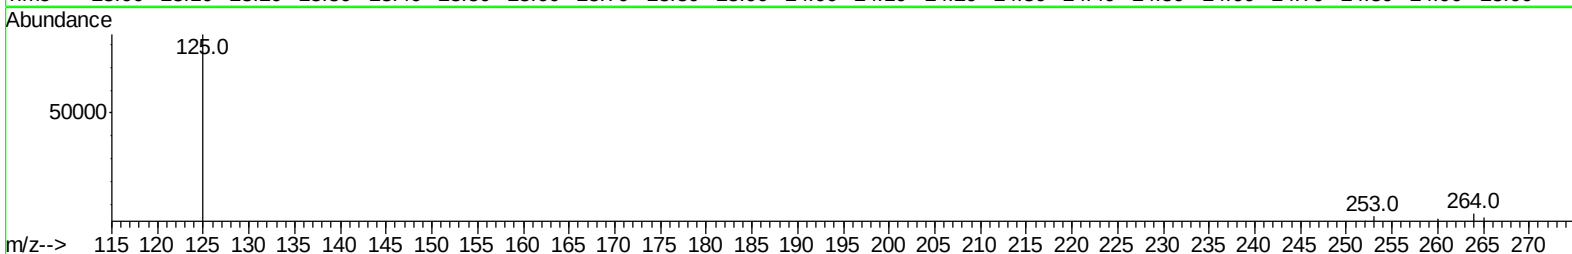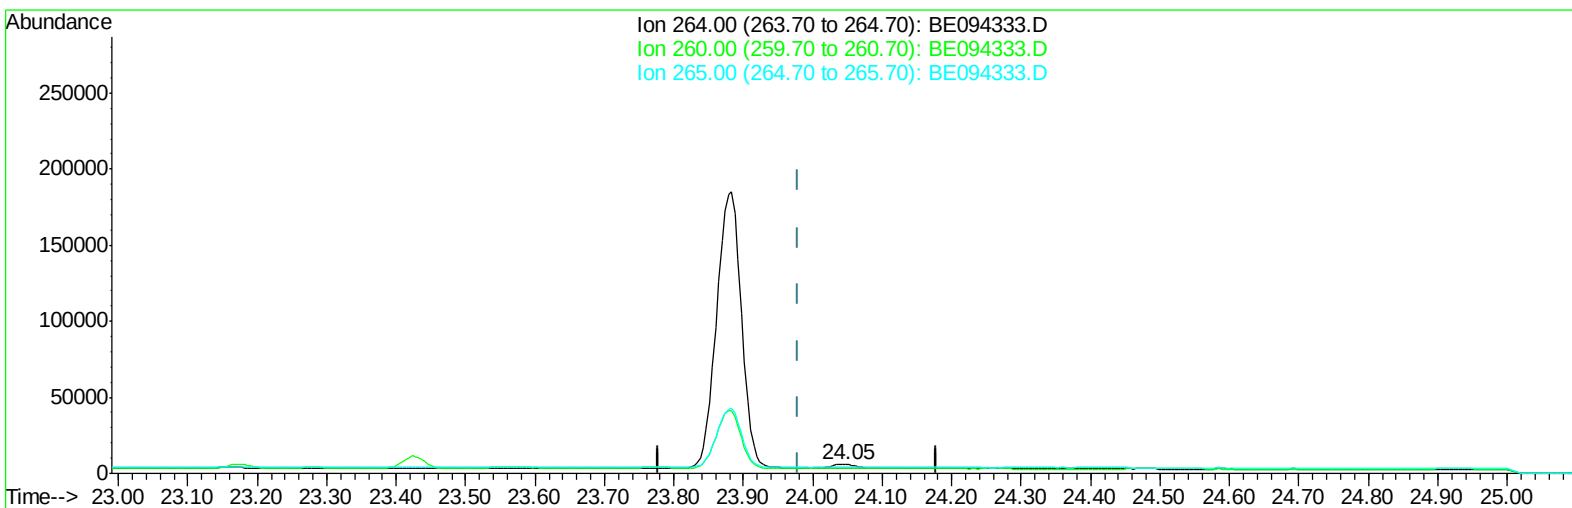

TIC: BE094333.D

(20) Perylene-d12 (I)

24.047min (+0.068) 0.40ng/ul m

response 6483

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	63.53#
265.00	103.50	75.57#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
 Data File : BE094333.D
 Acq On : 13 Oct 2017 21:14
 Operator : SJ/JU
 Sample : I5568-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 B-75(1-3)-092917

Manual Integrations
 APPROVED

Sohil
 10/16/2017 8:22:57 PM

Quant Time: Oct 14 04:24:01 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 03:57:24 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.95	152	5509	0.40	ng/ul	0.02
2) Naphthalene-d8	10.72	136	13855	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.54	164	5597	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.27	188	11440m	0.40	ng/ul	0.00
16) Chrysene-d12	21.46	240	6119	0.40	ng/ul	0.02
20) Perylene-d12	24.05	264	6483m	0.40	ng/ul	0.07
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	6353	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	7601	0.20	ng/ul	0.00
Target Compounds				Ovalue		
5) 2-Methylnaphthalene	12.37	142	5382	0.244	ng/ul	93
8) Acenaphthene	14.60	153	15106	0.841	ng/ul#	87
9) Fluorene	15.58	166	12665	0.602	ng/ul#	70
12) Phenanthrene	17.31	178	28399	0.950	ng/ul#	77
17) Pyrene	19.70	202	15596	0.916	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101317\
Data File : BE094333.D
Acq On : 13 Oct 2017 21:14
Operator : SJ/JU
Sample : I5568-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B-75(1-3)-092917

Manual Integrations
APPROVED

Sohil
10/16/2017 8:22:57 PM

Quant Time: Oct 14 04:24:01 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 03:57:24 2017
Response via : Initial Calibration

