

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101417\
 Data File : BE094355.D
 Acq On : 14 Oct 2017 15:06
 Operator : SJ/JU
 Sample : PB102872BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 15 01:08:15 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 05:22:31 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	942	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.70	136	4697	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	3186	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.27
16) Chrysene-d12	21.43	240	9390	0.40	ng/ul	0.00
20) Perylene-d12	23.79	264	514994	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	2462	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	8717	0.00	ng/ul	-0.01
Target Compounds						
17) Pyrene	19.65	202	1183	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE101417\
Data File : BE094355.D
Acq On : 14 Oct 2017 15:06
Operator : SJ/JU
Sample : PB102872BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 15 01:08:15 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 14 05:22:31 2017
Response via : Initial Calibration

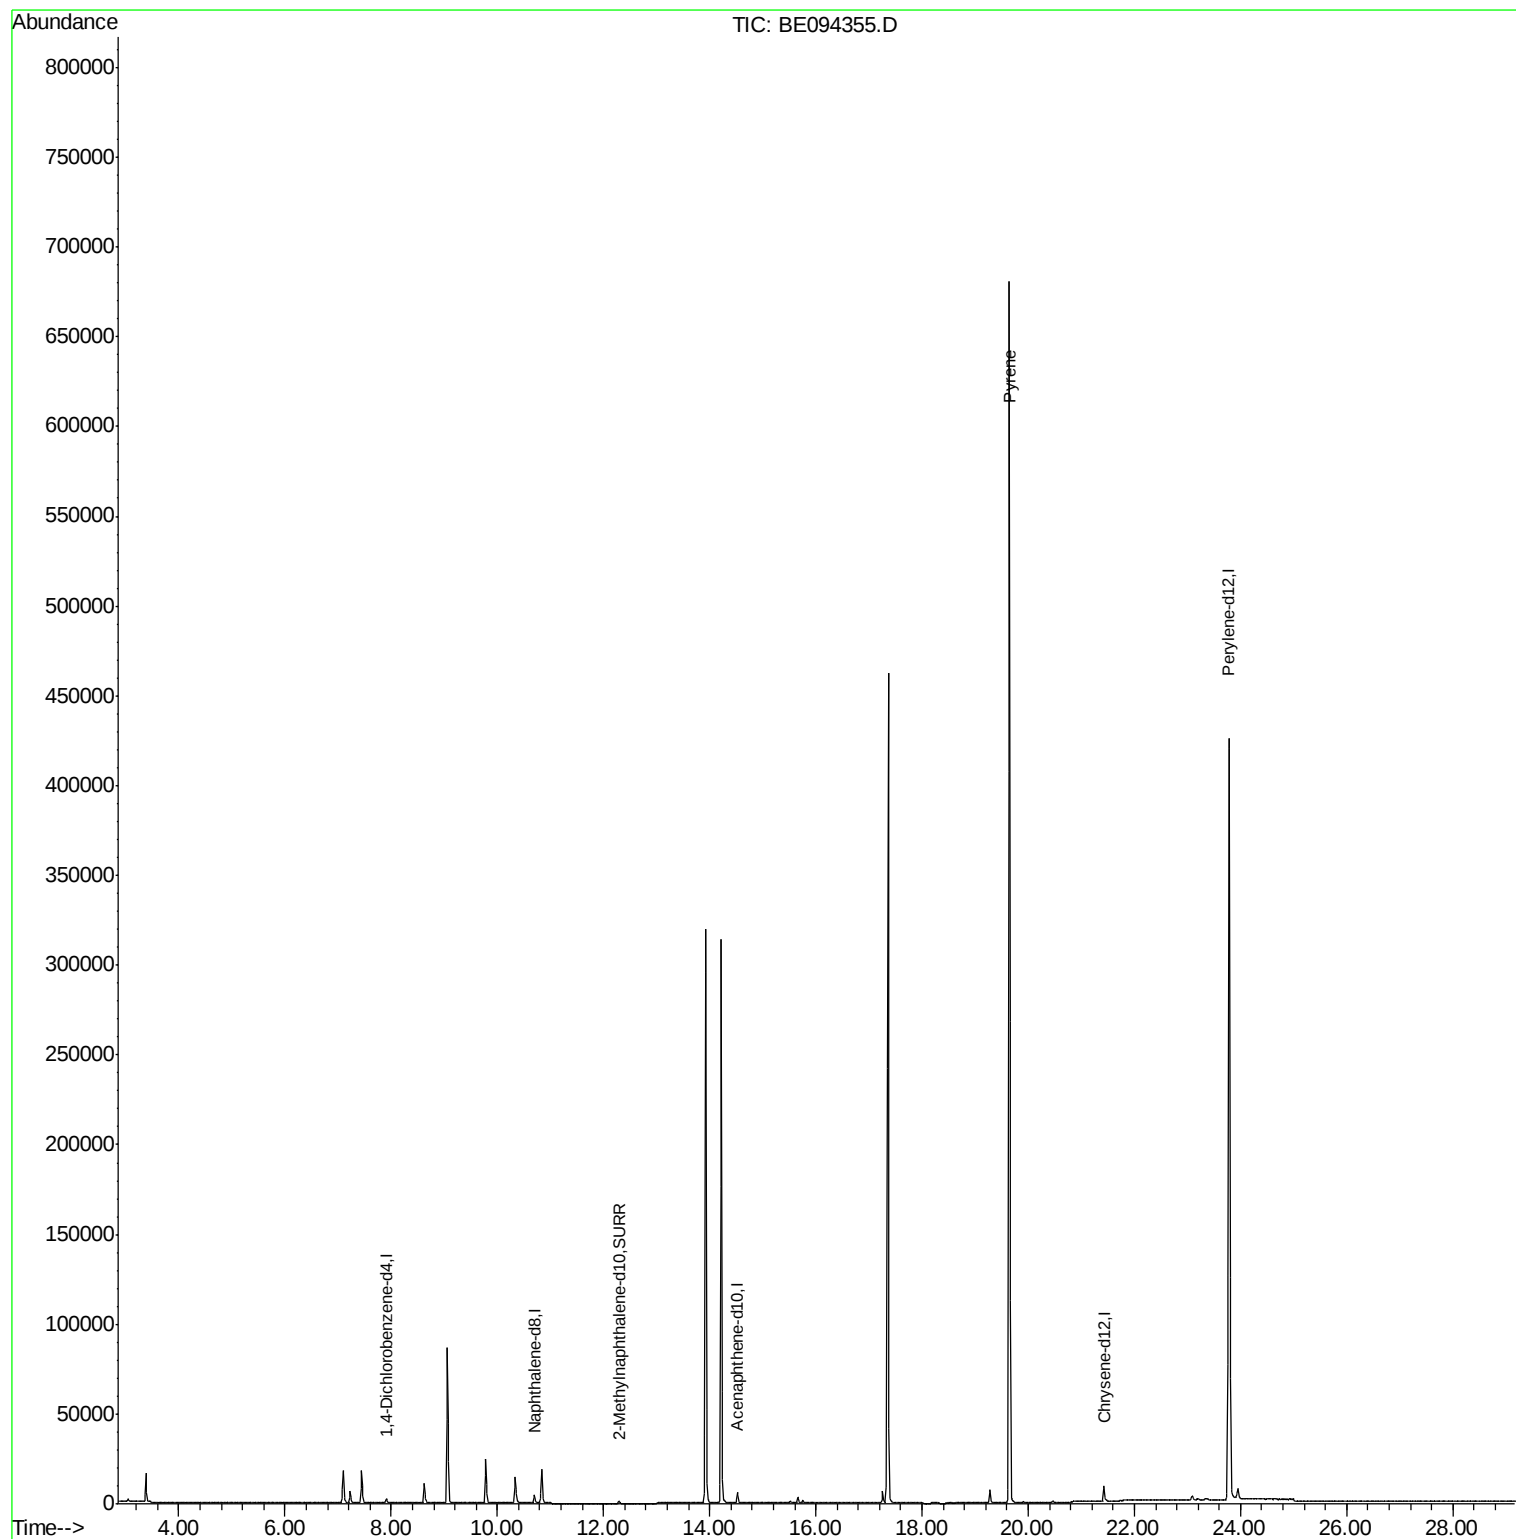


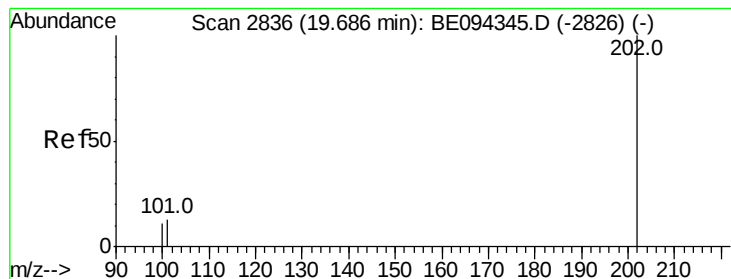

#17
 Pvrene
 Concen: 0.045 ng/ul
 RT: 19.65 min Scan# 2828
 Delta R.T. -0.04 min
 Lab File: BE094355.D
 Acq: 14 Oct 2017 15:06

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:202 Resp: 1183
 Ion Ratio Lower Upper
 202 100
 101 154.4 18.2 27.4#
 100 779.8 15.6 23.4#

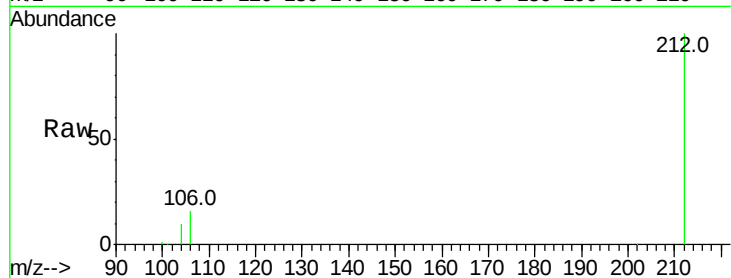

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): BE

