

Quantitation Report (QT Reviewed)


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA E\DATA\BE101417\
 Data File : BE094356.D
 Acq On : 14 Oct 2017 15:42
 Operator : SJ/JU
 Sample : PB102800BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK00

Manual Integrations
 APPROVED

Sohil
 10/16/2017 8:25:00 PM

Quant Time: Oct 15 01:25:52 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 05:22:31 2017
 Response via : Initial Calibration

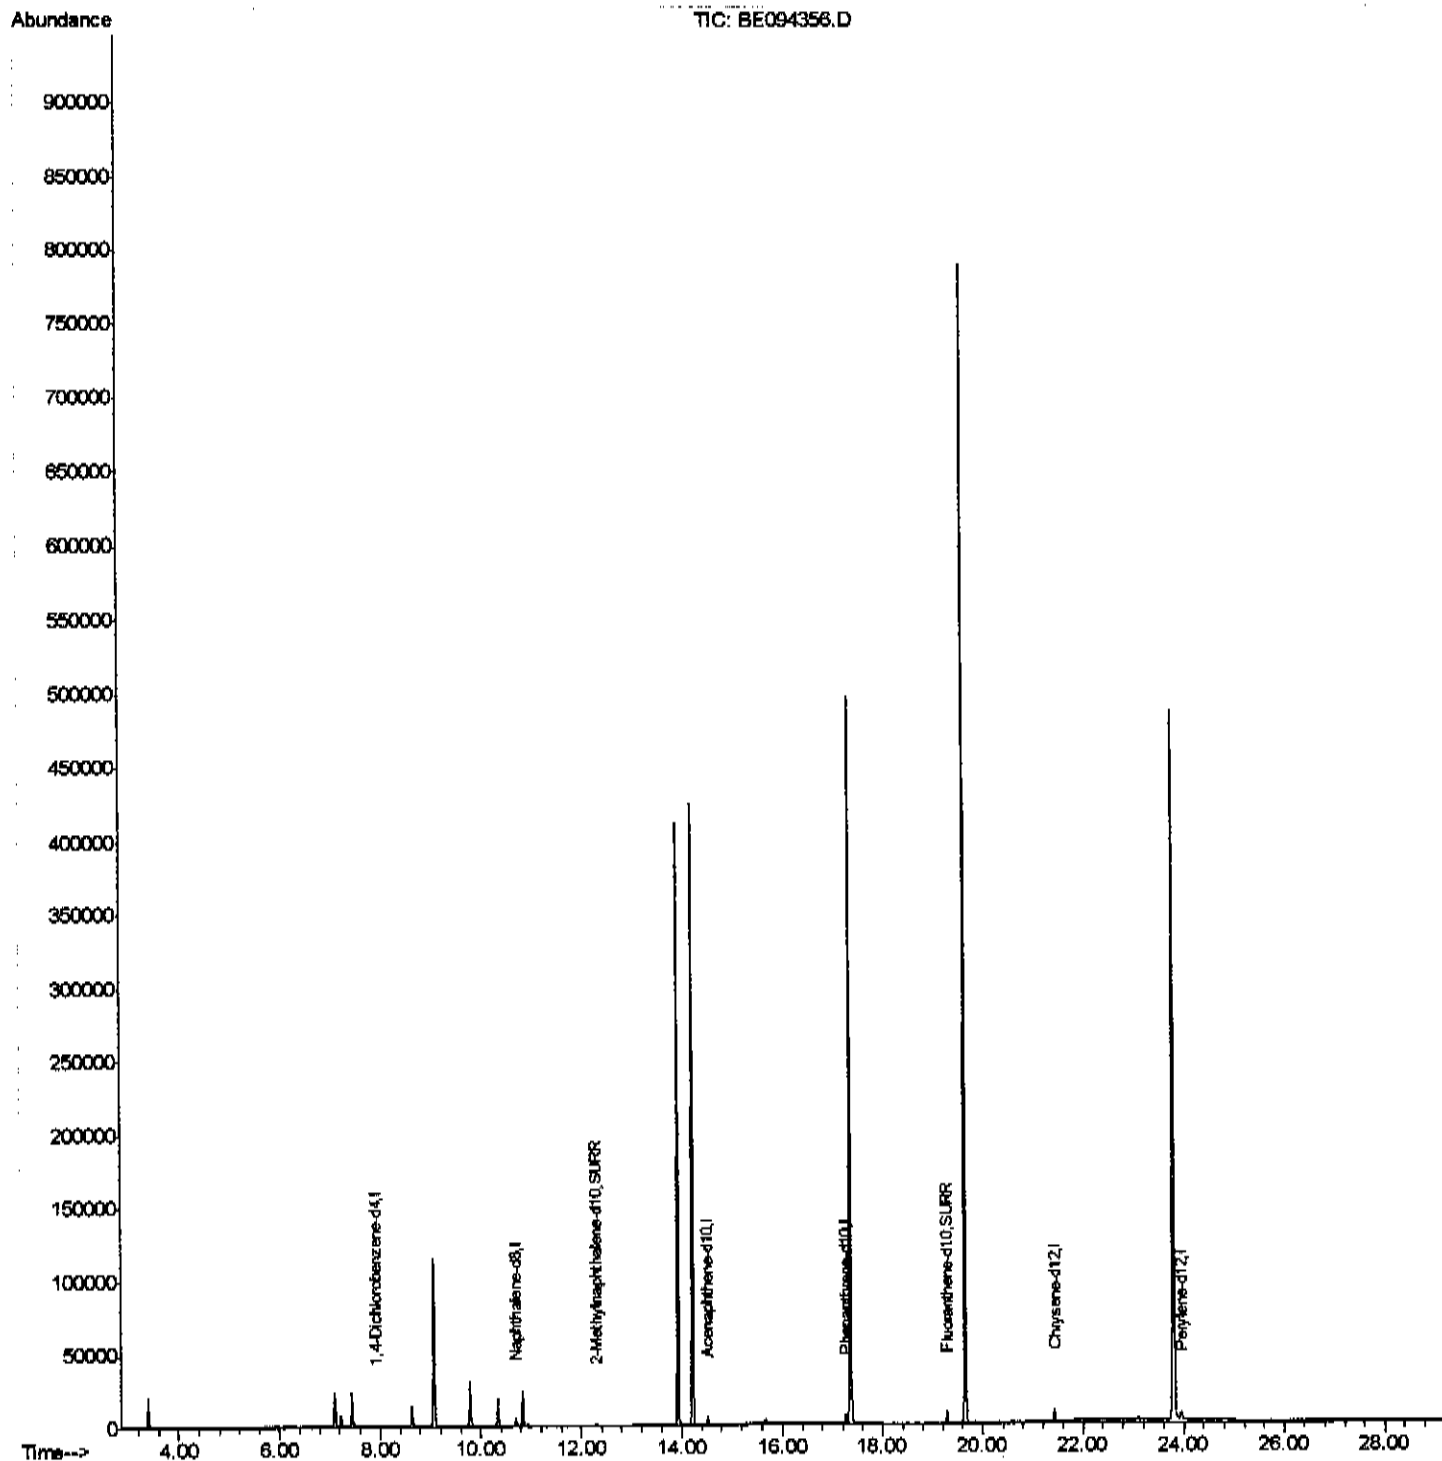

Quantitation Report (Qedit)


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA E\DATA\BE101417\
 Data File : BE094356.D
 Acq On : 14 Oct 2017 15:42
 Operator : SJ/JU
 Sample : PB102800BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK00

Manual Integrations
 APPROVED

Sohil
 10/16/2017 8:25:00 PM

Quant Time: Oct 15 01:08:22 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 05:22:31 2017
 Response via : Initial Calibration

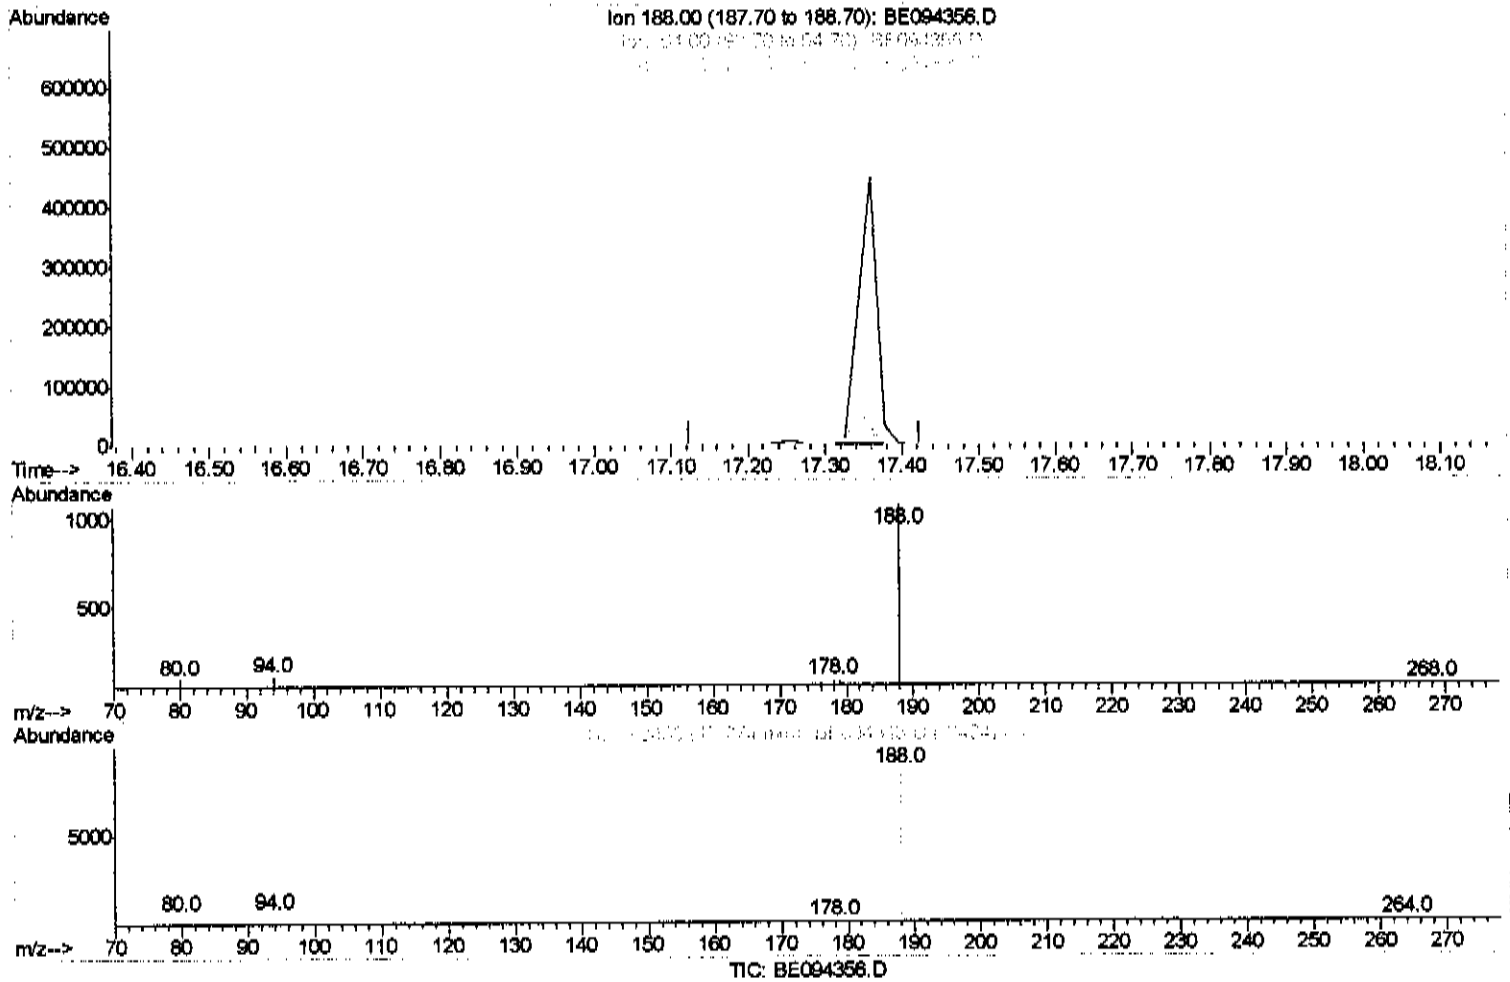

(10) Phenanthrene-d10 (I)
 17.274min (-17.274) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA E\DATA\BE101417\
 Data File : BE094356.D
 Acq On : 14 Oct 2017 15:42
 Operator : SJ/JU
 Sample : PB102800BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK00

Manual Integrations
 APPROVED

Sohil
 10/16/2017 8:25:00 PM

Quant Time: Oct 15 01:08:22 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 05:22:31 2017
 Response via : Initial Calibration

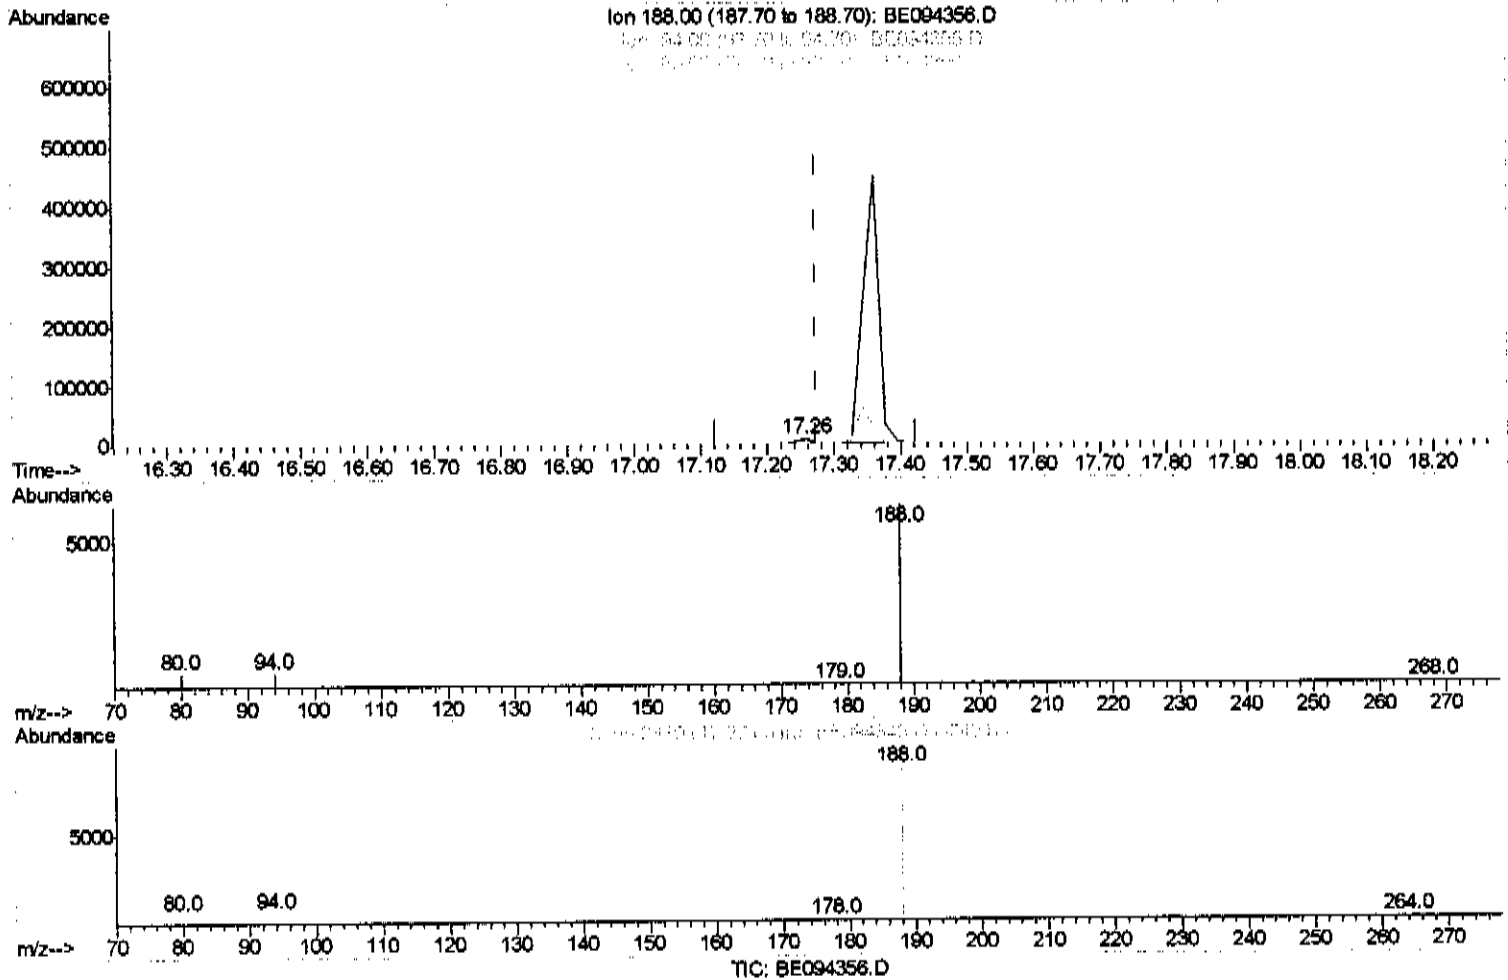

(10) Phenanthrene-d10 (I)

17.256min (-0.017) 0.40ng/ul m

response 8951

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	8.58#
80.00	11.80	8.35#
0.00	0.00	0.00

OK 10/16/17

Quantitation Report (Qedit)


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA E\DATA\BE101417\
 Data File : BE094356.D
 Acq On : 14 Oct 2017 15:42
 Operator : SJ/JU
 Sample : PB102800EL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK00

Manual Integrations
 APPROVED

Sohil
 10/16/2017 8:25:00 PM

Quant Time: Oct 15 01:23:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 14 05:22:31 2017
 Response via : Initial Calibration

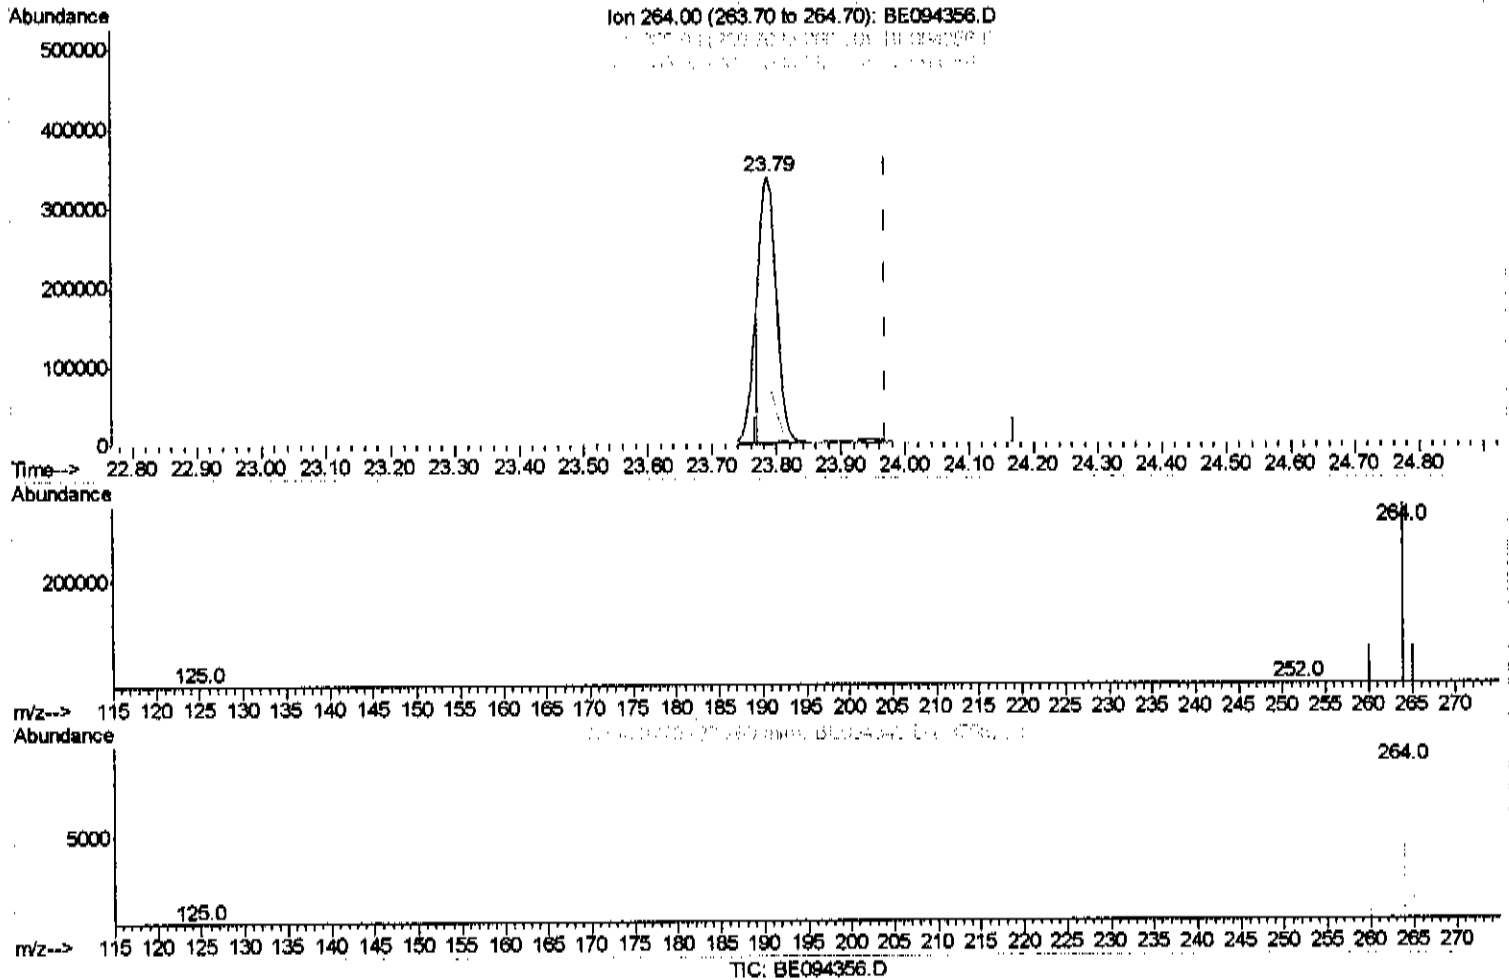

(20) Perylene-d12 (I)

23.787min (-0.182) 0.40ng/ui

response 597852

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.68#
265.00	103.50	21.55#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA E\DATA\BE101417\
 Data File : BE094356.D
 Acq On : 14 Oct 2017 15:42
 Operator : SJ/JU
 Sample : PB102800BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SBLK00

Manual Integrations
 APPROVED

Sohil
 10/16/2017 8:25:00 PM

Quant Time: Oct 15 01:23:50 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 OLast Update : Sat Oct 14 05:22:31 2017
 Response via : Initial Calibration

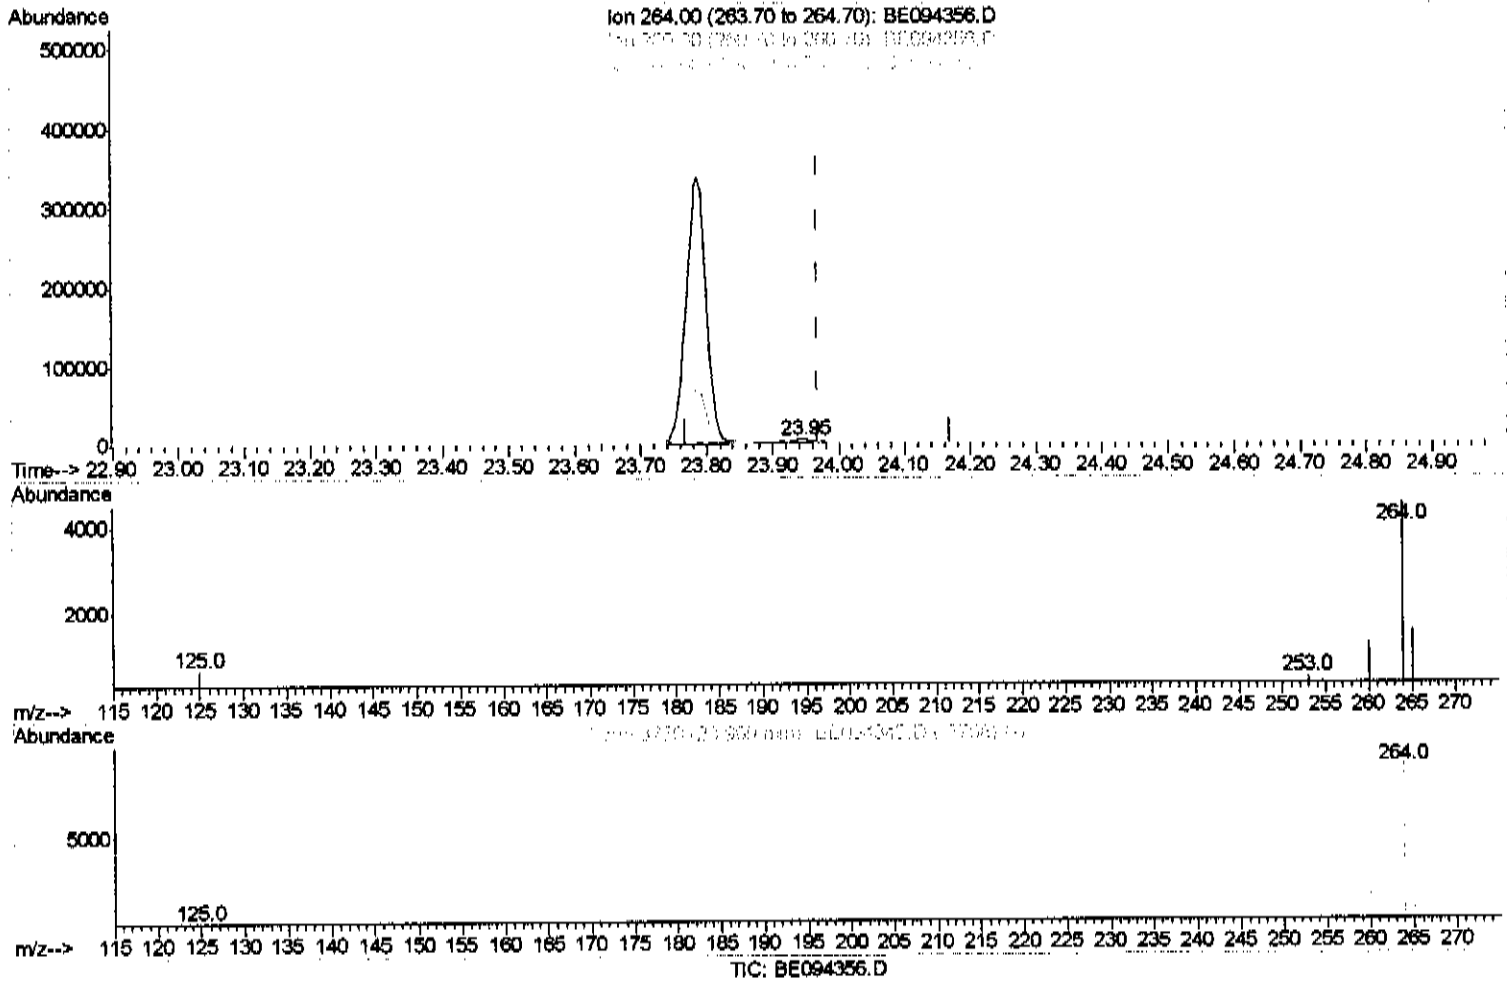

(20) Perylene-d12 (I)

23.948min (-0.023) 0.40ng/ul m *SJ 10/16/17*

response 8673

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	27.82
266.00	103.50	33.81#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampled :
SBLK00

Manual Integrations
APPROVED

Sohil
10/16/2017 8:25:00 PM

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA E\DATA\BE101417\
Data File : BE094356.D
Acq On : 14 Oct 2017 15:42
Operator : SJ/JU
Sample : PB102800BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 15 01:25:52 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Oct 14 05:22:31 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1105	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.70	136	5446	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	3637	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	8951m	0.40	ng/ul	>0.02
16) Chrysene-d12	21.43	240	9339	0.40	ng/ul	0.00
20) Perylene-d12	23.95	264	8673m	0.40	ng/ul	>0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.29	152	3165	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	9881	0.33	ng/ul	-0.01

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed