



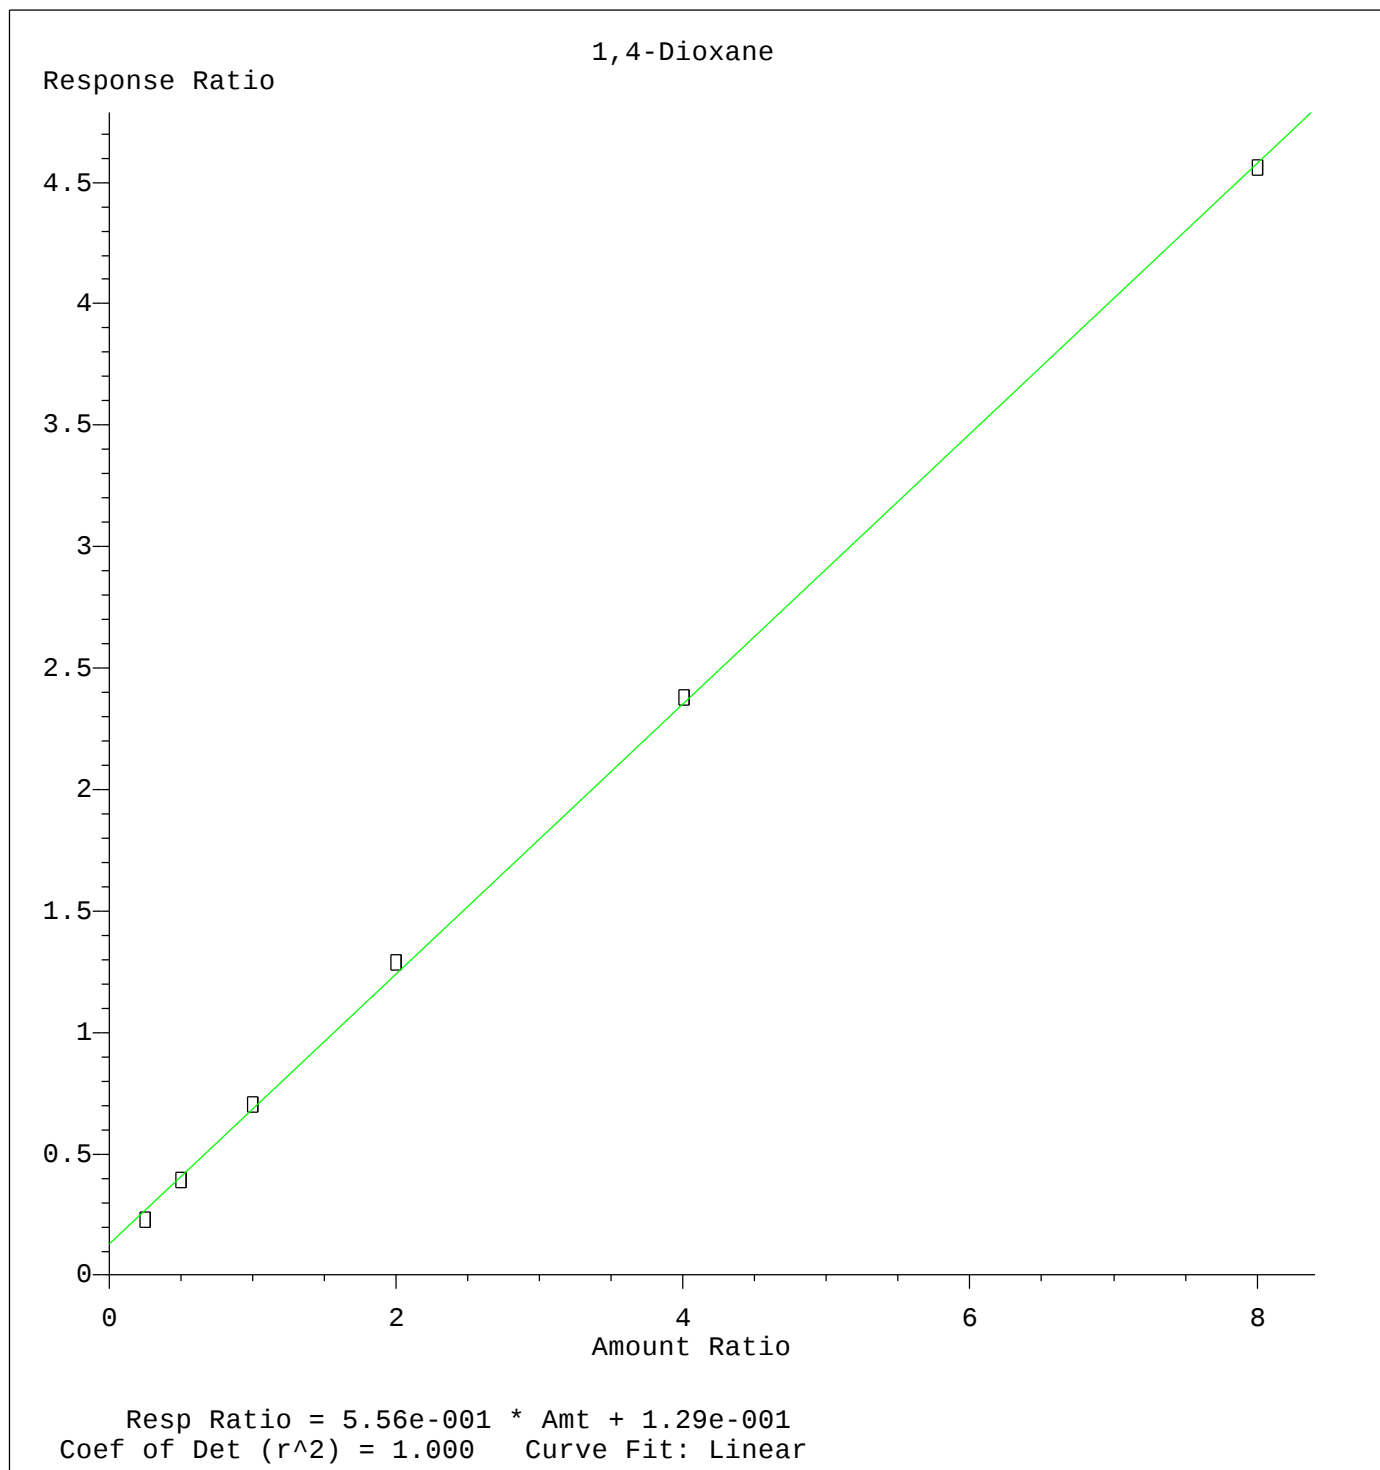

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101617.M
Calibration Table Last Updated: Mon Oct 16 14:54:40 2017


Hexachlorobenzene

Response Ratio

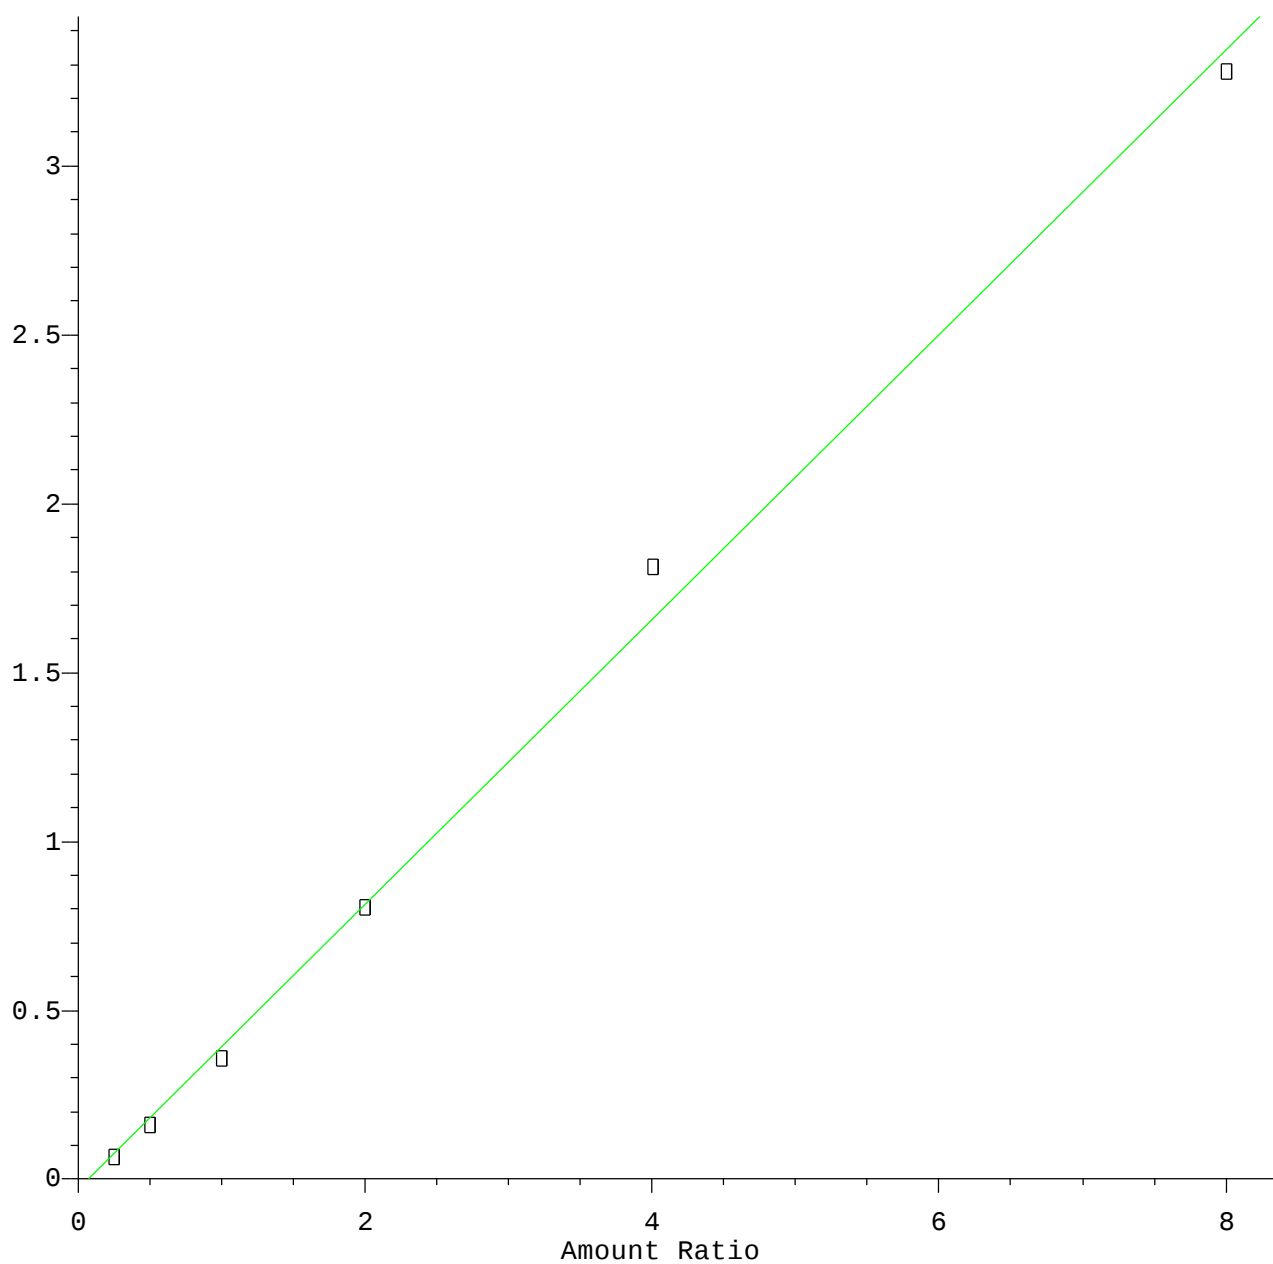

Resp Ratio = $4.22 \times 10^{-1} \times \text{Amt} - 2.84 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101617.M
Calibration Table Last Updated: Mon Oct 16 14:54:40 2017

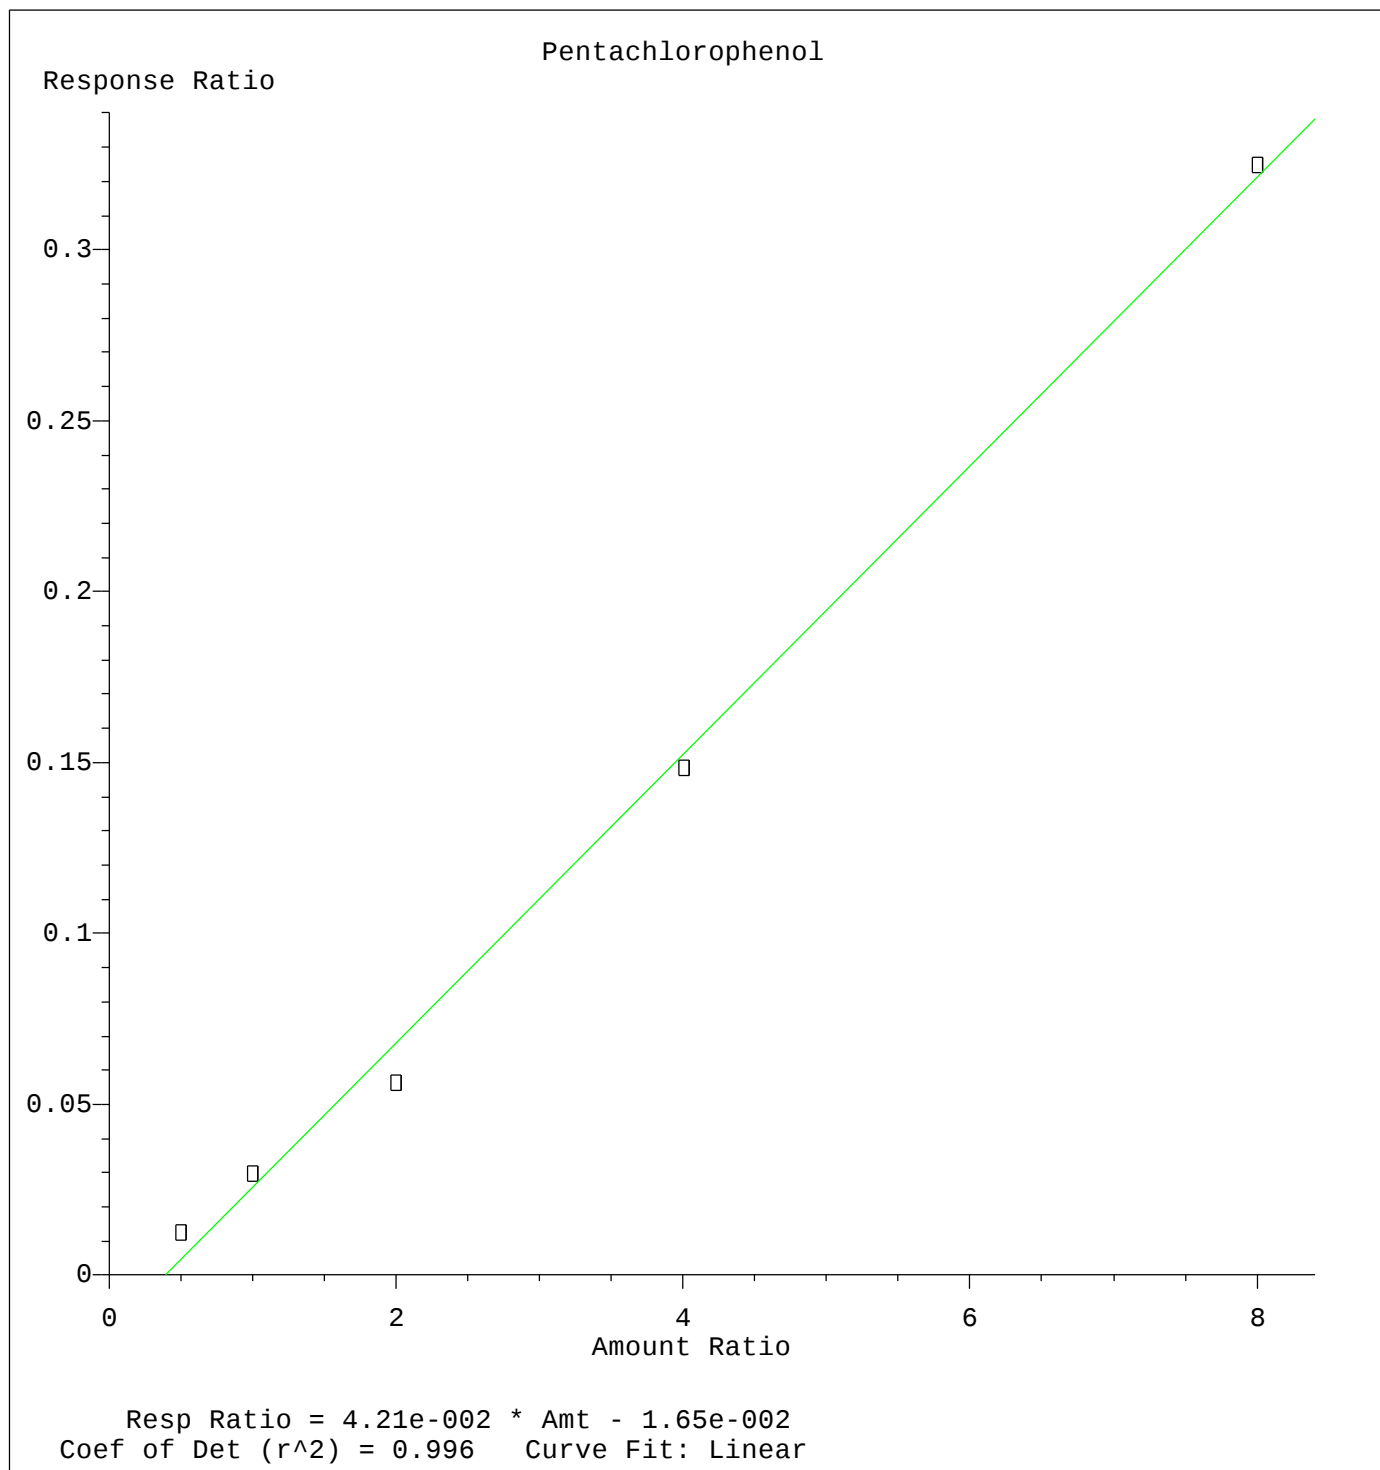

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101617.M
Calibration Table Last Updated: Mon Oct 16 14:54:40 2017