


Data Path : Z:\HPCHEM1\BNA_E\Data\BE101617\
Data File : BE094410.D
Acq On : 16 Oct 2017 10:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101617.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 16 14:54:40 2017

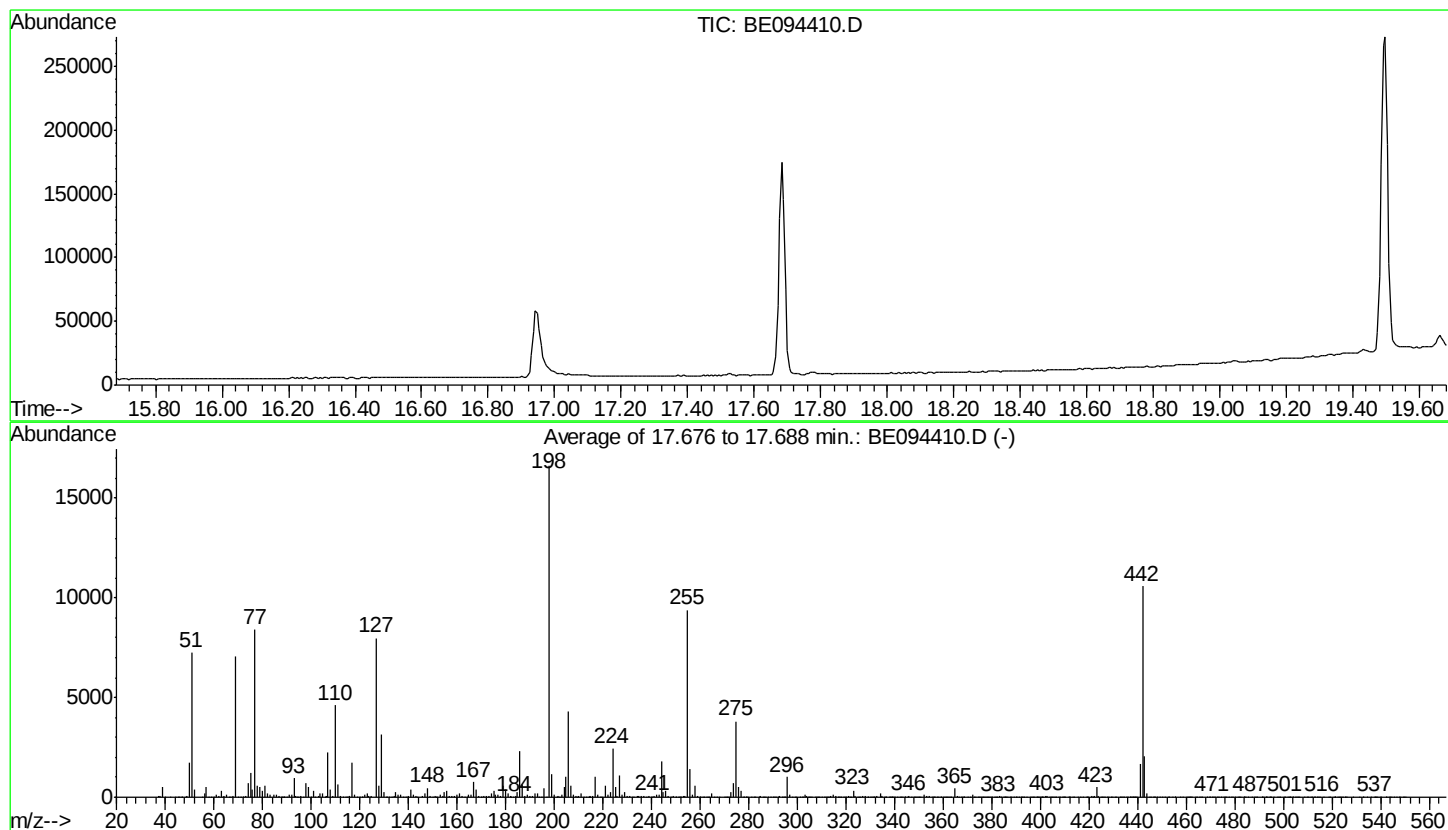

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	7241	PASS
68	69	0.00	2	1.3	95	PASS
69	198	0.00	100	42.4	7055	PASS
70	69	0.00	2	0.5	33	PASS
127	198	10	80	48.0	7989	PASS
197	198	0.00	2	0.1	11	PASS
198	198	100	100	100.0	16633	PASS
199	198	5	9	7.1	1177	PASS
275	198	10	60	22.9	3814	PASS
365	198	1	100	2.5	424	PASS
441	442	0.01	24	15.7	1665	PASS
442	198	50	100	63.7	10590	PASS
443	442	15	24	19.5	2066	PASS