


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE101717\
 Data File : BE094425.D
 Acq On : 17 Oct 2017 10:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\Methods\8270-SIM-BE101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 16 14:54:40 2017

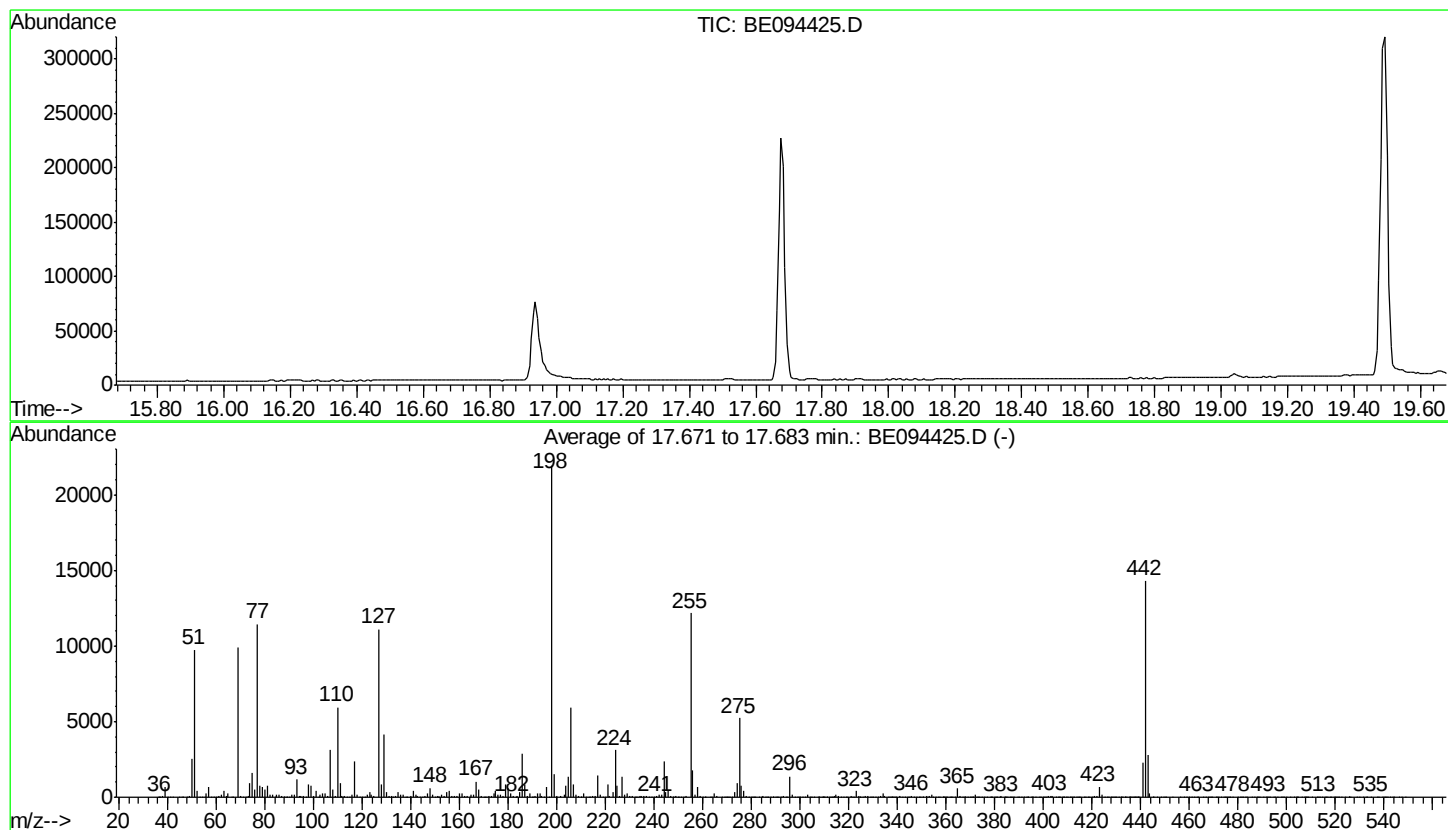

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	9756	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.1	9896	PASS
70	69	0.00	2	0.5	53	PASS
127	198	10	80	50.6	11089	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21924	PASS
199	198	5	9	7.0	1532	PASS
275	198	10	60	23.9	5246	PASS
365	198	1	100	2.6	572	PASS
441	442	0.01	24	16.2	2323	PASS
442	198	50	100	65.3	14314	PASS
443	442	15	24	19.3	2769	PASS