

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE101915\
 Data File : BE091024.D
 Acq On : 19 Oct 2015 17:16
 Operator : UM/NP
 Sample : G4075-17
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JG9M9

Quant Time: Oct 20 14:30:56 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE101415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 01:00:24 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 10/20/2015 6:28:08 PM

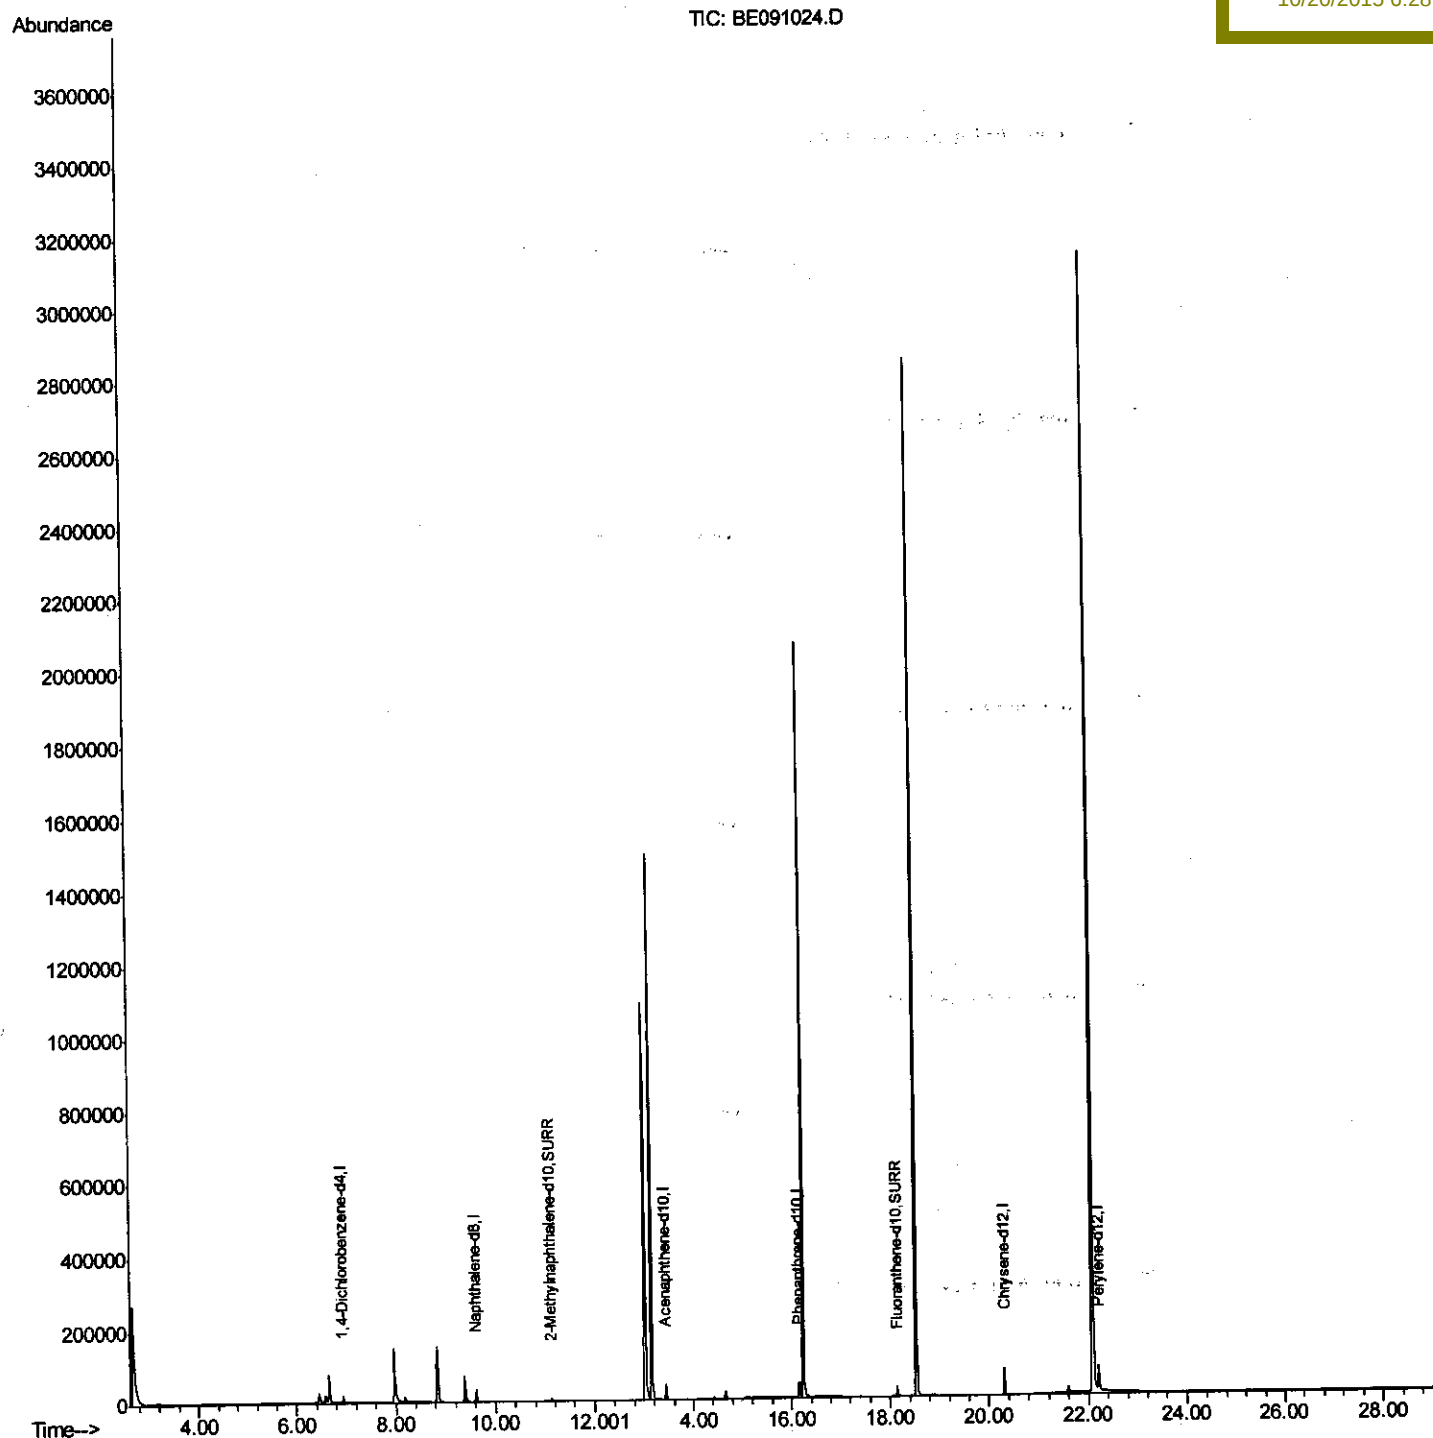

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE101915\
 Data File : BE091024.D
 Acq On : 19 Oct 2015 17:16
 Operator : UM/NP
 Sample : G4075-17
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JG9M9

Quant Time: Oct 20 14:28:04 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE101415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 01:00:24 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 10/20/2015 6:28:08 PM

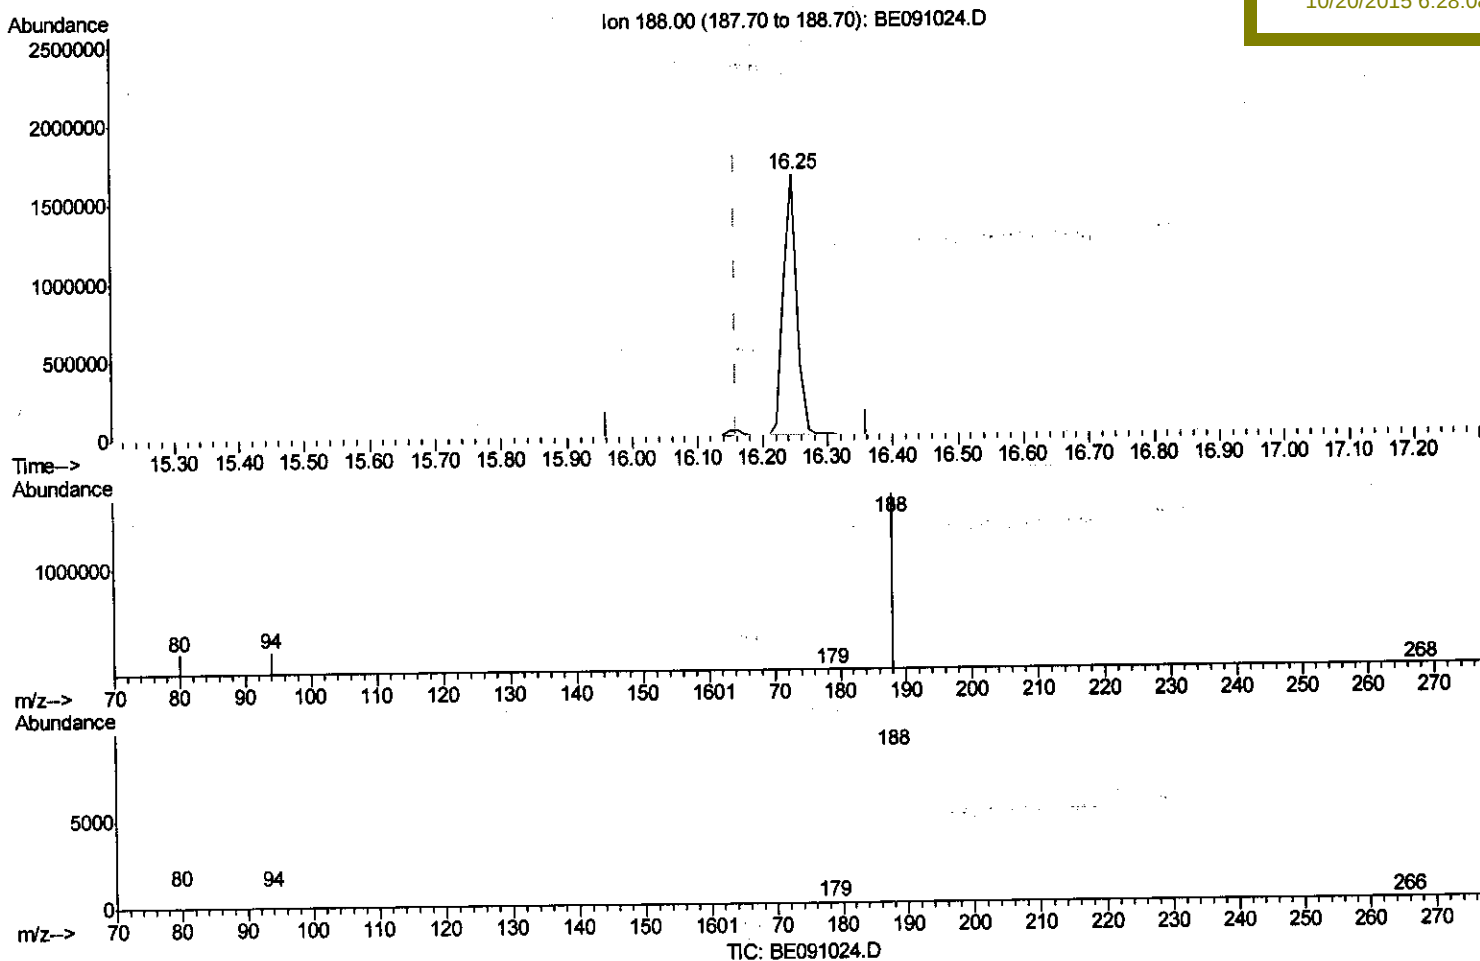

(10) Phenanthrene-d10 (I)

16.246min (+0.086) 0.40ng/ul

response 2345090

Ion	Exp%	Act%
188.00	100	100
94.00	16.90	12.61#
80.00	19.00	11.34#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_E\Data\BE101915\
 Data File : BE091024.D
 Acq On : 19 Oct 2015 17:16
 Operator : UM/NP
 Sample : G4075-17
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JG9M9

Quant Time: Oct 20 14:28:04 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE101415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 20 01:00:24 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMdadoda
 10/20/2015 6:28:08 PM

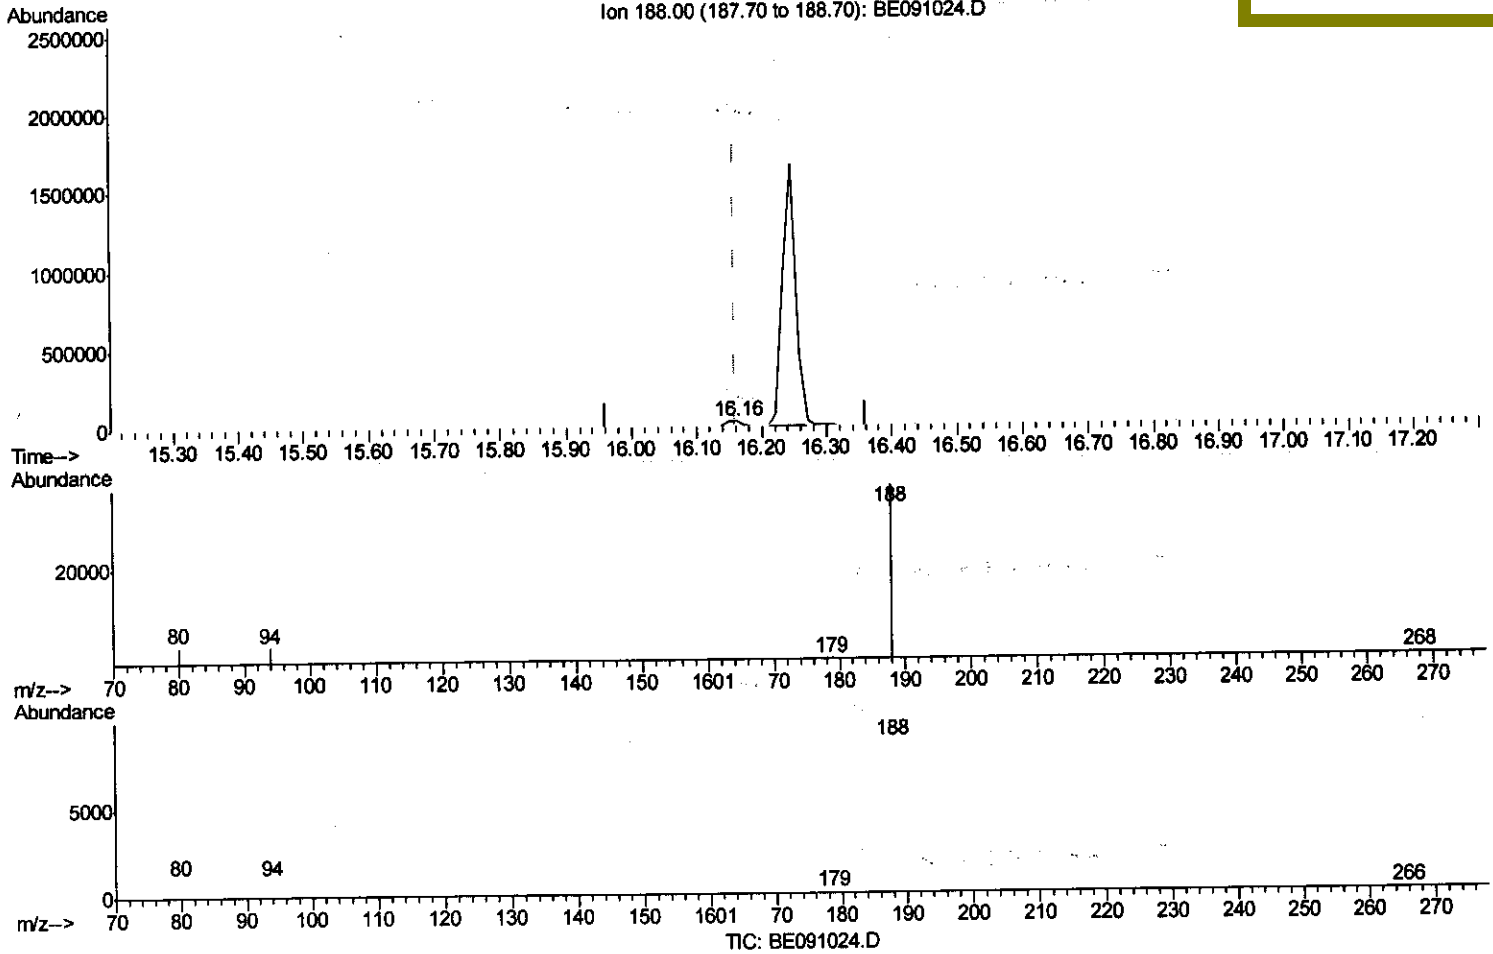

(10) Phenanthrene-d10 (I)

16.161min (+0.001) 0.40ng/ul m U.M
 response 55533 10/21/15

Ion	Exp%	Act%
188.00	100	100
94.00	16.90	8.98#
80.00	19.00	9.24#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE101915\
Data File : BE091024.D
Acq On : 19 Oct 2015 17:16
Operator : UM/NP
Sample : G4075-17
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JG9M9

Quant Time: Oct 20 14:30:56 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE101415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 20 01:00:24 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMdadoda
10/20/2015 6:28:08 PM

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	8686	0.40 ng/ul	0.00
2) Naphthalene-d8	9.61	136	41992	0.40 ng/ul	0.00
6) Acenaphthene-d10	13.43	164	24042	0.40 ng/ul	0.00
10) Phenanthrene-d10	16.16	188	55533m	0.40 ng/ul	0.00
16) Chrysene-d12	20.31	240	68560	0.40 ng/ul	0.00
20) Perylene-d12	22.21	264	98239	0.40 ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.12	152	11405	0.24 ng/ul	0.00
14) Fluoranthene-d10	18.15	212	31285	0.24 ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed