


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE101917\
Data File : BE094440.D
Acq On : 19 Oct 2017 9:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101617.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 16 14:54:40 2017

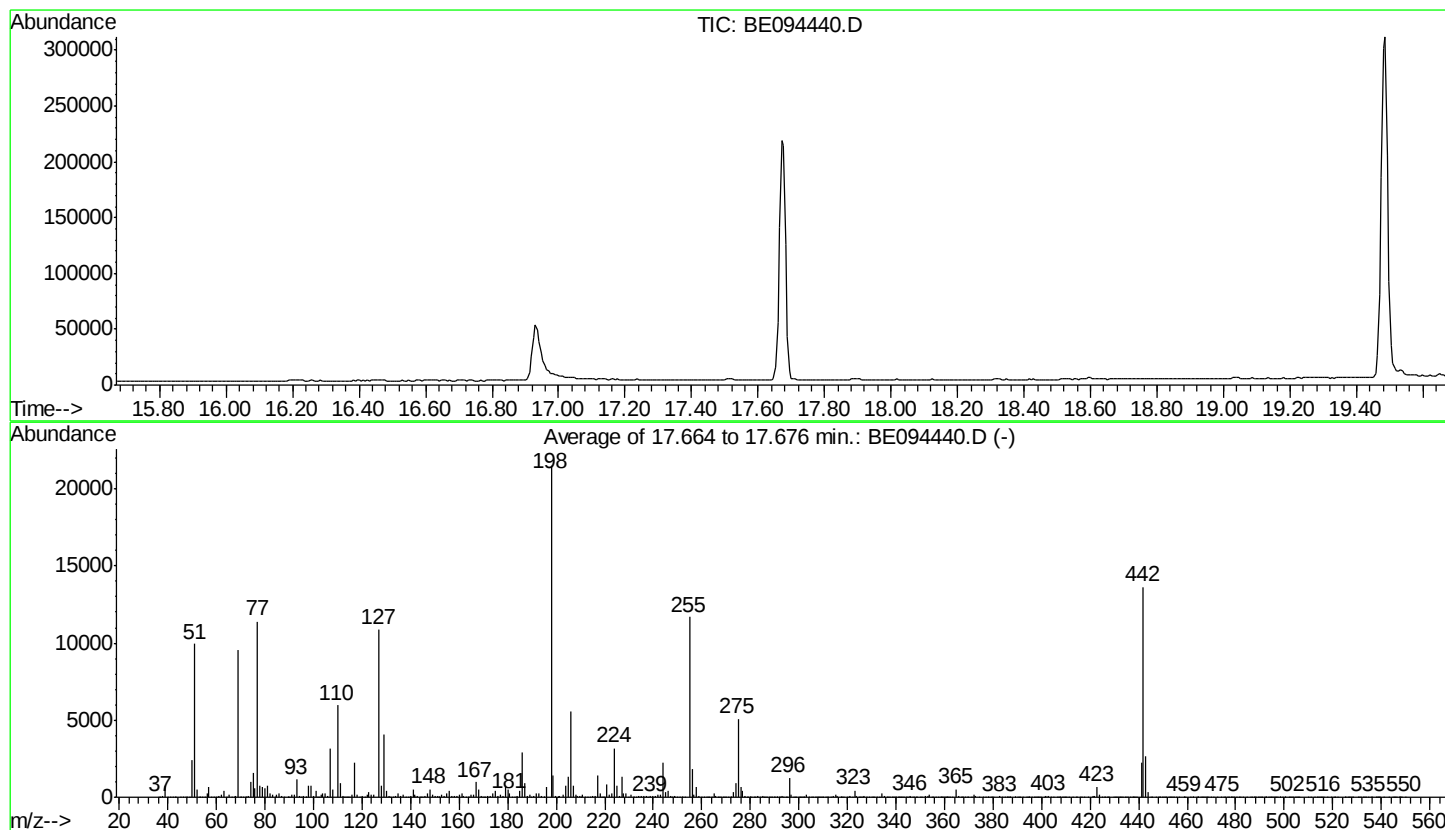

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	9935	PASS
68	69	0.00	2	0.8	74	PASS
69	198	0.00	100	44.4	9557	PASS
70	69	0.00	2	0.3	33	PASS
127	198	10	80	50.5	10867	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21503	PASS
199	198	5	9	6.7	1435	PASS
275	198	10	60	23.6	5084	PASS
365	198	1	100	2.5	532	PASS
441	442	0.01	24	16.2	2214	PASS
442	198	50	100	63.5	13657	PASS
443	442	15	24	19.3	2630	PASS