


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE101917\
 Data File : BE094456.D
 Acq On : 19 Oct 2017 20:51
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 16 14:54:40 2017

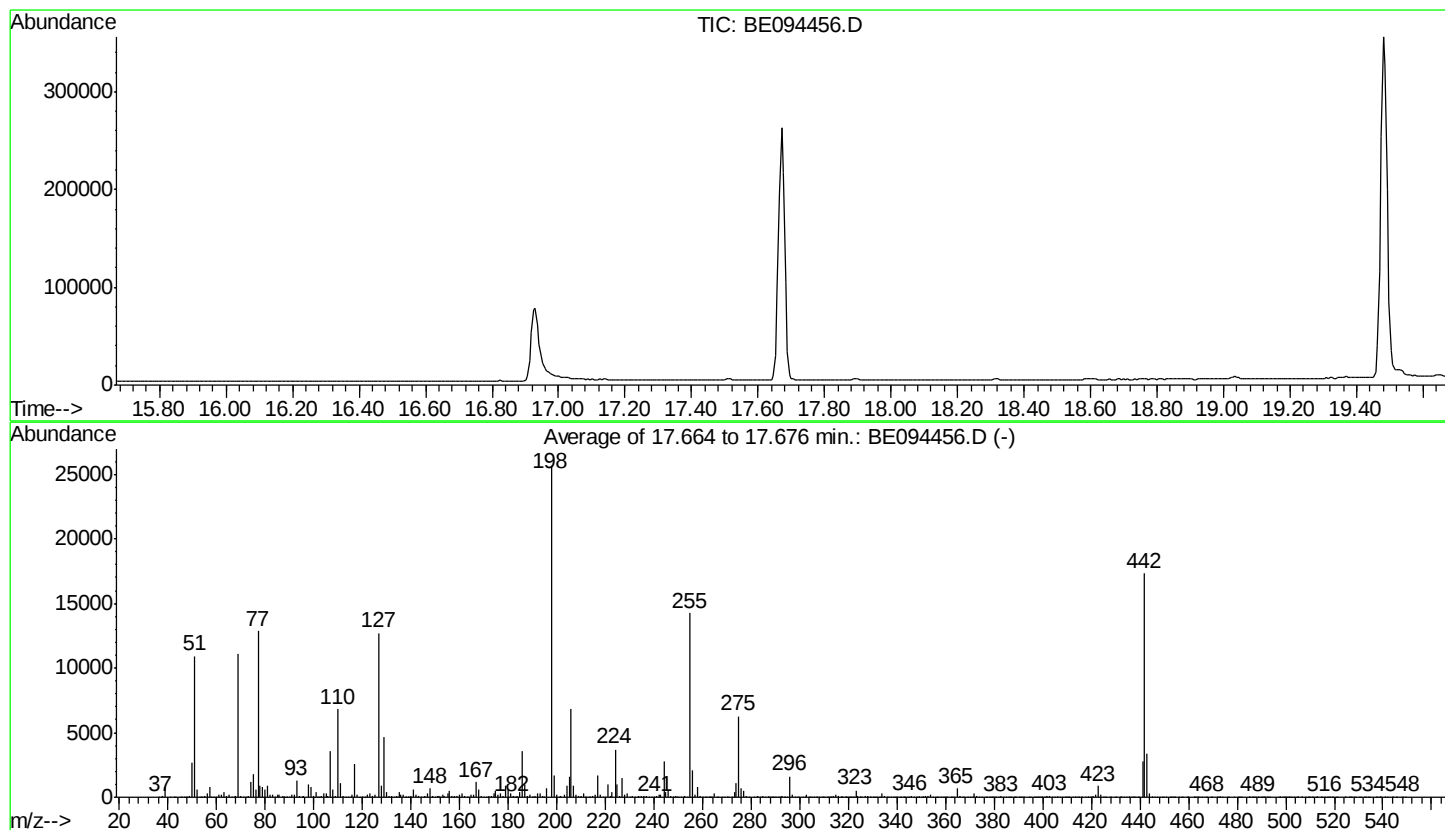

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	10945	PASS
68	69	0.00	2	0.5	57	PASS
69	198	0.00	100	43.2	11080	PASS
70	69	0.00	2	0.6	62	PASS
127	198	10	80	49.6	12736	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25670	PASS
199	198	5	9	6.6	1703	PASS
275	198	10	60	24.4	6251	PASS
365	198	1	100	2.6	662	PASS
441	442	0.01	24	16.0	2766	PASS
442	198	50	100	67.5	17337	PASS
443	442	15	24	19.6	3392	PASS