


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE101918\
 Data File : BE097984.D
 Acq On : 19 Oct 2018 9:07
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 15:36:44 2018

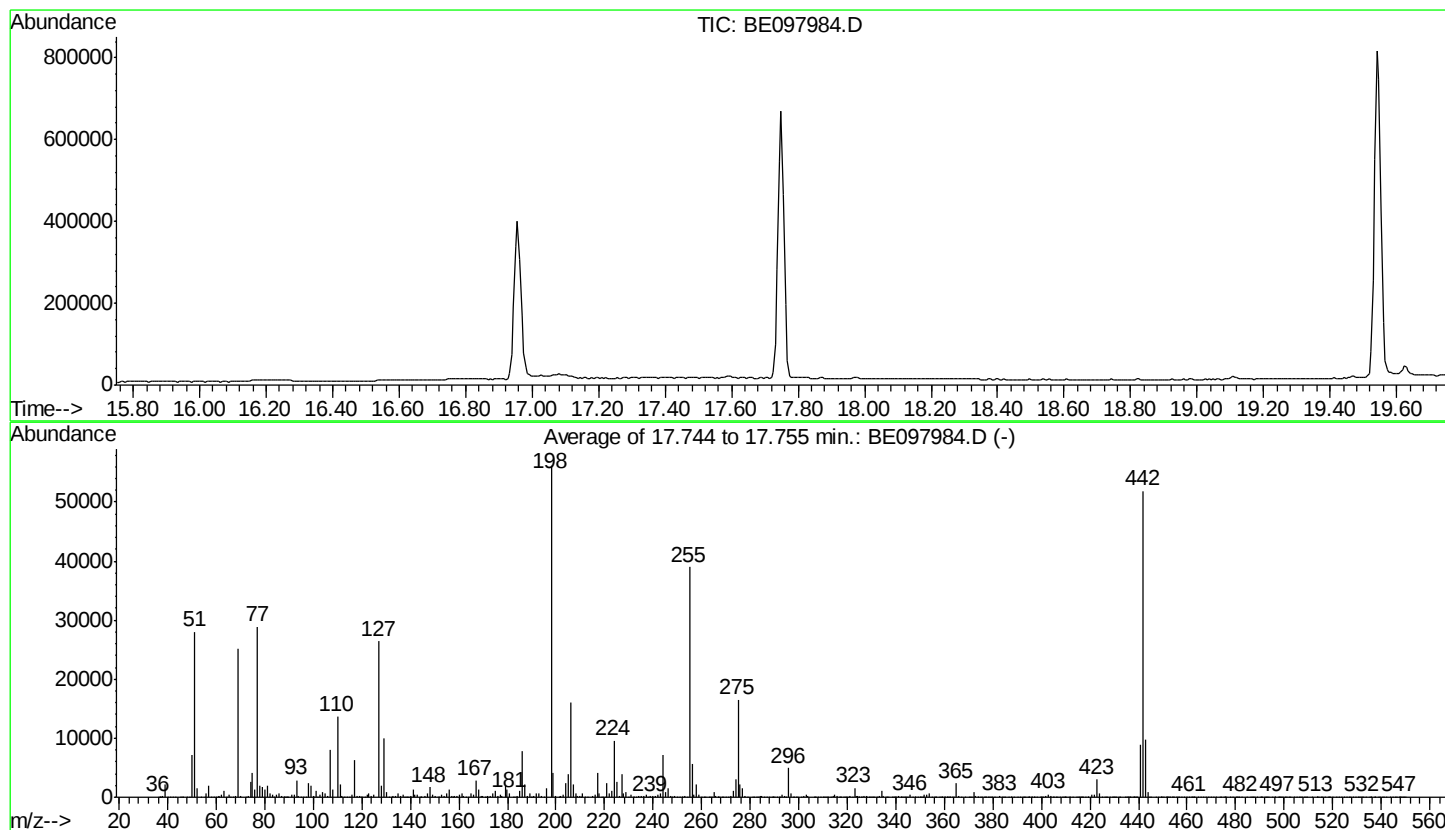

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.8	27991	PASS
68	69	0.00	2	0.5	136	PASS
69	198	0.00	100	44.9	25207	PASS
70	69	0.00	2	0.6	147	PASS
127	198	10	80	46.9	26355	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56173	PASS
199	198	5	9	7.2	4020	PASS
275	198	10	60	29.4	16489	PASS
365	198	1	100	4.1	2292	PASS
441	198	0.01	100	15.7	8808	PASS
442	198	50	100	92.5	51933	PASS
443	442	15	24	18.7	9692	PASS