


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE101918\
 Data File : BE097990.D
 Acq On : 19 Oct 2018 13:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE101618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 15:36:44 2018

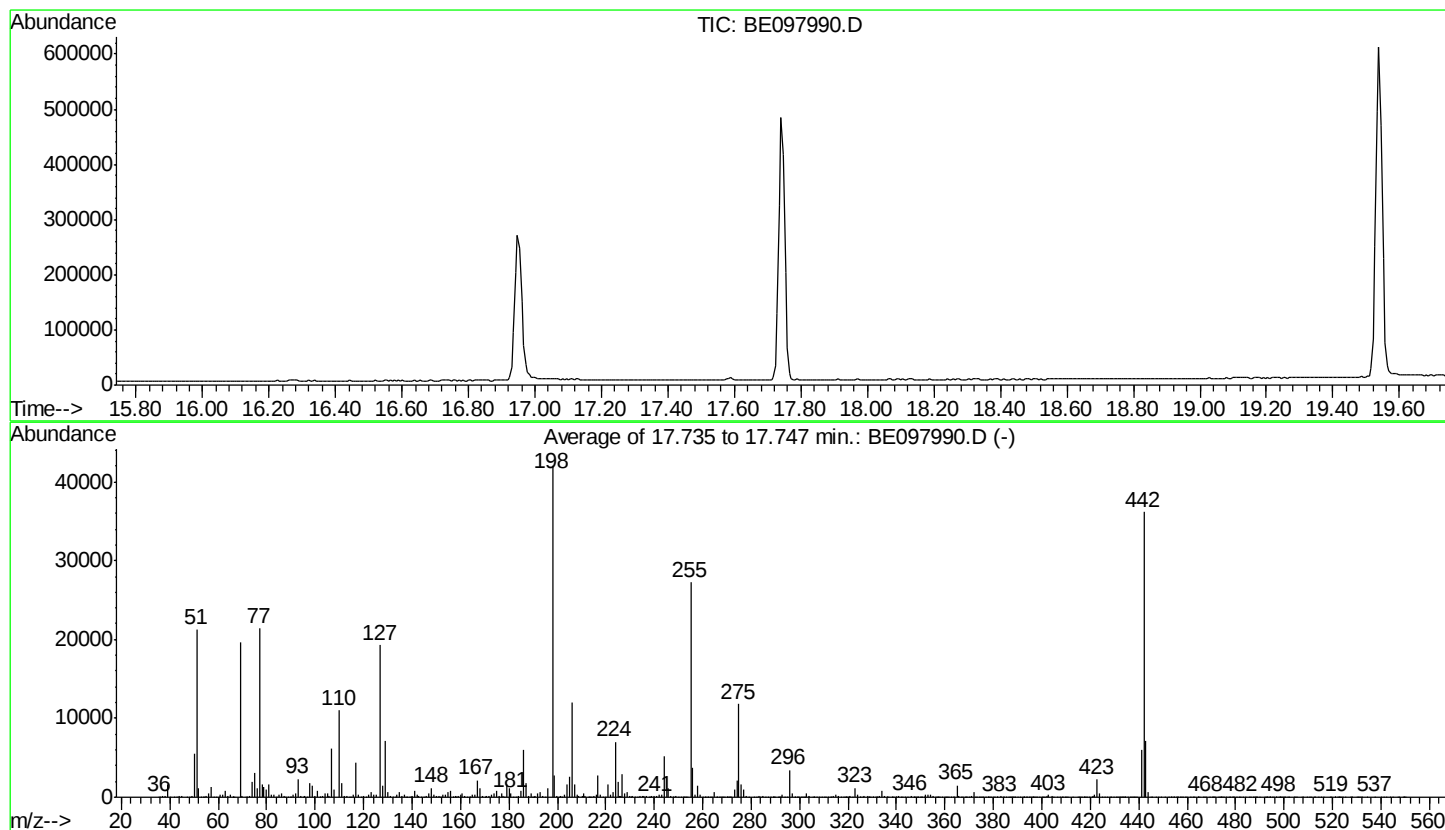

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	21192	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.6	19581	PASS
70	69	0.00	2	0.6	118	PASS
127	198	10	80	45.8	19275	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42042	PASS
199	198	5	9	6.6	2793	PASS
275	198	10	60	28.1	11806	PASS
365	198	1	100	3.6	1497	PASS
441	198	0.01	100	14.4	6067	PASS
442	198	50	100	86.0	36141	PASS
443	442	15	24	19.9	7180	PASS