


Data Path : Z:\HPCHEM1\BNA_E\Data\BE102014\
 Data File : Be088114.d
 Acq On : 20 Oct 2014 15:46
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE102014.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 21 02:11:14 2014

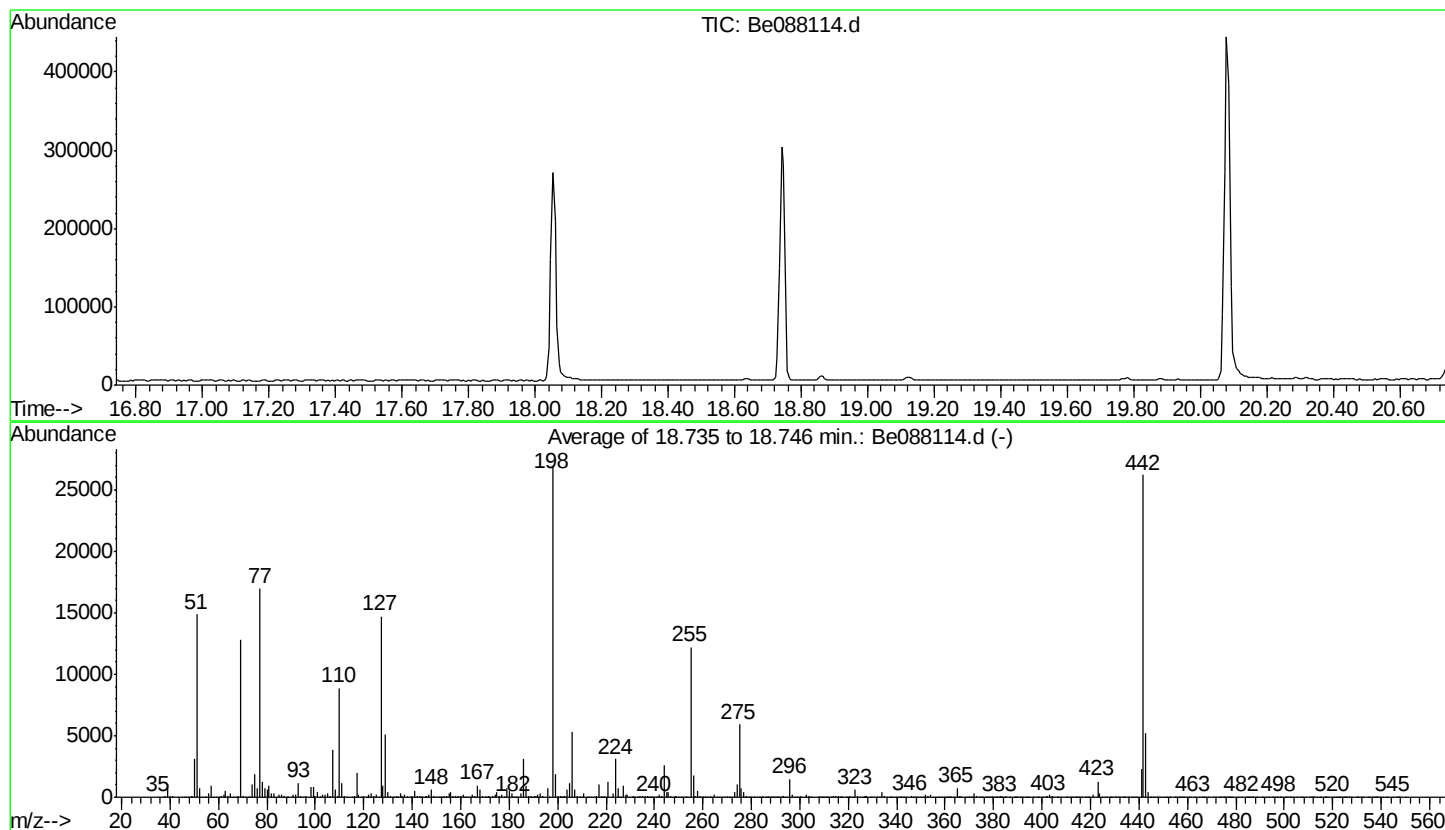

AutoFind: Scans 2646, 2647, 2648; Background Corrected with Scan 2639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.1	14854	PASS
68	69	0.00	2	0.8	97	PASS
69	198	0.00	100	47.3	12764	PASS
70	69	0.00	2	0.5	59	PASS
127	198	10	80	54.5	14706	PASS
197	198	0.00	2	0.1	29	PASS
198	198	100	100	100.0	26964	PASS
199	198	5	9	6.8	1843	PASS
275	198	10	60	21.9	5907	PASS
365	198	1	100	2.8	743	PASS
441	442	0.01	24	8.6	2246	PASS
442	198	50	100	97.2	26219	PASS
443	442	15	24	19.9	5212	PASS