

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
 Data File : BE094470.D
 Acq On : 20 Oct 2017 12:20
 Operator : SJ/JU
 Sample : PB103287BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 22 02:46:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 18 17:51:02 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1408	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	7637	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	4757	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.42	240	9993	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	683474	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	3985	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	9911	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
9) Fluorene	15.51	166	1182	0.066	ng/ul#	22
17) Pyrene	19.64	202	1254	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094470.D
Acq On : 20 Oct 2017 12:20
Operator : SJ/JU
Sample : PB103287BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 22 02:46:34 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

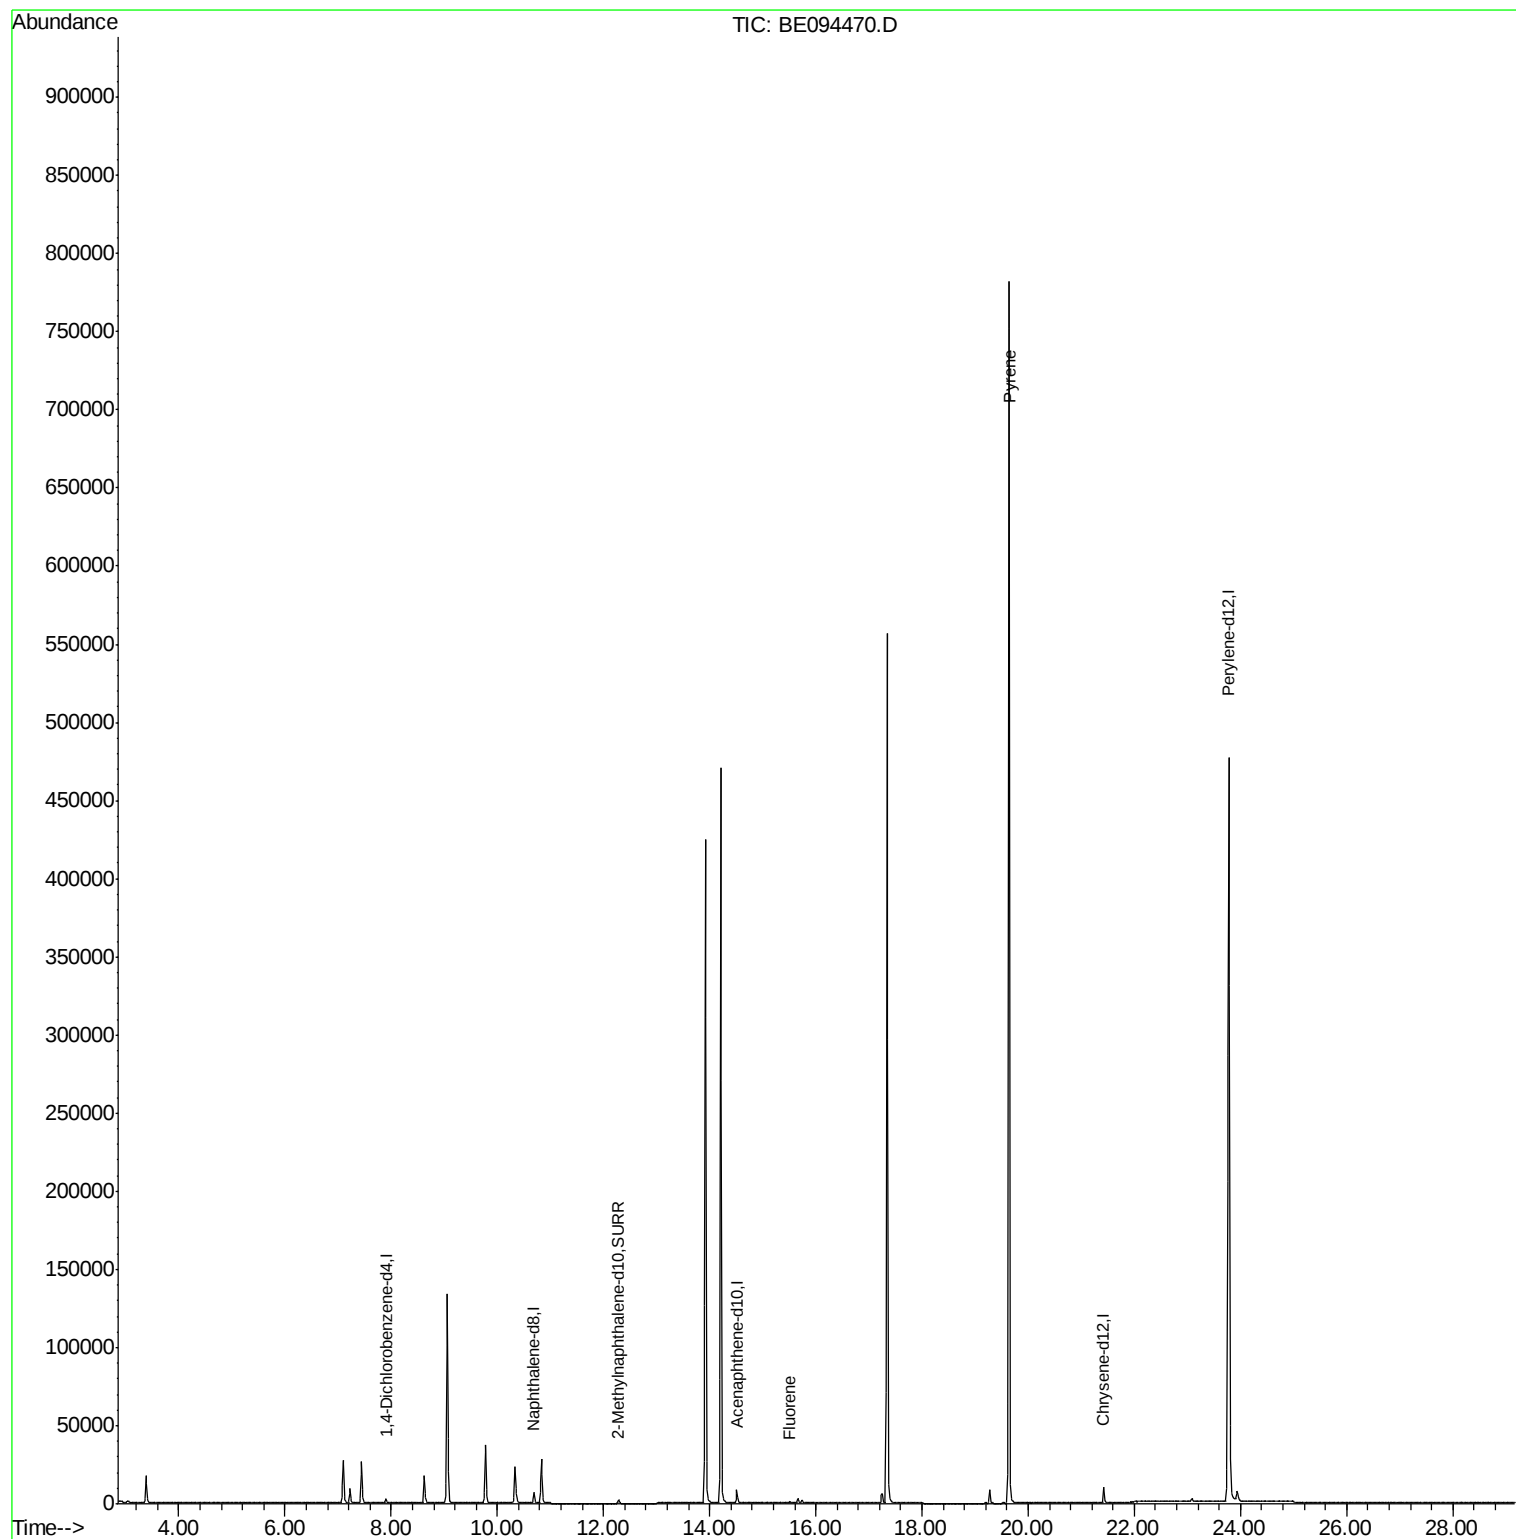

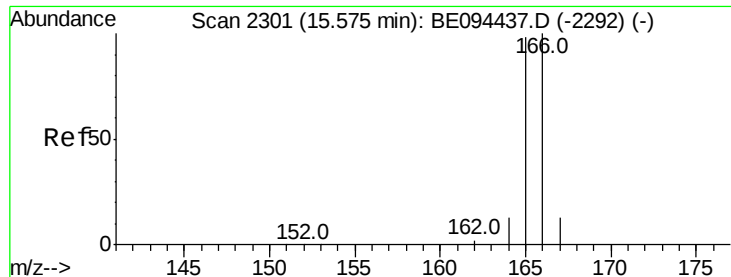

#9

Fluorene

Concen: 0.066 ng/ul

RT: 15.51 min Scan# 2292

Delta R.T. -0.07 min

Lab File: BE094470.D

Acq: 20 Oct 2017 12:20

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 1182

Ion Ratio Lower Upper

166 100

165 10.5 73.4 110.2#

167 36.0 14.6 22.0#

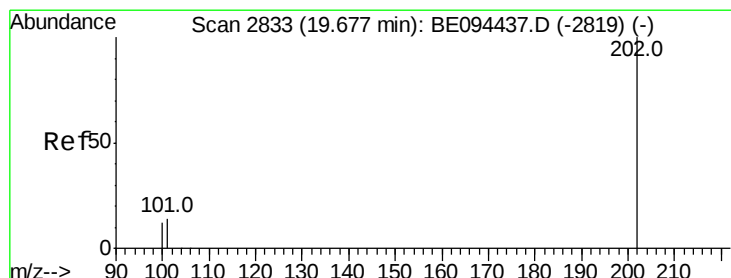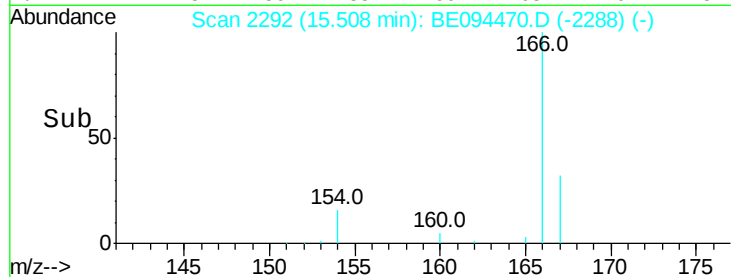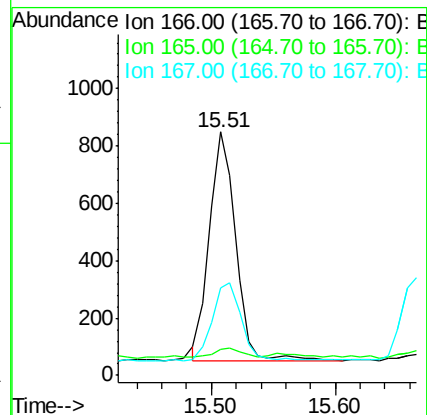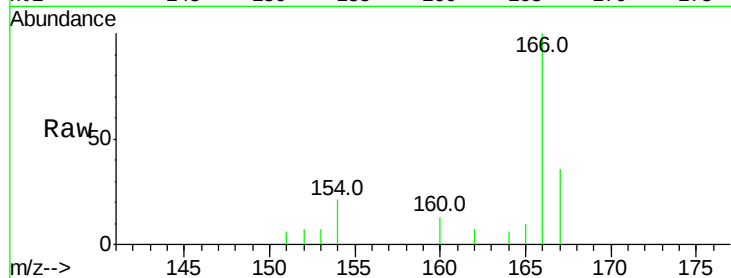

#17

Pyrene

Concen: 0.045 ng/ul

RT: 19.64 min Scan# 2826

Delta R.T. -0.04 min

Lab File: BE094470.D

Acq: 20 Oct 2017 12:20

Tgt Ion:202 Resp: 1254

Ion Ratio Lower Upper

202 100

101 165.9 18.2 27.4#

100 869.0 15.6 23.4#

