

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
 Data File : BE094472.D
 Acq On : 20 Oct 2017 13:32
 Operator : SJ/JU
 Sample : I5840-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 22 02:46:47 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 18 17:51:02 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1438	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	7991	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	5012	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.42	240	10381	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	806499	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	4342	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	11979	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.64	202	1594	0.055	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094472.D
Acq On : 20 Oct 2017 13:32
Operator : SJ/JU
Sample : I5840-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 22 02:46:47 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

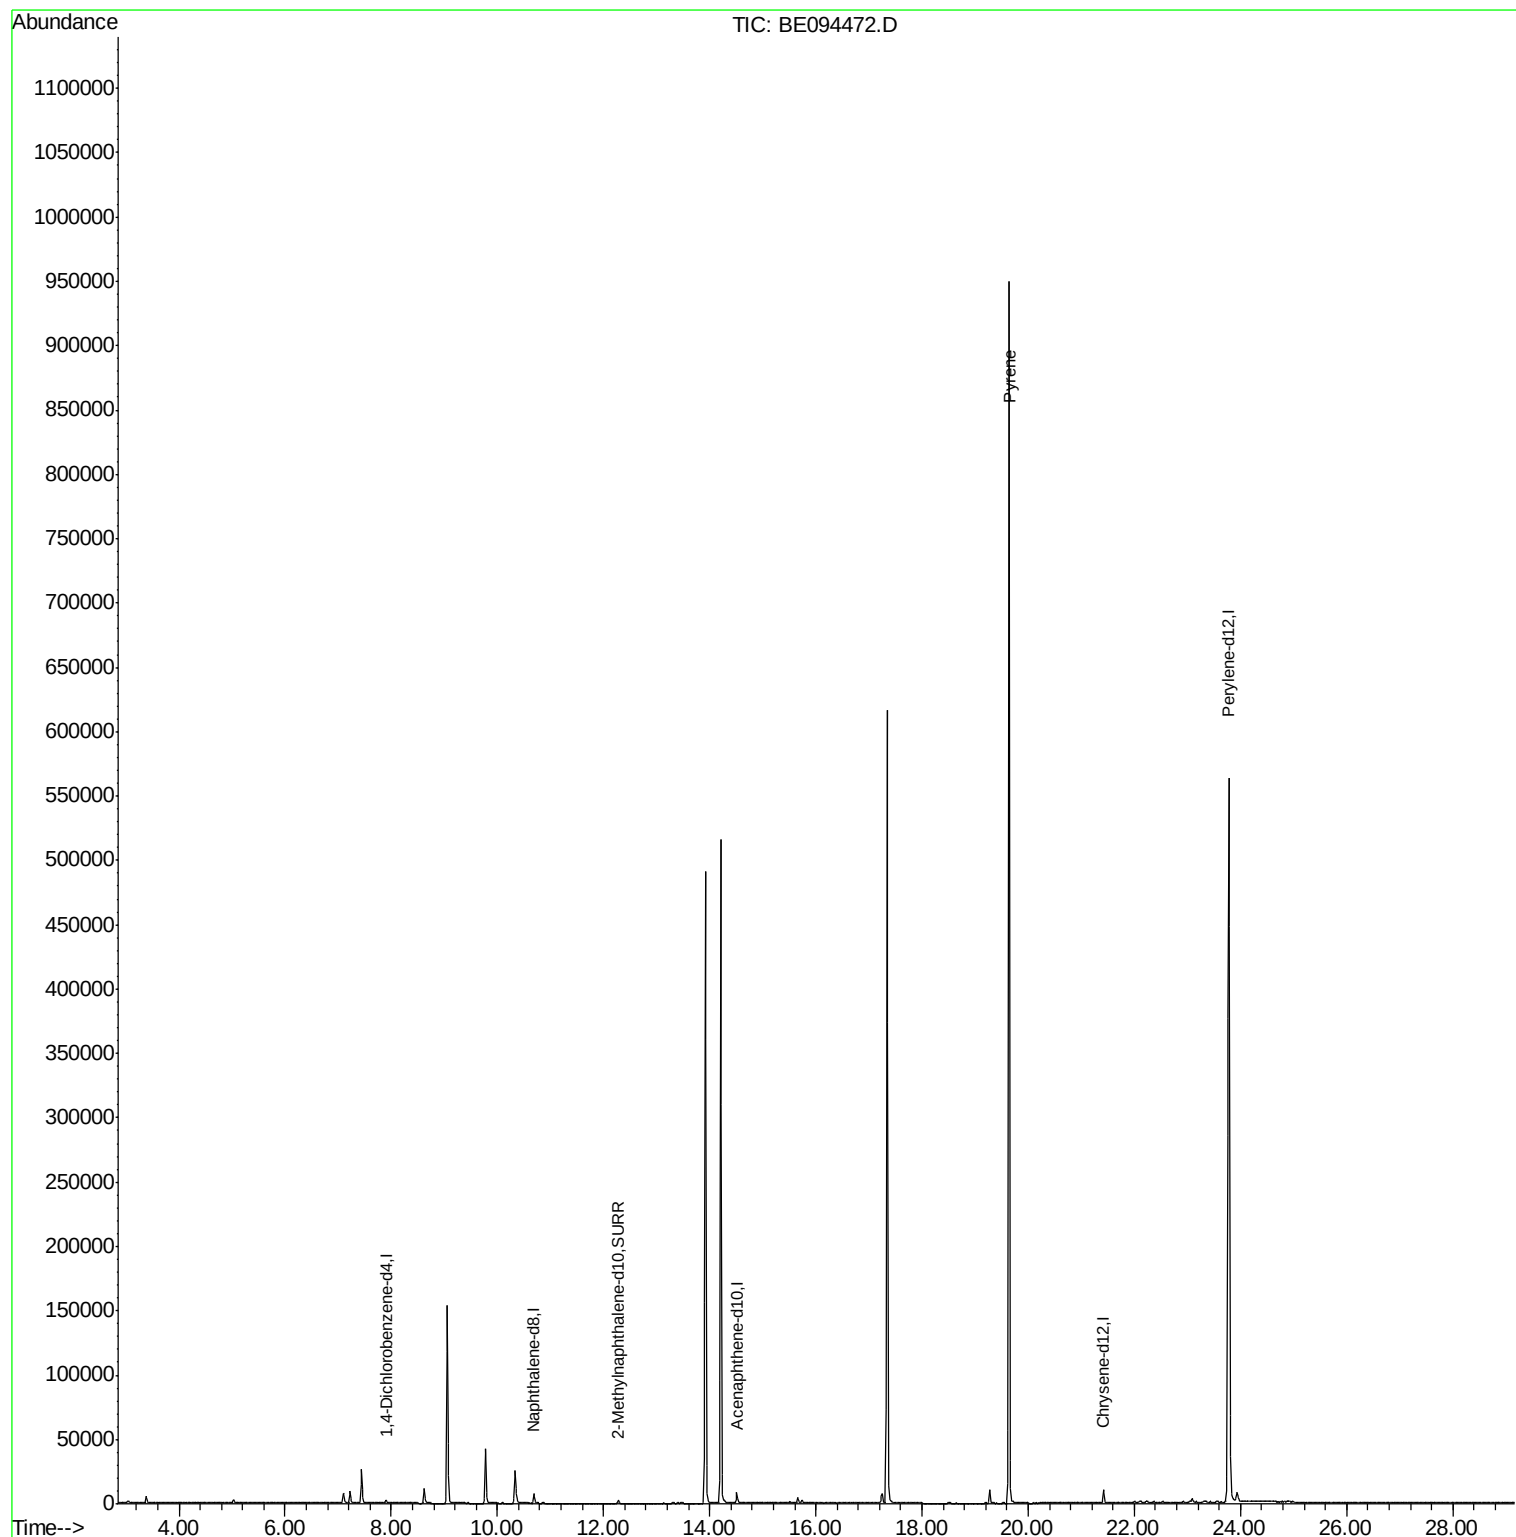


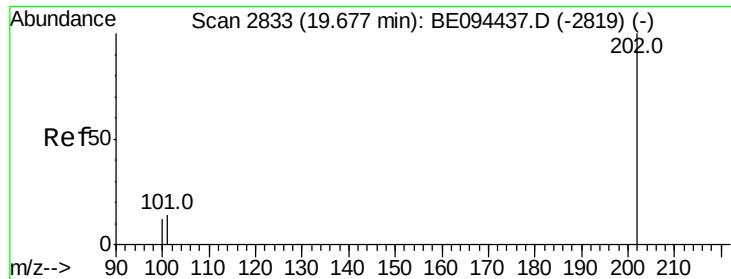

#17
 Pvrene
 Concen: 0.055 ng/ul
 RT: 19.64 min Scan# 2826
 Delta R.T. -0.04 min
 Lab File: BE094472.D
 Acq: 20 Oct 2017 13:32

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:202 Resp: 1594
 Ion Ratio Lower Upper
 202 100
 101 164.0 18.2 27.4#
 100 904.9 15.6 23.4#

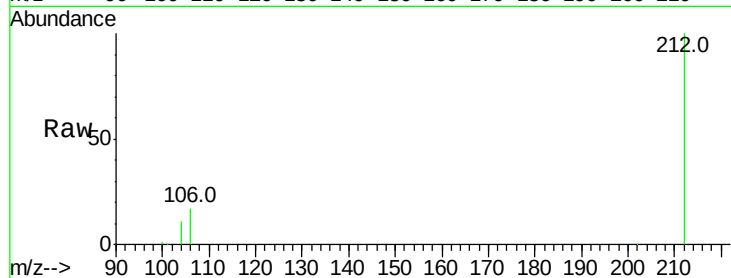

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): BE

