

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
 Data File : BE094490.D
 Acq On : 21 Oct 2017 00:34
 Operator : SJ/JU
 Sample : I5840-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Oct 22 02:49:10 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 18 17:51:02 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1355	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	7577	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	4890	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.26
16) Chrysene-d12	21.42	240	10634	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	748803	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	4111	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.27	212	11084	0.00	ng/ul	-0.01
Target Compounds						
3) Naphthalene	10.73	128	393	0.021	ng/ul#	60
17) Pyrene	19.64	202	1474	0.050	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094490.D
Acq On : 21 Oct 2017 00:34
Operator : SJ/JU
Sample : I5840-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Oct 22 02:49:10 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

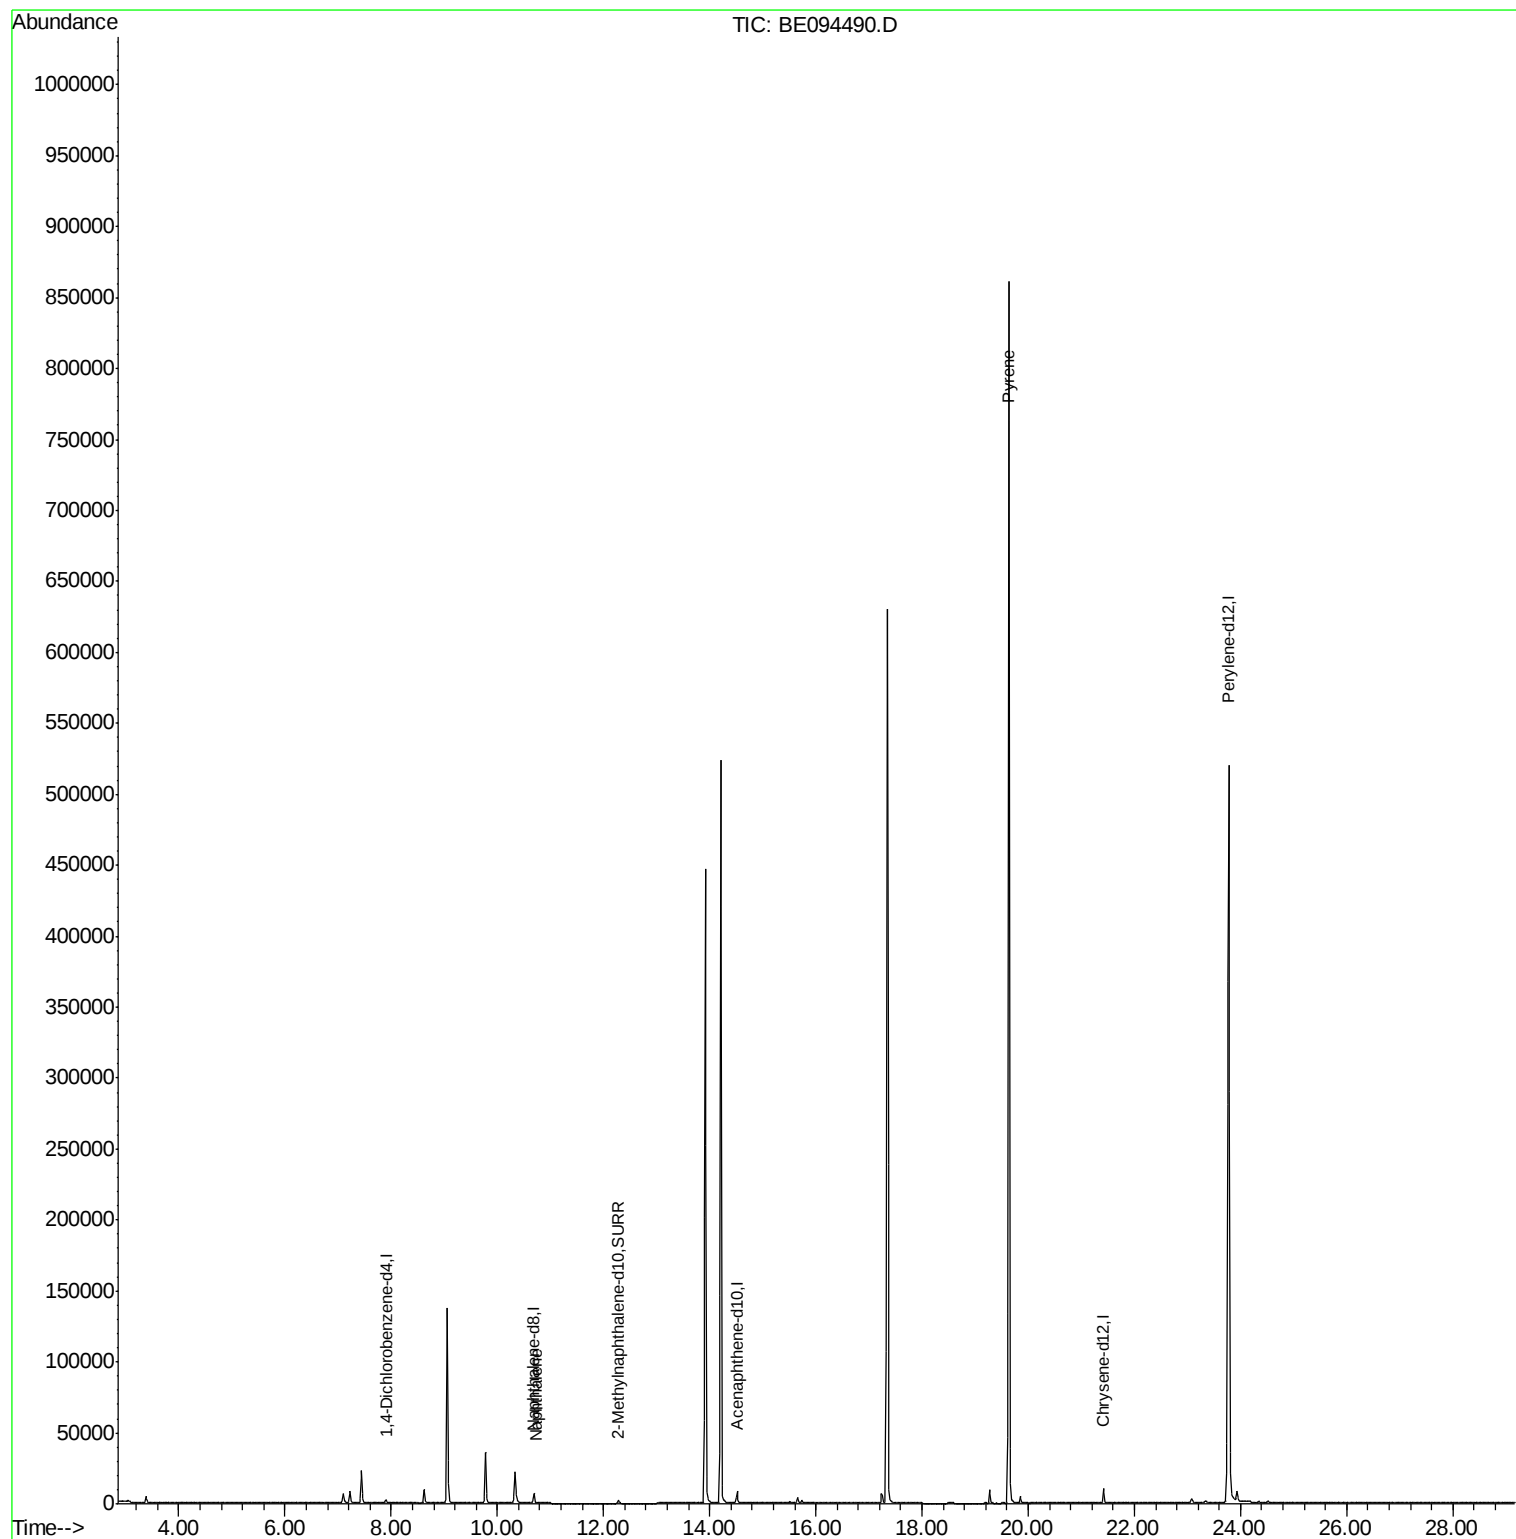

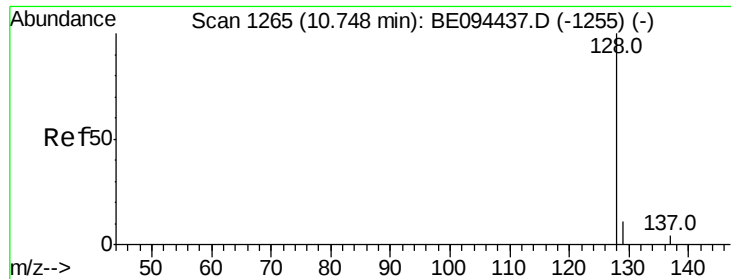

#3

Naphthalene

Concen: 0.021 ng/ul

RT: 10.73 min Scan# 1262

Delta R.T. -0.01 min

Lab File: BE094490.D

Acq: 21 Oct 2017 00:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 393

Ion Ratio Lower Upper

128 100

129 34.2 11.3 16.9#




127 0.0 4.0 6.0#

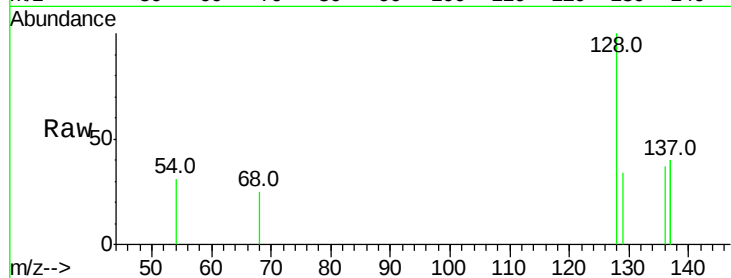

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

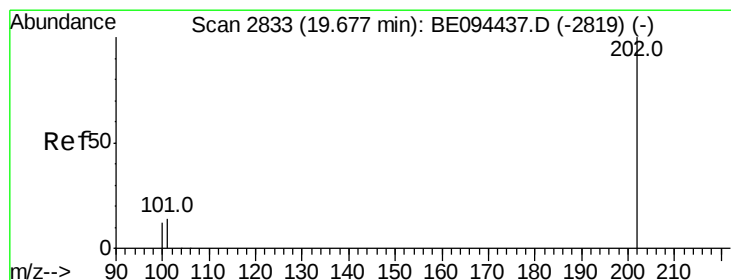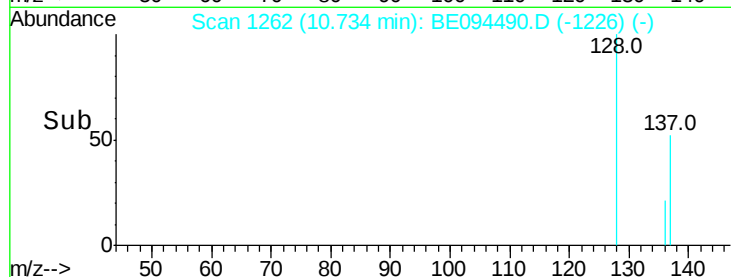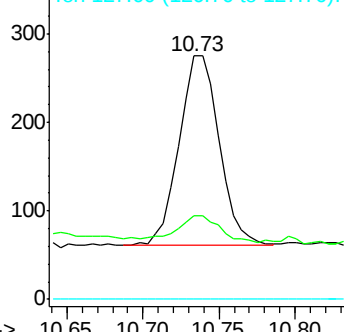

#17

Pyrene

Concen: 0.050 ng/ul

RT: 19.64 min Scan# 2825

Delta R.T. -0.04 min

Lab File: BE094490.D

Acq: 21 Oct 2017 00:34


Tgt Ion:202 Resp: 1474

Ion Ratio Lower Upper

202 100

101 163.0 18.2 27.4#

100 903.8 15.6 23.4#

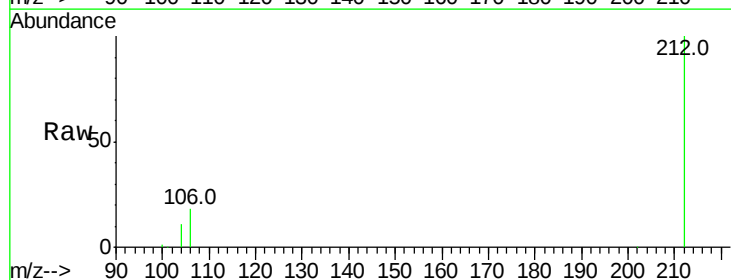

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

