




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094468.D
Acq On : 20 Oct 2017 11:05
Operator : SJ/JU
Sample : PB103279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK79

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:39 PM

Quant Time: Oct 22 02:46:18 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

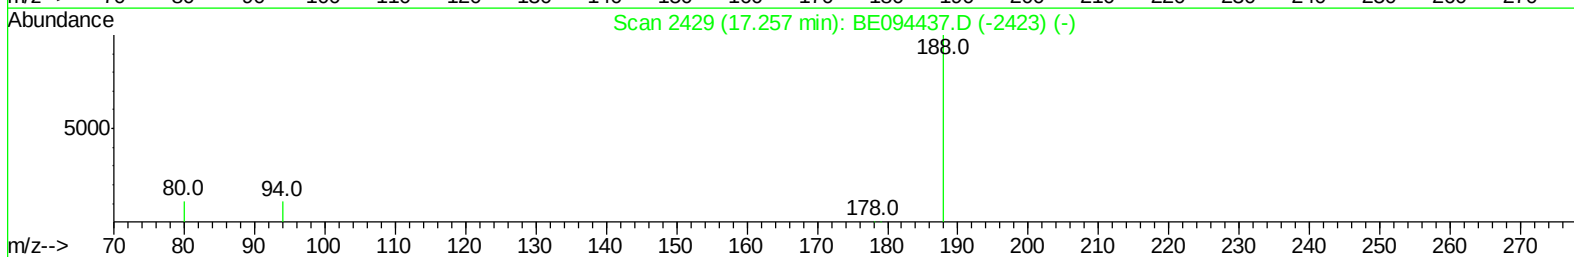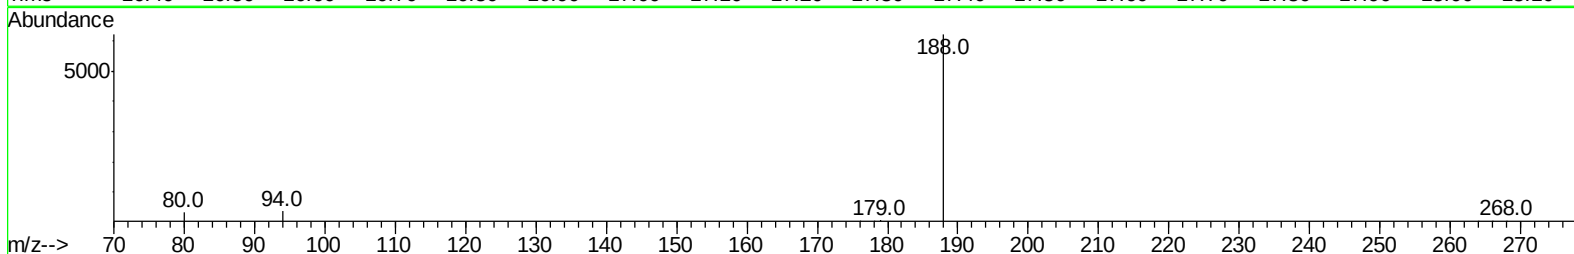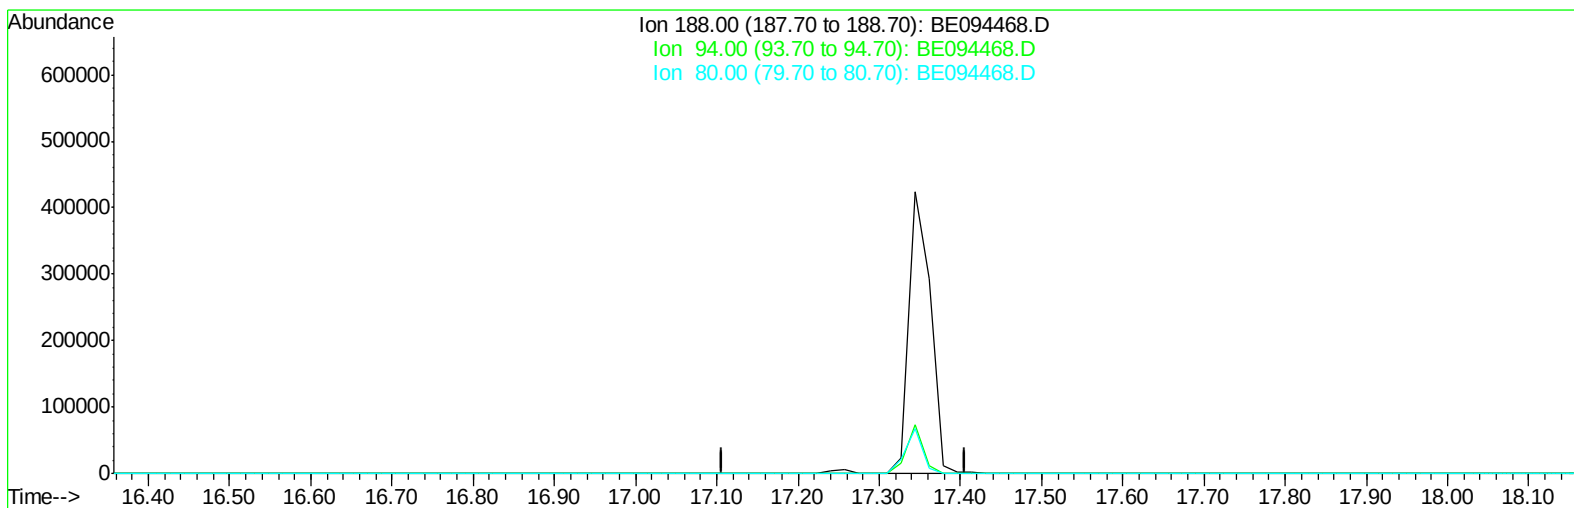

TIC: BE094468.D

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094468.D
Acq On : 20 Oct 2017 11:05
Operator : SJ/JU
Sample : PB103279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK79

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:39 PM

Quant Time: Oct 22 02:46:18 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

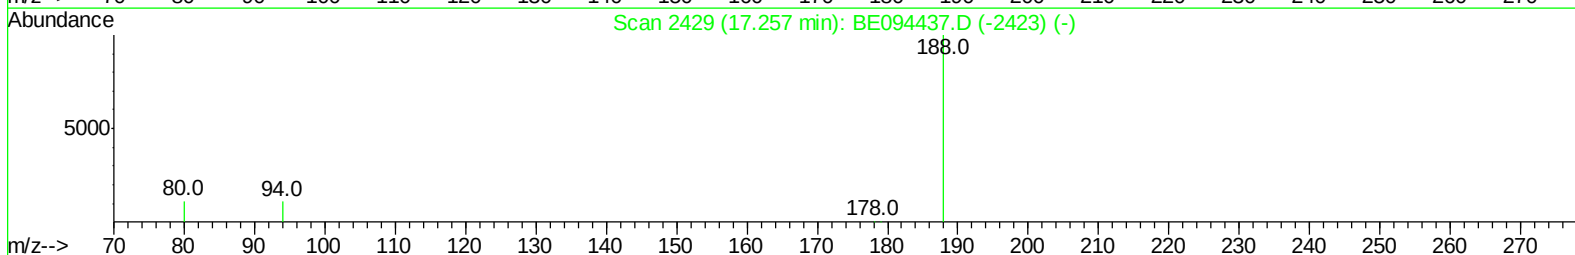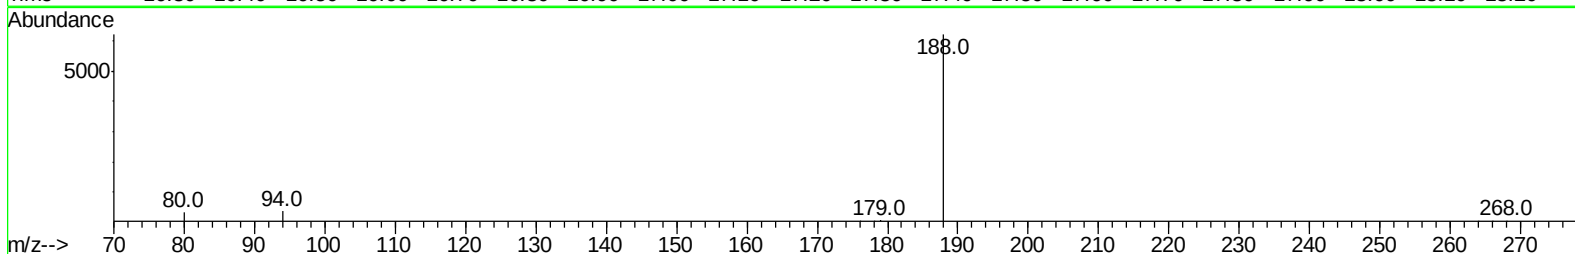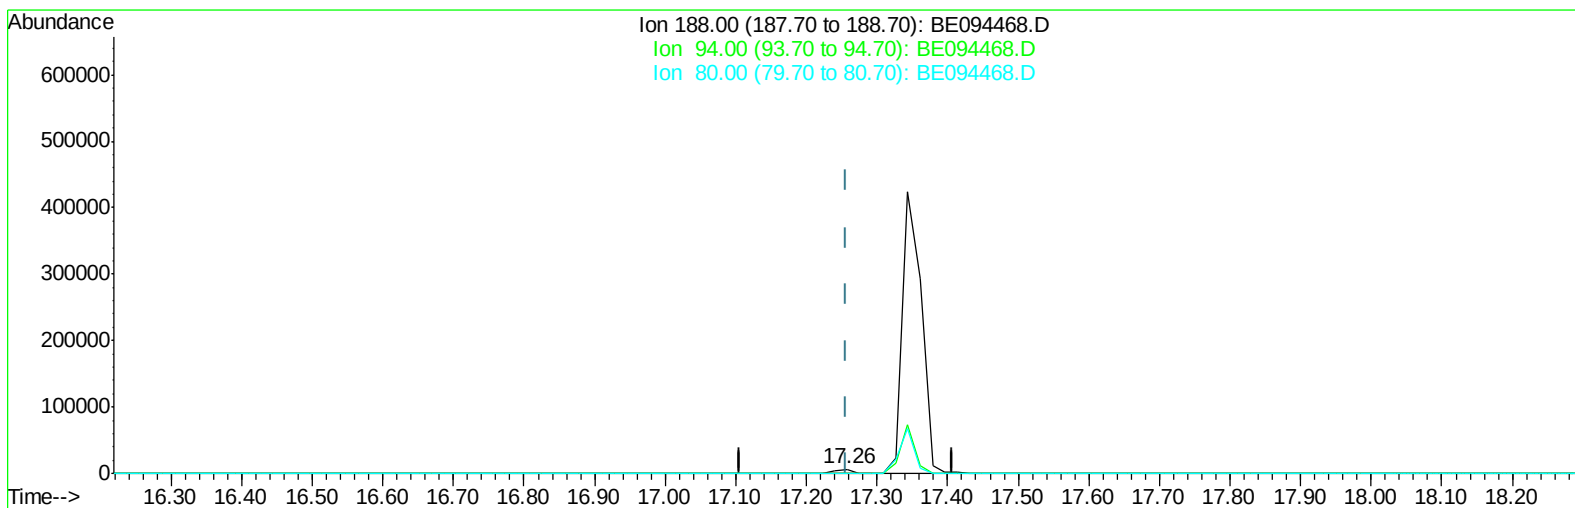

TIC: BE094468.D

(10) Phenanthrene-d10 (I)

17.257min (+0.000) 0.40ng/ul m

response 10589

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.00#
80.00	11.80	5.42#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094468.D
Acq On : 20 Oct 2017 11:05
Operator : SJ/JU
Sample : PB103279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK79

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:39 PM

Quant Time: Oct 22 02:53:41 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

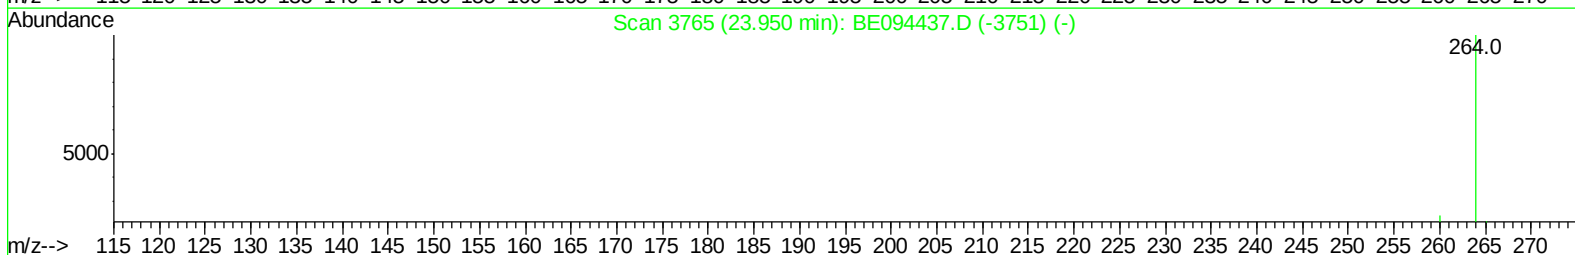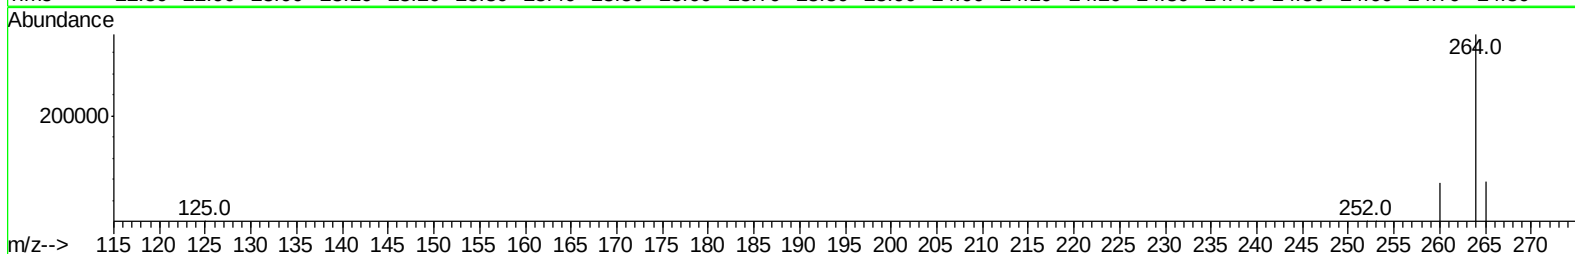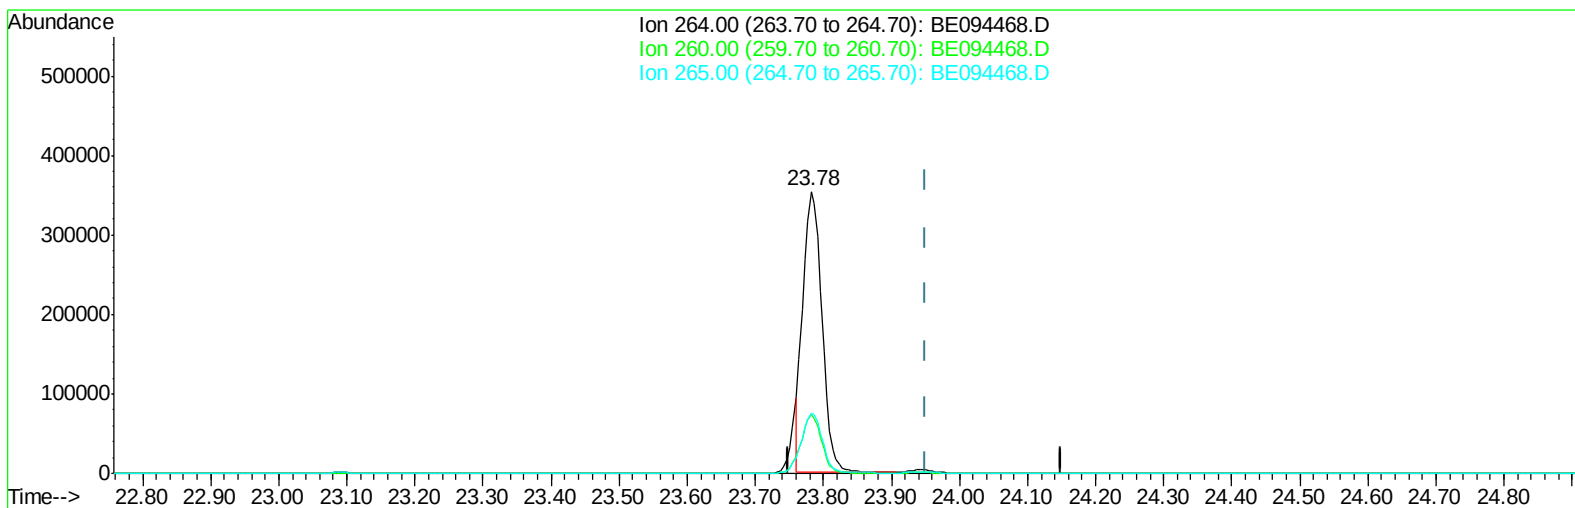

TIC: BE094468.D

(20) Perylene-d12 (I)

23.782min (-0.168) 0.40ng/ul

response 689920

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.84#
265.00	103.50	21.54#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094468.D
Acq On : 20 Oct 2017 11:05
Operator : SJ/JU
Sample : PB103279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK79

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:39 PM

Quant Time: Oct 22 02:55:19 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

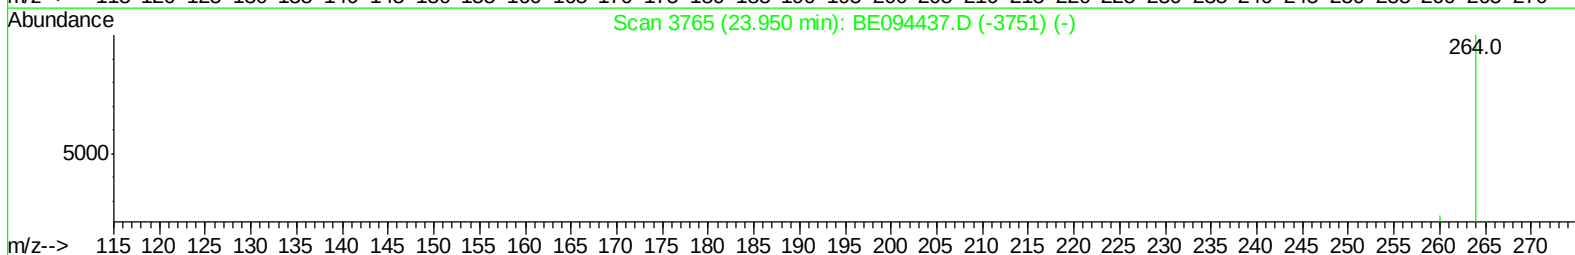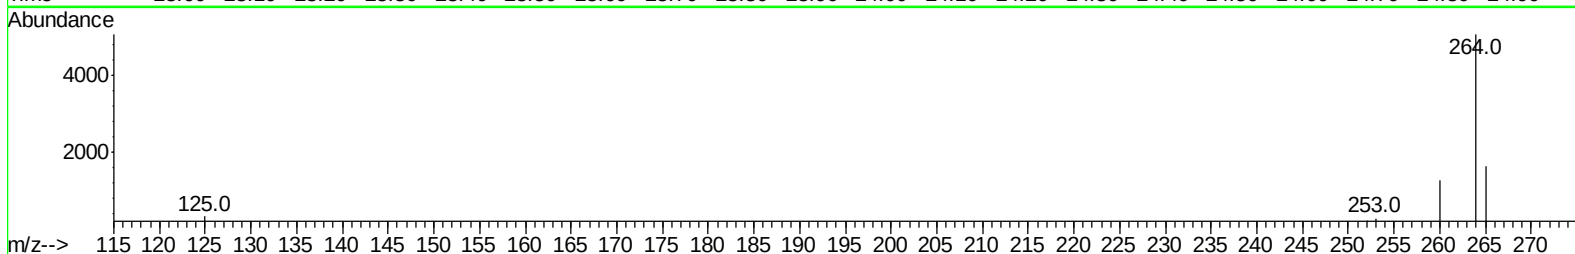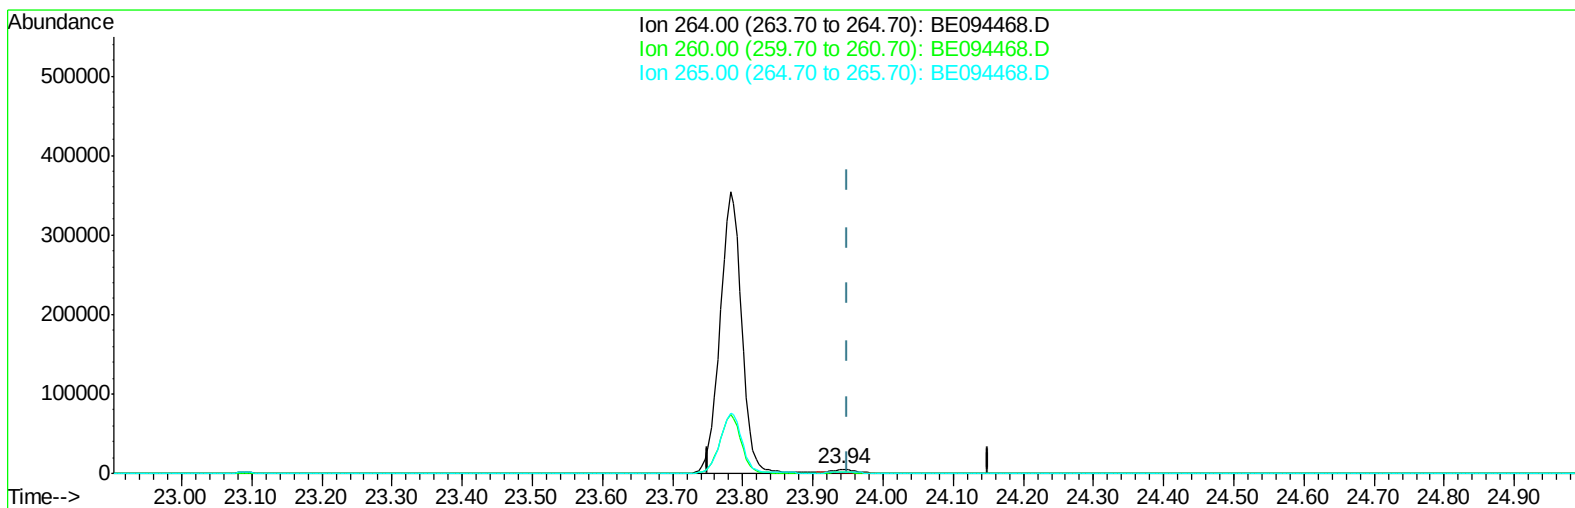

TIC: BE094468.D

(20) Perylene-d12 (I)

23.942min (-0.009) 0.40ng/ul m

response 9064

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.10
265.00	103.50	31.96#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
 Data File : BE094468.D
 Acq On : 20 Oct 2017 11:05
 Operator : SJ/JU
 Sample : PB103279BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK79

Manual Integrations
 APPROVED

Sohil
 10/23/2017 3:13:39 PM

Quant Time: Oct 22 02:55:19 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 18 17:51:02 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	1361	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	7444	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	4745	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	10589m	0.40	ng/ul	0.00
16) Chrysene-d12	21.43	240	10263	0.40	ng/ul	0.00
20) Perylene-d12	23.94	264	9064m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3889	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	10120	0.29	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094468.D
Acq On : 20 Oct 2017 11:05
Operator : SJ/JU
Sample : PB103279BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK79

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:39 PM

Quant Time: Oct 22 02:55:19 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

