




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094475.D
Acq On : 20 Oct 2017 15:22
Operator : SJ/JU
Sample : I5840-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:52 PM

Quant Time: Oct 22 02:47:12 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

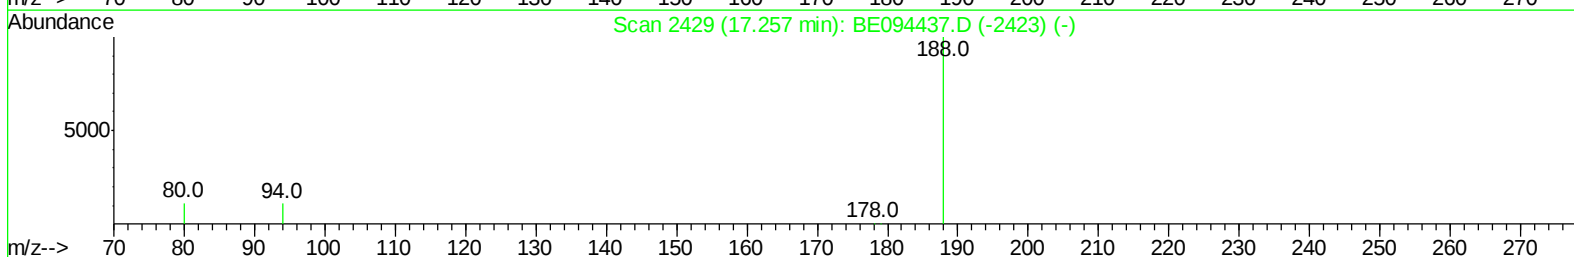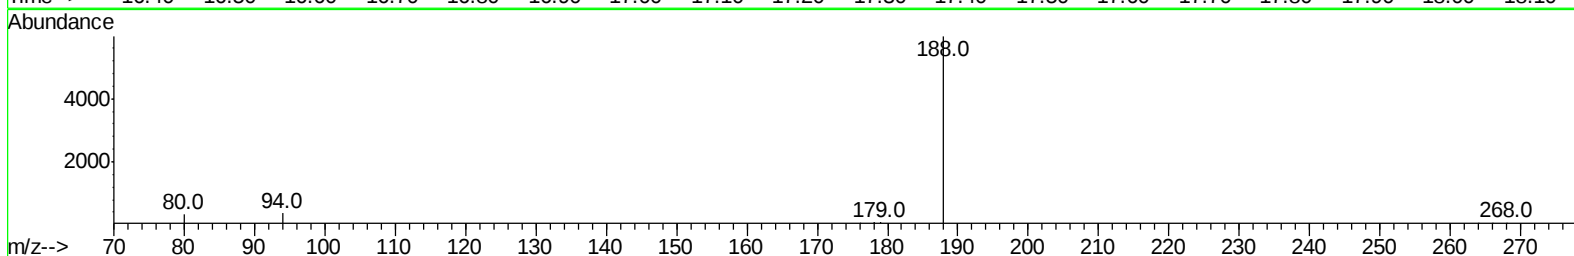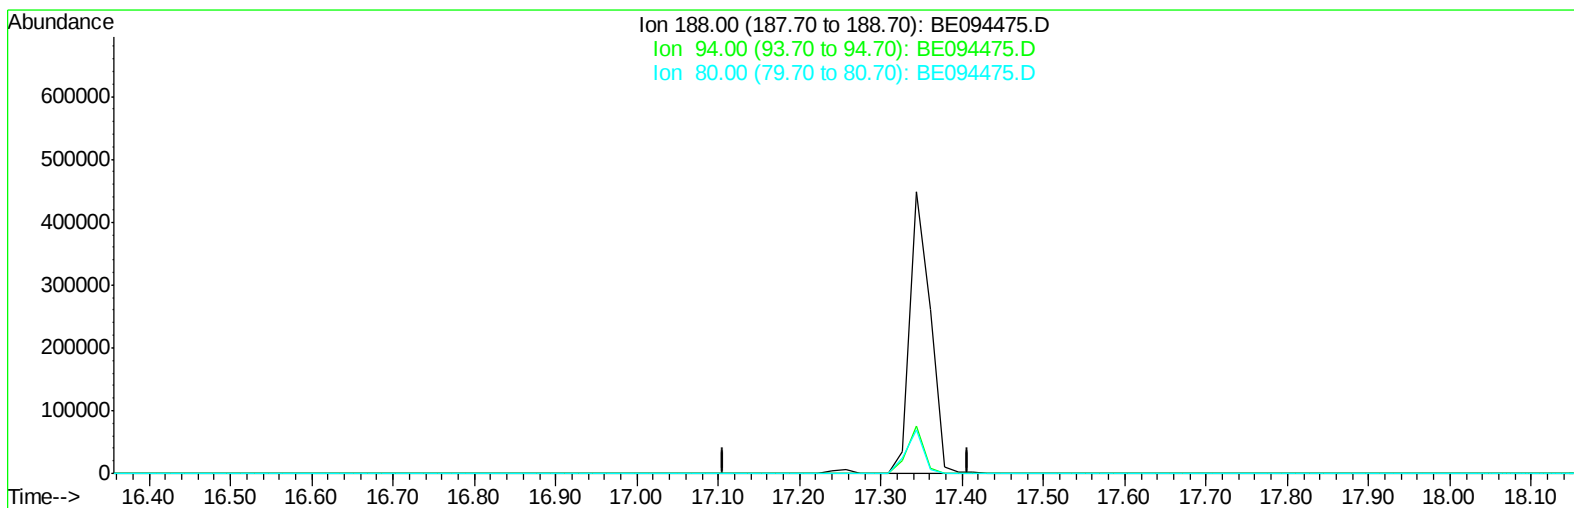

TIC: BE094475.D

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094475.D
Acq On : 20 Oct 2017 15:22
Operator : SJ/JU
Sample : I5840-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:52 PM

Quant Time: Oct 22 02:47:12 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

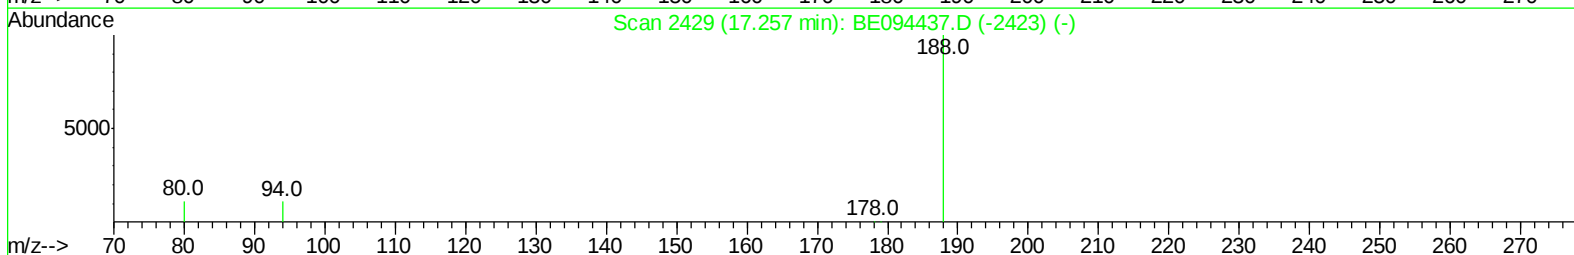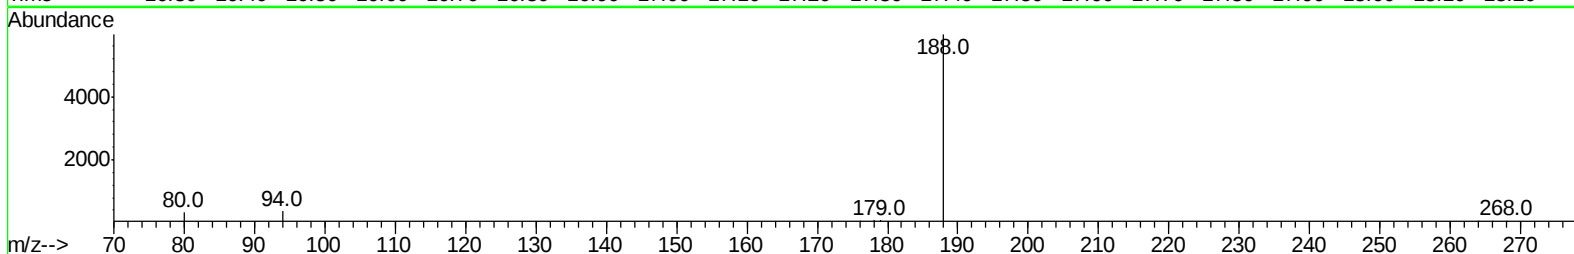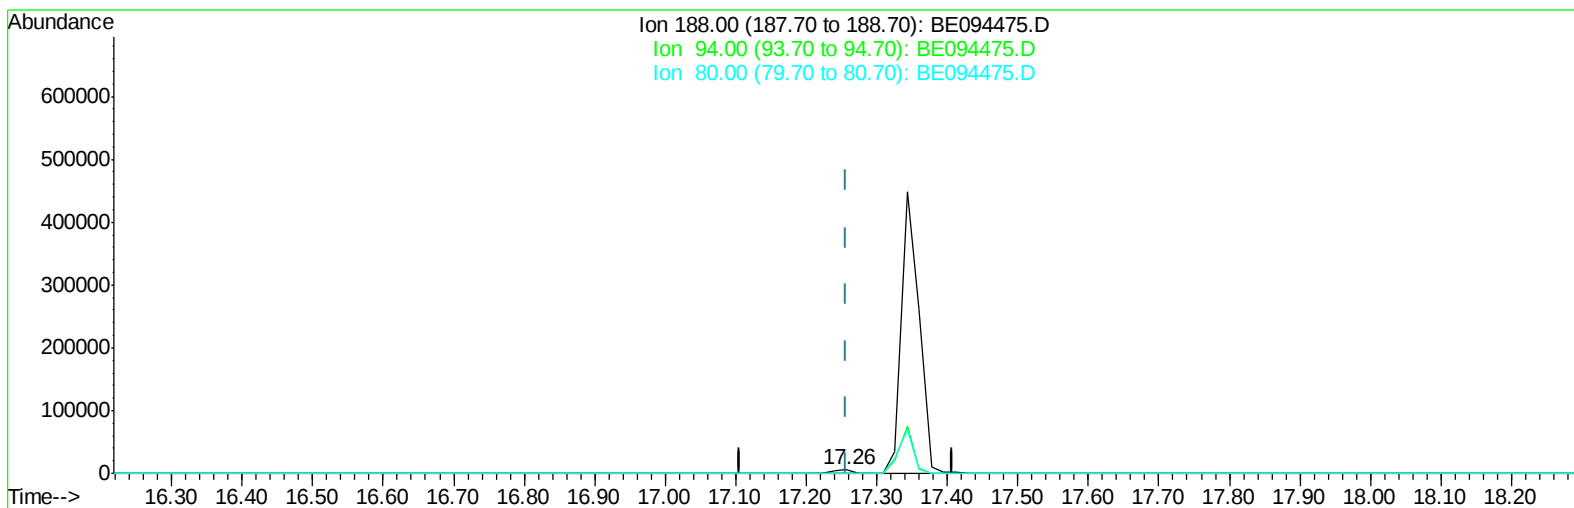

TIC: BE094475.D

(10) Phenanthrene-d10 (I)

17.257min (-0.000) 0.40ng/ul m

response 11498

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.03#
80.00	11.80	5.55#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094475.D
Acq On : 20 Oct 2017 15:22
Operator : SJ/JU
Sample : I5840-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:52 PM

Quant Time: Oct 22 03:34:09 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

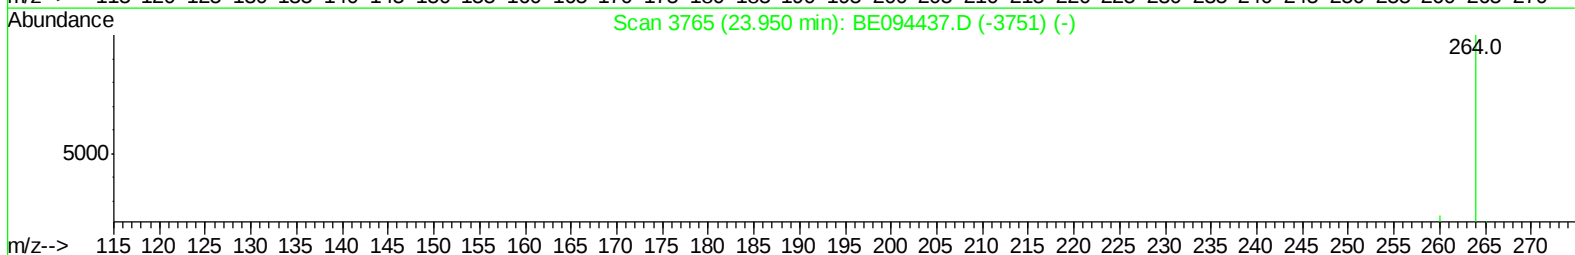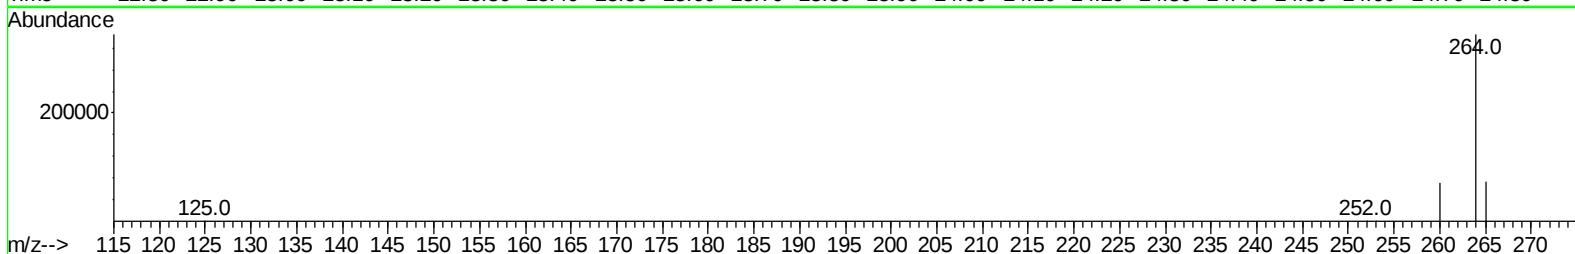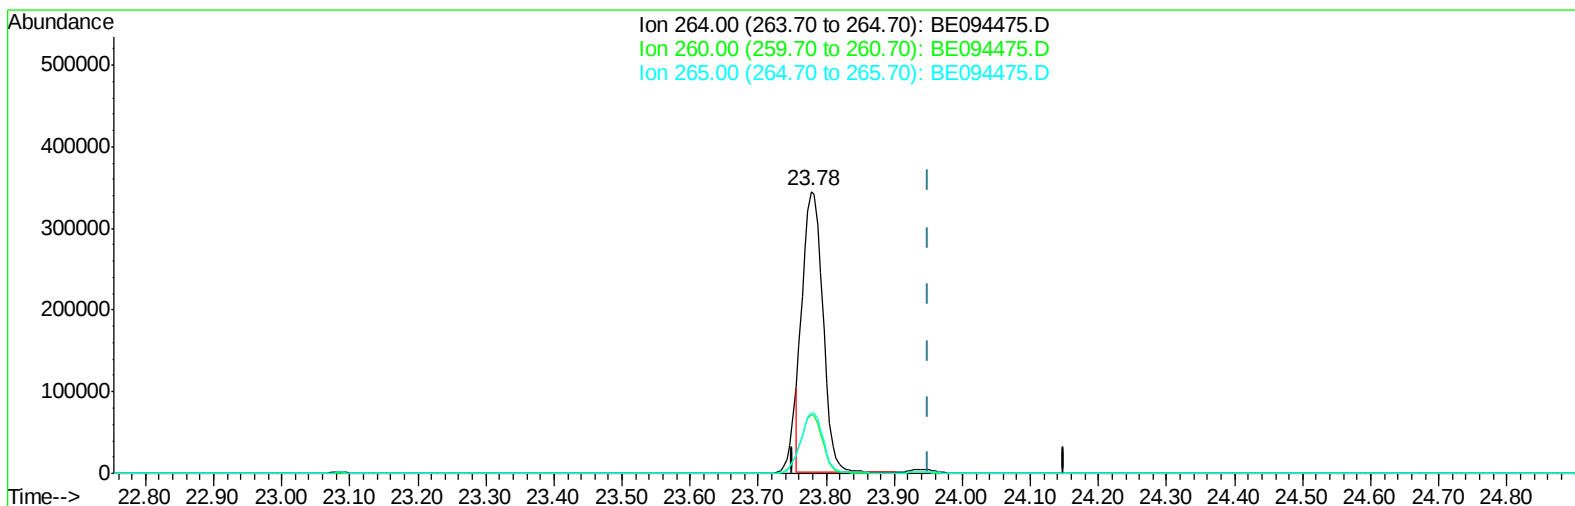

TIC: BE094475.D

(20) Perylene-d12 (I)

23.778min (-0.172) 0.40ng/ul

response 717171

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.86#
265.00	103.50	21.30#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094475.D
Acq On : 20 Oct 2017 15:22
Operator : SJ/JU
Sample : I5840-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:52 PM

Quant Time: Oct 22 03:34:09 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

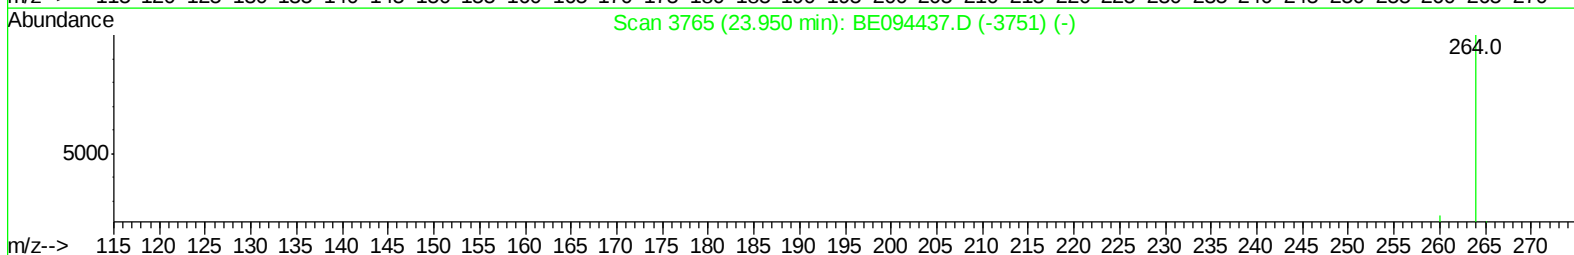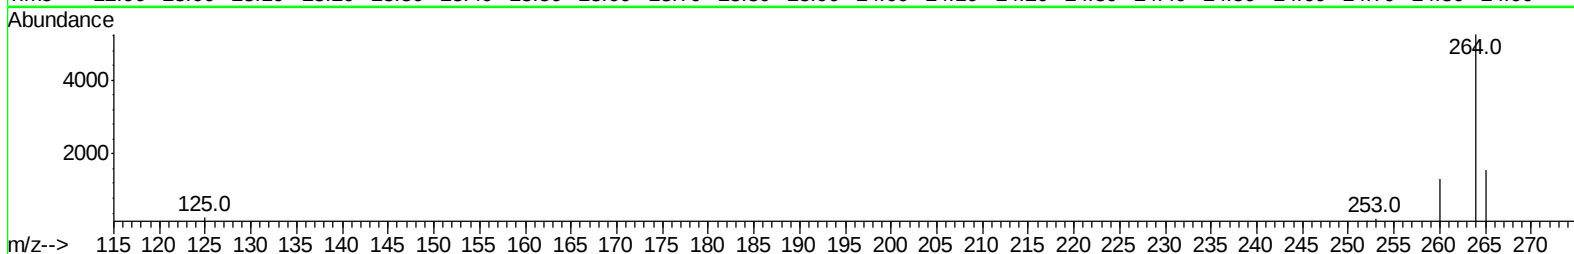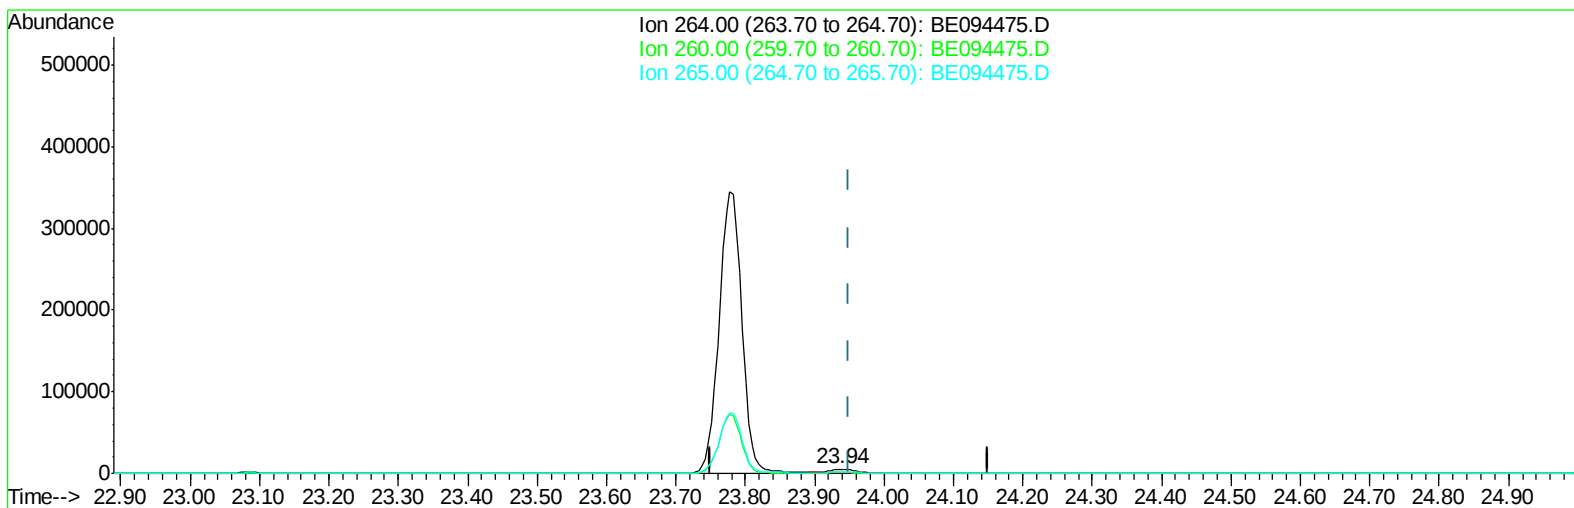

TIC: BE094475.D

(20) Perylene-d12 (I)

23.937min (-0.013) 0.40ng/ul m

response 9970

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.33
265.00	103.50	30.02#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094475.D
Acq On : 20 Oct 2017 15:22
Operator : SJ/JU
Sample : I5840-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:52 PM

Quant Time: Oct 22 03:35:37 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1504	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	8292	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.51	164	5173	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	11498m	0.40	ng/ul	0.00
16) Chrysene-d12	21.42	240	10879	0.40	ng/ul	0.00
20) Perylene-d12	23.94	264	9970m	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3760	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.28	212	10510	0.27	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102017\
Data File : BE094475.D
Acq On : 20 Oct 2017 15:22
Operator : SJ/JU
Sample : I5840-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/23/2017 3:13:52 PM

Quant Time: Oct 22 03:35:37 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE092017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 17:51:02 2017
Response via : Initial Calibration

