

Data Path : Z:\HPCHEM1\BNA_E\Data\BE102114\
 Data File : BE088176.D
 Acq On : 22 Oct 2014 11:24
 Operator : TP/JJ
 Sample : F4312-16DL 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 YS19-SS02P-1014

Quant Time: Oct 22 12:53:49 2014
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE102014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 21 02:11:14 2014
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.14	152	23926	5.00	ng	0.00
3) Naphthalene-d8	8.70	136	94130	5.00	ng	0.00
7) Acenaphthene-d10	10.85	164	48242	5.00	ng	0.00
12) Phenanthrene-d10	12.96	188	73615	5.00	ng	0.00
16) Chrysene-d12	18.39	240	46771	5.00	ng	0.00
22) Perylene-d12	21.44	264	46679	5.00	ng	0.00
System Monitoring Compounds						
4) Nitrobenzene-d5	7.83	82	81322	11.98	ng	0.00
8) 2-Fluorobiphenyl	10.04	172	137538	10.32	ng	0.00
18) Terphenyl-d14	16.15	244	101257	13.45	ng	0.00
Target Compounds						Qvalue
5) Naphthalene	8.72	128	2114	0.11	ng	96
6) 2-Methylnaphthalene	9.58	142	767	0.07	ng	# 93
9) Acenaphthylene	10.67	152	5940	0.08	ng	98
10) Acenaphthene	10.88	154	4133	0.36	ng	97
11) Fluorene	11.55	166	3983	0.33	ng	98
13) Phenanthrene	13.01	178	294408	5.45	ng	95
14) Anthracene	13.01	178	294408	5.12	ng	99
15) Fluoranthene	15.25	202	108996	7.78	ng	99
17) Pyrene	15.25	202	108137	8.50	ng	100
19) Benzo(a)anthracene	18.36	228	157164	3.78	ng	99
20) Chrysene	18.44	228	165405	4.05	ng	98
21) Indeno(1,2,3-cd)pyrene	23.64	276	112986	2.49	ng	# 88
23) Benzo(b)fluoranthene	20.69	252	52004	4.68	ng	99
24) Benzo(k)fluoranthene	20.74	252	22627	1.90	ng	98
25) Benzo(a)pyrene	21.32	252	36864	3.60	ng	98
26) Dibenzo(a,h)anthracene	23.73	278	5209	0.52	ng	# 93
27) Benzo(g,h,i)perylene	24.27	276	113313	2.55	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE102114\
Data File : BE088176.D
Acq On : 22 Oct 2014 11:24
Operator : TP/JJ
Sample : F4312-16DL 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
YS19-SS02P-1014

Quant Time: Oct 22 12:53:49 2014
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE102014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 21 02:11:14 2014
Response via : Initial Calibration

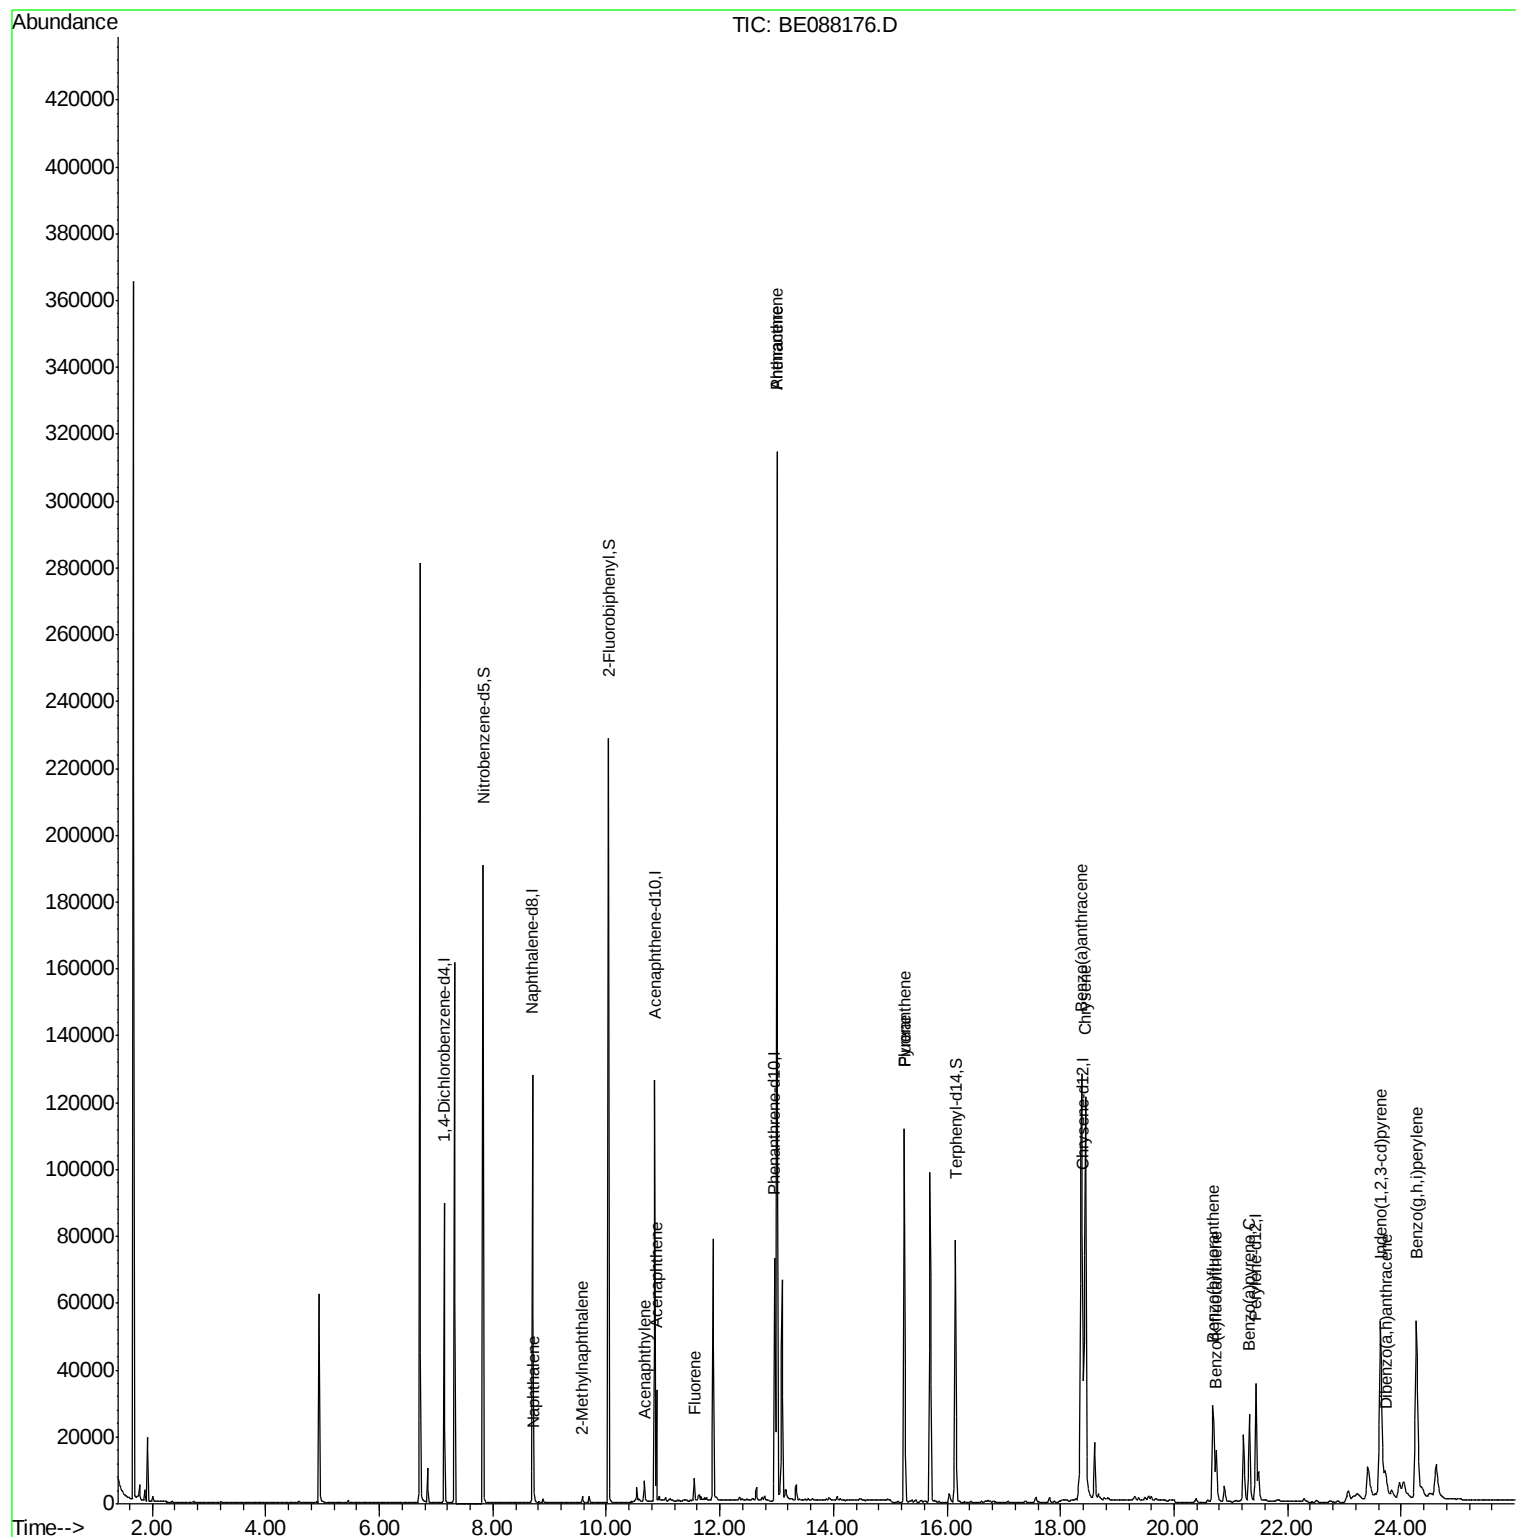

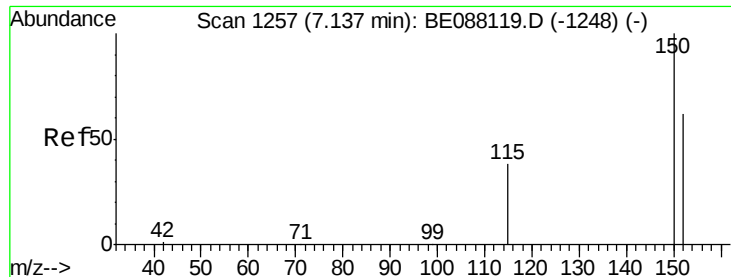

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.14 min Scan# 1258

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014


Tgt Ion:152 Resp: 23926

Ion Ratio Lower Upper

152 100

150 158.1 129.2 193.8




115 58.7 49.3 73.9

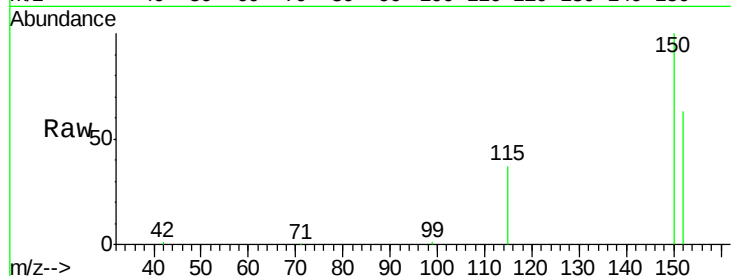

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

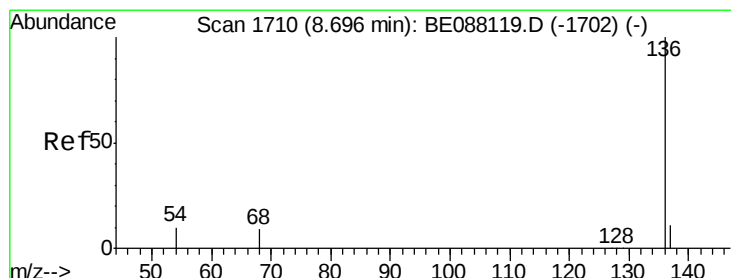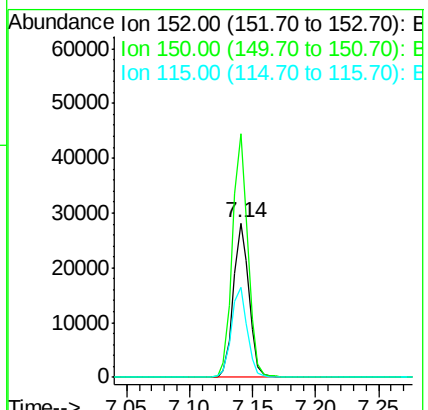

#3

Naphthalene-d8

Concen: 5.00 ng

RT: 8.70 min Scan# 1711

Delta R.T. 0.01 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24


Tgt Ion:136 Resp: 94130

Ion Ratio Lower Upper

136 100

137 11.1 8.6 12.8



54 5.9 7.7 11.5#




Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

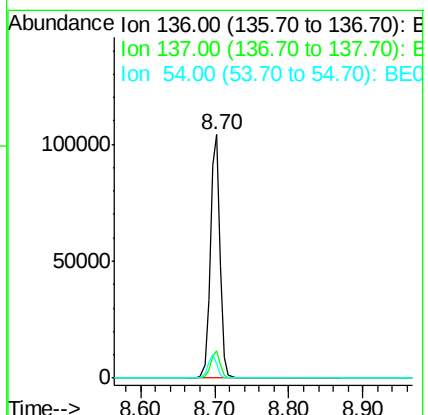

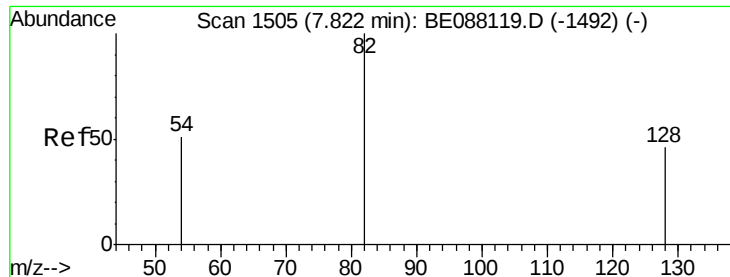

#4

Nitrobenzene-d5

Concen: 11.98 ng

RT: 7.83 min Scan# 1507

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014


Tgt Ion: 82 Resp: 81322

Ion Ratio Lower Upper

82 100

128 47.4 37.1 55.7




54 51.5 41.1 61.7

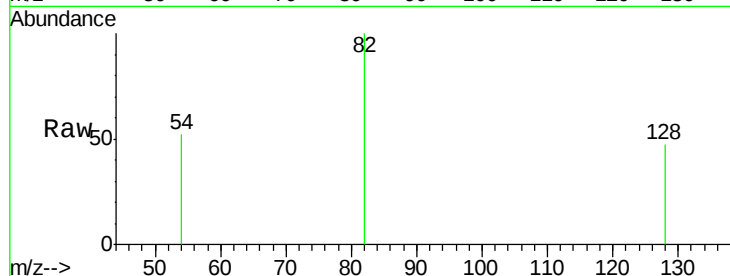

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

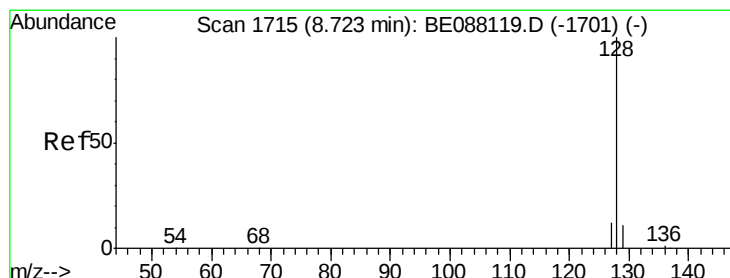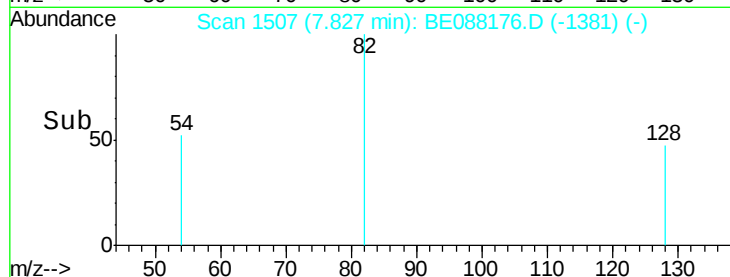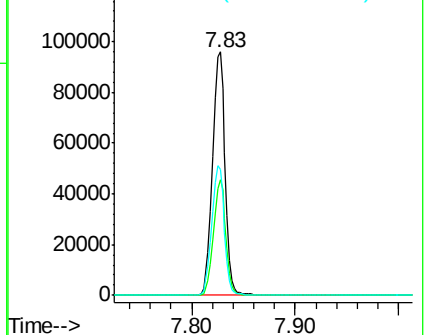

#5

Naphthalene

Concen: 0.11 ng

RT: 8.72 min Scan# 1715

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24


Tgt Ion: 128 Resp: 2114

Ion Ratio Lower Upper

128 100

129 12.2 8.9 13.3



127 14.1 9.7 14.5

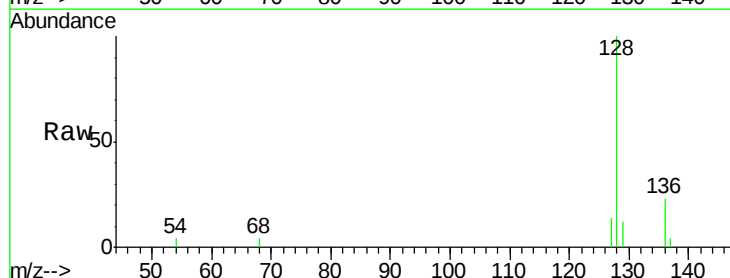


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

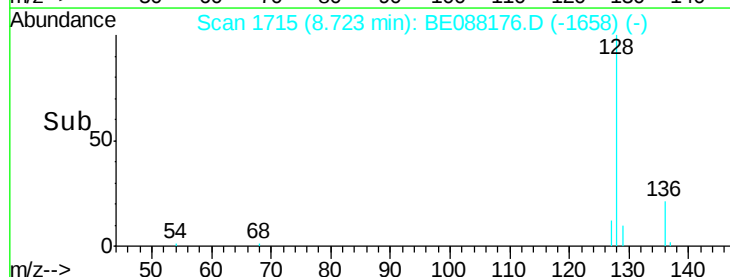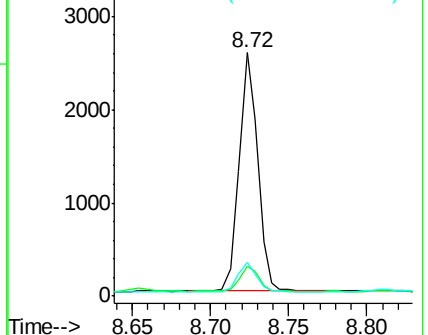

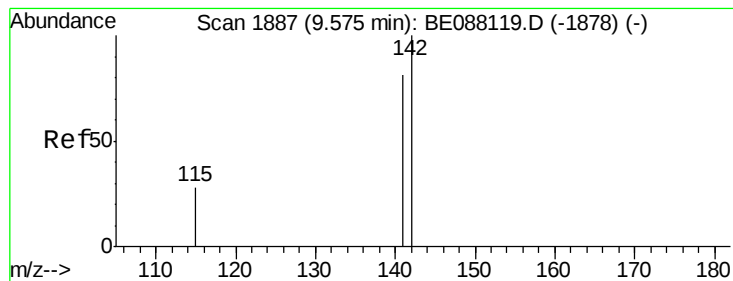

#6

2-Methylnaphthalene

Concen: 0.07 ng

RT: 9.58 min Scan# 1887

Delta R.T. -0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014


Tgt Ion:142 Resp: 767

Ion Ratio Lower Upper

142 100

141 85.1 64.6 97.0




115 35.6 22.6 34.0#

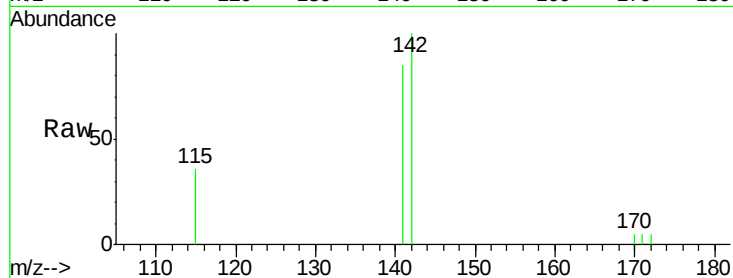

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

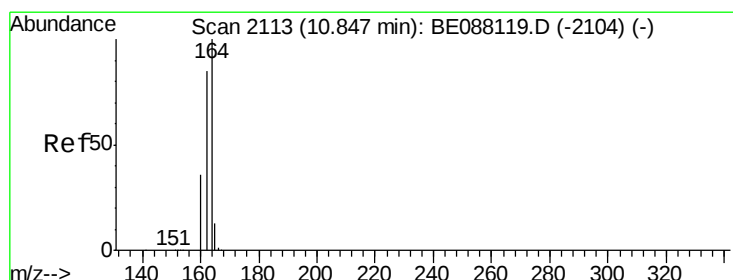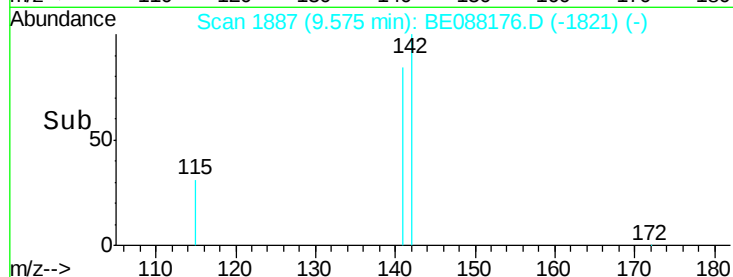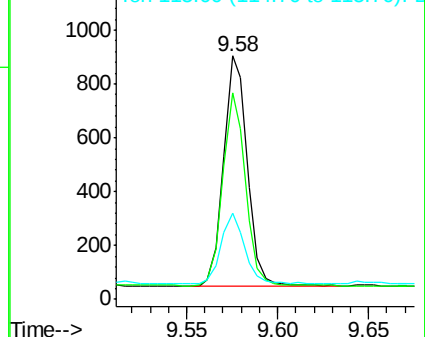

#7

Acenaphthene-d10

Concen: 5.00 ng

RT: 10.85 min Scan# 2113

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24


Tgt Ion:164 Resp: 48242

Ion Ratio Lower Upper

164 100

162 88.4 68.3 102.5



160 38.7 28.7 43.1

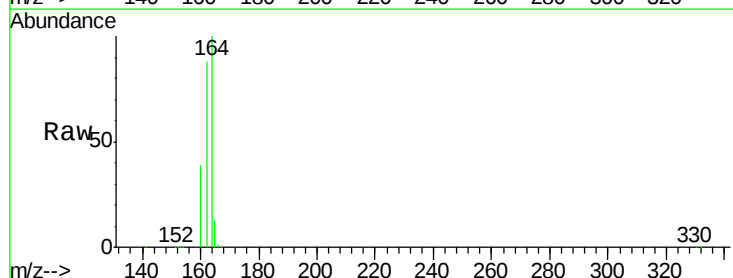

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

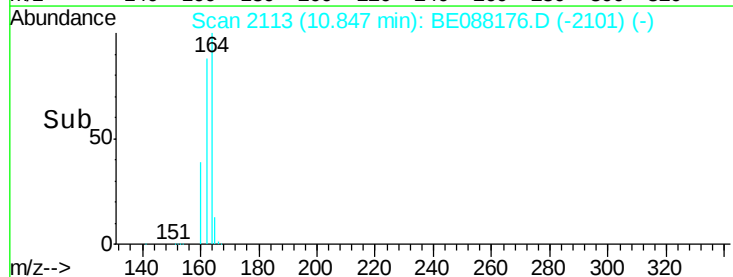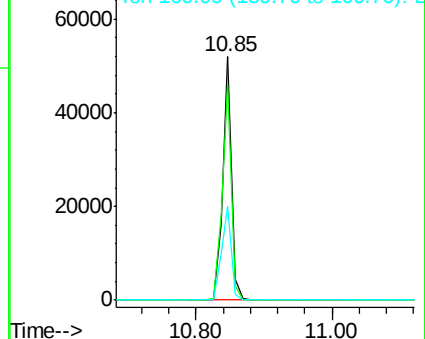



#8

2-Fluorobiphenyl

Concen: 10.32 ng

RT: 10.04 min Scan# 1989

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014





Tgt Ion:172 Resp: 137538

Ion Ratio Lower Upper

172 100

171 30.4 25.4 38.2

170 19.5 17.4 26.2

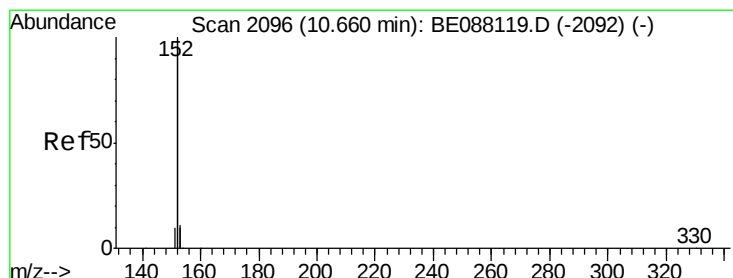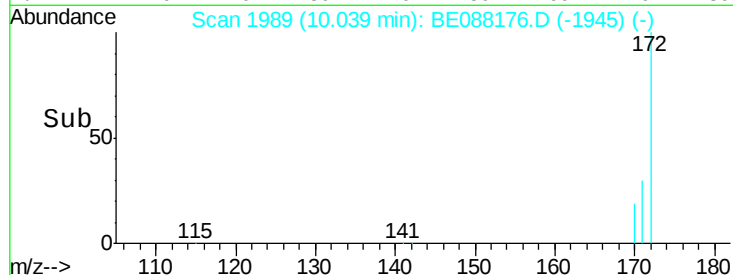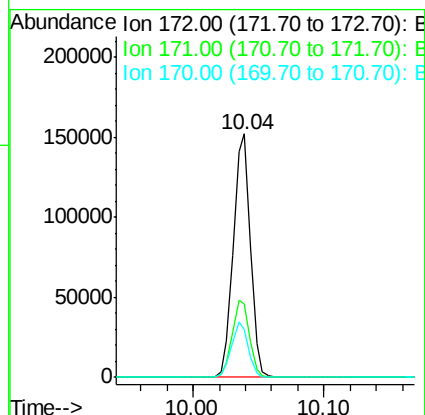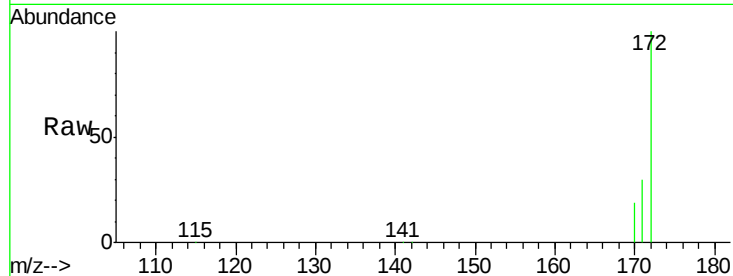

#9

Acenaphthylene

Concen: 0.08 ng

RT: 10.67 min Scan# 2097

Delta R.T. 0.01 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24




Tgt Ion:152 Resp: 5940


Ion Ratio Lower Upper

152 100

151 4.8 3.7 5.5

153 14.2 10.4 15.6

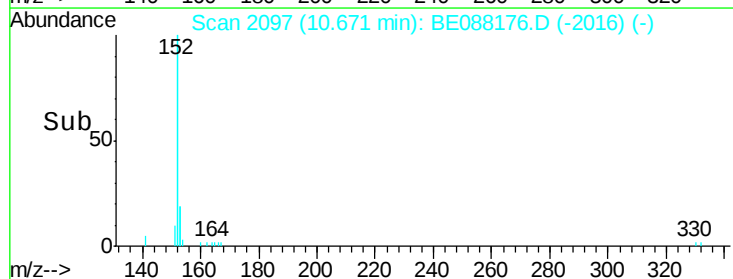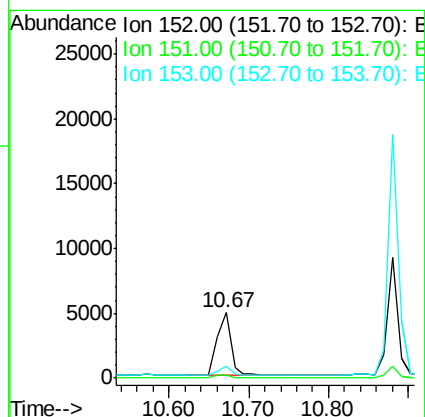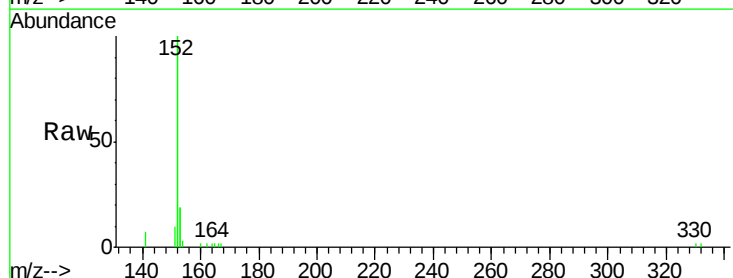

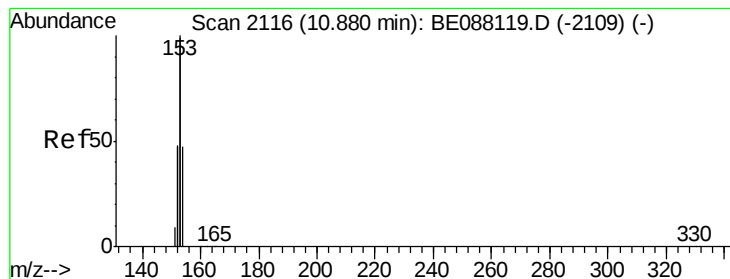

#10

Acenaphthene

Concen: 0.36 ng

RT: 10.88 min Scan# 2116

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014


Tgt Ion:154 Resp: 4133

Ion Ratio Lower Upper

154 100

153 402.2 327.8 491.6




152 200.5 157.6 236.4

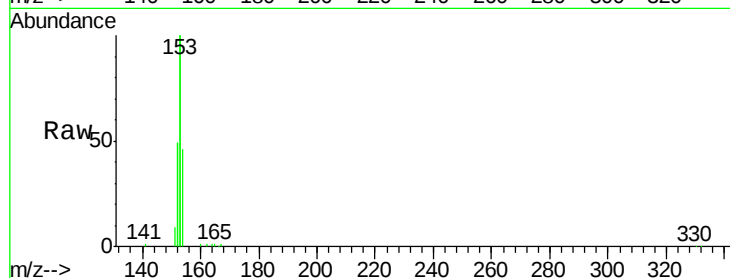

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

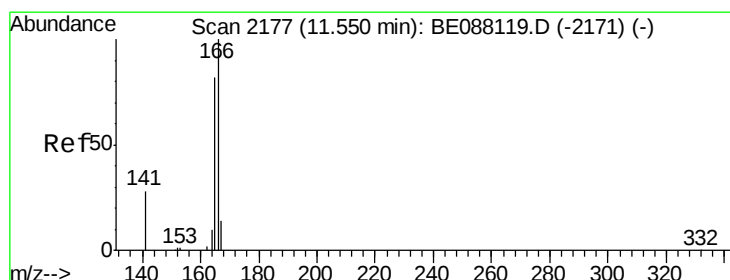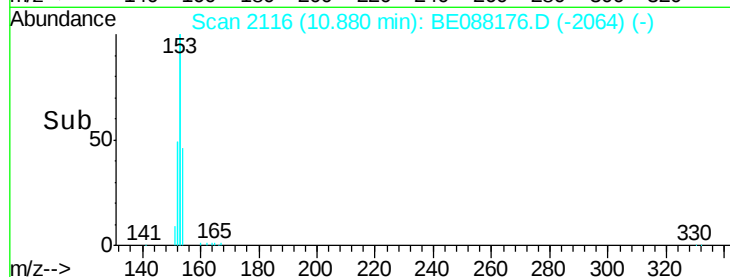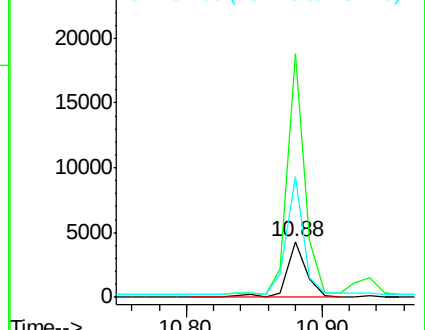

#11

Fluorene

Concen: 0.33 ng

RT: 11.55 min Scan# 2177

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24


Tgt Ion:166 Resp: 3983

Ion Ratio Lower Upper

166 100

165 90.5 71.4 107.2



167 14.7 10.6 16.0

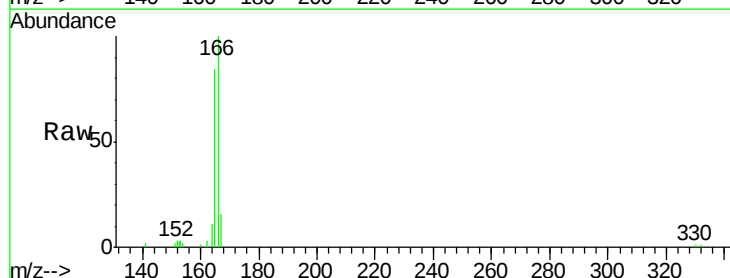


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

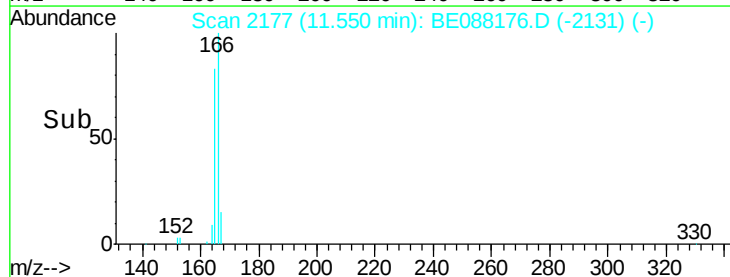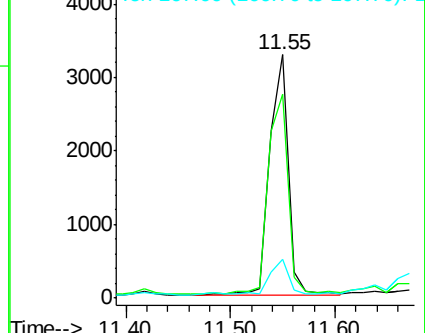

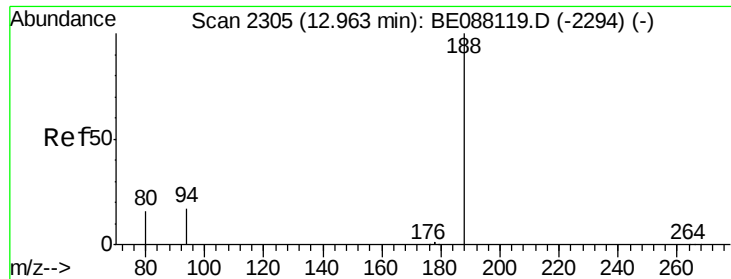

#12

Phenanthrene-d10

Concen: 5.00 ng

RT: 12.96 min Scan# 2305

Delta R.T. -0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014


Tgt Ion:188 Resp: 73615

Ion Ratio Lower Upper

188 100

94 18.1 13.9 20.9




80 17.3 12.9 19.3

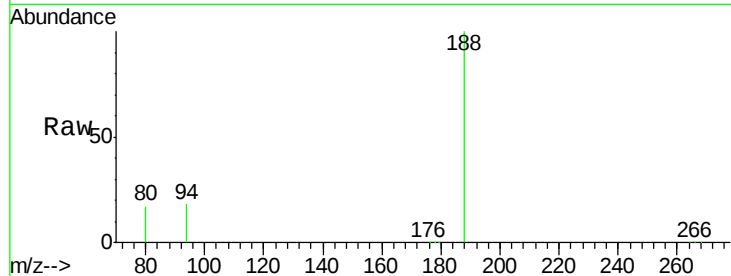

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

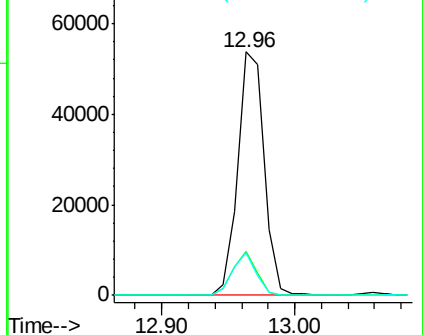

#13

Phenanthrene

Concen: 5.45 ng

RT: 13.01 min Scan# 2310

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24


Tgt Ion:178 Resp: 294408

Ion Ratio Lower Upper

178 100

176 18.6 12.5 18.7



179 15.2 13.5 20.3




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

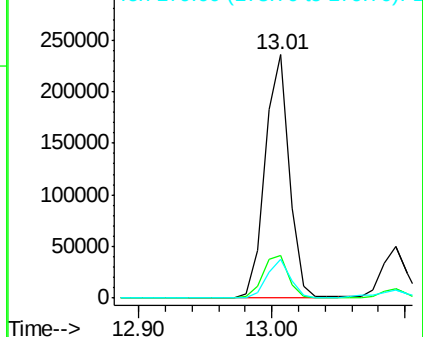

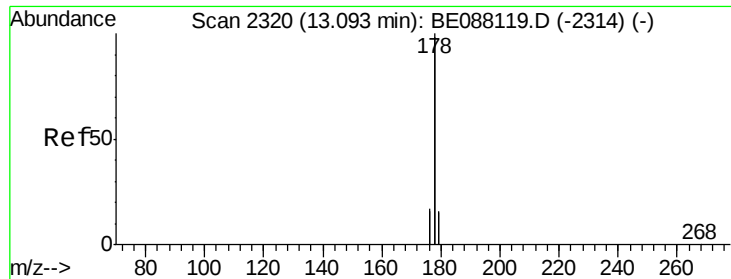

#14

Anthracene

Concen: 5.12 ng

RT: 13.01 min Scan# 2310

Delta R.T. -0.09 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014


Tgt Ion:178 Resp: 294408

Ion Ratio Lower Upper

178 100

176 18.6 14.6 21.8




179 15.2 12.5 18.7

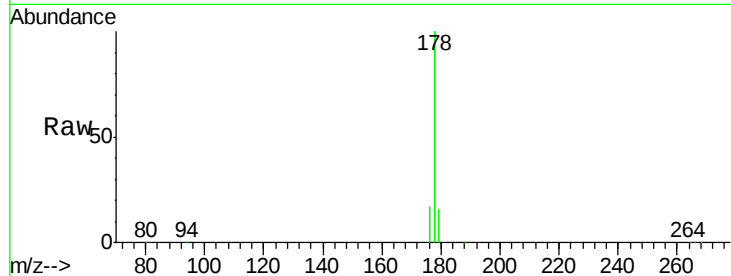

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

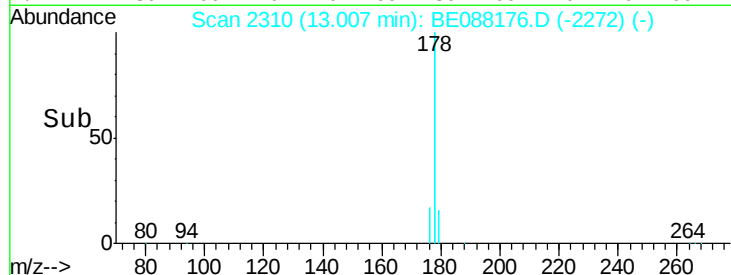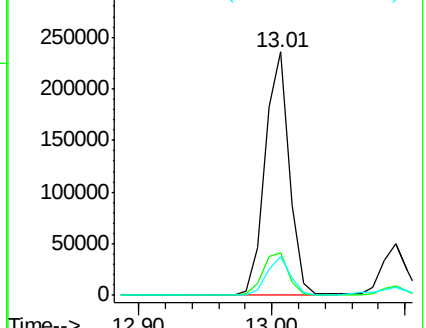

#15

Fluoranthene

Concen: 7.78 ng

RT: 15.25 min Scan# 2585

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24


Tgt Ion:202 Resp: 108996

Ion Ratio Lower Upper

202 100

101 18.2 14.8 22.2



203 17.3 13.5 20.3




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E




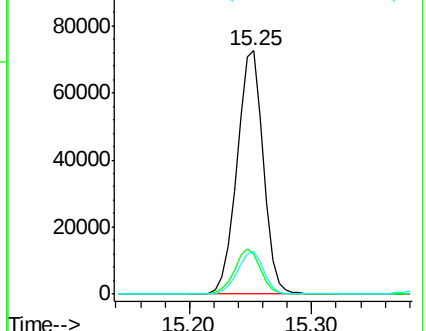


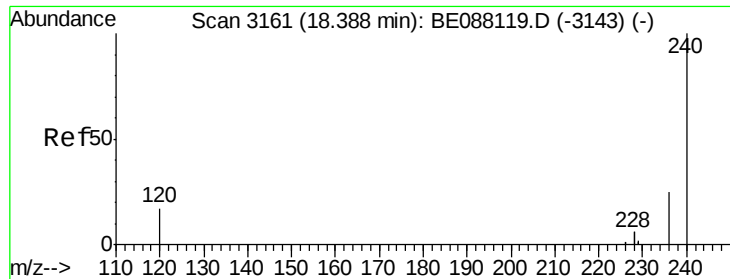

#16
Chrysene-d12
Concen: 5.00 ng
RT: 18.39 min Scan# 3161
Delta R.T. 0.00 min
Lab File: BE088176.D
Acq: 22 Oct 2014 11:24




Instrument :
BNA_E
ClientSampleId :
YS19-SS02P-1014


Tgt Ion:240 Resp: 46771
Ion Ratio Lower Upper
240 100
120 15.9 13.9 20.9
236 24.9 19.9 29.9

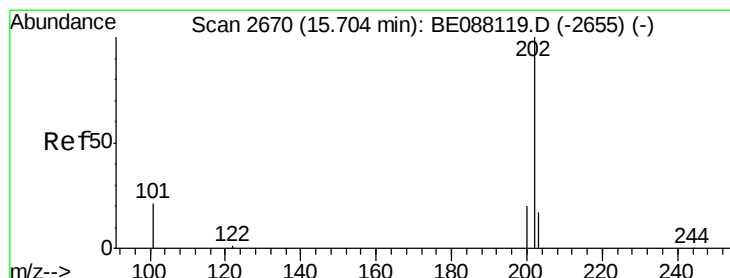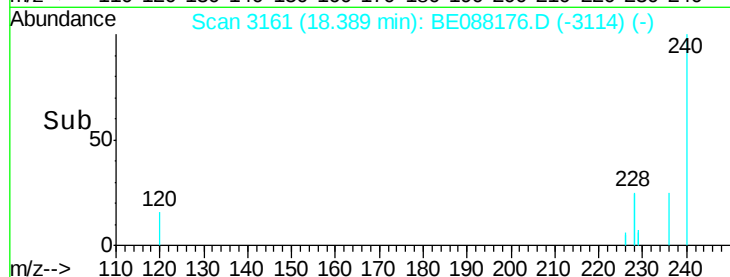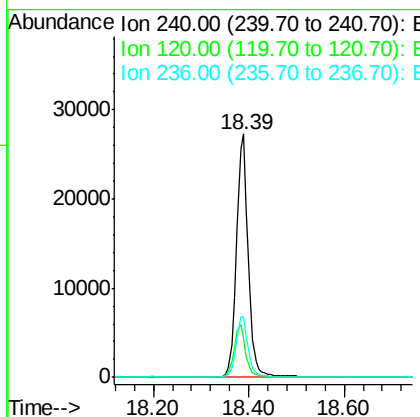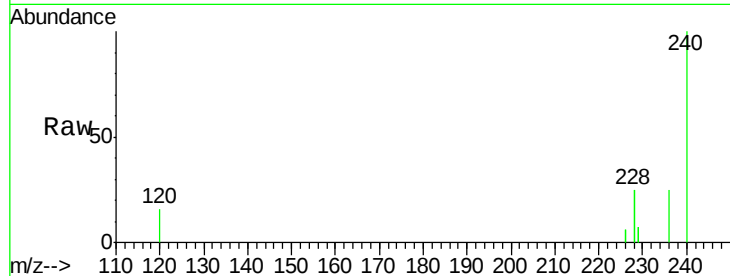

#17
Pyrene
Concen: 8.50 ng
RT: 15.25 min Scan# 2585
Delta R.T. -0.45 min
Lab File: BE088176.D
Acq: 22 Oct 2014 11:24

Tgt Ion:202 Resp: 108137
Ion Ratio Lower Upper
202 100
200 20.1 16.1 24.1
203 17.3 13.9 20.9

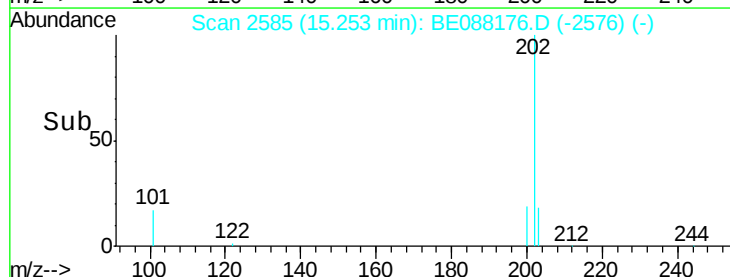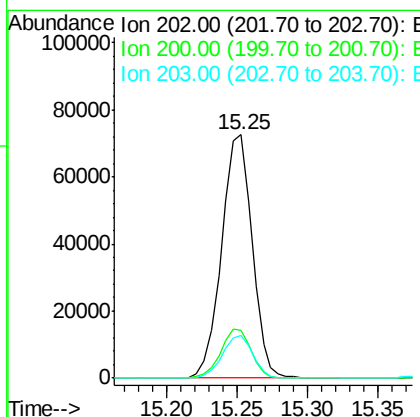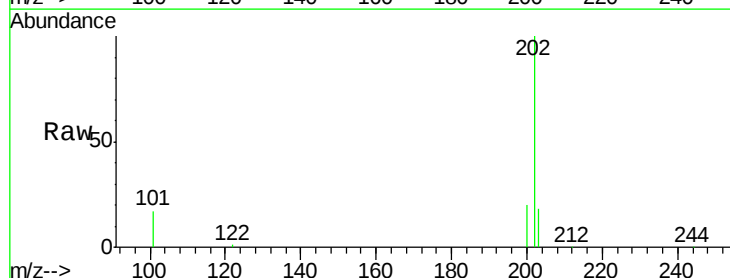

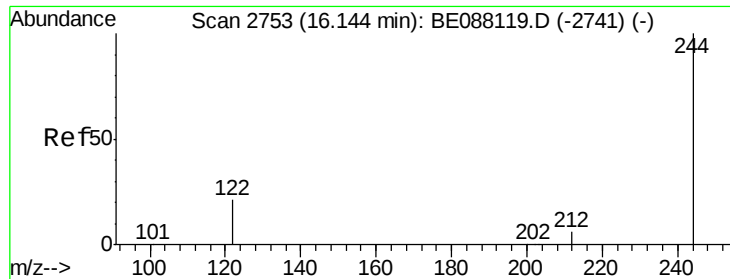

#18

Terphenyl-d14

Concen: 13.45 ng

RT: 16.15 min Scan# 2754

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014


Tgt Ion:244 Resp: 101257

Ion Ratio Lower Upper

244 100

212 6.6 5.4 8.0




122 20.5 17.5 26.3

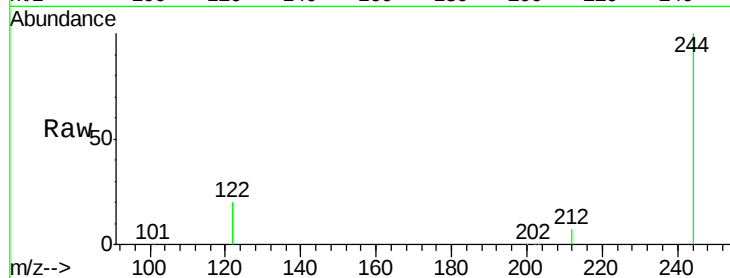

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

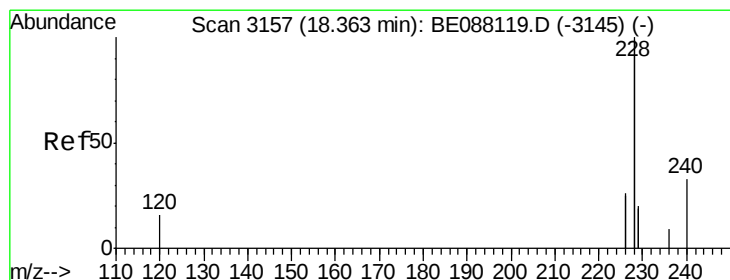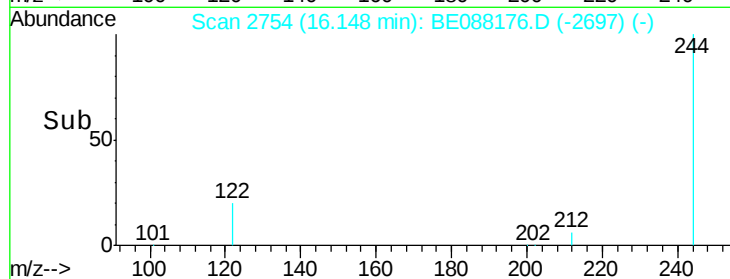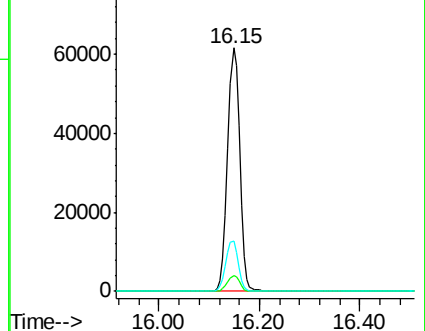

#19

Benzo(a)anthracene

Concen: 3.78 ng

RT: 18.36 min Scan# 3157

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24


Tgt Ion:228 Resp: 157164

Ion Ratio Lower Upper

228 100

226 26.3 20.8 31.2



229 20.3 15.6 23.4

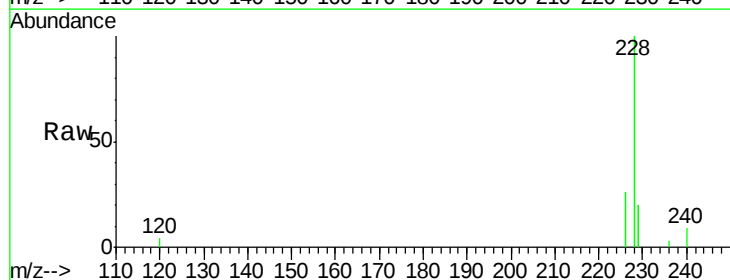


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

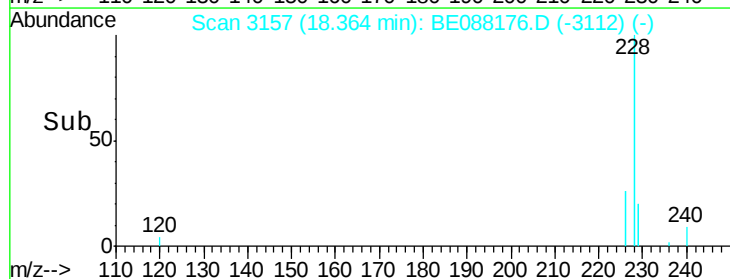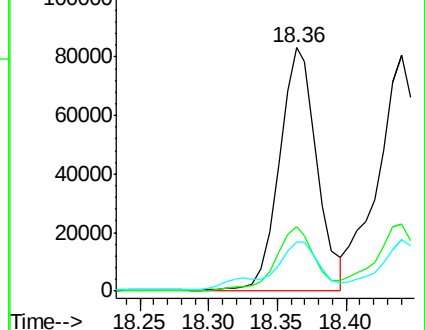

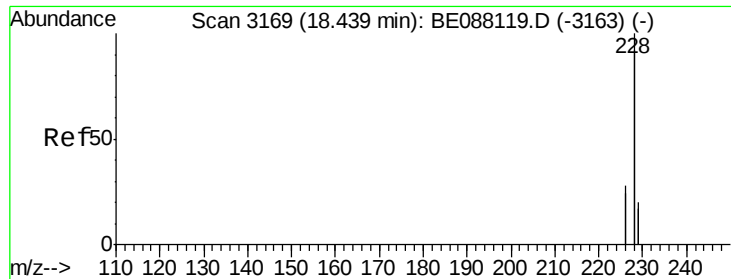

#20

Chrysene

Concen: 4.05 ng

RT: 18.44 min Scan# 3169

Delta R.T. 0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014





Tgt Ion:228 Resp: 165405

Ion Ratio Lower Upper

228 100

226 28.3 22.7 34.1

229 21.7 15.8 23.6

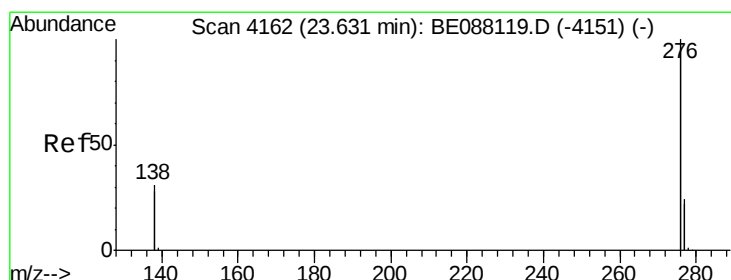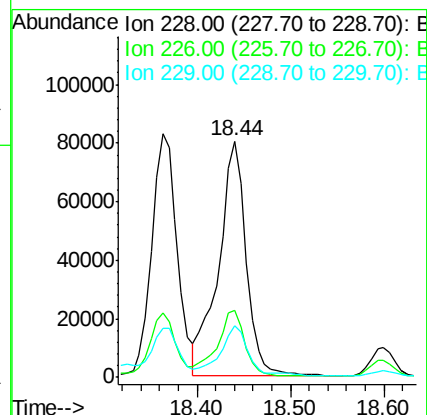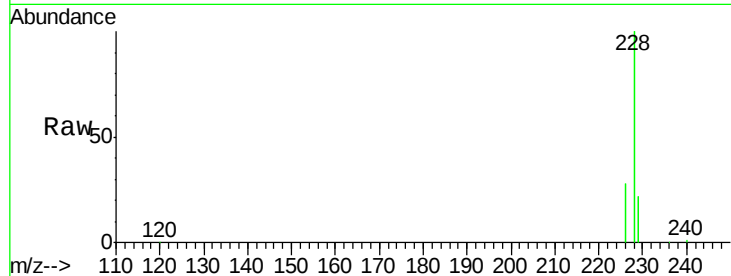

#21

Indeno(1,2,3-cd)pyrene

Concen: 2.49 ng

RT: 23.64 min Scan# 4163

Delta R.T. 0.01 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24




Tgt Ion:276 Resp: 112986


Ion Ratio Lower Upper

276 100

138 27.1 18.5 27.7

277 25.3 14.6 21.8#


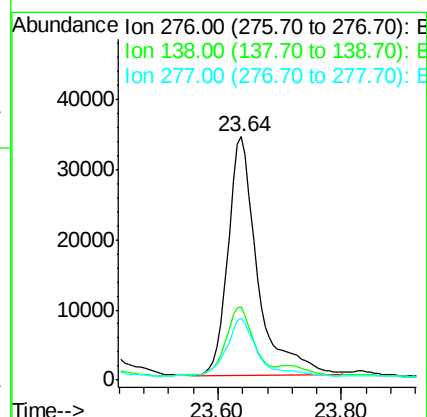




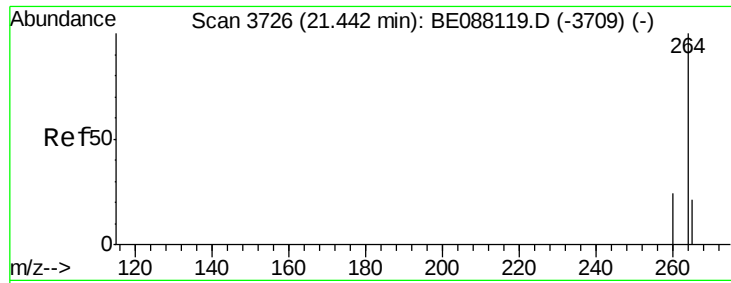

#22
Perylene-d12
Concen: 5.00 ng
RT: 21.44 min Scan# 3726
Delta R.T. -0.00 min
Lab File: BE088176.D
Acq: 22 Oct 2014 11:24




Instrument :
BNA_E
ClientSampleId :
YS19-SS02P-1014


Tgt Ion:264 Resp: 46679
Ion Ratio Lower Upper
264 100
260 24.0 19.0 28.4
265 21.8 17.2 25.8

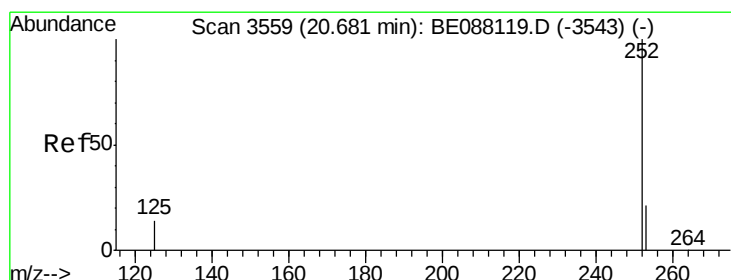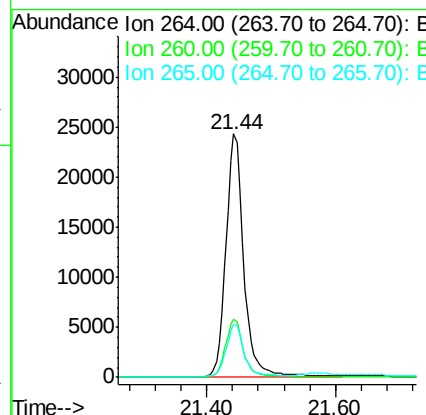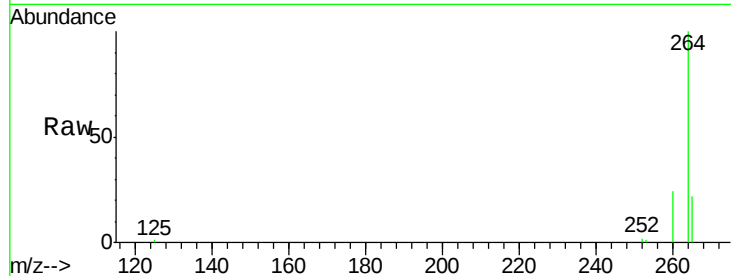

#23
Benzo(b)fluoranthene
Concen: 4.68 ng
RT: 20.69 min Scan# 3560
Delta R.T. 0.00 min
Lab File: BE088176.D
Acq: 22 Oct 2014 11:24

Tgt Ion:252 Resp: 52004
Ion Ratio Lower Upper
252 100
253 22.7 17.4 26.0
125 14.9 11.8 17.8

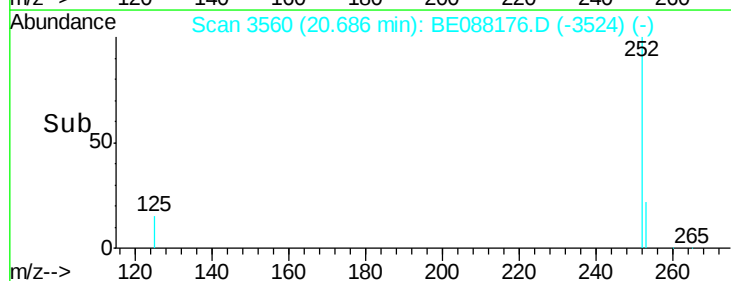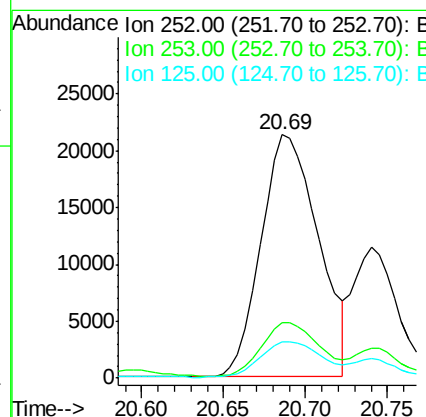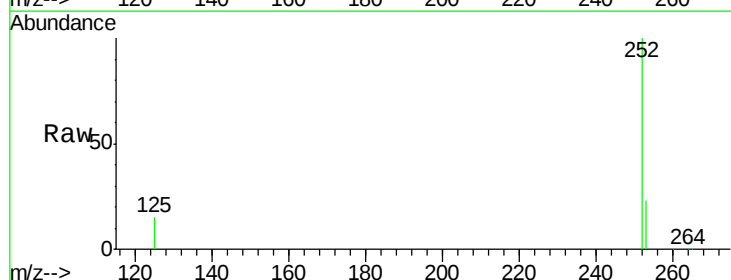

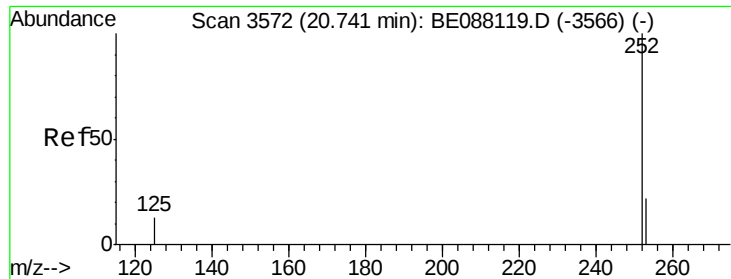

#24

Benzo(k)fluoranthene

Concen: 1.90 ng

RT: 20.74 min Scan# 3572

Delta R.T. -0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24

Instrument :

BNA_E

ClientSampleId :

YS19-SS02P-1014


Tgt Ion:252 Resp: 22627

Ion Ratio Lower Upper

252 100

253 23.2 17.6 26.4




125 14.6 11.5 17.3

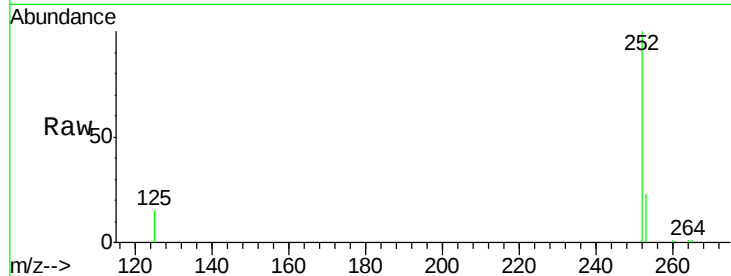

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

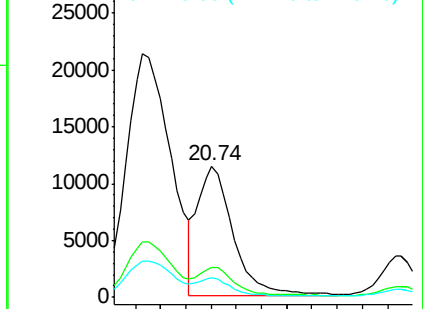

#25

Benzo(a)pyrene

Concen: 3.60 ng

RT: 21.32 min Scan# 3700

Delta R.T. -0.00 min

Lab File: BE088176.D

Acq: 22 Oct 2014 11:24


Tgt Ion:252 Resp: 36864

Ion Ratio Lower Upper

252 100

253 23.2 17.5 26.3



125 15.7 13.0 19.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



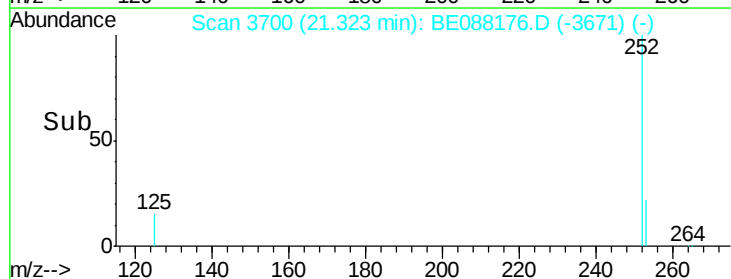
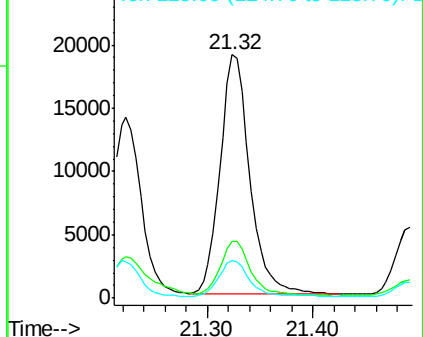




#26
Dibenzo(a,h)anthracene
Concen: 0.52 ng
RT: 23.73 min Scan# 4177
Delta R.T. 0.00 min
Lab File: BE088176.D
Acq: 22 Oct 2014 11:24

Instrument :
BNA_E
ClientSampleId :
YS19-SS02P-1014

Tgt Ion: 278 Resp: 5209
Ion Ratio Lower Upper
278 100
139 26.9 20.9 31.3
279 30.8 19.8 29.8#

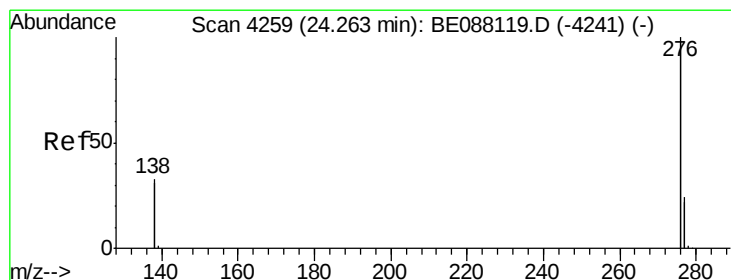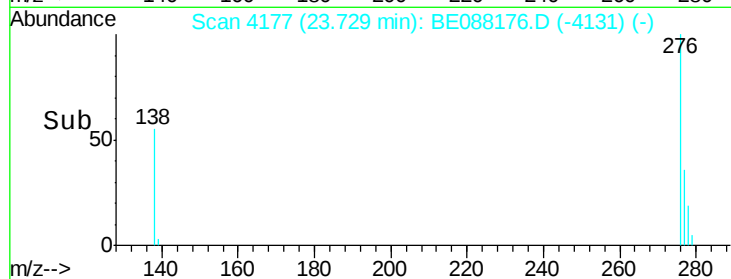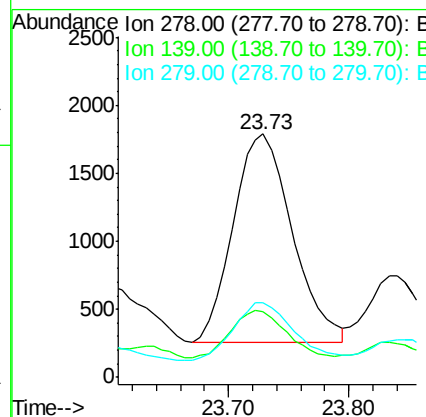

#27
Benzo(g,h,i)perylene
Concen: 2.55 ng
RT: 24.27 min Scan# 4260
Delta R.T. 0.01 min
Lab File: BE088176.D
Acq: 22 Oct 2014 11:24

Tgt Ion: 276 Resp: 113313
Ion Ratio Lower Upper
276 100
277 24.5 19.2 28.8
138 32.5 26.6 40.0

