


Data Path : Z:\HPCHEM1\BNA_E\Data\BE102114\
 Data File : Be088140.d
 Acq On : 21 Oct 2014 13:34
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE102014.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 21 02:11:14 2014

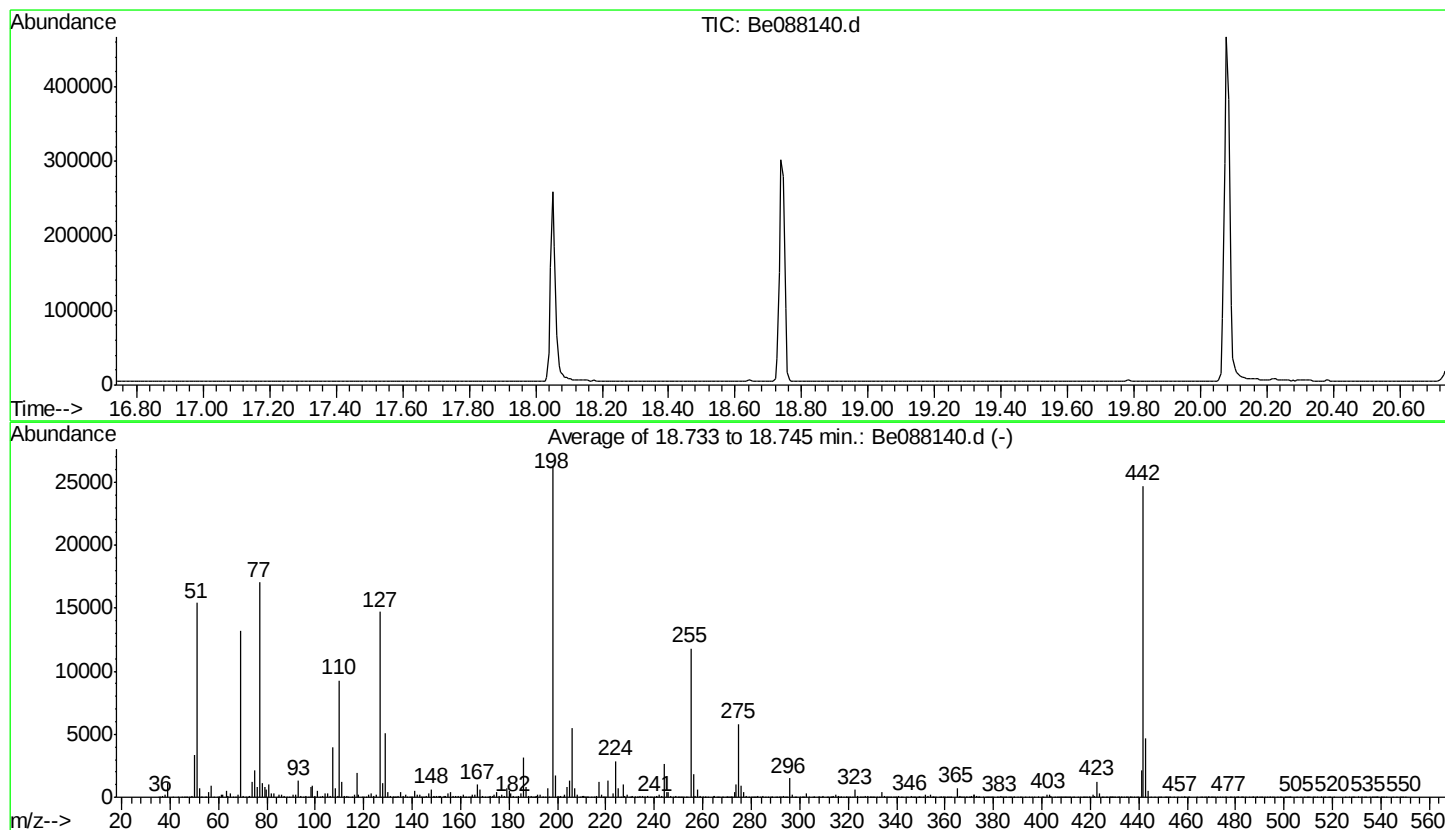

AutoFind: Scans 2646, 2647, 2648; Background Corrected with Scan 2639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	15424	PASS
68	69	0.00	2	1.3	176	PASS
69	198	0.00	100	50.1	13180	PASS
70	69	0.00	2	0.4	58	PASS
127	198	10	80	55.9	14710	PASS
197	198	0.00	2	0.2	48	PASS
198	198	100	100	100.0	26319	PASS
199	198	5	9	6.7	1763	PASS
275	198	10	60	22.2	5838	PASS
365	198	1	100	2.9	751	PASS
441	442	0.01	24	8.7	2153	PASS
442	198	50	100	94.0	24731	PASS
443	442	15	24	18.9	4662	PASS