

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE102116\
 Data File : BE092466.D
 Acq On : 21 Oct 2016 14:30
 Operator : UM/SJ
 Sample : PB94258BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB94258BL

Quant Time: Oct 21 17:23:39 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 21 17:07:17 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	11580	5.00	ng	0.00
7) Naphthalene-d8	10.95	136	48185	5.00	ng	0.00
12) Acenaphthene-d10	14.81	164	29633	5.00	ng	0.00
18) Phenanthrene-d10	17.58	188	55639	5.00	ng	0.00
24) Chrysene-d12	21.75	240	75863	5.00	ng	0.00
31) Perylene-d12	24.12	264	69867	5.00	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.67	112	21486	7.87	ng	-0.01
5) Phenol-d6	7.34	99	26416	6.79	ng	-0.02
8) Nitrobenzene-d5	9.34	82	11291	3.31	ng	-0.02
13) 2,4,6-Tribromophenol	16.32	330	4911	4.74	ng	0.00
14) 2-Fluorobiphenyl	13.45	172	29519	4.21	ng	0.00
26) Terphenyl-d14	20.17	244	36802	3.91	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE102116\
Data File : BE092466.D
Acq On : 21 Oct 2016 14:30
Operator : UM/SJ
Sample : PB94258BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB94258BL

Quant Time: Oct 21 17:23:39 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 17:07:17 2016
Response via : Initial Calibration

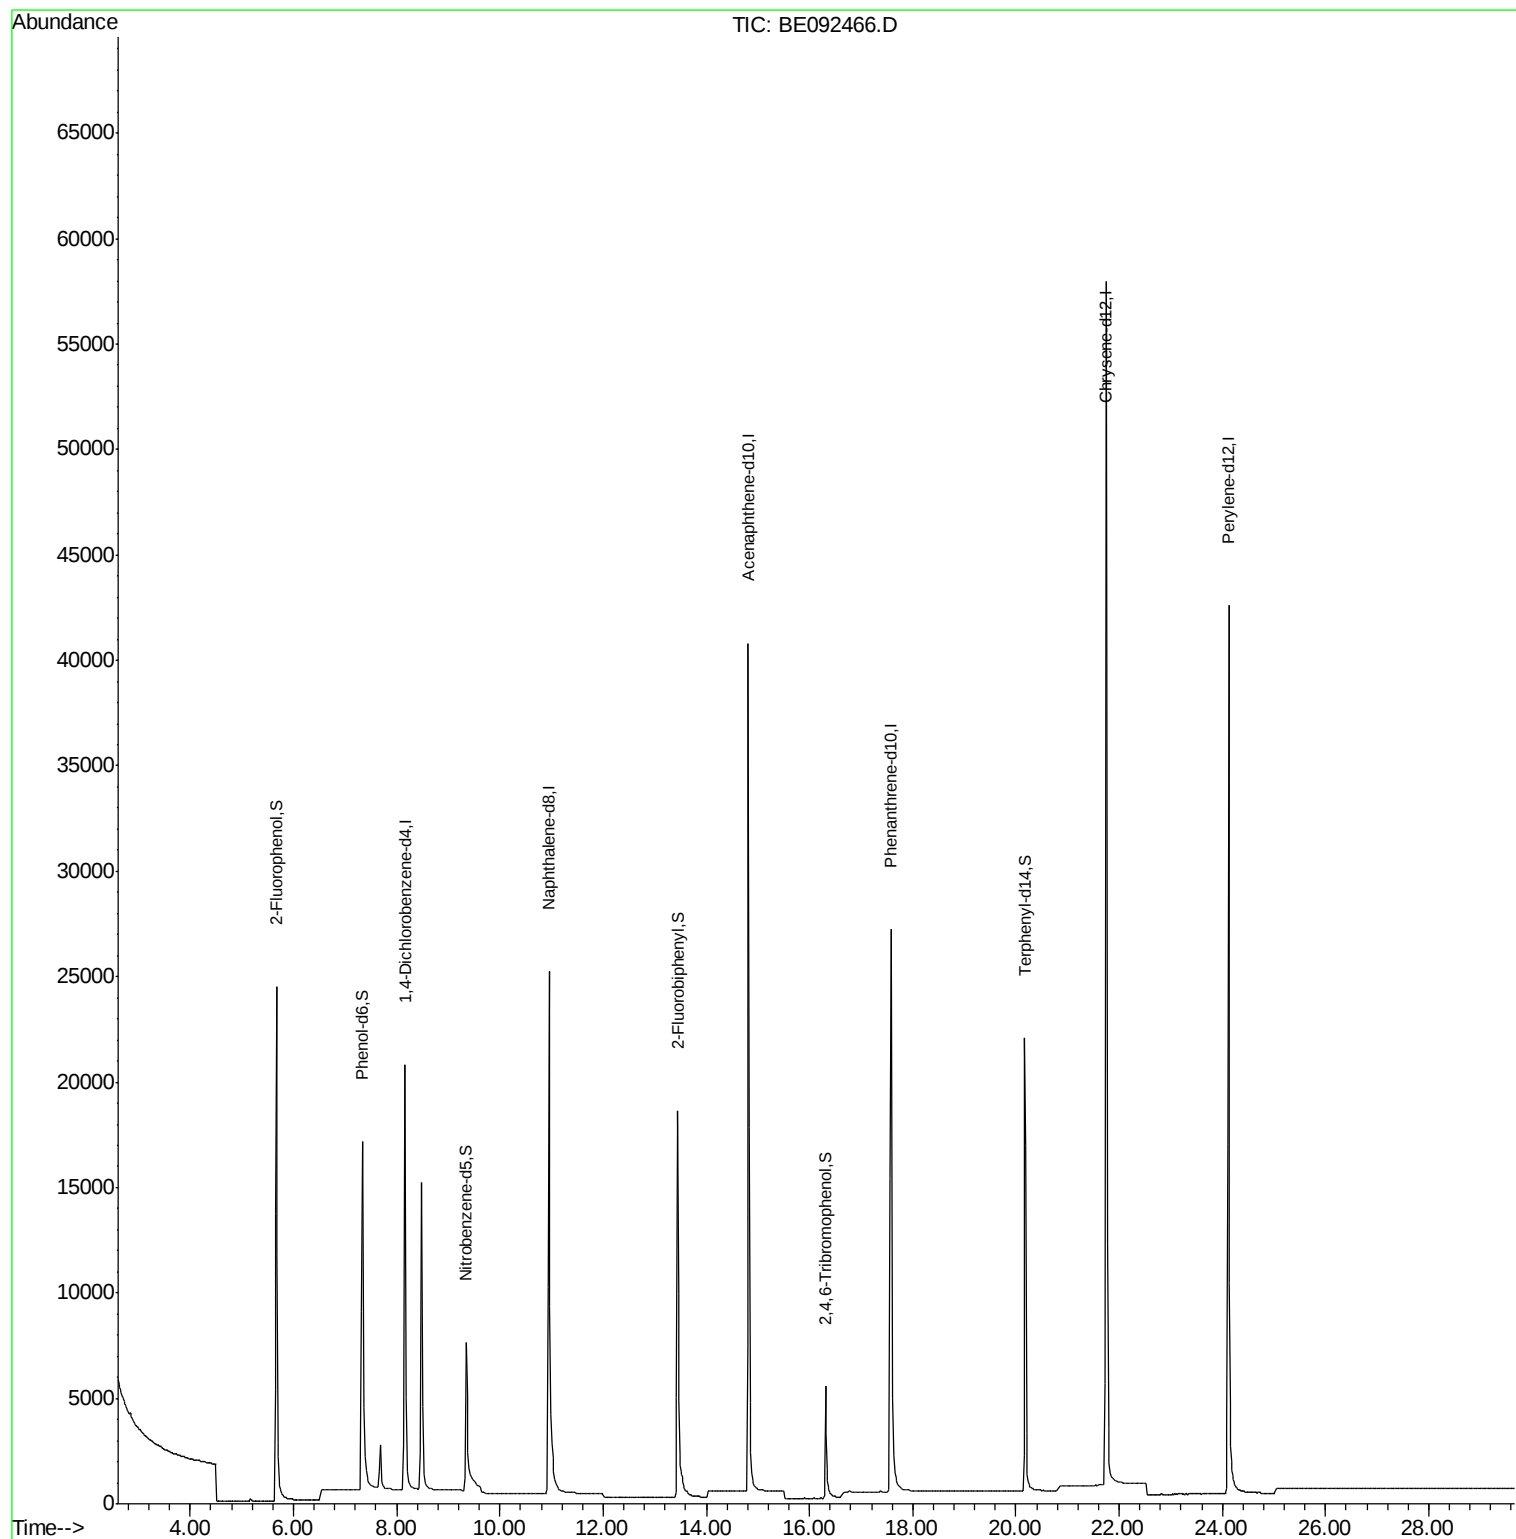

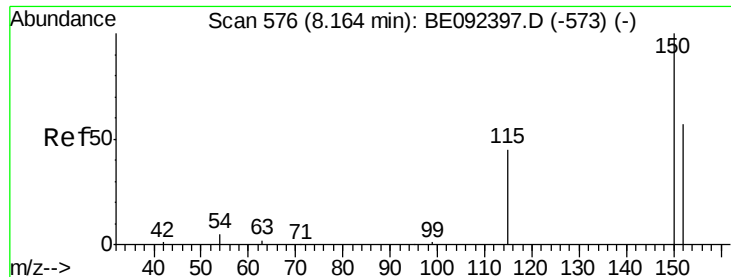

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.16 min Scan# 576

Delta R.T. -0.00 min

Lab File: BE092466.D

Acq: 21 Oct 2016 14:30

Instrument :

BNA_E

ClientSampleId :

PB94258BL


Tgt Ion:152 Resp: 11580

Ion Ratio Lower Upper

152 100

150 162.3 106.0 159.0#




115 63.6 31.2 46.8#

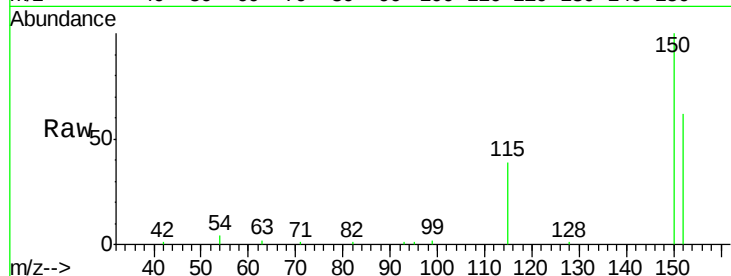

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

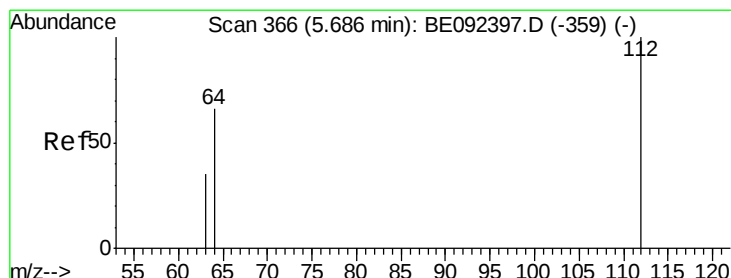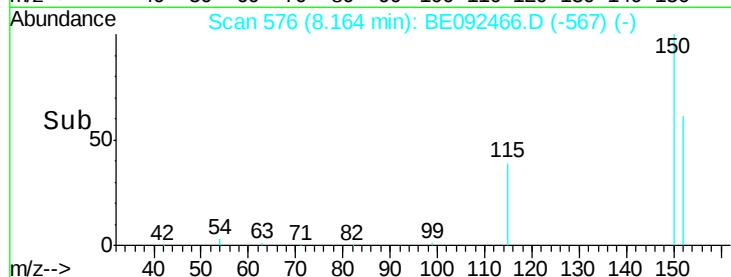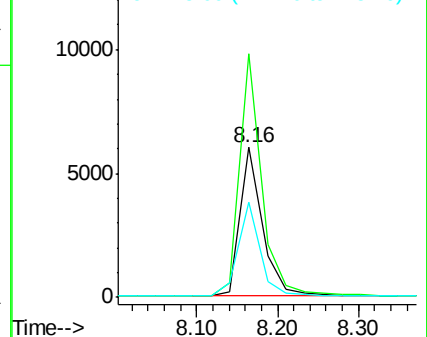

#4

2-Fluorophenol

Concen: 7.87 ng

RT: 5.67 min Scan# 363

Delta R.T. -0.01 min

Lab File: BE092466.D

Acq: 21 Oct 2016 14:30


Tgt Ion:112 Resp: 21486

Ion Ratio Lower Upper

112 100

64 67.8 53.5 80.3



63 36.4 27.9 41.9

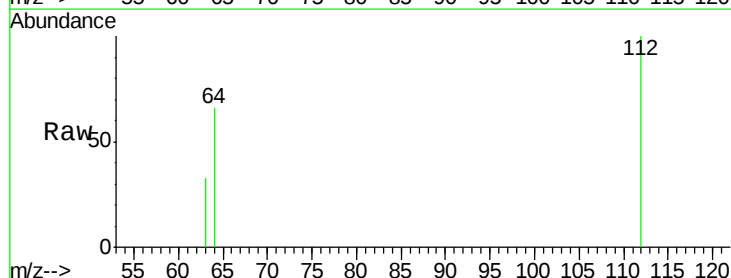


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

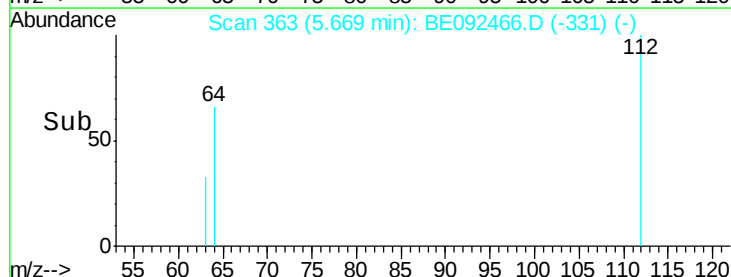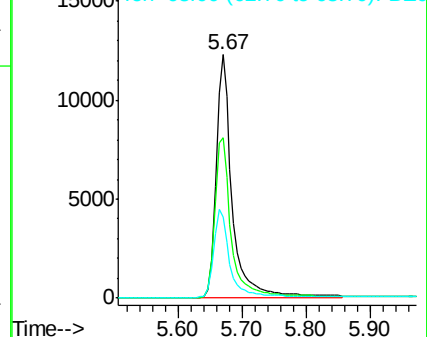

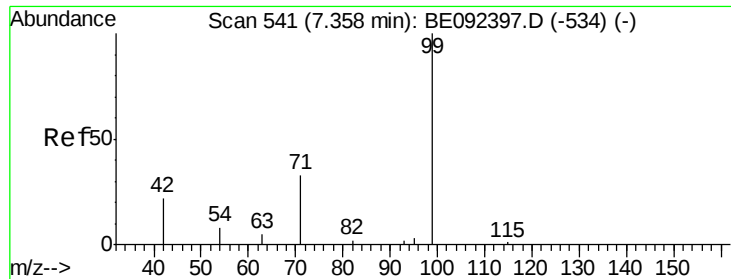

#5

Phenol-d6

Concen: 6.79 ng

RT: 7.34 min Scan# 540

Delta R.T. -0.02 min

Lab File: BE092466.D

Acq: 21 Oct 2016 14:30

Instrument :

BNA_E

ClientSampleId :

PB94258BL


Tgt Ion: 99 Resp: 26416

Ion Ratio Lower Upper

99 100

42 0.0 16.0 24.0#




71 34.6 30.6 45.8

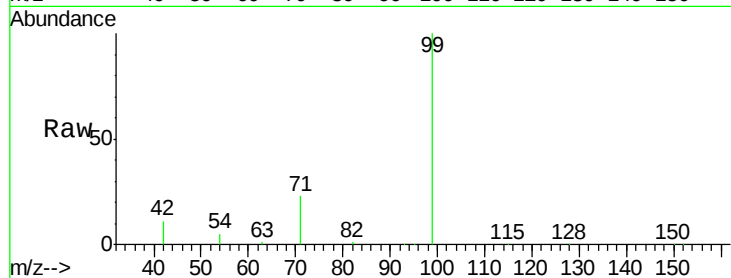

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

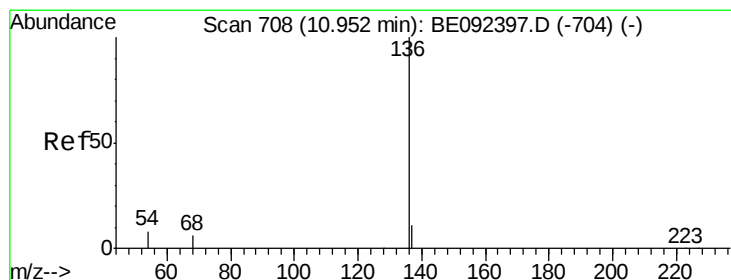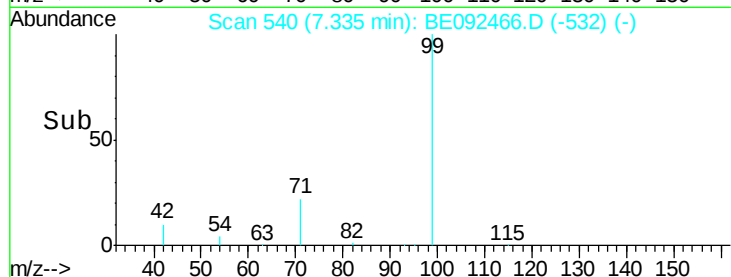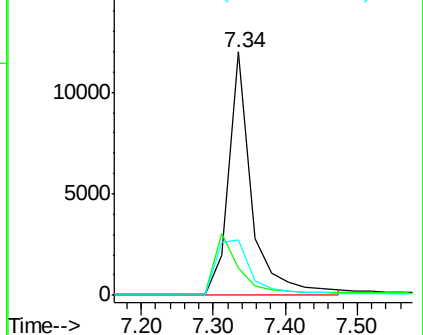

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.95 min Scan# 708

Delta R.T. 0.00 min

Lab File: BE092466.D

Acq: 21 Oct 2016 14:30

Tgt Ion: 136 Resp: 48185


Ion Ratio Lower Upper

136 100

137 11.2 8.2 12.4

54 7.1 9.6 14.4#

68 5.2 6.7 10.1#


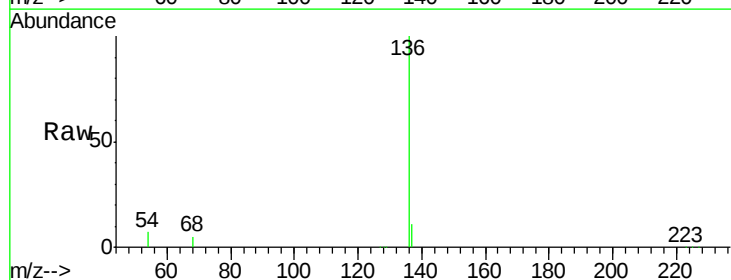



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

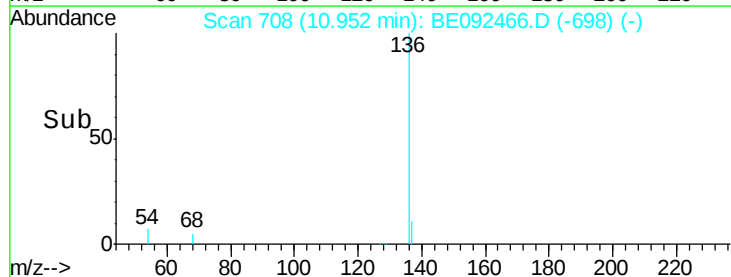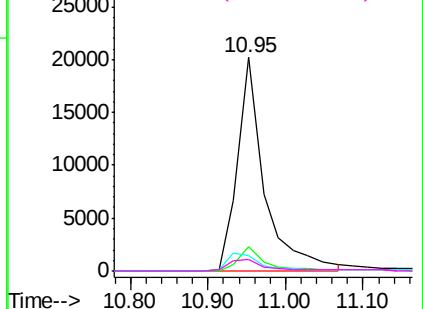

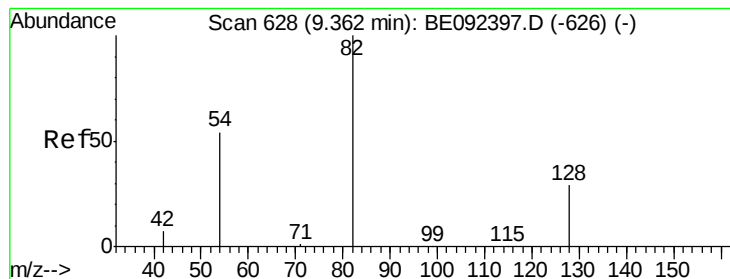

#8

Nitrobenzene-d5

Concen: 3.31 ng

RT: 9.34 min Scan# 627

Delta R.T. -0.02 min

Lab File: BE092466.D

Acq: 21 Oct 2016 14:30

Instrument :

BNA_E

ClientSampleId :

PB94258BL


Tgt Ion: 82 Resp: 11291

Ion Ratio Lower Upper

82 100

128 20.5 39.0 58.4#




54 64.4 44.8 67.2

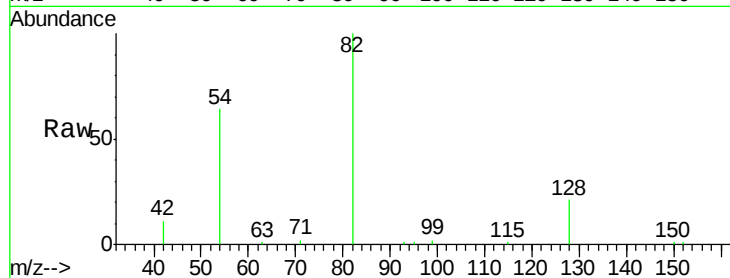

Abundance Ion 82.00 (81.70 to 82.70): BE092397.D (-626) (-)

Ion 128.00 (127.70 to 128.70): BE092397.D (-626) (-)

Ion 54.00 (53.70 to 54.70): BE092397.D (-626) (-)

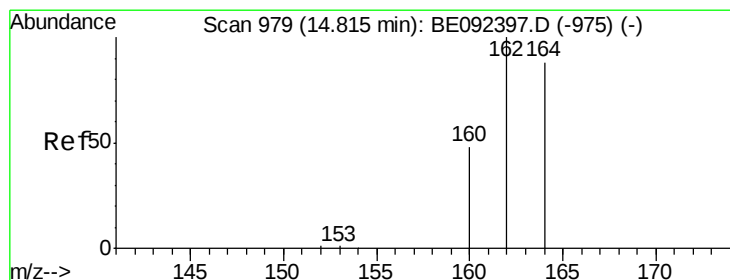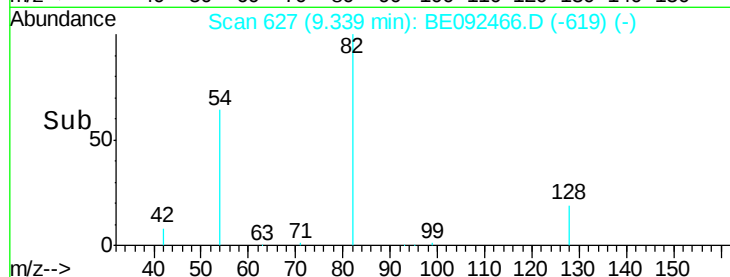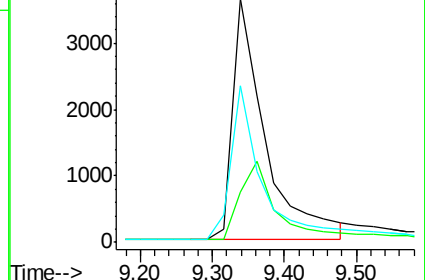

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.81 min Scan# 980

Delta R.T. -0.00 min

Lab File: BE092466.D

Acq: 21 Oct 2016 14:30


Tgt Ion: 164 Resp: 29633

Ion Ratio Lower Upper

164 100

162 106.8 71.4 107.0



160 49.5 27.4 41.2#

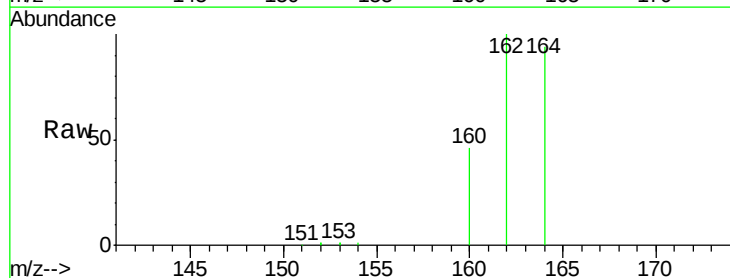


Abundance Ion 164.00 (163.70 to 164.70): BE092397.D (-975) (-)

Ion 162.00 (161.70 to 162.70): BE092397.D (-975) (-)

Ion 160.00 (159.70 to 160.70): BE092397.D (-975) (-)



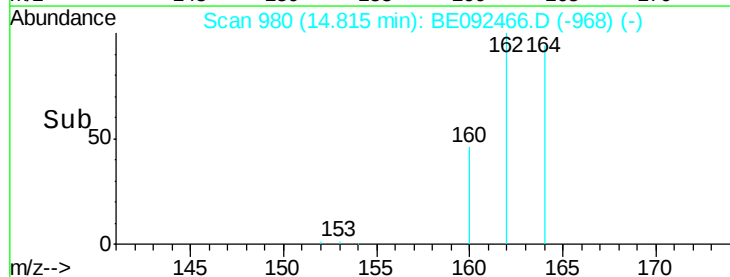
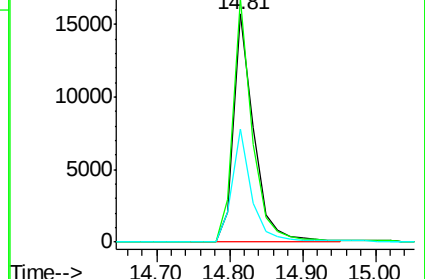


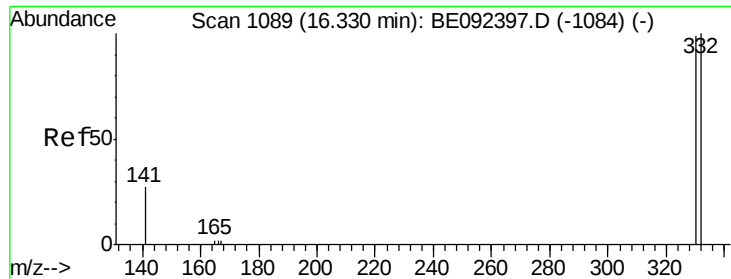

#13
 2,4,6-Tribromophenol
 Concen: 4.74 ng
 RT: 16.32 min Scan# 1089
 Delta R.T. 0.00 min
 Lab File: BE092466.D
 Acq: 21 Oct 2016 14:30




Instrument :
 BNA_E
 ClientSampleId :
 PB94258BL


Tgt Ion:330 Resp: 4911
 Ion Ratio Lower Upper
 330 100
 332 96.9 75.4 113.0
 141 44.8 31.0 46.6

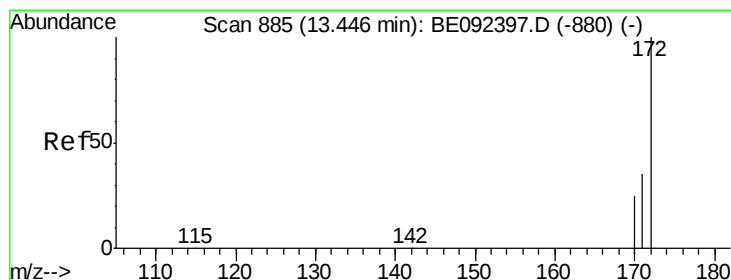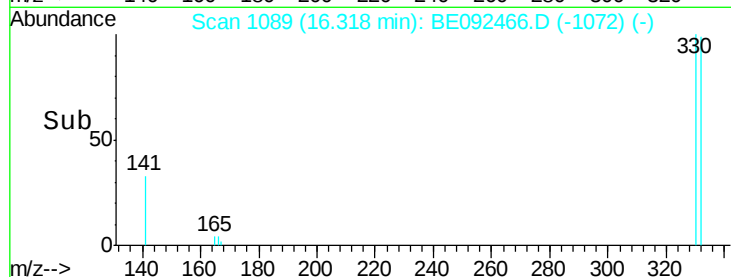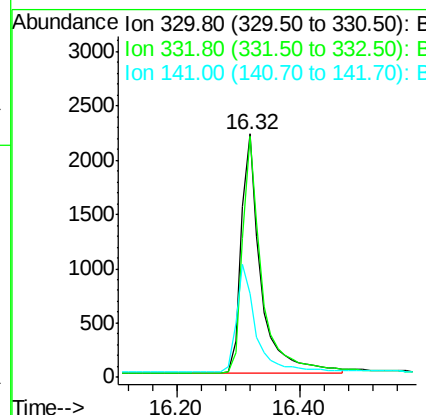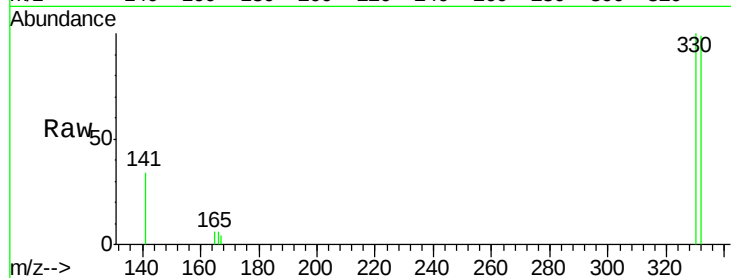

#14
 2-Fluorobiphenyl
 Concen: 4.21 ng
 RT: 13.45 min Scan# 885
 Delta R.T. 0.00 min
 Lab File: BE092466.D
 Acq: 21 Oct 2016 14:30

Tgt Ion:172 Resp: 29519
 Ion Ratio Lower Upper
 172 100
 171 31.6 30.1 45.1
 170 20.2 21.8 32.6#

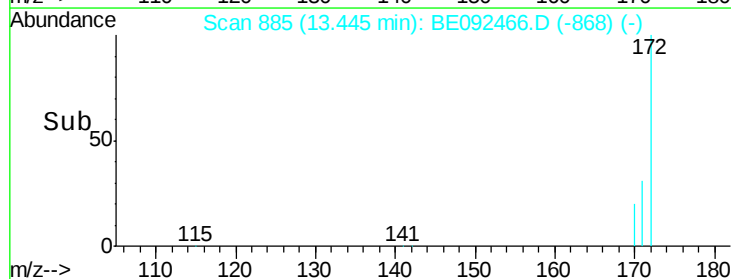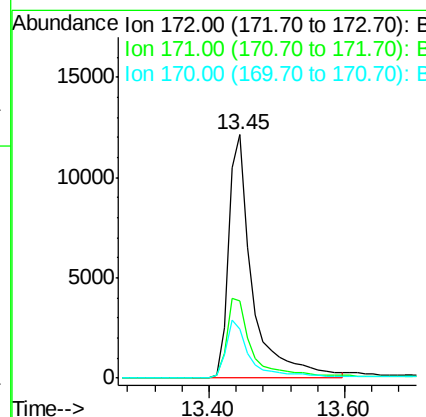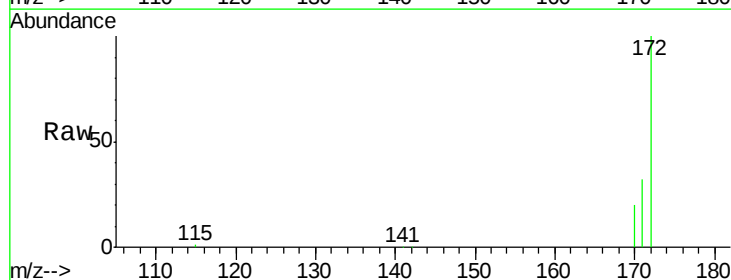

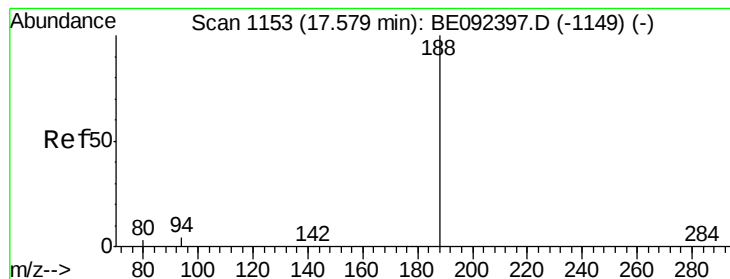

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.58 min Scan# 1154

Delta R.T. 0.00 min

Lab File: BE092466.D

Acq: 21 Oct 2016 14:30

Instrument :

BNA_E

ClientSampleId :

PB94258BL


Tgt Ion:188 Resp: 55639

Ion Ratio Lower Upper

188 100

94 5.1 3.2 4.8#




80 4.8 2.6 3.8#

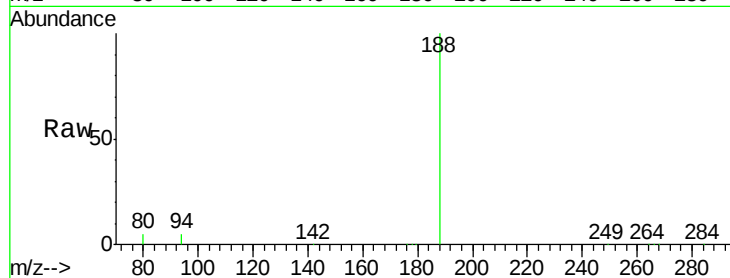

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

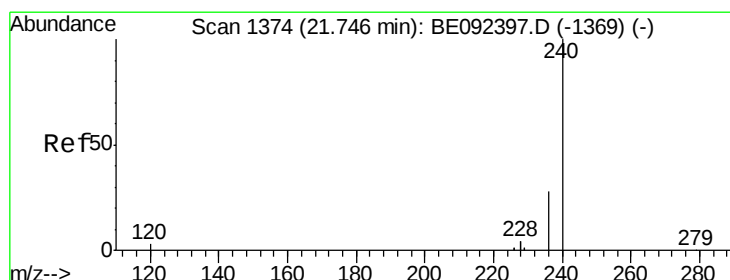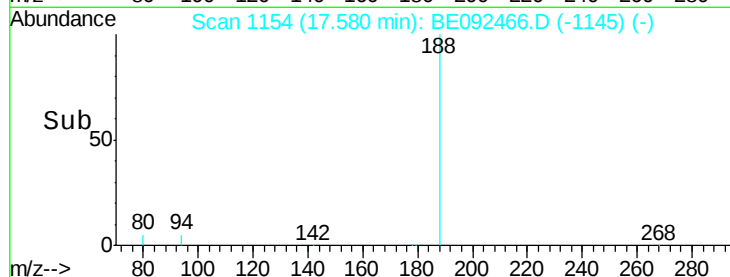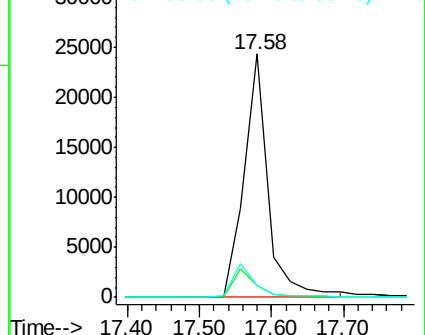

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.75 min Scan# 1375

Delta R.T. 0.00 min

Lab File: BE092466.D

Acq: 21 Oct 2016 14:30


Tgt Ion:240 Resp: 75863

Ion Ratio Lower Upper

240 100

120 3.9 2.6 4.0



236 27.8 24.6 37.0

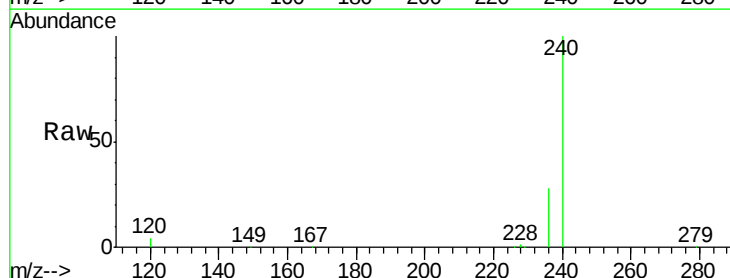


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



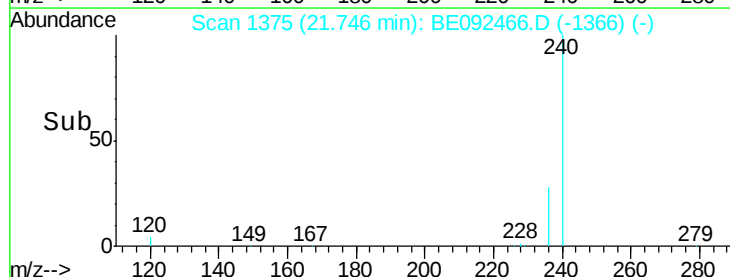
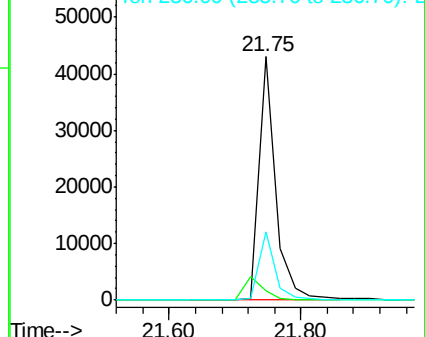


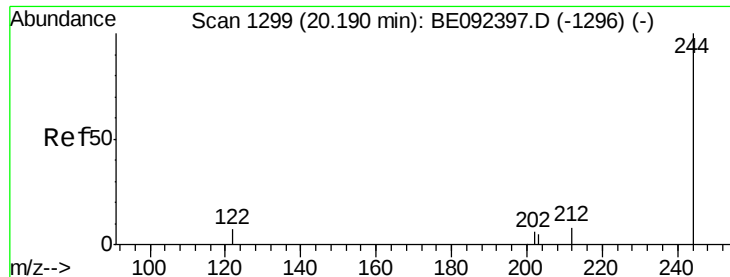

#26
 Terphenyl-d14
 Concen: 3.91 ng
 RT: 20.17 min Scan# 1299
 Delta R.T. -0.02 min
 Lab File: BE092466.D
 Acq: 21 Oct 2016 14:30

Instrument :
 BNA_E
 ClientSampleId :
 PB94258BL

Tgt Ion: 244 Resp: 36802
 Ion Ratio Lower Upper
 244 100
 212 10.0 6.7 10.1
 122 17.2 3.6 5.4#

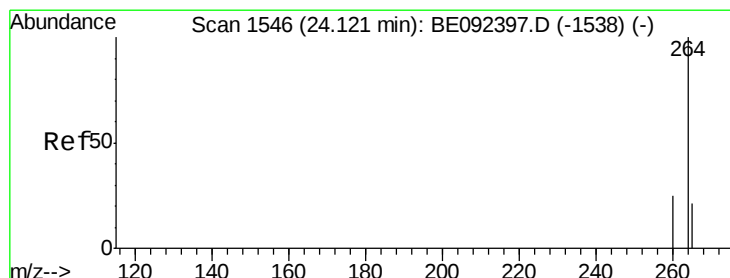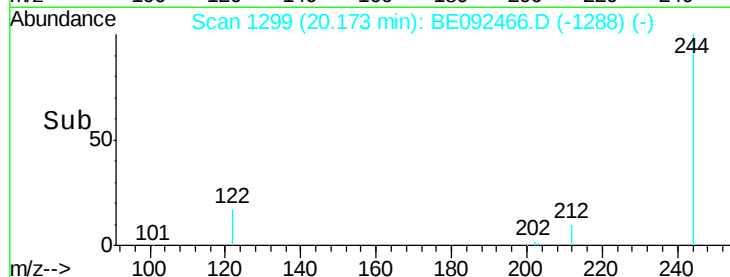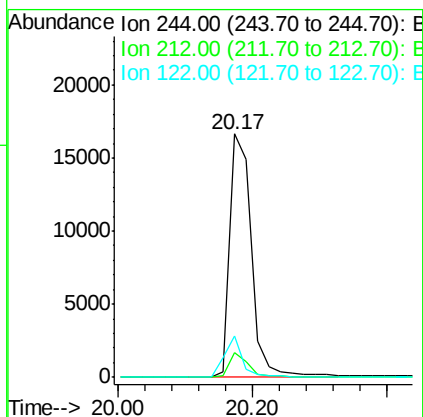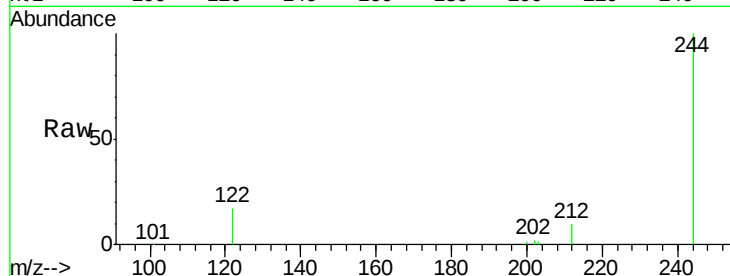

#31
 Perylene-d12
 Concen: 5.00 ng
 RT: 24.12 min Scan# 1547
 Delta R.T. 0.01 min
 Lab File: BE092466.D
 Acq: 21 Oct 2016 14:30

Tgt Ion: 264 Resp: 69867
 Ion Ratio Lower Upper
 264 100
 260 24.4 20.1 30.1
 265 22.4 17.9 26.9

