
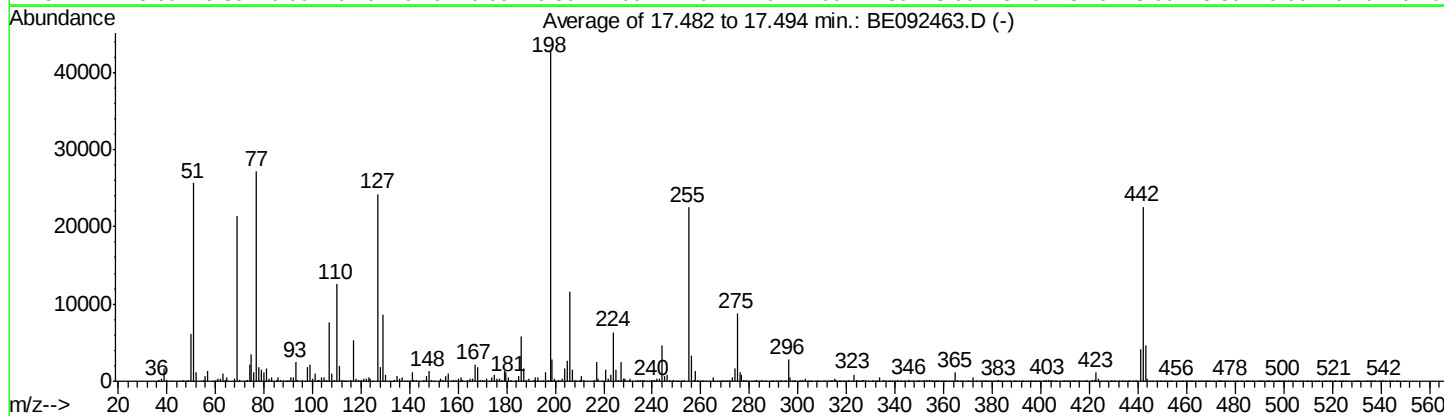


Data Path : Z:\HPCHEM1\BNA_E\Data\Be102116\
Data File : BE092463.D
Acq On : 21 Oct 2016 11:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092216.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 22 18:25:56 2016

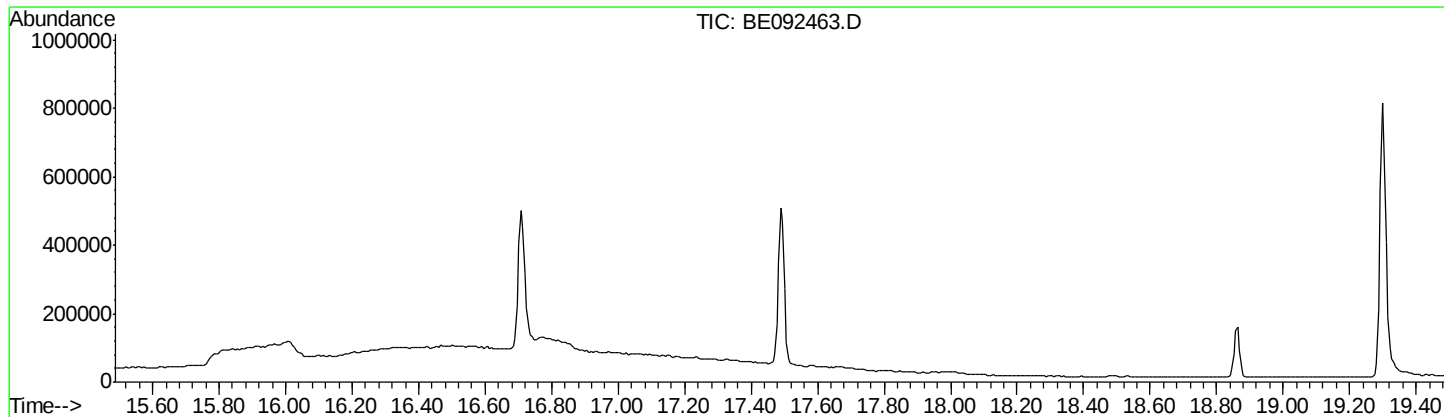

AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2525

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.8	25679	PASS
68	69	0.00	2	1.8	383	PASS
69	198	0.00	100	49.9	21436	PASS
70	69	0.00	2	0.5	117	PASS
127	198	10	80	56.4	24205	PASS
197	198	0.00	2	0.4	162	PASS
198	198	100	100	100.0	42935	PASS
199	198	5	9	6.4	2740	PASS
275	198	10	60	20.3	8732	PASS
365	198	1	100	2.6	1129	PASS
441	442	0.01	24	18.1	4090	PASS
442	198	50	100	52.5	22550	PASS
443	442	15	24	20.4	4590	PASS