


Data Path : Z:\HPCHEM1\BNA_E\Data\BE102214\
Data File : BE088179.D
Acq On : 22 Oct 2014 13:02
Operator : TP/JJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE102014.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 21 02:11:14 2014

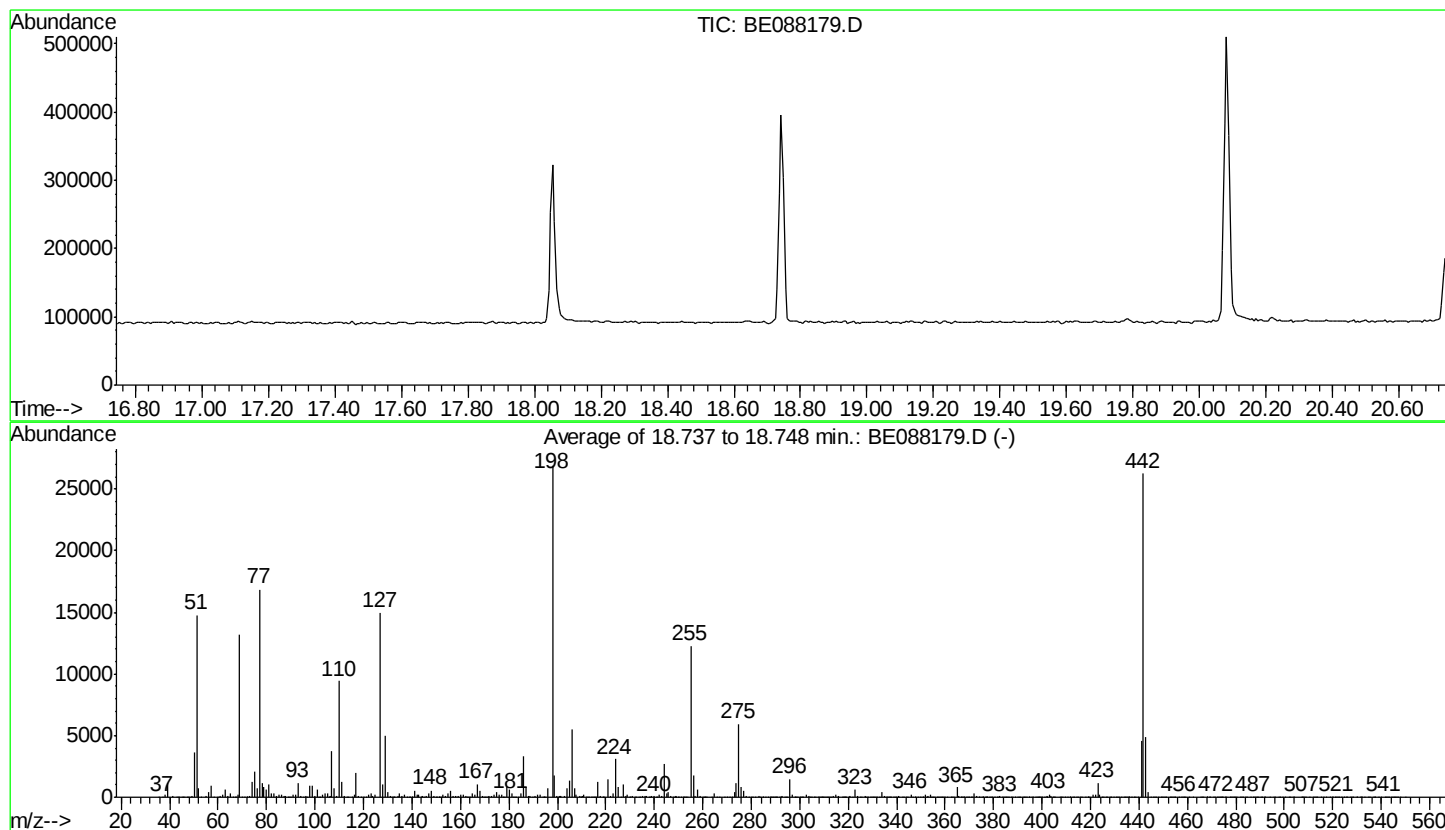

AutoFind: Scans 2646, 2647, 2648; Background Corrected with Scan 2638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.9	14782	PASS
68	69	0.00	2	1.3	175	PASS
69	198	0.00	100	49.1	13210	PASS
70	69	0.00	2	0.4	48	PASS
127	198	10	80	55.6	14958	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26902	PASS
199	198	5	9	6.7	1808	PASS
275	198	10	60	22.1	5937	PASS
365	198	1	100	3.0	797	PASS
441	442	0.01	24	17.6	4624	PASS
442	198	50	100	97.6	26255	PASS
443	442	15	24	18.7	4911	PASS