


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE102315\
Data File : BE091034.D
Acq On : 23 Oct 2015 12:44
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE092815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 07 17:11:43 2015

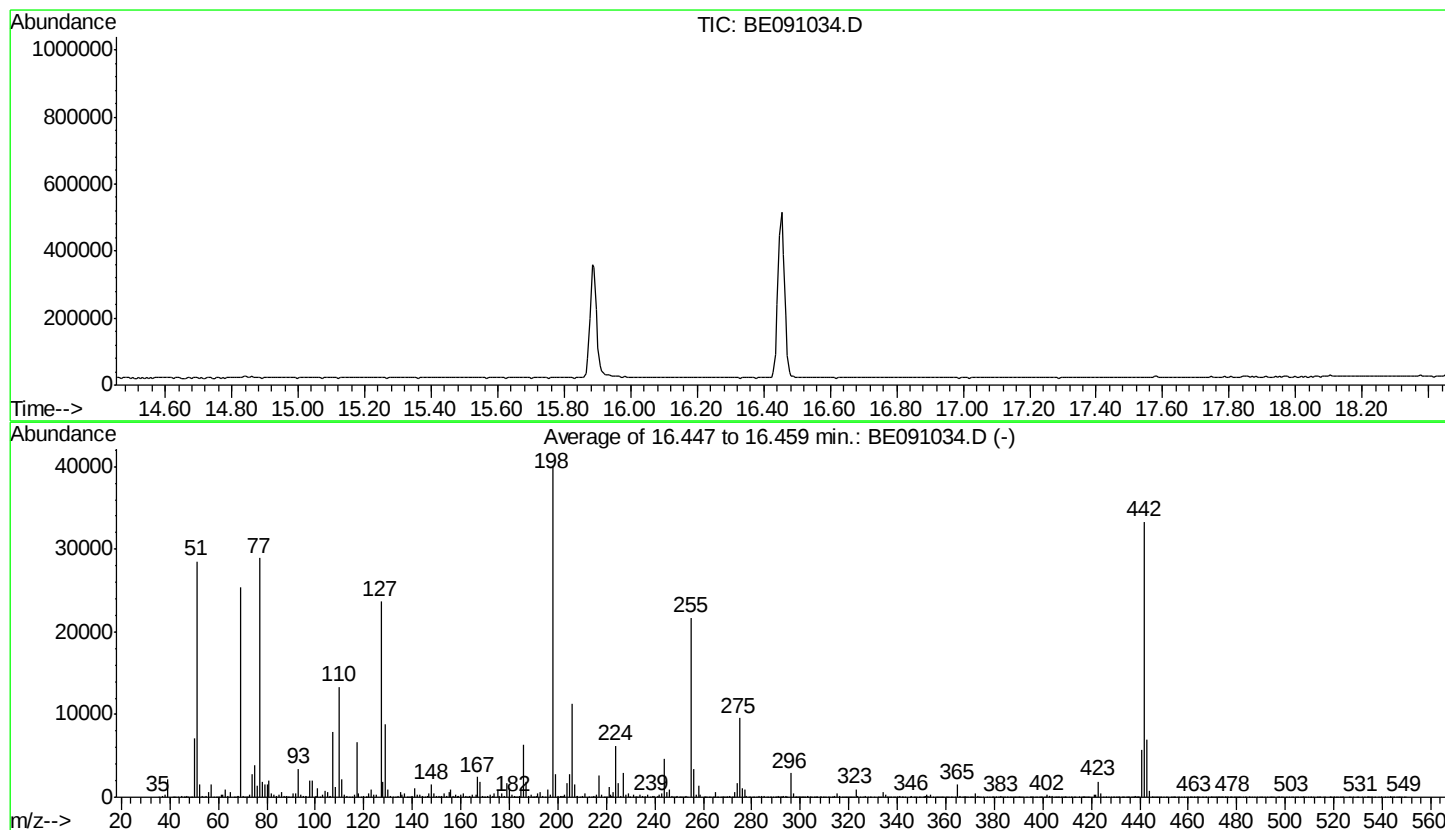

AutoFind: Scans 2359, 2360, 2361; Background Corrected with Scan 2351

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	71.1	28504	PASS
68	69	0.00	2	0.8	213	PASS
69	198	0.00	100	63.4	25417	PASS
70	69	0.00	2	0.7	183	PASS
127	198	10	80	58.9	23626	PASS
197	198	0.00	2	0.6	257	PASS
198	198	100	100	100.0	40114	PASS
199	198	5	9	7.1	2864	PASS
275	198	10	60	23.8	9537	PASS
365	198	1	100	3.8	1509	PASS
441	442	0.01	24	17.0	5670	PASS
442	198	50	100	83.1	33332	PASS
443	442	15	24	20.9	6950	PASS