
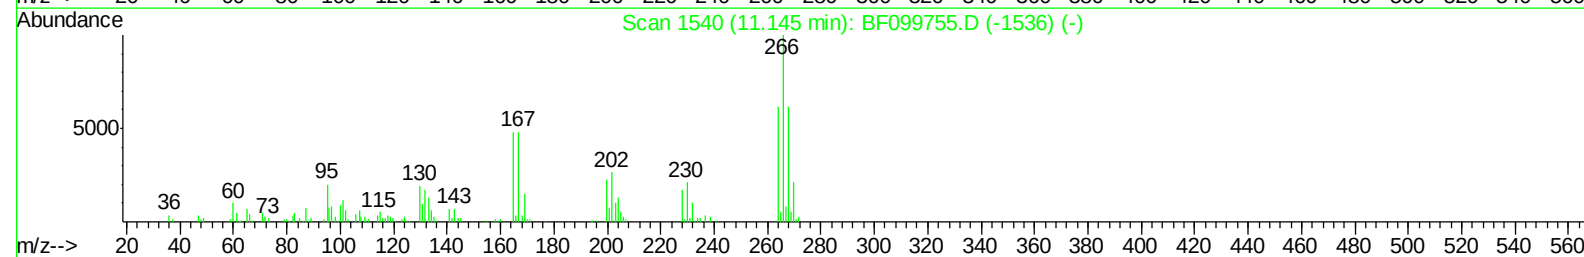
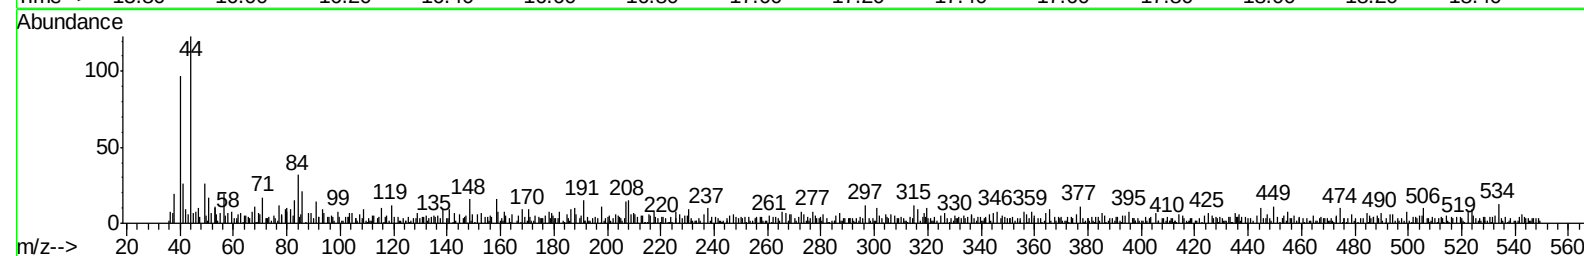


Data Path : Z:\HPCHEM1\BNA E\DATA\BE102317\
 Data File : BE094494.D
 Acq On : 23 Oct 2017 14:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 02:40:59 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 23 23:39:26 2017
 Response via : Initial Calibration

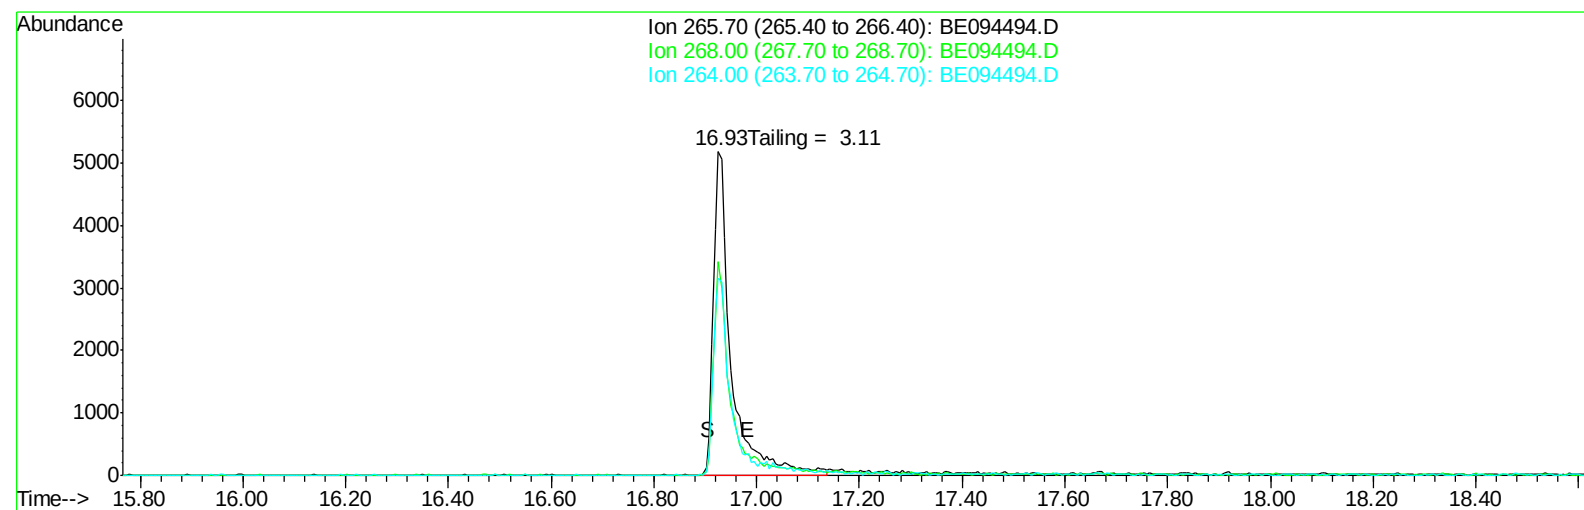

TIC: BE094494.D

(69) Pentachlorophenol (C)




10.962min (-0.184) 118.52ng

response 6

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	75.00
264.00	61.90	62.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102317\
 Data File : BE094494.D
 Acq On : 23 Oct 2017 14:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 02:40:59 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 23 23:39:26 2017
 Response via : Initial Calibration

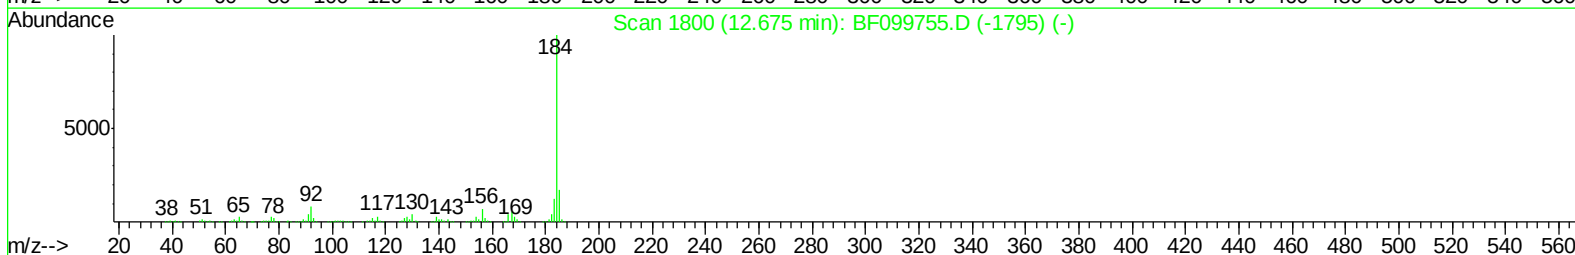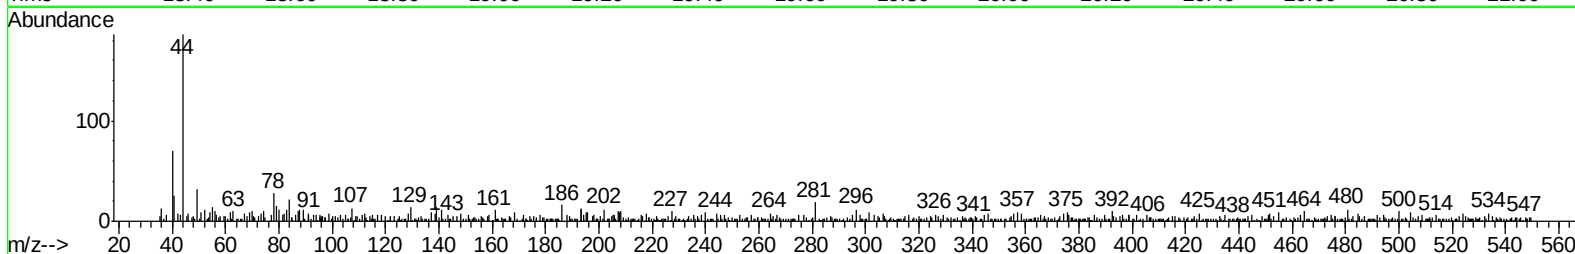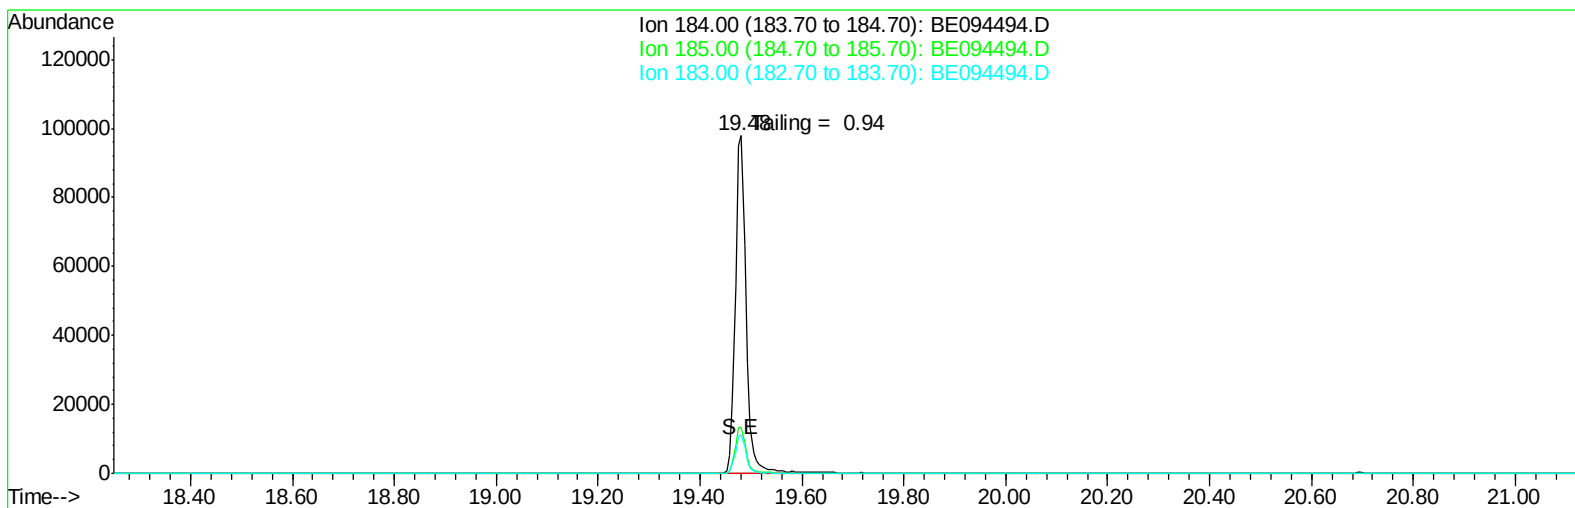

TIC: BE094494.D

(76) Benzidine

12.366min (-0.309) 12.47ng

response 6

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	33.33#
183.00	11.60	22.22#
0.00	0.00	0.00