


Data Path : Z:\HPCHEM1\BNA E\DATA\BE102317\
Data File : BE094494.D
Acq On : 23 Oct 2017 14:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 23 22:40:47 2017

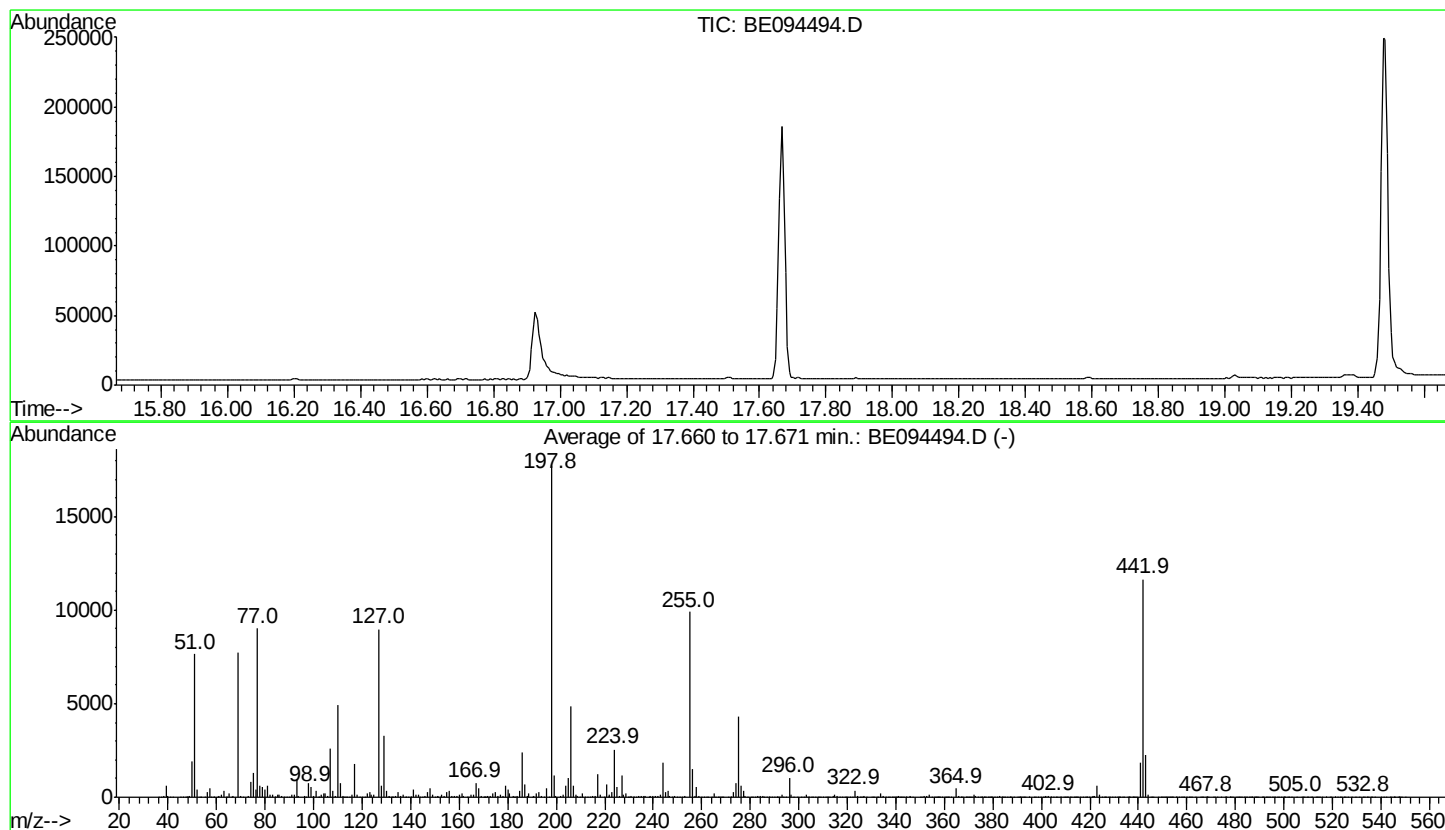

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	7647	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.6	7725	PASS
70	69	0.00	2	0.6	46	PASS
127	198	10	80	50.7	8987	PASS
197	198	0.00	2	0.1	25	PASS
198	198	100	100	100.0	17723	PASS
199	198	5	9	6.5	1155	PASS
275	198	10	60	24.5	4342	PASS
365	198	1	100	2.7	472	PASS
441	442	0.01	24	15.9	1849	PASS
442	198	50	100	65.8	11658	PASS
443	442	15	24	19.7	2292	PASS