


Data Path : Z:\HPCHEM1\BNA_E\Data\Be102414\
 Data File : BE088206.D
 Acq On : 24 Oct 2014 11:18
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE102414.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 27 13:04:40 2014

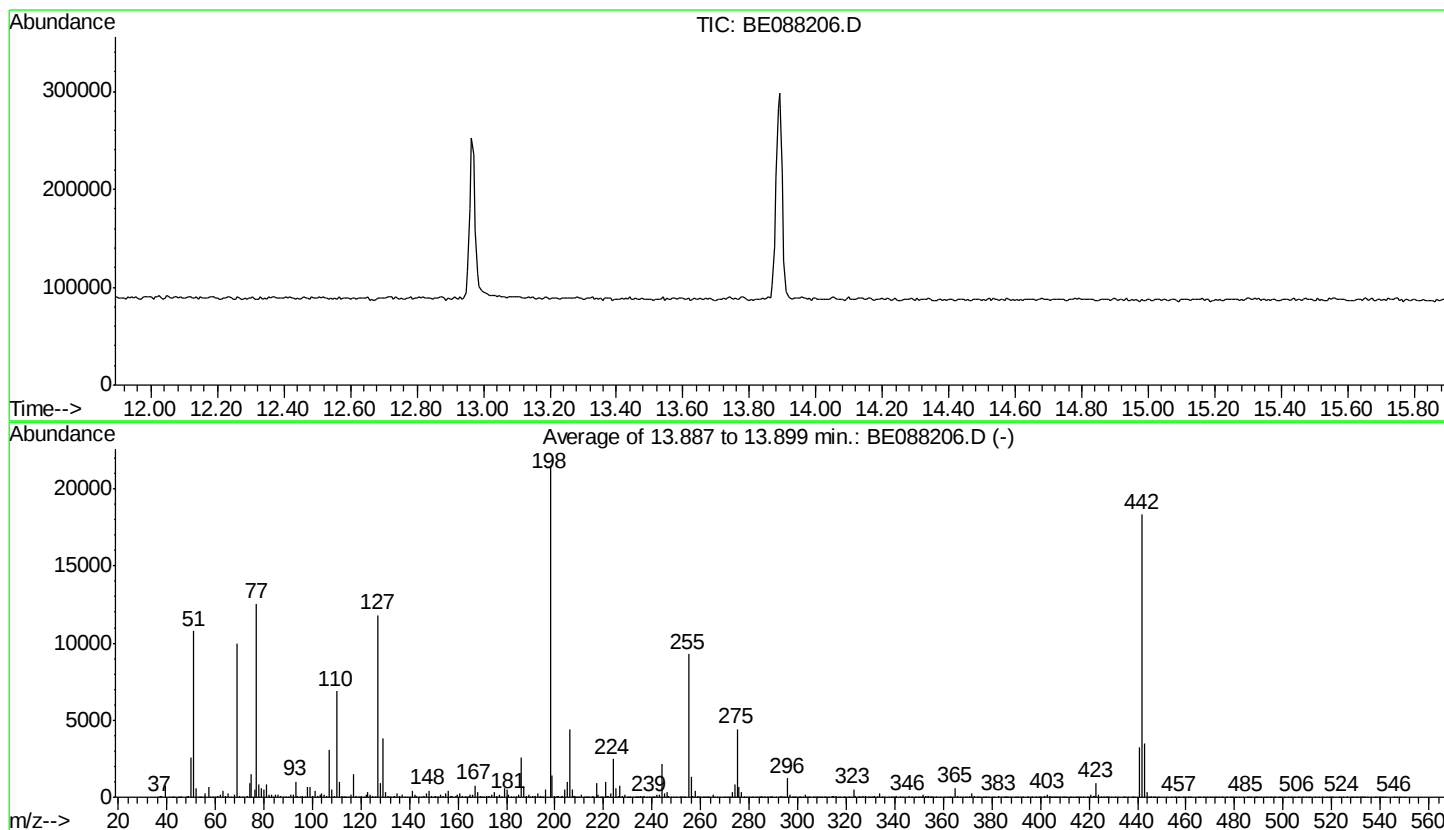

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	10779	PASS
68	69	0.00	2	1.3	129	PASS
69	198	0.00	100	46.2	9933	PASS
70	69	0.00	2	0.5	53	PASS
127	198	10	80	54.9	11804	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21508	PASS
199	198	5	9	6.5	1396	PASS
275	198	10	60	20.6	4438	PASS
365	198	1	100	2.7	588	PASS
441	442	0.01	24	17.6	3230	PASS
442	198	50	100	85.3	18341	PASS
443	442	15	24	19.1	3499	PASS