


Data Path : Z:\HPCHEM1\BNA_E\Data\Be102414\
Data File : Be088226.d
Acq On : 25 Oct 2014 00:34
Operator : TP/JJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BE102414.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 27 13:04:40 2014

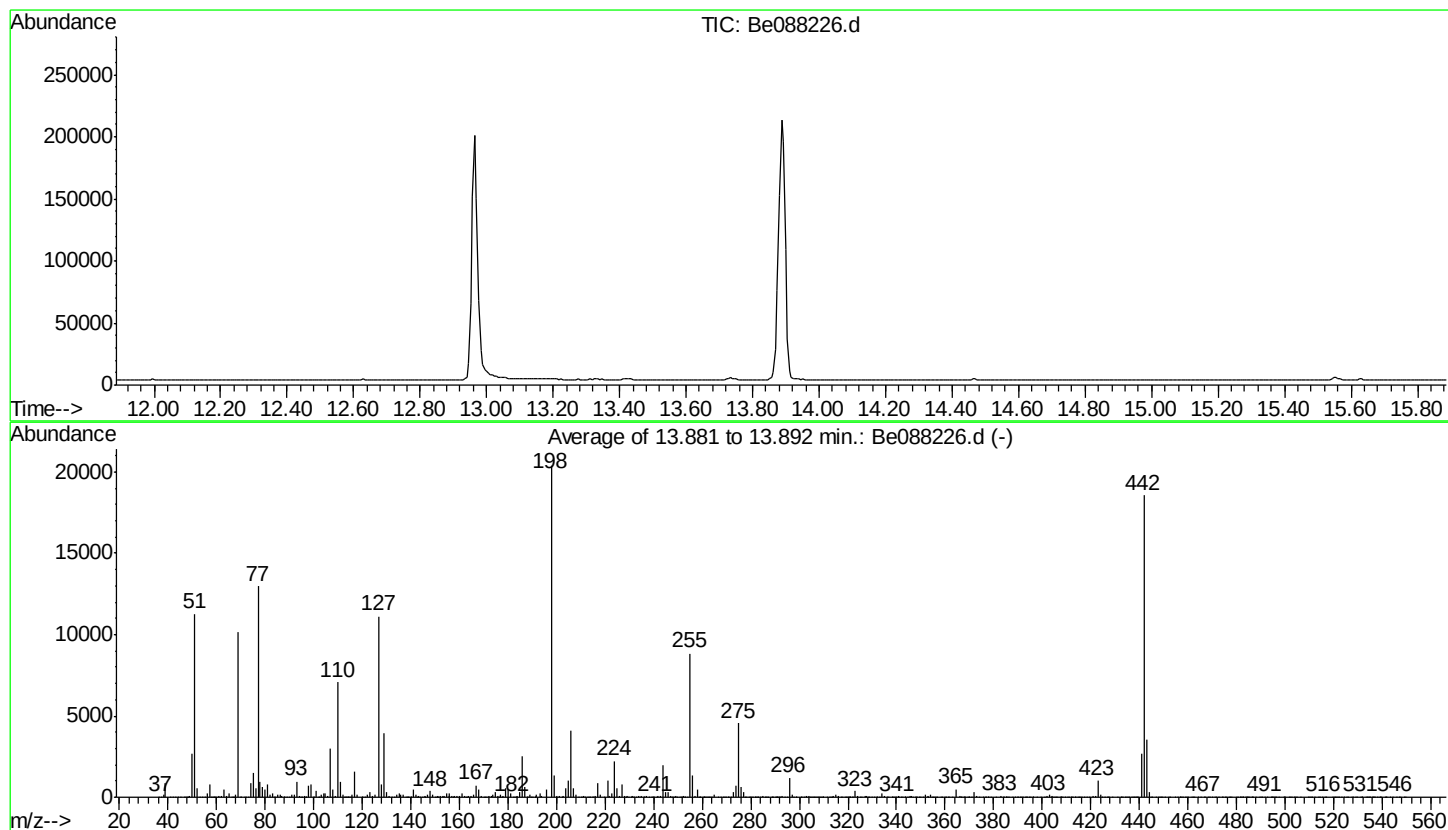

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.3	11279	PASS
68	69	0.00	2	1.4	144	PASS
69	198	0.00	100	49.9	10184	PASS
70	69	0.00	2	0.3	29	PASS
127	198	10	80	54.6	11139	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20389	PASS
199	198	5	9	6.7	1364	PASS
275	198	10	60	22.3	4550	PASS
365	198	1	100	2.4	496	PASS
441	442	0.01	24	14.4	2662	PASS
442	198	50	100	90.9	18543	PASS
443	442	15	24	19.2	3559	PASS