
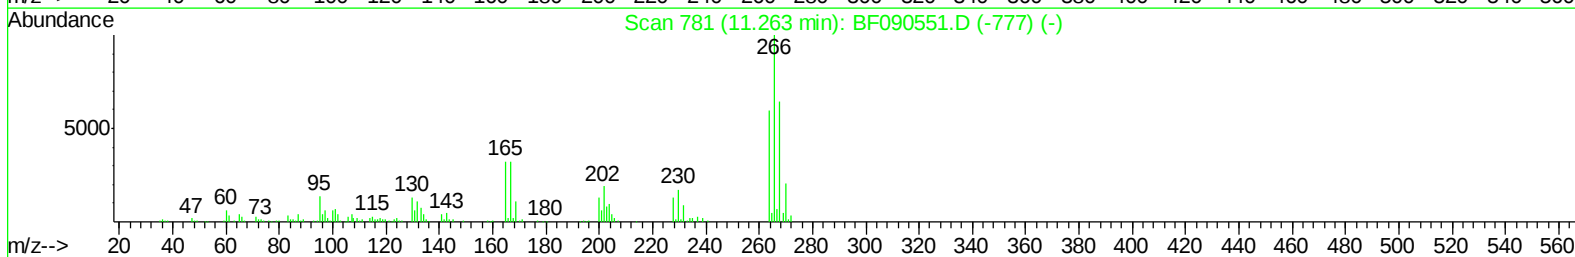
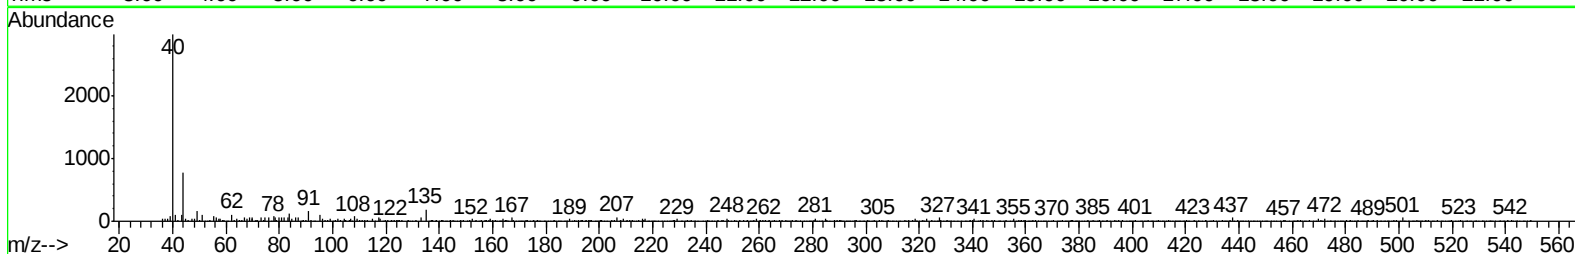


Data Path : Z:\HPCHEM1\BNA E\DATA\BE102516\
Data File : BE092470.D
Acq On : 25 Oct 2016 8:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 18:52:02 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 19 15:13:23 2016
Response via : Initial Calibration

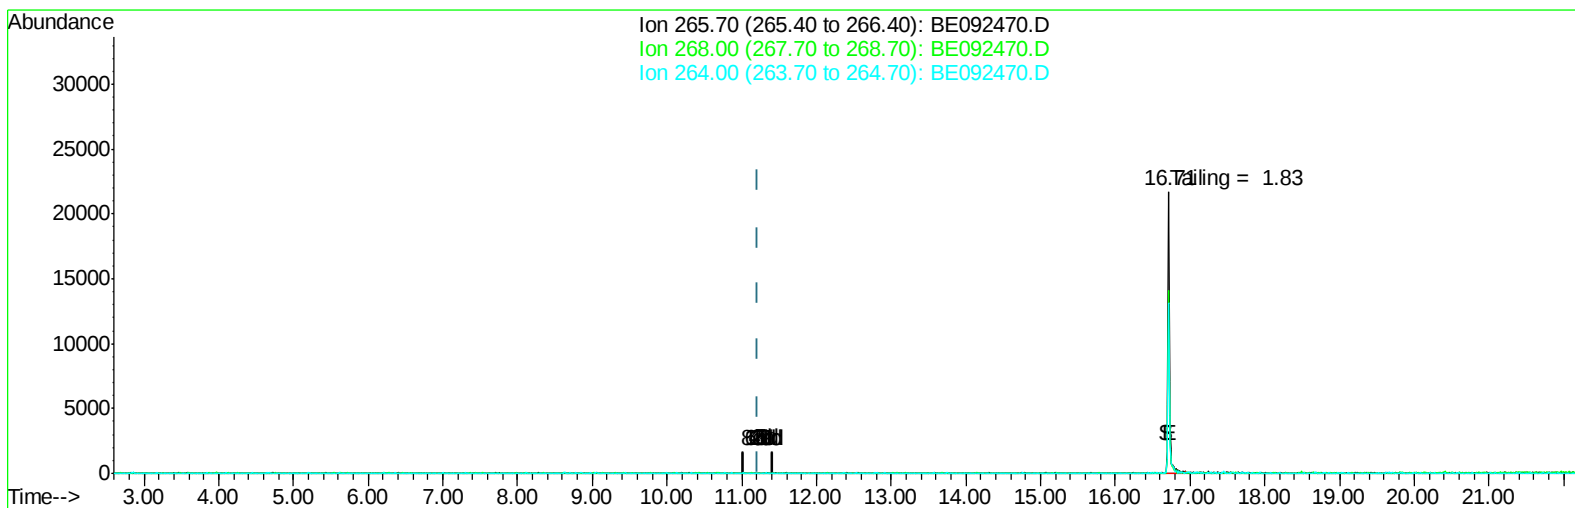

TIC: BE092470.D

(69) Pentachlorophenol (C)




11.138min (-0.091) 66.61ng

response 10

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	66.67
264.00	59.90	62.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE102516\
 Data File : BE092470.D
 Acq On : 25 Oct 2016 8:36
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 18:52:02 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 19 15:13:23 2016
 Response via : Initial Calibration

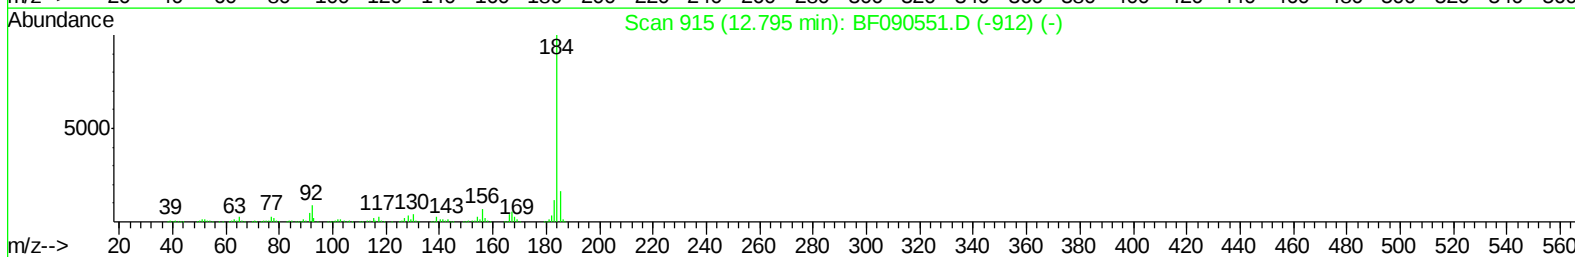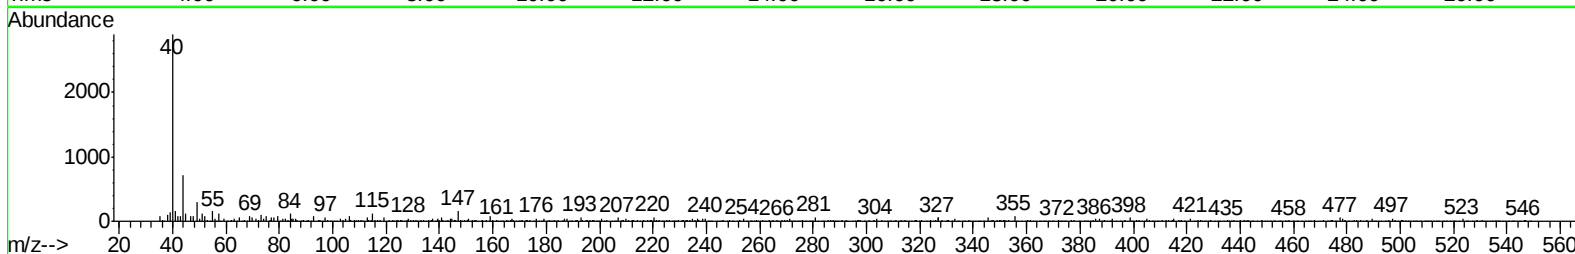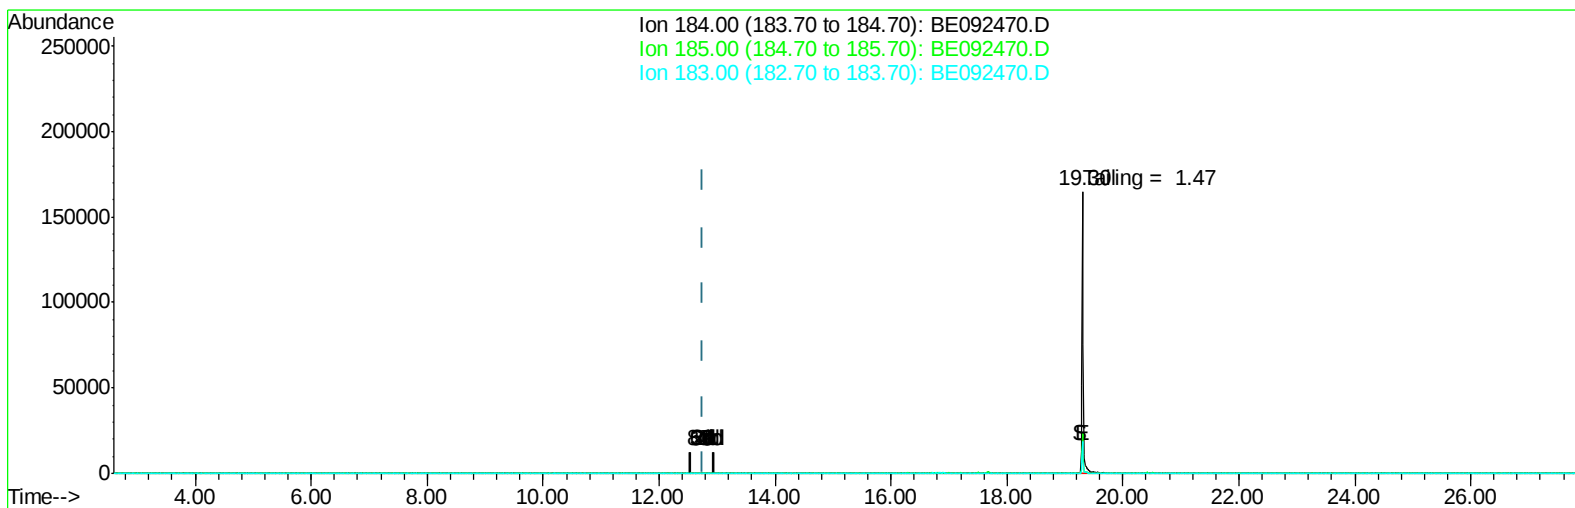

TIC: BE092470.D

(76) Benzidine

12.819min (+0.058) 53.59ng

response 16

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	0.00#
183.00	11.70	114.81#
0.00	0.00	0.00