


Data Path : Z:\HPCHEM1\BNA E\DATA\BE102516\
Data File : BE092470.D
Acq On : 25 Oct 2016 8:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE102516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 25 15:25:33 2016

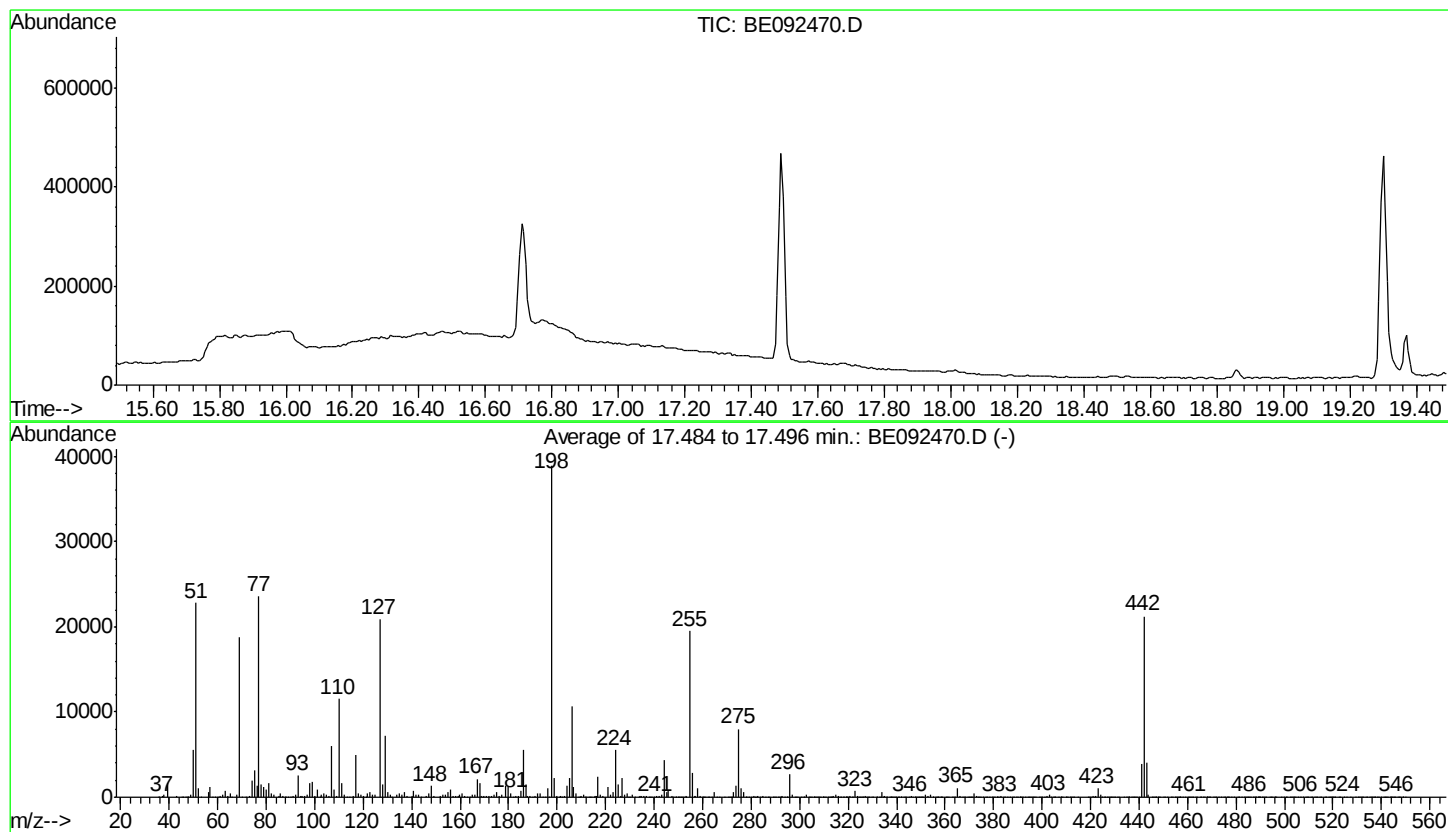

AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.7	22836	PASS
68	69	0.00	2	1.2	232	PASS
69	198	0.00	100	48.2	18779	PASS
70	69	0.00	2	0.4	78	PASS
127	198	10	80	53.6	20874	PASS
197	198	0.00	2	0.2	69	PASS
198	198	100	100	100.0	38927	PASS
199	198	5	9	5.7	2216	PASS
275	198	10	60	20.6	8034	PASS
365	198	1	100	2.7	1067	PASS
441	442	0.01	24	18.2	3871	PASS
442	198	50	100	54.5	21214	PASS
443	442	15	24	19.1	4055	PASS