




Data Path : Z:\HPCHEM1\BNA_E\Data\BE102517\
Data File : BE094522.D
Acq On : 24 Oct 2017 19:41
Operator : SJ/JU
Sample : SST3.252
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTD3.252

Manual Integrations
APPROVED

Sohil
10/27/2017 8:56:20 AM

Quant Time: Oct 24 20:16:30 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 24 18:46:10 2017
Response via : Initial Calibration

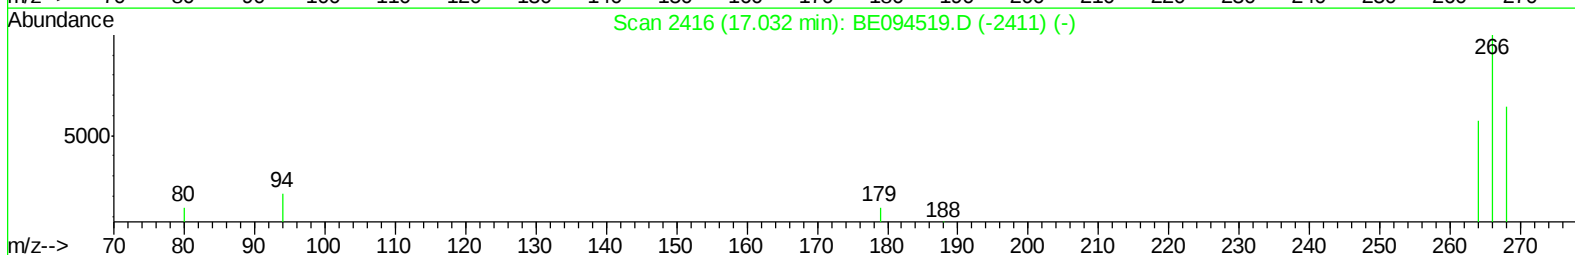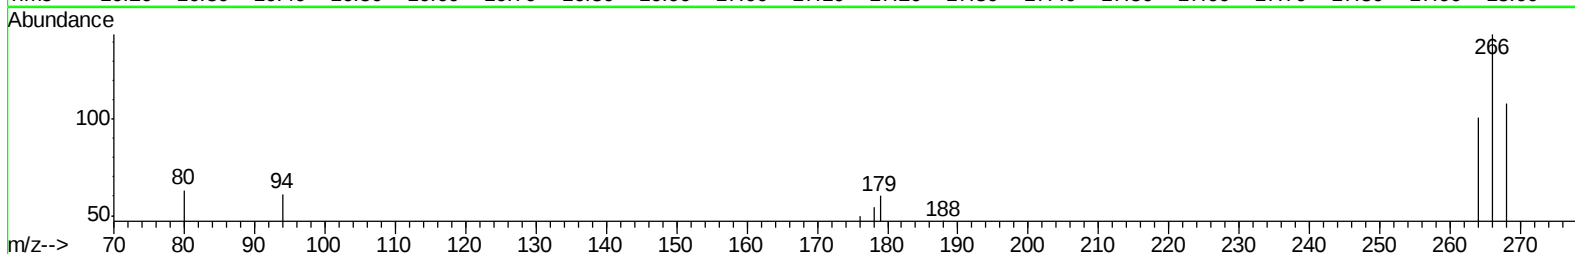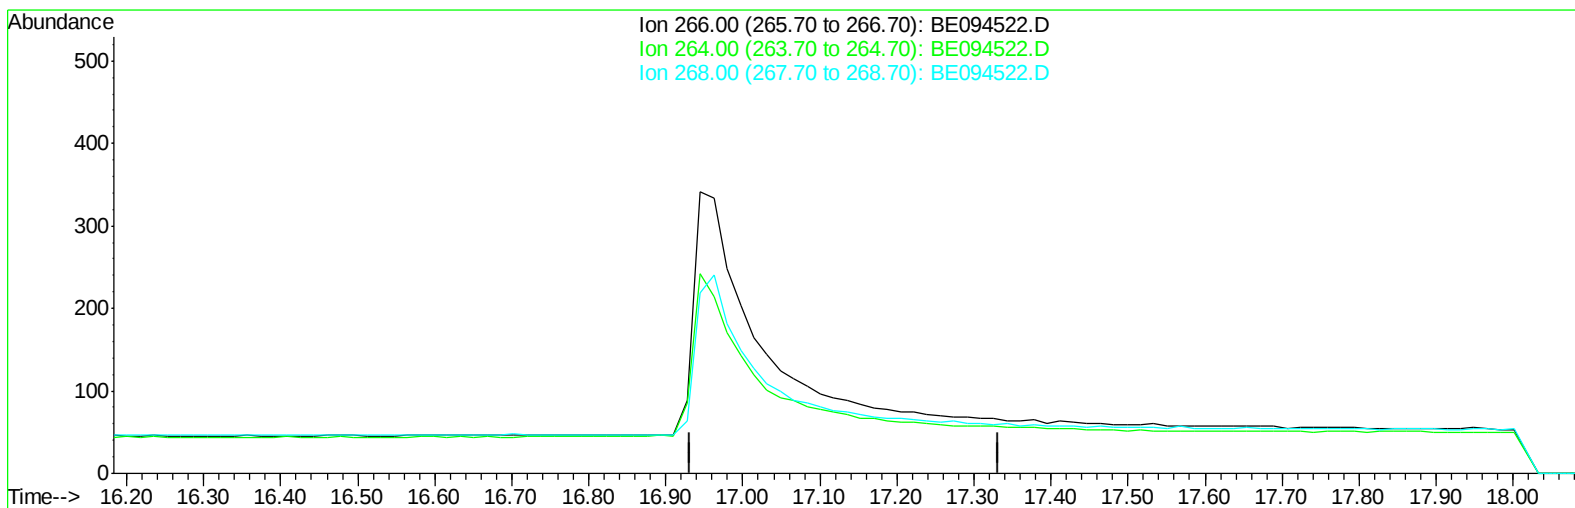

TIC: BE094522.D

(11) Pentachlorophenol

17.032min (-17.032) 0.00ng/ul

response 0

Ion	Exp%	Act%
266.00	100	0.00
264.00	59.90	0.00#
268.00	62.30	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE102517\
Data File : BE094522.D
Acq On : 24 Oct 2017 19:41
Operator : SJ/JU
Sample : SSTD3.252
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTD3.252

Manual Integrations
APPROVED

Sohil
10/27/2017 8:56:20 AM

Quant Time: Oct 24 20:16:30 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 24 18:46:10 2017
Response via : Initial Calibration

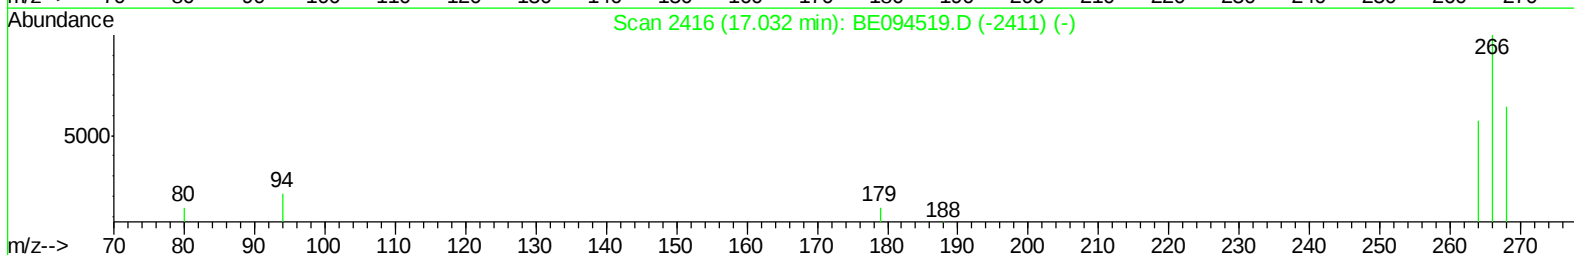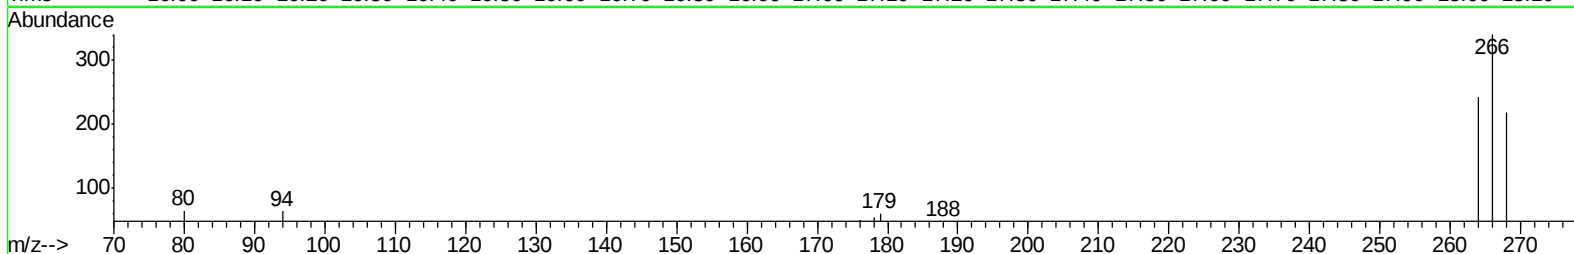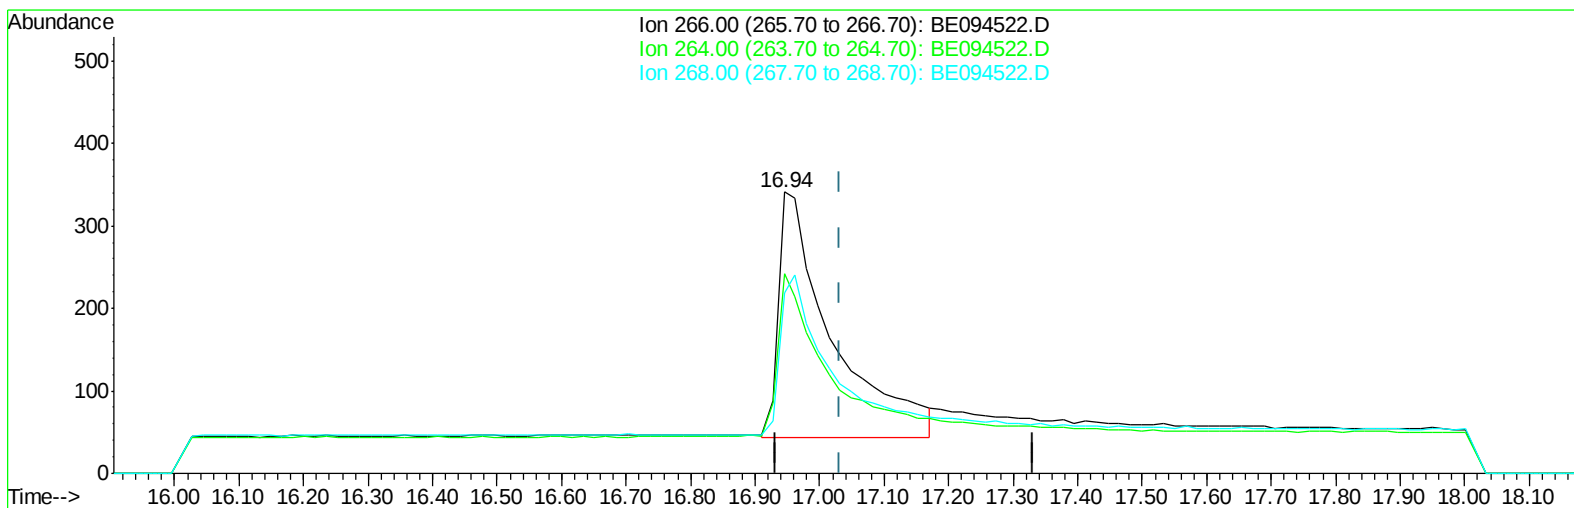

TIC: BE094522.D

(11) Pentachlorophenol
16.945min (-0.087) 1.71ng/ul m
response 1727

Ion	Exp%	Act%
266.00	100	100
264.00	59.90	0.00#
268.00	62.30	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE102517\
 Data File : BE094522.D
 Acq On : 24 Oct 2017 19:41
 Operator : SJ/JU
 Sample : SSTD3.252
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTD3.252

Manual Integrations
 APPROVED

Sohil
 10/27/2017 8:56:20 AM

Quant Time: Oct 24 20:19:07 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 24 18:46:10 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1176	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	6646	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	3805	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.24	188	8591	0.40	ng/ul	-0.02
16) Chrysene-d12	21.42	240	8997	0.40	ng/ul	0.00
20) Perylene-d12	23.95	264	8463	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul
14) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul

Target Compounds

					Qvalue
11) Pentachlorophenol	16.94	266	1727m	1.713	ng/ul

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE102517\
Data File : BE094522.D
Acq On : 24 Oct 2017 19:41
Operator : SJ/JU
Sample : SST3.252
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTD3.252

Manual Integrations
APPROVED

Sohil
10/27/2017 8:56:20 AM

Quant Time: Oct 24 20:19:07 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 24 18:46:10 2017
Response via : Initial Calibration

