




Data Path : Z:\HPCHEM1\BNA_E\Data\BE102517\
Data File : BE094527.D
Acq On : 25 Oct 2017 10:54
Operator : SJ/JU
Sample : PB103071BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK71

Manual Integrations
APPROVED

Sohil
10/27/2017 8:28:29 AM

Quant Time: Oct 25 18:20:08 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 17:03:27 2017
Response via : Initial Calibration

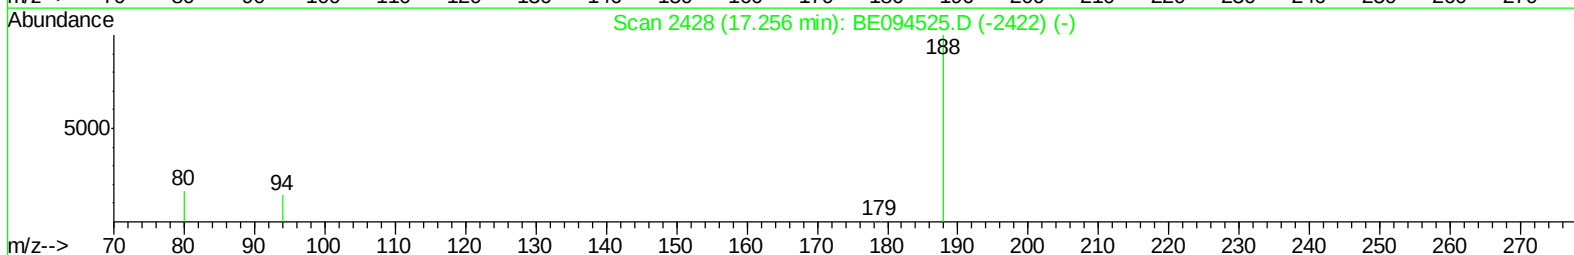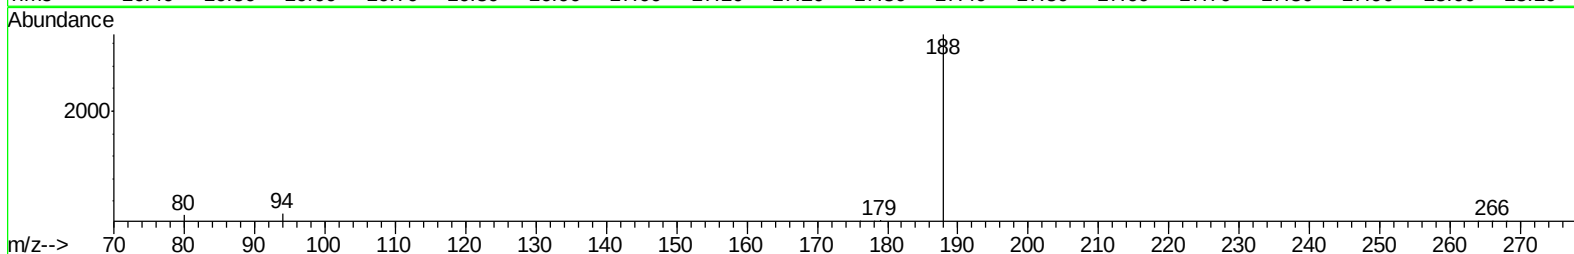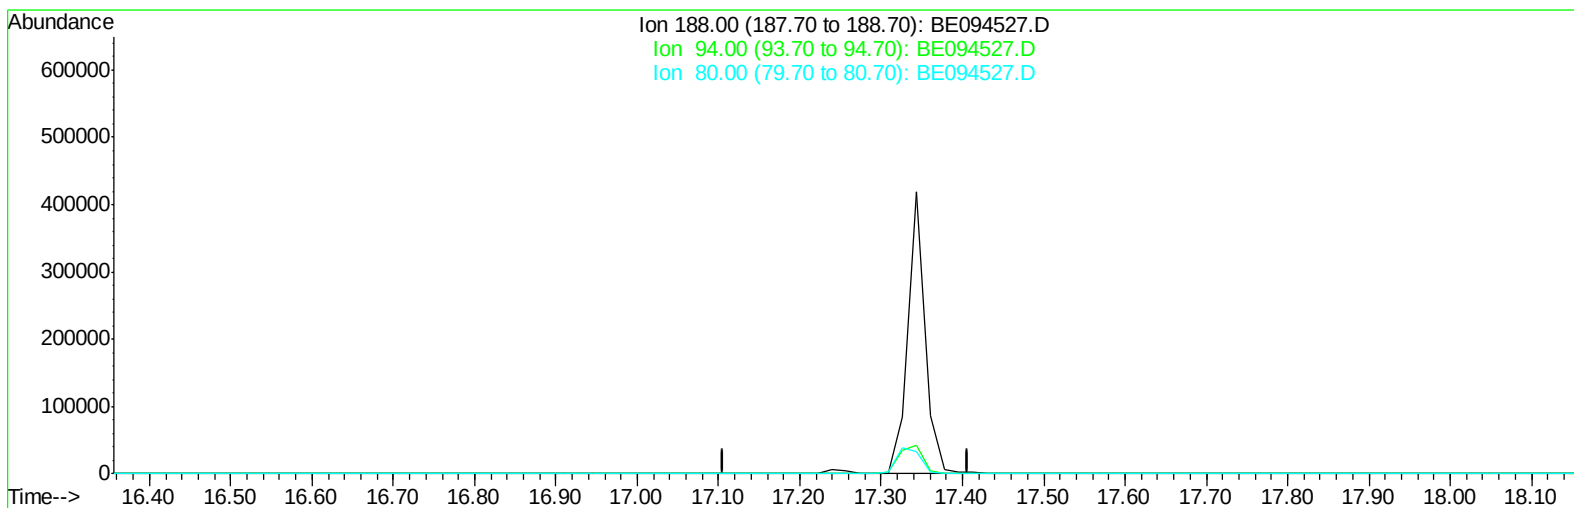

TIC: BE094527.D

(10) Phenanthrene-d10 (I)

17.257min (-17.257) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE102517\
Data File : BE094527.D
Acq On : 25 Oct 2017 10:54
Operator : SJ/JU
Sample : PB103071BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK71

Manual Integrations
APPROVED

Sohil
10/27/2017 8:28:29 AM

Quant Time: Oct 25 18:20:08 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 17:03:27 2017
Response via : Initial Calibration

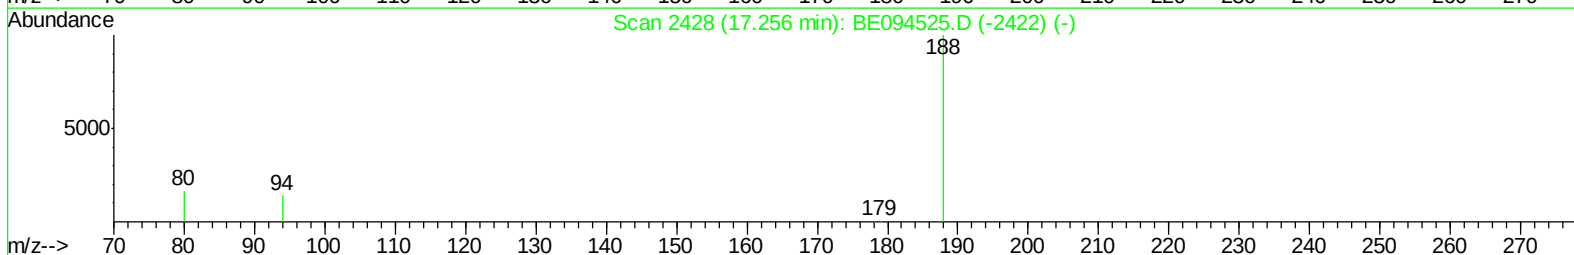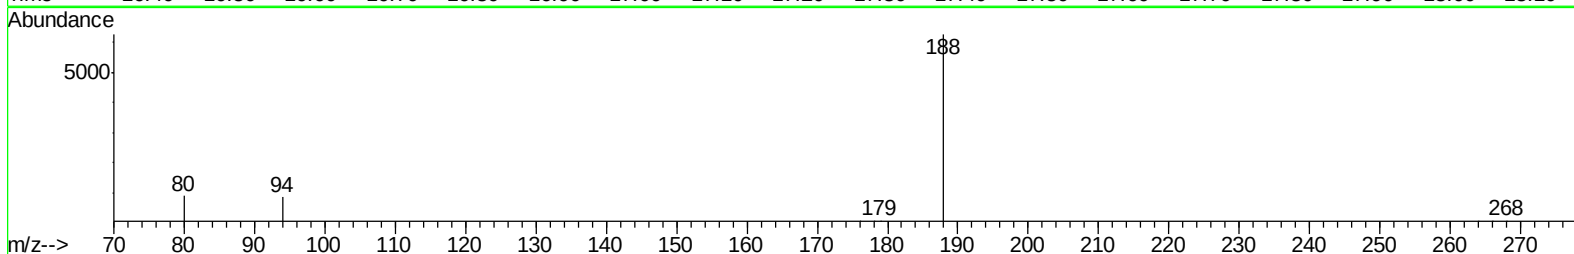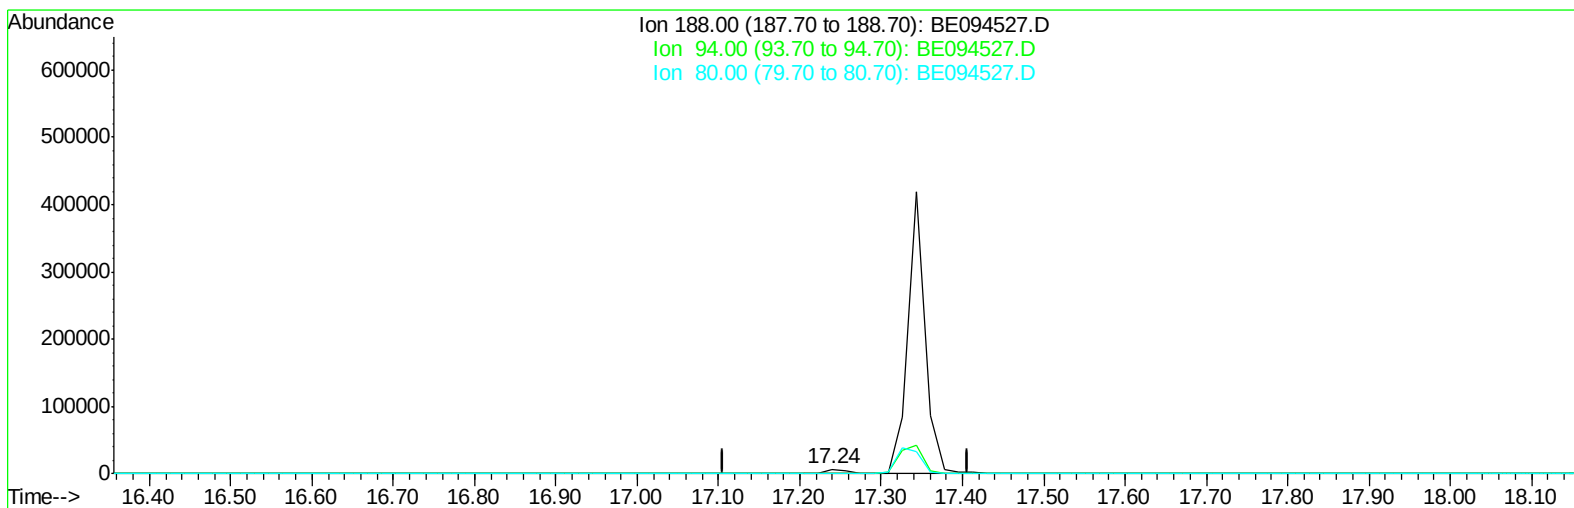

TIC: BE094527.D

(10) Phenanthrene-d10 (I)

17.239min (-0.018) 0.40ng/ul m

response 10748

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.38#
80.00	11.80	14.29#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE102517\
 Data File : BE094527.D
 Acq On : 25 Oct 2017 10:54
 Operator : SJ/JU
 Sample : PB103071BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK71

Manual Integrations
 APPROVED

Sohil
 10/27/2017 8:28:29 AM

Quant Time: Oct 25 18:22:36 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 25 17:03:27 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	1201	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	6970	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.51	164	4733	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.24	188	10748m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.42	240	11017	0.40	ng/ul	0.00
20) Perylene-d12	23.94	264	15685	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	3142	0.28	ng/ul	-0.02
14) Fluoranthene-d10	19.27	212	7716	0.24	ng/ul	-0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE102517\
Data File : BE094527.D
Acq On : 25 Oct 2017 10:54
Operator : SJ/JU
Sample : PB103071BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK71

Manual Integrations
APPROVED

Sohil
10/27/2017 8:28:29 AM

Quant Time: Oct 25 18:22:36 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE102517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 17:03:27 2017
Response via : Initial Calibration

